# Oregon Capacity System

Equipment Configurator Instructions

Use the **Equipment Configurator** to set the inventory for Vents, CRRT and ECMO. Select the icon labeled '**Tile Configure'** and then the '**Equipment Inventory'.** Use the drop-down list to select relevant hospitals and equipment type. Click the blue pencil (edit) icon and type in the quantity and select save.
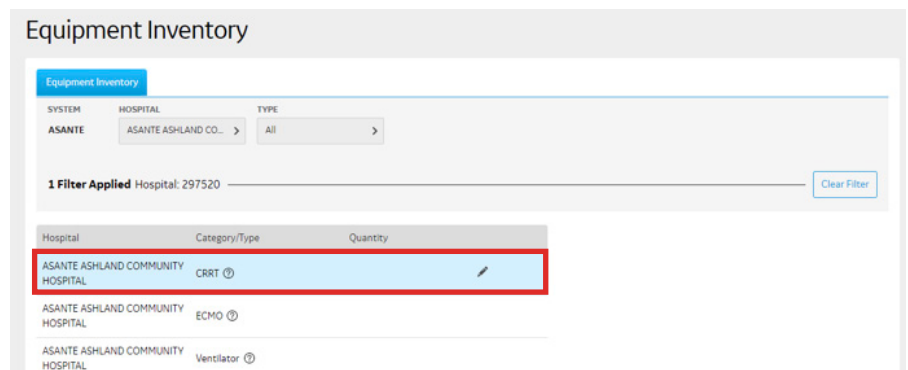
1.

Select **Tile Configure** from Home Page
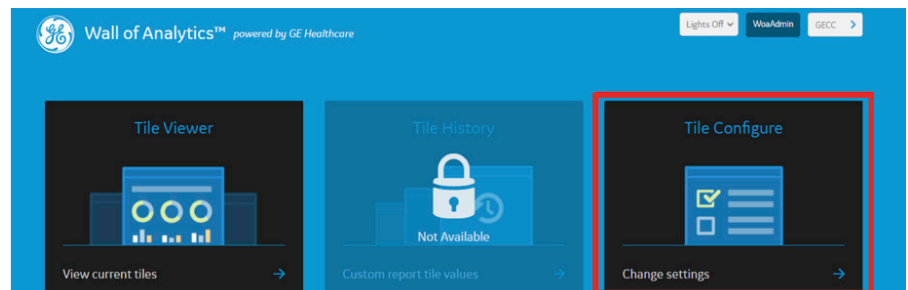
2.

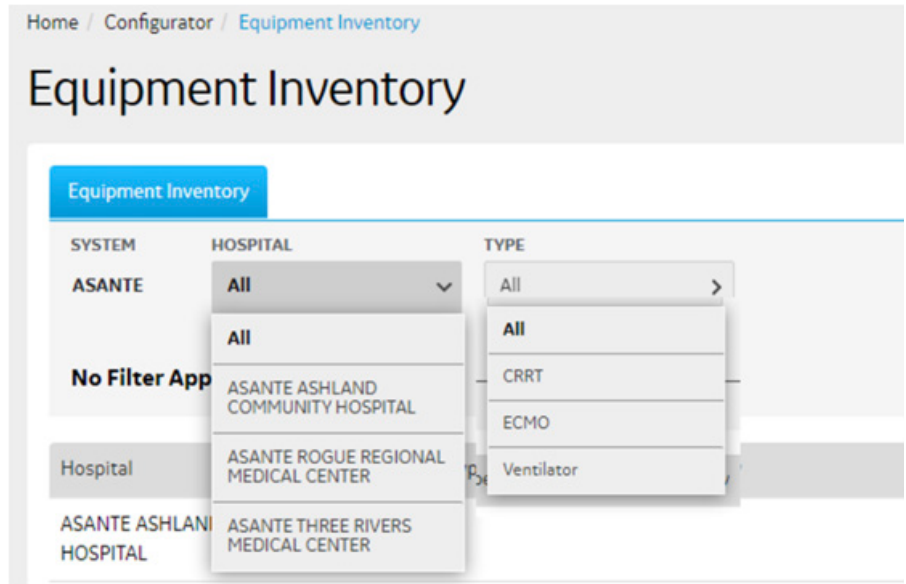Select **Equipment Inventory**
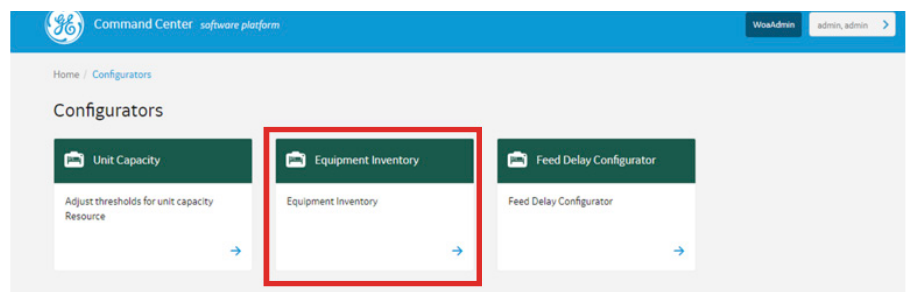
3.

Hover over the hospital you would like to edit and select the pencil icon.

4.

Note: you can use the filters to narrow down our search by hospital and equipment.

5.

Enter the quantity value and select the check mark to save.