



**Direct Nasopharyngeal Swab Procedure**

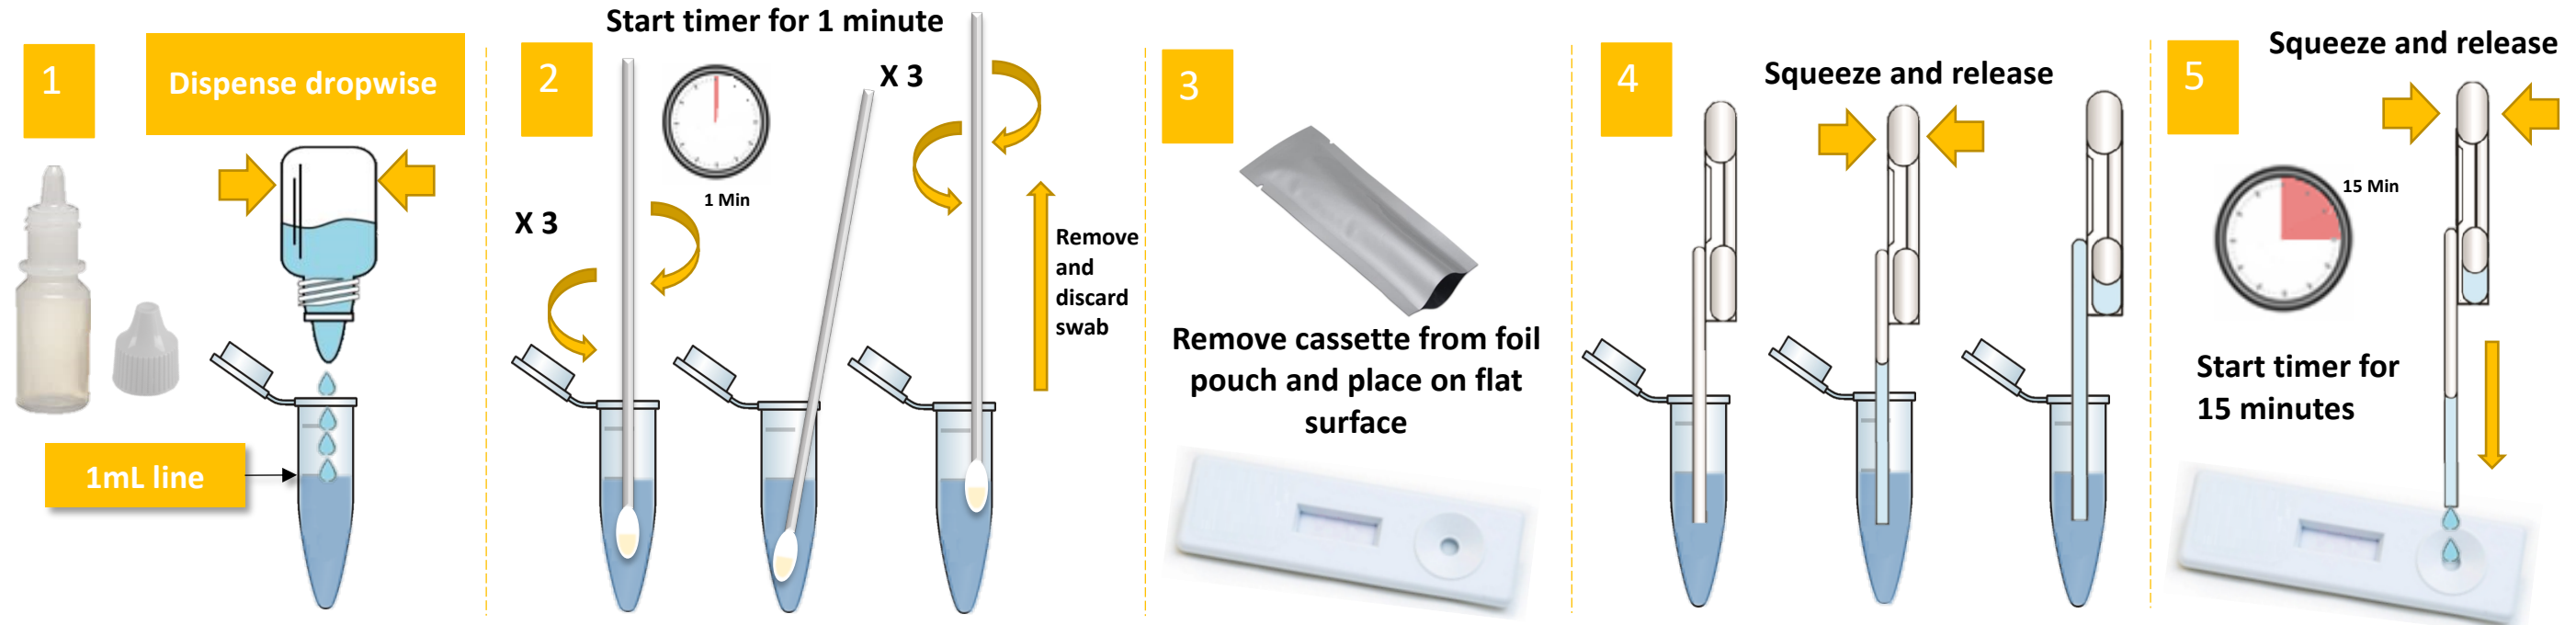


**Positive**

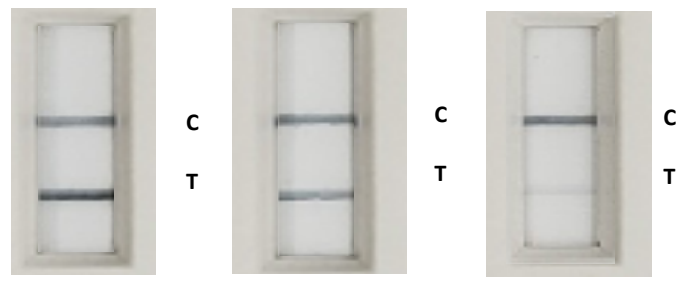

**Negative**



**Invalid**

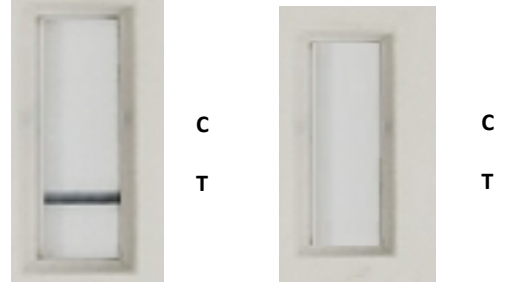

T = COVID-19 Test Line

C = Control Line



Consult Instructions for Use



OBELIS S.A  
Bd. General Wahis, 53, 1030 Brussels, Belgium.  
E-mail: mail@obelis.net  
TEL: +32-2-732-59-54 FAX: +32-2-732-60-03




Sona Nanotech  
Dartmouth, NS B2Y 4M9 Canada  
Sonanano.com

**External Control Dropper Bottle Procedure**




**Positive**

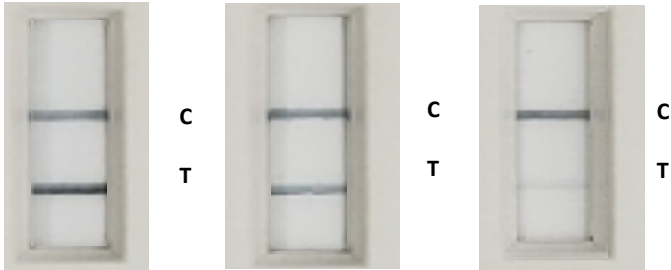

**Negative**



**Invalid**

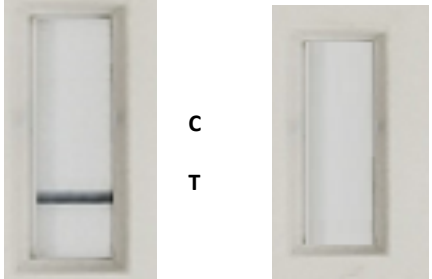

T = COVID-19 Test Line

C = Control Line



Consult Instructions for Use



OBELIS S.A  
Bd. General Wahis, 53, 1030 Brussels, Belgium.  
E-mail: mail@obelis.net  
TEL: +32-2-732-59-54 FAX: +32-2-732-60-03



Sona Nanotech  
Dartmouth, NS B2Y 4M9 Canada  
Sonanano.com