



I'm not a robot





Continue

Relion thermometer 06429 manual



TAKING A RECTAL TEMPERATURE Rectal temperatures should only be taken when it is impossible or impractical to take an oral or axillary temperature. THE THERMOMETER TIP SHOULD BE INSERTED A MAXIMUM OF 1/2" INTO THE RECTUM. The temperature reading should take approximately sixty seconds. The unit will continue to flash during the reading of the temperature. When the peak temperature has been reached, the unit will stop flashing and the thermometer will sound four long beeps if the temperature is below 99.5°F. If the temperature is above 99.5°F the unit will sound four sets of three short beeps each.

To turn the unit off, press the ON/OFF button. The unit will automatically power down after approximately ten minutes. **REMEMBER:** Rectal temperatures are generally 1.0°F higher than oral readings. **USING DISPOSABLE THERMOMETER TIP COVERS** It is recommended to use disposable thermometer tip covers in order to prevent cross-contamination. ReliOn® thermometer tip covers can be purchased from your local Wal-Mart retailer or with the order form provided. **CHANGING THE BATTERY** The battery in your digital thermometer needs to be replaced when " " appears in the lower right of the display. Replace the battery with an LR41 alkaline or SR41 silver oxide type. To replace the battery, slide the battery cap away from the unit. Remove the battery using a non-metal tool. Insert the new battery with the positive (+) side facing up. Carefully slide the battery cap back into place. **SPECIFICATIONS** **DISPLAY:** LIQUID CRYSTAL DISPLAY **RESOLUTION:** 4 DIGITS **(1/10 CFA DEGREE INCLEMENTS)** **MEASUREMENT RANGE:** 89.6°F to 111.2°F **ACCURACY:** ±0.2°F **BETWEEN** 95.9°F AND 107.6°F **BATTERY:** ONE 1.5V BUTTON SIZE BATTERY LR41 OR EQUIVALENT **BATTERY LIFE:** APPROXIMATELY 24 MONTHS **AUTOMATIC SHUT-OFF:** AFTER APPROXIMATELY TEN MINUTES **OPERATING TEMPERATURE:** 50.0°F - 140.0°F **STORAGE TEMPERATURE:** 14.0°F - 140.0°F **DIMENSIONS:** 5-1/8" X 3/4" X 3/8" **WEIGHT:** 0.38 OUNCES **Specifications** are subject to change without notice. Manufactured for: MABIS Healthcare Inc. 1931 Norman Drive Waukegan, IL 60085 USA **Meets ASTM Standard E1112** Made in China ReliOn® is a trademark under license by MABIS Healthcare Inc. #44-MT-18-F 12/04 © 2004 ReliOn® **PARTS OF YOUR DIGITAL THERMOMETER** BODY TEMPERATURE Body temperature can vary from 97°F to 99°F. The generally accepted "normal" temperature is 98.6°F. Usually your temperature is lower in the morning than in the afternoon. Normal temperature varies according to the location of the temperature reading. While the oral temperature follows the guidelines previously described, a rectal temperature is generally 1.0°F higher. Conversely, an axillary (under the arm) temperature will be 1.0°F lower. **GENERAL CARE AND USE** The thermometer should be held during use. The patient should be seated upright. **TEMPERATURES SHOULD ONLY BE TAKEN UNDER THE SUPERVISION OF AN ADULT.** You can clean your Digital Thermometer by wiping it with soap and water or 70% Isopropyl Alcohol. **THE UNIT MUST NEVER BE SUBMERSED IN ANY LIQUID OR STERILIZED IN ANY WAY (GAS OR STEAM AUTOCLAVES).** Failure to follow these instructions will cause severe damage to your unit and void your warranty. **1.** The thermometer should only be used under the supervision of an adult. **2.** Do not walk, run or talk during temperature taking. **3.** Clean the thermometer before and after each use. **4.** Store the unit in the protective case when not in use. **5.** Do not bite the thermometer tip. **6.** Do not store the unit where it will be exposed to direct sunlight, dust or humidity. Avoid extreme temperatures. **7.** Dropping or subjecting your thermometer to strong shocks should be avoided. **8.** Do not attempt to disassemble the unit, except to replace the battery. **9.** If the unit displays an error message and measurement is not attainable, the unit must be replaced. **NOTE:** Performance of the device may be degraded if operated outside of the stated temperature and humidity range; stored outside of stated temperature and humidity range; thermometer undergoes mechanical shock (drop); patient temperature is below ambient temperature. **OPERATING YOUR DIGITAL THERMOMETER** Press the ON/OFF button to activate the thermometer. The digital display will show the following and the thermometer will beep. This is the LCD display test. This insures all parts of the display are functioning properly. By continuing to hold the button down, the last measured temperature will be displayed until the button is released. Once the button is released or if no reading is stored, an L with a flashing 0°F will appear in the display followed by a brief flash of 97.7°F followed by an L with a flashing 0°F to indicate that the thermometer is ready for measurement. **NOTE:** If the room temperature is above 89.6°F, the room temperature will display instead of the L. **TAKING A ORAL TEMPERATURE** Using the diagram on the right, place the thermometer tip under the tongue as near as possible to the heat pocket. The diagram also shows the temperature variables by not placing the tip in the heat pocket area. The temperature reading should take approximately sixty seconds. The unit will continue to flash during the reading of the temperature. When the peak temperature has been reached, the unit will stop flashing and the thermometer will sound four long beeps if the temperature is below 99.5°F. If the temperature is above 99.5°F the unit will sound four sets of three short beeps each. To turn the unit off, press the ON/OFF button. The unit will automatically power down after approximately ten minutes. **NOTE:** The mouth must remain closed during the measurement to insure accurate readings. **TAKING AN AXILLARY TEMPERATURE** (under the arm) The thermometer tip should be placed under the arm so the tip is touching the skin.

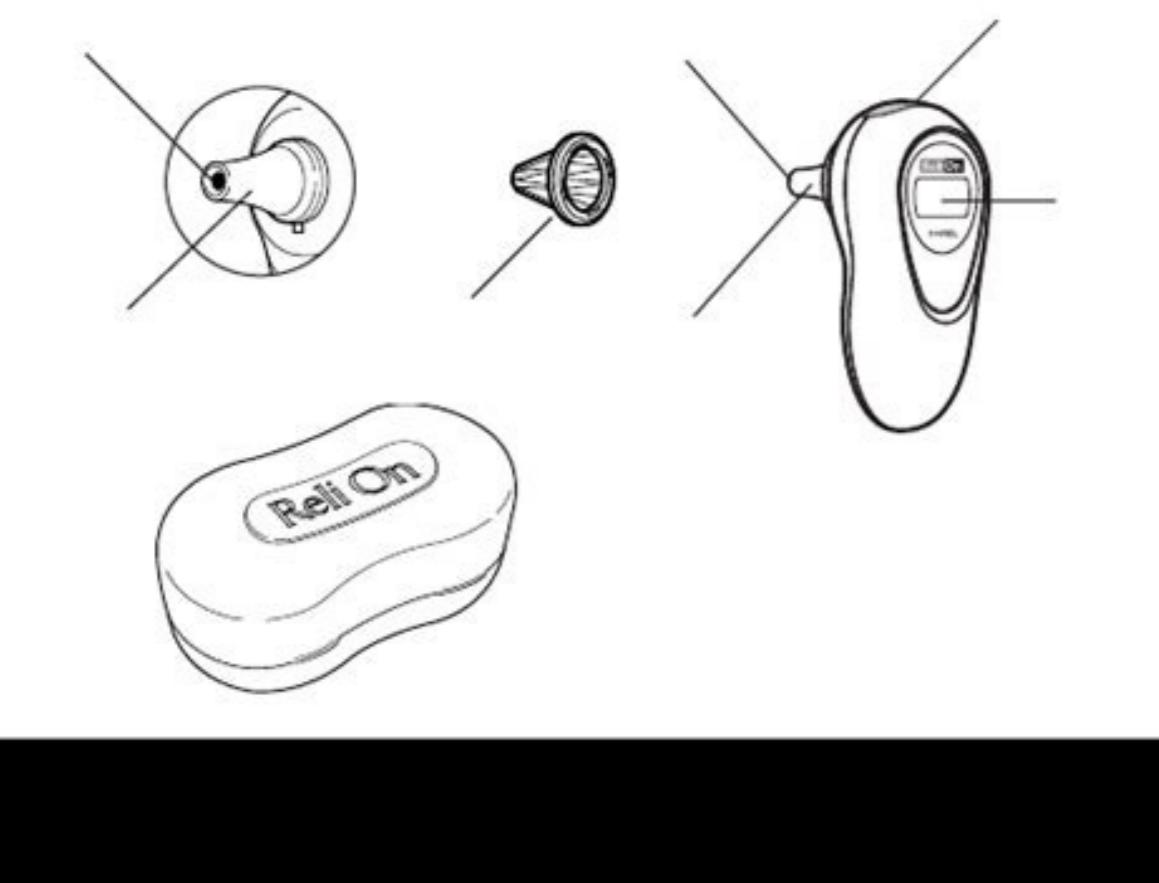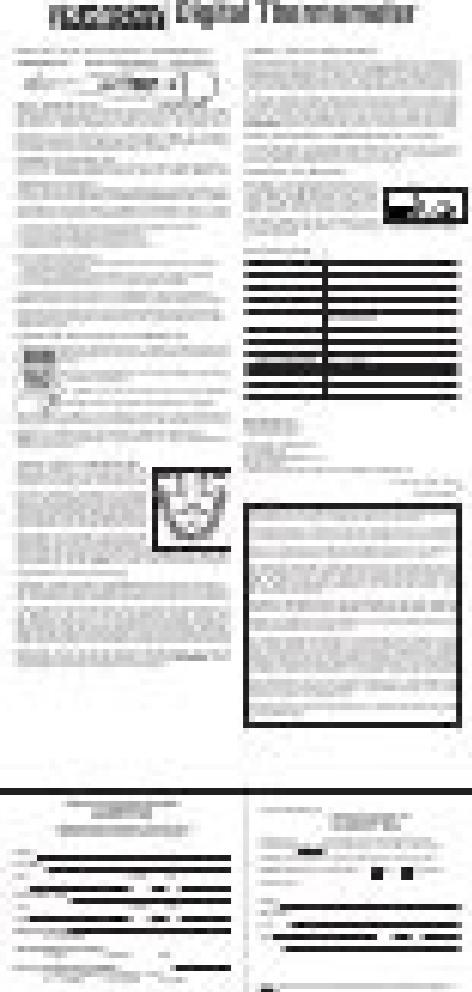

The warrantor shall not be liable to the purchaser for any amount in excess of the cost of repair and/or replacement of the unit, or the purchase price of the unit. Some states do not allow the exclusive or limitation of incidental or consequential damages, so the above limitation or exclusion may not apply to you. This warranty gives you specific legal rights, and you may also have other rights which vary from state to state.

Relion Thermometer 06429 Manual. Web personal care manuals and free healthcare pdf instructions. Web page 1 instruction manual instant ear thermometer please read this detailed guidebook completely before operating this unit. Relion Digital Thermometer Instruction Booklet Manual. Makes it easy from user manual wiki. Web personal care manuals and free healthcare pdf instructions. Web comfier touchless forehead thermometer for adults and kids, infrared digital thermometer for home with fast and. Press and release the scan button. Source: usermanual.wiki Find the personal care product manual that you need at manualsonline. Place the thermometer probe in the center of the temporal area. Source: usermanual.wiki Web relion 60 second digital thermometer relion thermometer 06429 manual.



Between the eye socket and the hairline. Source: usermanual.wikiWeb page 1 instruction manual instant ear thermometer please read this detailed guidebook completely before operating this unit. Web personal care manuals and free healthcare pdf instructions. Source: www.manualsdir.com 4.3 4.3 out of 5 stars (42) \$4.59 \$4. Web thermometer relion digital temple thermometer instructions for use. Web take a measurement in 9 seconds.

