



## Division of Criminal Justice Services

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 107808, performed on November 04, 2019 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Joshua Vinehout".

Digitally signed under ESRA  
by Joshua Vinehout  
on 11/6/2019 12:08 PM

**Joshua Vinehout**  
Supervisor of Public Safety Programs  
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Serial Number: 107808

Date: November 04, 2019

Reference Solution Lot Number: 19180

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.102 %	34.00 degrees centigrade
2	0.102 %	34.00 degrees centigrade
3	0.103 %	34.01 degrees centigrade
4	0.103 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under  
ESRA by Joseph Iavarone  
on 11/4/2019 11:12 AM

**Joseph Iavarone**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 11/6/2019 9:29 AM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department  
Manufacturer: NAT'L PATENT ANALYTICAL SYS  
Model: DATAMASTER DMT  
Serial Number: 107808  
Date: November 04, 2019

1. General Appearance and condition of this device -----: N/A
2. Check controls and indicators -----: OK
3. Check breath flow system -----: OK
4. Check printer operation -----: N/A
5. System cycles through all modes -----: OK
6. Record any repairs made to this instrument and list services provided: **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**


Performed by:



Digitally signed under  
ESRA by Joseph Iavarone  
on 11/4/2019 11:12 AM

**Joseph Iavarone**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 11/6/2019 9:29 AM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

-----  
CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808  
-----

Date: 11/04/2019

Nominal = 0.100 g/210L

BLANK TEST	0.000	10:21
INTERNAL STANDARD	VERIFIED	10:21
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.102	10:22
BLANK TEST	0.000	10:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.102	10:23
BLANK TEST	0.000	10:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.103	10:24
BLANK TEST	0.000	10:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.103	10:25
BLANK TEST	0.000	10:26

Average = 0.1025

Std Dev = 0.0006



## Supervisor Record

Σ3

## Control Test Record

Serial Number: 107808

Test Date: 11/01/2019 10:13:08

Location: 308

CICERO TOWN POLICE DEPT.

## Supervisor Information

First Name: Michael J

Last Name: Serafin

Permit: 37161

Agency: CICERO TOWN PD

## Simulator Information

Lot: 19180 Nominal: 0.100

## Test Results


Alcohol 1: 0.10 34.01

Alcohol 2: 0.10 34.00

Alcohol 3: 0.10 34.00

Solution Change: ☒

Plot 1 of 3 &lt;=&gt;



## Status

Status Code: Date Time: Message:



## Division of Criminal Justice Services

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 107808, performed on May 04, 2020 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Joshua Vinehout".

Digitally signed under  
ESRA by Joshua Vinehout  
on 5/11/2020 3:25 PM

**Joshua Vinehout**  
Supervisor of Public Safety Programs  
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Date: May 04, 2020

Serial Number: 107808

Reference Solution Lot Number: 19281

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.02 degrees centigrade
2	0.100 %	34.02 degrees centigrade
3	0.100 %	34.02 degrees centigrade
4	0.100 %	34.02 degrees centigrade

Reference Solution Lot Number: 20020

Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.079 %	33.97 degrees centigrade
2	0.080 %	33.99 degrees centigrade
3	0.080 %	33.99 degrees centigrade
4	0.080 %	33.98 degrees centigrade

Reference Solution Lot Number: 19210


Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.181 %	33.98 degrees centigrade
2	0.181 %	33.99 degrees centigrade
3	0.181 %	33.99 degrees centigrade
4	0.181 %	33.99 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under  
ESRA by Jonathan Mascolo  
on 5/4/2020 4:12 PM

**Jonathan Mascolo**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 45339

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 5/6/2020 1:47 PM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor


**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department  
Manufacturer: NAT'L PATENT ANALYTICAL SYS  
Model: DATAMASTER DMT  
Serial Number: 107808  
Date: May 04, 2020

1. General Appearance and condition of this device -----: OK
2. Check controls and indicators -----: OK
3. Check breath flow system -----: OK
4. Check printer operation -----: OK
5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.


Performed by:



Digitally signed under  
ESRA by Jonathan Mascolo  
on 5/4/2020 4:12 PM

**Jonathan Mascolo**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 45339

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 5/6/2020 1:47 PM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/04/2020

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 19281

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.099	12:00
BLANK TEST	0.000	12:01
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	12:01
BLANK TEST	0.000	12:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	12:03
BLANK TEST	0.000	12:03
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	12:04
BLANK TEST	0.000	12:05

Average = 0.0998  
Std Dev = 0.0005



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/04/2020

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 20020

Nominal = 0.080 g/210L

BLANK TEST	0.000	11:52
INTERNAL STANDARD	VERIFIED	11:52
REFERENCE STANDARD TEMP	33.97c	
REFERENCE STANDARD	0.079	11:52
BLANK TEST	0.000	11:53
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.080	11:54
BLANK TEST	0.000	11:54
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.080	11:55
BLANK TEST	0.000	11:56
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.080	11:56
BLANK TEST	0.000	11:57

Average = 0.0798  
Std Dev = 0.0005



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/04/2020

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 19210

Nominal = 0.180 g/210L

BLANK TEST	0.000	12:07
INTERNAL STANDARD	VERIFIED	12:07
REFERENCE STANDARD TEMP	33.98c	
REFERENCE STANDARD	0.181	12:08
BLANK TEST	0.000	12:09
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.181	12:09
BLANK TEST	0.000	12:10
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.181	12:10
BLANK TEST	0.000	12:11
REFERENCE STANDARD TEMP	33.99c	
REFERENCE STANDARD	0.181	12:11
BLANK TEST	0.000	12:12

Average = 0.1810  
Std Dev = 0.0000




New York State Division of Criminal Justice Services  
**SERVICE AUTHORIZATION FORM**

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE.

**SECTION I - AGENCY INFORMATION**

Name of Agency Town of Cicero		Today's Date 05/04/20
Address 6200 State Route 31		City, State, ZIP Cicero NY 13039
Contact Person Sgt Steven Amyot		Contact Telephone 315-445-4515
Contact Telephone 315-699-3677	Contact Facsimile 315-699-8128	Contact Email Jasnell@ciceropd.us

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer NPAS		Model Number Datamaster DMT
Instrument Serial Number 107808	Antenna Serial Number (if applicable)	
Date of Malfunction none	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction calibration		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units. All cables and cord including simulator mp4243		
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein.		
Signature 		Date 05/04/20

**DCJS USE ONLY**

Inspected instrument, checked setup voltages print & Remote operation. Performed Calibration/Adjustment procedure, Ran subject, technician & Diagnostic tests, Verified Calibration.





## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 107808, performed on November 04, 2020 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Joshua Vinehout".

Digitally signed under ESRA  
by Joshua Vinehout  
on 11/12/2020 10:09 AM

---

**Joshua Vinehout**  
Supervisor of Public Safety Programs  
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Serial Number: 107808

Date: November 04, 2020

Reference Solution Lot Number: 20340

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.02 degrees centigrade
2	0.100 %	34.02 degrees centigrade
3	0.100 %	34.02 degrees centigrade
4	0.101 %	34.02 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under  
ESRA by Joseph Iavarone  
on 11/4/2020 2:44 PM

**Joseph Iavarone**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 11/5/2020 1:39 PM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department  
Manufacturer: NAT'L PATENT ANALYTICAL SYS  
Model: DATAMASTER DMT  
Serial Number: 107808  
Date: November 04, 2020

1. General Appearance and condition of this device -----: N/A

2. Check controls and indicators -----: OK

3. Check breath flow system -----: OK

4. Check printer operation -----: N/A

5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided: **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**


Performed by:



Digitally signed under  
ESRA by Joseph Iavarone  
on 11/4/2020 2:44 PM

**Joseph Iavarone**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 44106

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 11/5/2020 1:39 PM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

-----  
CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808  
-----

Date: 11/04/2020

Nominal = 0.100 g/210L

BLANK TEST	0.000	14:34
INTERNAL STANDARD	VERIFIED	14:34
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	14:34
BLANK TEST	0.000	14:35
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	14:35
BLANK TEST	0.000	14:36
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.100	14:36
BLANK TEST	0.000	14:37
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.101	14:38
BLANK TEST	0.000	14:38

Average = 0.1003  
Std Dev = 0.0005

## Control Test Record

Serial Number: 107808

Test Date: 10/31/2020 06:42:25

Location: 308

CICERO TOWN POLICE DEPT.

## Supervisor Information

First Name: Michael

Last Name: Serafin

Permit: 37161

Agency: CICERO TOWN PD

## Simulator Information

Lot: 20340

Nominal: 0.100

## Test Results


Alcohol 1: 0.10 34.01

Alcohol 2: 0.10 34.01

Alcohol 3: 0.10 34.02

Solution Change: ☒

Plot 1 of 3



## Status

Status Code:

Date Time:

Message:



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 107808, performed on May 12, 2021 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under  
ESRA by Joshua Vinehout  
on 5/20/2021 8:31 AM

---

**Joshua Vinehout**  
**Supervisor of Public Safety Programs**  
**Office of Public Safety**

An Equal Opportunity/Affirmative Action Agency

# BREATH TEST INSTRUMENT RECORD OF INSPECTION / MAINTENANCE / CALIBRATION

Name of Submitting Agency: Cicero Town Police Department

Manufacturer: NAT'L PATENT ANALYTICAL SYS

Model: DATAMASTER DMT

Date: May 12, 2021

Serial Number: 107808

Reference Solution Lot Number: 20361

Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.099 %	34.01 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.100 %	34.01 degrees centigrade
4	0.100 %	34.00 degrees centigrade

Reference Solution Lot Number: 20470

Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.079 %	34.02 degrees centigrade
2	0.080 %	34.02 degrees centigrade
3	0.079 %	34.02 degrees centigrade
4	0.079 %	34.02 degrees centigrade

Reference Solution Lot Number: 20290

Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.179 %	34.01 degrees centigrade
2	0.179 %	34.01 degrees centigrade
3	0.180 %	34.01 degrees centigrade
4	0.179 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under  
ESRA by Jonathan Mascolo  
on 5/12/2021 3:17 PM

**Jonathan Mascolo**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit # 45339

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 5/17/2021 9:41 AM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Cicero Town Police Department  
**Manufacturer:** NAT'L PATENT ANALYTICAL SYS  
**Model:** DATAMASTER DMT  
**Serial Number:** 107808  
**Date:** May 12, 2021

**1. General Appearance and condition of this device -----: OK**

**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: OK**

**5. System cycles through all modes -----: OK**

**6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

Performed by:



Digitally signed under  
ESRA by Jonathan Mascolo  
on 5/12/2021 3:17 PM

---

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 45339**

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 5/17/2021 9:41 AM

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808





Date: 05/12/2021

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 20361

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:27
INTERNAL STANDARD	VERIFIED	12:28
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:28
BLANK TEST	0.000	12:29
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	12:29
BLANK TEST	0.000	12:30
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.100	12:30
BLANK TEST	0.000	12:31
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.100	12:31
BLANK TEST	0.000	12:32

Average = 0.0995  
Std Dev = 0.0006



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/12/2021

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 20470

Nominal = 0.080 g/210L

BLANK TEST	0.000	12:20
INTERNAL STANDARD	VERIFIED	12:20
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	12:21
BLANK TEST	0.000	12:22
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.080	12:22
BLANK TEST	0.000	12:23
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	12:23
BLANK TEST	0.000	12:24
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.079	12:24
BLANK TEST	0.000	12:25

Average = 0.0792  
Std Dev = 0.0005





# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808





Date: 05/12/2021

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 20290

Nominal = 0.180 g/210L

BLANK TEST	0.000	12:36
INTERNAL STANDARD	VERIFIED	12:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.179	12:36
BLANK TEST	0.000	12:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.179	12:37
BLANK TEST	0.000	12:38
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:38
BLANK TEST	0.000	12:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.179	12:40
BLANK TEST	0.000	12:41

Average = 0.1792  
Std Dev = 0.0005




**SERVICE AUTHORIZATION FORM**  
Highway Safety Technology Unit  
80 South Swan Street  
Albany, NY 12210  
Ph: 518-485-7636 / 518-402-0689  
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

## SECTION I – AGENCY INFORMATION

Name of Agency		Today's Date
Town of Cicero Police Dept.		05/12/2021
Address	City, State, ZIP	
6200 Rte 31	Cicero, NY 13039	
Contact Person	Contact Telephone	
Michael Serafin	315-699-3677 ext216	
Contact Email	Best Way to Reach You During Appointment Period	
mserafin@ciceropd.us	315-247-6318	

## SECTION II—INSTRUMENT INFORMATION

SECTION II - INSTRUMENT INFORMATION					
Instrument Manufacturer (Please Circle) NPAS DMT    GUTH    Applied Concepts (Stalker)    Decatur (Genesis)    Kustom (Eagle/Falcon)    MPH    Alco-Sensor    Other:					
Model Number <b>DataMaster</b>			Instrument Serial Number <b>107808</b>		
Antenna Serial Number (if applicable) Antenna 1 --                                  /    Antenna 2 --				Type of maintenance (check appropriate) <input type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction     					
List all parts, cables and/or accessories being submitted. <b>Tuning forks must accompany all radar units (if applicable).</b> (Please Circle)					
DMT/SIM:  DMT                      SIM                      Tubes  Keyboard                Other:			Radar:  Control Unit              Antenna(s)              Antenna Cable(s)  Power Cord               Forks                      Other:		
<i>I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.</i>					
Signature 			Date <b>05/12/2021</b>		

DCJS USE ONLY

Inspected instrument, checked Setup Voltages Print & Remote Operation. Performed Calibration/Adjustment Procedure, Ran Subject, technician & Diagnostic tests, Verified Calibration.



## Division of Criminal Justice Services

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 107808, performed on November 08, 2021 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance/calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Joshua Vinehout".

Digitally signed under ESRA  
by **Joshua Vinehout**  
on 11/22/2021 7:41 AM

---

**Joshua Vinehout**  
**Supervisor of Public Safety Programs**  
**Office of Public Safety**

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NAT'L PATENT ANALYTICAL SYS**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: November 08, 2021**

**Reference Solution Lot Number: 21280**

**Reference Solution Standard: 0.10 % at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.102 %	34.02 degrees centigrade
2	0.103 %	34.02 degrees centigrade
3	0.102 %	34.02 degrees centigrade
4	0.102 %	34.02 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under  
ESRA by Joseph Iavarone  
on 11/8/2021 2:29 PM

**Joseph Iavarone**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 44106**

Reviewed by:



Digitally signed under  
ESRA by Frank Sgarlata  
on 11/18/2021 6:47 AM

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department  
Manufacturer: NAT'L PATENT ANALYTICAL SYS  
Model: DATAMASTER DMT  
Serial Number: 107808  
Date: November 08, 2021

1. General Appearance and condition of this device -----: N/A
2. Check controls and indicators -----: OK
3. Check breath flow system -----: OK
4. Check printer operation -----: N/A
5. System cycles through all modes -----: OK
6. Record any repairs made to this instrument and list services provided: **CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**



Performed by:

A handwritten signature in cursive script that reads "Joe Iavarone".

Digitally signed under  
ESRA by Joseph Iavarone  
on 11/8/2021 2:29 PM

**Joseph Iavarone**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit # 44106**

Reviewed by:

A handwritten signature in cursive script that reads "Frank Sgarlata".

Digitally signed under  
ESRA by Frank Sgarlata  
on 11/18/2021 6:47 AM

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

-----  
CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808  
-----

Date: 11/08/2021

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:51
INTERNAL STANDARD	VERIFIED	11:51
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.102	11:51
BLANK TEST	0.000	11:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.103	11:52
BLANK TEST	0.000	11:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.102	11:54
BLANK TEST	0.000	11:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.102	11:55
BLANK TEST	0.000	11:56

Average = 0.1022

Std Dev = 0.0005



## Supervisor Record



## Control Test Record

Serial Number: 107808

Test Date: 11/08/2021 11:35:09

Location: 308

CICERO TOWN POLICE DEPT.

## Supervisor Information

First Name: John J

Last Name: Cottrell

Pemit: 35845

Agency: CICERO TOWN PD

## Simulator Information

Lot: 21280 Nominal: 0.100

## Test Results


Alcohol 1: 0.10 34.02

Alcohol 2: 0.10 34.02

Alcohol 3: 0.10 34.02

Solution Change: ☒

Plot 1 of 3 &lt;=&gt;



## Status

Status Code: Date Time: Message:



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 107808, performed on May 03, 2022 by Office of Public Safety employee George Coffin, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA  
by Steven J. Carluccio  
on 05/13/2022 10:12 AM

---

**Steven J. Carluccio**  
**Highway Safety Equipment Technical Supervisor**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: May 03, 2022**

**Reference Solution Lot Number : 21200**

**Reference Solution Standard : 0.10% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.102 %	34.01 degrees centigrade
2	0.103 %	34.01 degrees centigrade
3	0.103 %	34.01 degrees centigrade
4	0.103 %	34.01 degrees centigrade

**Reference Solution Lot Number : 21310**

**Reference Solution Standard : 0.08% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.080 %	34.01 degrees centigrade
2	0.080 %	34.01 degrees centigrade
3	0.081 %	34.01 degrees centigrade
4	0.081 %	34.01 degrees centigrade

**Reference Solution Lot Number : 22060**

**Reference Solution Standard : 0.18% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.183 %	34.01 degrees centigrade
2	0.184 %	34.01 degrees centigrade
3	0.183 %	34.01 degrees centigrade
4	0.184 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by George Coffin  
on 05/03/2022 01:38 PM

Reviewed by:

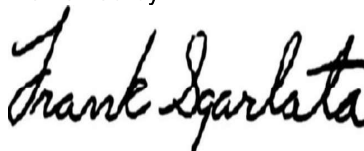

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/03/2022 01:49 PM

**George Coffin**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #48534**

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: May 03, 2022**

**1. General appearance and condition of this device -----: OK**

**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: OK**

**5. System cycles through all modes -----: OK**

**6. Record any repairs made to this instrument and list services provided : INSPECTED  
INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION.  
PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT,  
TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**



Performed by:

A handwritten signature in black ink that reads "George Coffin".

Digitally signed under ESRA  
by George Coffin  
on 05/03/2022 01:38 PM

---

**George Coffin  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #48534**

Reviewed by:

A handwritten signature in black ink that reads "Frank Sgarlata".

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/03/2022 01:49 PM

---

**Frank Sgarlata  
Breath Analysis Technical Supervisor**

# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808





Date: 05/03/2022

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 21310

Nominal = 0.080 g/210L

BLANK TEST	0.000	12:22
INTERNAL STANDARD	VERIFIED	12:22
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	12:23
BLANK TEST	0.000	12:24
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.080	12:24
BLANK TEST	0.000	12:25
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.081	12:25
BLANK TEST	0.000	12:26
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.081	12:26
BLANK TEST	0.000	12:27

Average = 0.0805  
Std Dev = 0.0006





# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/03/2022

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 21200

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:31
INTERNAL STANDARD	VERIFIED	12:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.102	12:32
BLANK TEST	0.000	12:33
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.103	12:33
BLANK TEST	0.000	12:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.103	12:34
BLANK TEST	0.000	12:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.103	12:35
BLANK TEST	0.000	12:36

Average = 0.1028  
Std Dev = 0.0005



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808





Date: 05/03/2022

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 22060

Nominal = 0.180 g/210L

BLANK TEST	0.000	12:39
INTERNAL STANDARD	VERIFIED	12:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	12:39
BLANK TEST	0.000	12:40
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.184	12:41
BLANK TEST	0.000	12:41
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	12:42
BLANK TEST	0.000	12:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.184	12:43
BLANK TEST	0.000	12:44

Average = 0.1835  
Std Dev = 0.0006



# SERVICE AUTHORIZATION FORM

Highway Safety Technology Unit

**Albany, NY 12210**

**Fax: 518-457-6869**

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

## SECTION I - AGENCY INFORMATION

Name of Agency Town of Cicero Police Department		Today's Date 05/03/2022
Address 6200 State Route 31	City, State, ZIP Cicero, NY 13039	
Contact Person Inv Michael Serafin	Contact Telephone 315-247-6318	
Contact Email jasnell@ciceropd.us	Best Way to Reach You During Appointment Period 315-247-6318	

## SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT   GUTH   Applied Concepts (Stalker)   Decatur (Genesis)   Kustom (Eagle/Falcon)   MPH   Alco-Sensor   Other:					
Model Number <b>Datamaster DMT</b>			Instrument Serial Number <b>107808</b>		
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --				Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction					
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)					
DMT/SIM: <div style="display: flex; justify-content: space-around;"> <span><b>DMT</b></span> <span><b>SIM</b></span> <span>Tubes</span> </div> Keyboard      Other:			Radar: <div style="display: grid; grid-template-columns: repeat(3, 1fr); gap: 10px;"> <div>Control Unit</div> <div>Antenna(s)</div> <div>Antenna Cable(s)</div> <div>Power Cord</div> <div>Forks</div> <div>Other:</div> </div>		
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.					
Signature 				Date <b>5/3/22</b>	

## DCJS USE ONLY

Inspected instrument, checked setup voltages print & remote operation. Performed calibration / adjustment procedure, ran subject, technician & diagnostic tests, verified calibration.





## Division of Criminal Justice Services

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of GUTH LABORATORIES, 12V500 SIMULATOR, serial number MP4243, performed on May 03, 2022 by Office of Public Safety employee George Coffin, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio". The signature is written in a cursive style.

Digitally signed under ESRA  
by Steven J. Carluccio  
on 05/13/2022 10:16 AM

---

**Steven J. Carluccio**  
**Highway Safety Equipment Technical Supervisor**  
**Office of Public Safety**

**SIMULATOR  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Cicero Town Police Department

**Manufacturer:** GUTH LABORATORIES

**Model:** 12V500

**Serial Number:** MP4243

**Date:** May 03, 2022

<b>Breath Simulator Temperature</b>
34.03 degrees centigrade



**Division of Criminal  
Justice Services**

**I hereby certify that I have performed any necessary maintenance procedures and verified the calibration of GUTH LABORATORIES simulator model 12V500, serial number MP4243, and have determined that it is accurate.**

**I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified simulator was performed, or within a reasonable time thereafter.**

A handwritten signature in black ink that reads "George Coffin".

Digitally signed under ESRA  
by George Coffin  
on 05/03/2022 02:35 PM

---

**George Coffin  
Highway Safety Equipment Technician  
Office of Public Safety**

**SIMULATOR**  
**RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Cicero Town Police Department

**Manufacturer:** GUTH LABORATORIES

**Model:** 12V500

**Serial Number:** MP4243

**Date:** May 03, 2022

1. General appearance and condition of this device -----: OK

2. Check propeller rotation -----: OK

3. Check for air leaks -----: OK

4. Check for proper temperature -----: OK

5. Record any repairs made to this instrument and list services provided : VERIFIED  
CALIBRATION



Division of Criminal  
Justice Services

A handwritten signature in black ink that reads "George Coffin".

Digitally signed under ESRA  
by George Coffin  
on 05/03/2022 02:35 PM

---

**George Coffin**  
**Highway Safety Equipment Technician**  
**Office of Public Safety**

625 East Bunker Court  
Vernon Hills, Illinois 60061  
PH: 866-466-6225  
Fax: 847-327-2993  
www.innocalsolutions.com

# NIST Traceable Calibration Report



Reference Number: 1405165  
PO Number: SCALUCCIO061421

New York State Division Criminal Justice Services  
80 South Swan Street  
Albany, NY 12210 United States

Manufacturer: Ertco  
Model Number: 4400  
Description: Temperature, Dig thermometer w/probe  
Asset Number: 304011  
Serial Number: 304011  
Procedure: DS Eutechnics 4400-EP642

Calibration Date: 06/17/2021  
Calibration Due Date: 06/17/2022  
Condition As Found: In Tolerance  
Condition As Left: In Tolerance, No adjustment

**Remarks:**

NIST-traceable calibration performed on the unit referenced above in accordance with customer requirements, published specifications and the lab's standard operating procedures. No adjustments were made to the unit.

## Standards Utilized

Asset No.	Manufacturer	Model No.	Description	Cal. Date	Due Date
CP144317	Fluke Corporation	1595A	Thermometer, Readout, Precision Thermometer	01/28/2020	02/28/2022
CP32032	Hart Scientific	5628	Temperature, Probe	10/19/2020	04/30/2022
CP32034	Hart Scientific	5628	Temperature, Probe	01/22/2020	10/31/2021
CP32042	Hart Scientific	5680	Temperature, Probe, SPRT	03/31/2021	04/30/2022
CP53595	Hart Scientific	5628	Temperature, Probe	01/28/2020	02/28/2022

## Calibration Data

FUNCTION TESTED	Nominal Value	As Found	Out of Tol	As Left	Out of Tol	CALIBRATION TOLERANCE
Temperature Accuracy	-15.000 °C	-14.97		Same		-15.050 to -14.950 °C [EMU 0.013 °C][TUR 3.8:1]
	0.000 °C	0.01		Same		-0.030 to 0.030 °C [EMU 0.012 °C][TUR 2.5:1]
	75.000 °C	75.01		Same		74.970 to 75.030 °C [EMU 0.015 °C][TUR 2.0:1]
	125.000 °C	124.99		Same		124.950 to 125.050 °C [EMU 0.015 °C][TUR 3.4:1]

Temperature: 21° C  
Humidity: 49% RH  
Rpt. No.: 1655081

Calibration Performed By:				Quality Reviewer:	
Sittinger, Jennifer	330	Metrologist	847-327-5317	Ziegler, Jeff	06/18/2021
Name	ID #	Title	Phone	Name	Date

This report may not be reproduced, except in full, without written permission of Innocal. The results stated in this report relate only to the items tested or calibrated. Measurements reported herein are traceable to SI units via national standards maintained by NIST and were performed in compliance with MIL-STD-45662A, ANSI/ASCE Z540-1-1994, 10CFR50, Appendix B, ISO 9002-94, and ISO 17025:2017. Guard Banding, if reported on this certificate, is applied at a Z-factor of 30% for test points with a test uncertainty ratio (TUR) below 4:1. In Tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The estimated measurement uncertainty (EMU), if reported on this certificate, is being reported at a confidence level of 95% or K=2 unless otherwise noted in the remarks section.



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 107808, performed on May 09, 2023 by Office of Public Safety employee George Coffin, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA  
by Steven J. Carluccio  
on 05/16/2023 11:29 AM

---

**Steven J. Carluccio**  
**Highway Safety Equipment Technical Supervisor**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: May 09, 2023**

**Reference Solution Lot Number : 23050**

**Reference Solution Standard : 0.10% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.098 %	34.01 degrees centigrade
2	0.098 %	34.01 degrees centigrade
3	0.098 %	34.01 degrees centigrade
4	0.099 %	34.01 degrees centigrade

**Reference Solution Lot Number : 22210**

**Reference Solution Standard : 0.08% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.079 %	34.00 degrees centigrade
2	0.078 %	34.00 degrees centigrade
3	0.079 %	34.00 degrees centigrade
4	0.079 %	34.00 degrees centigrade

**Reference Solution Lot Number : 22450**

**Reference Solution Standard : 0.18% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.179 %	34.00 degrees centigrade
2	0.180 %	34.00 degrees centigrade
3	0.180 %	34.00 degrees centigrade
4	0.181 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by George Coffin  
on 05/09/2023 02:24 PM

Reviewed by:

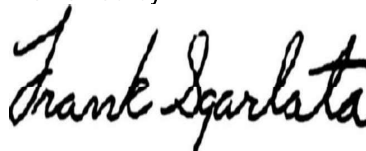

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/10/2023 08:28 AM

**George Coffin**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #48534**

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: May 09, 2023**

**1. General appearance and condition of this device -----: OK**

**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: OK**

**5. System cycles through all modes -----: OK**

**6. Record any repairs made to this instrument and list services provided : INSPECTED  
INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION.  
PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT,  
TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**



Performed by:

A handwritten signature in black ink that reads "George Coffin".

Digitally signed under ESRA  
by George Coffin  
on 05/09/2023 02:24 PM

---

**George Coffin  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #48534**

Reviewed by:

A handwritten signature in black ink that reads "Frank Sgarlata".

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/10/2023 08:28 AM

---

**Frank Sgarlata  
Breath Analysis Technical Supervisor**

# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/09/2023

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 22210

Nominal = 0.080 g/210L

BLANK TEST	0.000	11:43
INTERNAL STANDARD	VERIFIED	11:43
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	11:44
BLANK TEST	0.000	11:45
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.078	11:45
BLANK TEST	0.000	11:46
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	11:46
BLANK TEST	0.000	11:47
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	11:47
BLANK TEST	0.000	11:48

Average = 0.0788  
Std Dev = 0.0005





# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808





Date: 05/09/2023

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 23050

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:35
INTERNAL STANDARD	VERIFIED	11:35
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	11:36
BLANK TEST	0.000	11:36
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	11:37
BLANK TEST	0.000	11:37
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	11:38
BLANK TEST	0.000	11:39
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	11:39
BLANK TEST	0.000	11:40

Average = 0.0982  
Std Dev = 0.0005



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/09/2023

OPERATOR NAME:  
GEORGE R COFFIN  
Permit #: 48534  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 22450

Nominal = 0.180 g/210L

BLANK TEST	0.000	11:22
INTERNAL STANDARD	VERIFIED	11:22
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.179	11:22
BLANK TEST	0.000	11:23
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.180	11:23
BLANK TEST	0.000	11:24
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.180	11:24
BLANK TEST	0.000	11:25
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.181	11:26
BLANK TEST	0.000	11:26

Average = 0.1800  
Std Dev = 0.0008





GRC  
5/9/23


**SERVICE AUTHORIZATION FORM**  
Highway Safety Technology Unit  
80 South Swan Street  
Albany, NY 12210  
Ph: 518-485-7636 / 518-402-0689  
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

**SECTION I - AGENCY INFORMATION**

Name of Agency Town of Cicero Police Dept.		Today's Date 05/08/2023
Address 6200 Rte 31		City, State, ZIP Cicero, NY 13039
Contact Person Micheal Serafin		Contact Telephone 315-699-3677 ext 247
Contact Email jsnell@ciceronypd.gov		Best Way to Reach You During Appointment Period 315-247-6318

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer (Please Circle) <u>NPAS DMT</u> GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number DMT		Instrument Serial Number 107808
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction calibration		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle) DMT/SIM: <u>DMT</u> <u>SIM</u> <u>mp4243</u> <u>Tubes</u> <u>Keyboard</u> Other: <u>Cables</u>		
Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:		
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. <b>PLEASE SIGN AND DATE.</b>		
Signature 		Date 05/08/2023

**DCJS USE ONLY**

*Inspected instrument, checked setup voltages, print + remote operation. Performed calibration / adjustment procedure, ran subject, technician + diagnostic tests, verified calibration.*


**SERVICE AUTHORIZATION FORM**  
**Highway Safety Technology Unit**  
**80 South Swan Street**  
**Albany, NY 12210**  
**Ph: 518-485-7636 / 518-402-0689**  
**Fax: 518-457-6869**

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

**SECTION I - AGENCY INFORMATION**

Name of Agency <b>Town of Cicero Police Department</b>		Today's Date <b>05/03/2022</b>
Address <b>6200 State Route 31</b>	City, State, ZIP <b>Cicero, NY 13039</b>	
Contact Person <b>Inv Michael Serafin</b>	Contact Telephone <b>315-247-6318</b>	
Contact Email <b>jasnell@ciceropd.us</b>	Best Way to Reach You During Appointment Period <b>315-247-6318</b>	

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer (Please Circle) NPAS DMT   GUTH   Applied Concepts(Stalker)   Decatur(Genesis)   Kustom(Eagle/Falcon)   MPH   Alco-Sensor   Other:		
Model Number <b>12V500</b>	Instrument Serial Number <b>MP4243</b>	
Antenna Serial Number (if applicable) Antenna 1 --                      /   Antenna 2 --	Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: DMT                      SIM                      Tubes Keyboard              Other:	Radar: Control Unit              Antenna(s)              Antenna Cable(s) Power Cord              Forks                      Other:	
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. <b>PLEASE SIGN AND DATE.</b>		
Signature 		Date <b>5/3/22</b>

**DCJS USE ONLY**

Export °C <u>34.02</u>	Digital °C <u>34.03</u>	Thermometer: <u>304011</u>
<u>34.02</u>	<u>34.03</u>	Calibration Due: <u>6/17/22</u>
<u>34.02</u>	<u>34.03</u>	Air Leak Test: <u>OK</u> Propeller Rotation: <u>OK</u>



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 107808, performed on November 02, 2023 by Office of Public Safety employee Joseph Iavarone, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA  
by Steven J. Carluccio  
on 11/13/2023 12:10 PM

---

**Steven J. Carluccio**  
**Highway Safety Equipment Technical Supervisor**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Cicero Town Police Department  
**Manufacturer:** NATL PATENT ANALYTICAL SYSTEM  
**Model:** DATAMASTER DMT  
**Serial Number:** 107808  
**Date:** November 02, 2023


**Reference Solution Lot Number :** 23270  
**Reference Solution Standard :** 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.101 %	34.02 degrees centigrade
2	0.101 %	34.02 degrees centigrade
3	0.102 %	34.02 degrees centigrade
4	0.102 %	34.02 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:




Digitally signed under ESRA  
by Joseph Iavarone  
on 11/02/2023 11:58 AM

---

**Joseph Iavarone**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #44106**

Reviewed by:

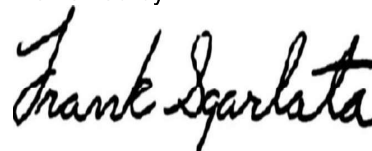

Digitally signed under ESRA  
by Frank Sgarlata  
on 11/02/2023 11:59 AM

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: November 02, 2023**

**1. General appearance and condition of this device -----: N/A**

**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: N/A**

**5. System cycles through all modes -----: OK**

**6. Record any repairs made to this instrument and list services provided : CHECKED REMOTE OPERATION, RAN DIAGNOSTIC AND TECHNICIAN TESTS, VERIFIED CALIBRATION.**



Performed by:

A handwritten signature in black ink that reads "Joe Iavarone".

Digitally signed under ESRA  
by Joseph Iavarone  
on 11/02/2023 11:58 AM

Reviewed by:

A handwritten signature in black ink that reads "Frank Sgarlata".

Digitally signed under ESRA  
by Frank Sgarlata  
on 11/02/2023 11:59 AM

---

**Joseph Iavarone**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #44106**

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

-----  
CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808  
-----

Date: 11/02/2023

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:28
INTERNAL STANDARD	VERIFIED	11:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.101	11:28
BLANK TEST	0.000	11:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.101	11:29
BLANK TEST	0.000	11:30
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.102	11:30
BLANK TEST	0.000	11:31
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.102	11:31
BLANK TEST	0.000	11:32

Average = 0.1015

Std Dev = 0.0006



## Supervisor Record

88

## Control Test Record

Serial Number: 107808

Test Date: 10/31/2023 01:32:44

Location: 308

CICERO TOWN POLICE DEPT.

## Supervisor Information

First Name: Casey

Last Name: Placito

Permit: 47415

Agency: CICERO TOWN PD

## Simulator Information

Lot: 23270

Nominal: 0.100

## Test Results

Alcohol 1: 0.10 34.02


Alcohol 2: 0.10 34.02

Alcohol 3: 0.10 34.02

Solution Change: ☒

Plot 1 of 3

&lt;=&gt;



## Status

Status Code:

Date Time:

Message:



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Martin Schilling, Highway Safety Equipment Technician 2, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 107808, performed on May 03, 2024 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Martin Schilling".

Digitally signed under ESRA  
by Martin Schilling  
on 05/06/2024 10:39 AM

---

**Martin Schilling**  
**Highway Safety Equipment Technician 2**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department  
Manufacturer: NATL PATENT ANALYTICAL SYSTEM  
Model: DATAMASTER DMT  
Serial Number: 107808  
Date: May 03, 2024

Reference Solution Lot Number : 23451  
Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.01 degrees centigrade
2	0.101 %	34.00 degrees centigrade
3	0.101 %	34.01 degrees centigrade
4	0.101 %	34.00 degrees centigrade

Reference Solution Lot Number : 24011  
Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.082 %	34.03 degrees centigrade
2	0.082 %	34.02 degrees centigrade
3	0.082 %	34.02 degrees centigrade
4	0.082 %	34.02 degrees centigrade

Reference Solution Lot Number : 23380  
Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.183 %	34.00 degrees centigrade
2	0.183 %	34.00 degrees centigrade
3	0.182 %	34.00 degrees centigrade
4	0.182 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 05/03/2024 02:51 PM

**Jonathan Mascolo**  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #45339

Reviewed by:



Digitally signed under ESRA  
by Frank Sgarlata  
on 05/03/2024 03:37 PM

**Frank Sgarlata**  
Breath Analysis Technical Supervisor



**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: Cicero Town Police Department  
Manufacturer: NATL PATENT ANALYTICAL SYSTEM  
Model: DATAMASTER DMT  
Serial Number: 107808  
Date: May 03, 2024

1. General appearance and condition of this device -----: OK
2. Check controls and indicators -----: OK
3. Check breath flow system -----: OK
4. Check printer operation -----: OK
5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided : INSPECTED  
INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION.  
PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT,  
TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

**THIS CERTIFICATE EXPIRES 365 DAYS FROM THE DATE AT THE TOP OF THIS  
PAGE.**


Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 05/03/2024 02:51 PM

**Jonathan Mascolo  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #45339**

Reviewed by:

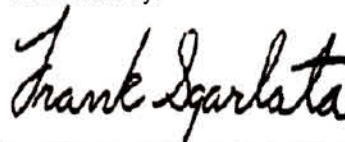

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/03/2024 03:37 PM

**Frank Sgarlata  
Breath Analysis Technical Supervisor**

# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/03/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 24011

Nominal = 0.080 g/210L

BLANK TEST	0.000	10:47
INTERNAL STANDARD	VERIFIED	10:47
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.082	10:47
BLANK TEST	0.000	10:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.082	10:48
BLANK TEST	0.000	10:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.082	10:49
BLANK TEST	0.000	10:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.082	10:50
BLANK TEST	0.000	10:51

Average = 0.0820  
Std Dev = 0.0000



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/03/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 23451

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:04
INTERNAL STANDARD	VERIFIED	11:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.100	11:04
BLANK TEST	0.000	11:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	11:05
BLANK TEST	0.000	11:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.101	11:06
BLANK TEST	0.000	11:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	11:08
BLANK TEST	0.000	11:08

Average = 0.1008  
Std Dev = 0.0005





# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/03/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 23380

Nominal = 0.180 g/210L

BLANK TEST	0.000	11:11
INTERNAL STANDARD	VERIFIED	11:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.183	11:11
BLANK TEST	0.000	11:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.183	11:12
BLANK TEST	0.000	11:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.182	11:14
BLANK TEST	0.000	11:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.182	11:15
BLANK TEST	0.000	11:16

Average = 0.1825  
Std Dev = 0.0006






**SERVICE AUTHORIZATION FORM**  
Highway Safety Technology Unit  
80 South Swan Street  
Albany, NY 12210  
Ph: 518-485-7636 / 518-402-0689  
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

## SECTION I - AGENCY INFORMATION

Name of Agency Town of Cicero Police Dept.		Today's Date 05/03/2024
Address 6200 Rte 31	City, State, ZIP Cicero, NY 13039	
Contact Person Sean Wallace	Contact Telephone 315-699-3677 ext 258	
Contact Email swallace@ciceronypd.gov	Best Way to Reach You During Appointment Period 315-664-2755	

## SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle)		MPH		Alco-Sensor		Other:	
NPAS DMT		GUTH		Applied Concepts (Stalker)		Decatur (Genesis)	
Kustom (Eagle/Falcon)		MPH		Alco-Sensor		Other:	
Model Number				Instrument Serial Number			
Data master DMT				107808			
Antenna Serial Number (if applicable)						Type of maintenance (check appropriate)	
Antenna 1 --						<input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Antenna 2 --							
Brief Description of Malfunction							
Calibration							
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)							
DMT/SIM:				Radar:			
DMT <input checked="" type="checkbox"/> Keyboard <input checked="" type="checkbox"/> Other:				Control Unit <input type="checkbox"/> Power Cord <input type="checkbox"/> Antenna(s) <input type="checkbox"/> Forks <input type="checkbox"/> Antenna Cable(s) <input type="checkbox"/> Other:			
Tubes <input checked="" type="checkbox"/> Breath tube <input checked="" type="checkbox"/> Simulator tube <input checked="" type="checkbox"/>							
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.							
Signature						Date	
						05/03/2024	

DCJS USE ONLY

Inspected instrument, checked setup voltages, print and remote operation. Performed calibration/adjustment procedure, ran subject, technician and diagnostic tests, verified calibration.

\* @ 5-3-24



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Martin Schilling, Highway Safety Equipment Technician 2, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 107808, performed on May 03, 2024 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Martin Schilling".

Digitally signed under ESRA  
by Martin Schilling  
on 05/06/2024 10:39 AM

---

**Martin Schilling**  
**Highway Safety Equipment Technician 2**  
**Office of Public Safety**



**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Cicero Town Police Department

**Manufacturer:** NATL PATENT ANALYTICAL SYSTEM

**Model:** DATAMASTER DMT

**Serial Number:** 107808

**Date:** May 03, 2024

**Reference Solution Lot Number :** 23451

**Reference Solution Standard :** 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.100 %	34.01 degrees centigrade
2	0.101 %	34.00 degrees centigrade
3	0.101 %	34.01 degrees centigrade
4	0.101 %	34.00 degrees centigrade

**Reference Solution Lot Number :** 24011

**Reference Solution Standard :** 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.082 %	34.03 degrees centigrade
2	0.082 %	34.02 degrees centigrade
3	0.082 %	34.02 degrees centigrade
4	0.082 %	34.02 degrees centigrade

**Reference Solution Lot Number :** 23380

**Reference Solution Standard :** 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.183 %	34.00 degrees centigrade
2	0.183 %	34.00 degrees centigrade
3	0.182 %	34.00 degrees centigrade
4	0.182 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 05/03/2024 02:51 PM

Reviewed by:

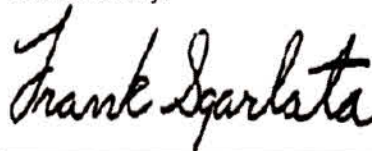

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/03/2024 03:37 PM

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #45339**

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency:** Cicero Town Police Department

**Manufacturer:** NATL PATENT ANALYTICAL SYSTEM

**Model:** DATAMASTER DMT

**Serial Number:** 107808

**Date:** May 03, 2024

1. General appearance and condition of this device -----: OK

2. Check controls and indicators -----: OK

3. Check breath flow system -----: OK

4. Check printer operation -----: OK

5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided : INSPECTED  
INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION.  
PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT,  
TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

**THIS CERTIFICATE EXPIRES 365 DAYS FROM THE DATE AT THE TOP OF THIS  
PAGE.**


Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 05/03/2024 02:51 PM

**Jonathan Mascolo  
Highway Safety Equipment Technician  
Breath Analysis Operator Permit #45339**

Reviewed by:

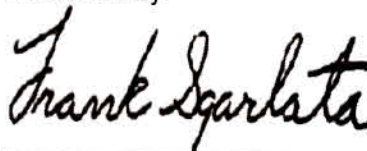

Digitally signed under ESRA  
by Frank Sgarlata  
on 05/03/2024 03:37 PM

**Frank Sgarlata  
Breath Analysis Technical Supervisor**



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/03/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 24011

Nominal = 0.080 g/210L

BLANK TEST	0.000	10:47
INTERNAL STANDARD	VERIFIED	10:47
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.082	10:47
BLANK TEST	0.000	10:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.082	10:48
BLANK TEST	0.000	10:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.082	10:49
BLANK TEST	0.000	10:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.082	10:50
BLANK TEST	0.000	10:51

Average = 0.0820  
Std Dev = 0.0000



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 05/03/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 23451

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:04
INTERNAL STANDARD	VERIFIED	11:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.100	11:04
BLANK TEST	0.000	11:05
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	11:05
BLANK TEST	0.000	11:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.101	11:06
BLANK TEST	0.000	11:07
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.101	11:08
BLANK TEST	0.000	11:08

Average = 0.1008  
Std Dev = 0.0005



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808





Date: 05/03/2024

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 23380

Nominal = 0.180 g/210L

BLANK TEST	0.000	11:11
INTERNAL STANDARD	VERIFIED	11:11
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.183	11:11
BLANK TEST	0.000	11:12
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.183	11:12
BLANK TEST	0.000	11:13
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.182	11:14
BLANK TEST	0.000	11:14
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.182	11:15
BLANK TEST	0.000	11:16

Average = 0.1825  
Std Dev = 0.0006






**SERVICE AUTHORIZATION FORM**  
Highway Safety Technology Unit  
80 South Swan Street  
Albany, NY 12210  
Ph: 518-485-7636 / 518-402-0689  
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

**SECTION I - AGENCY INFORMATION**

Name of Agency Town of Cicero Police Dept.		Today's Date 05/03/2024
Address 6200 Rte 31	City, State, ZIP Cicero, NY 13039	
Contact Person Sean Wallace	Contact Telephone 315-699-3677 ext 258	
Contact Email swallace@ciceronypd.gov	Best Way to Reach You During Appointment Period 315-664-2755	

**SECTION II - INSTRUMENT INFORMATION**

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts (Stalker) Decatur (Genesis) Kustom (Eagle/Falcon) MPH Alco-Sensor Other:			
Model Number DataMaster DMT		Instrument Serial Number 107808	
Antenna Serial Number (if applicable) Antenna 1 - / Antenna 2 -		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction Calibration			
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)			
DMT/SIM: DMT SIM Keyboard Other:		Radar: Control Unit Antenna(s) Antenna Cable(s) Power Cord Forks Other:	
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. <b>PLEASE SIGN AND DATE.</b>			
Signature 		Date 05/03/2024	

**DCJS USE ONLY**

Inspected instrument, checked setup voltages, print and remote operation. Performed calibration/adjustment procedure, ran subject, technician and diagnostic tests, verified calibration.  *@ 5-3-24
---



## Division of Criminal Justice Services

---

### **CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Martin Schilling, Highway Safety Equipment Technician 2, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 107808, performed on April 28, 2025 by Office of Public Safety employee Jonathan Mascolo, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink, appearing to read "Martin Schilling".

Digitally signed under ESRA  
by Martin Schilling  
on 04/28/2025 01:19 PM

---

**Martin Schilling**  
**Highway Safety Equipment Technician 2**  
**Office of Public Safety**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**

**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**

**Model: DATAMASTER DMT**

**Serial Number: 107808**

**Date: April 28, 2025**

**Reference Solution Lot Number : 24371**

**Reference Solution Standard : 0.10% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.099 %	34.02 degrees centigrade
2	0.098 %	34.03 degrees centigrade
3	0.098 %	34.02 degrees centigrade
4	0.098 %	34.02 degrees centigrade

**Reference Solution Lot Number : 24421**

**Reference Solution Standard : 0.08% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.080 %	34.00 degrees centigrade
2	0.079 %	34.00 degrees centigrade
3	0.079 %	34.00 degrees centigrade
4	0.080 %	34.00 degrees centigrade

**Reference Solution Lot Number : 24290**

**Reference Solution Standard : 0.18% at 34.0 degrees centigrade**

Test No	Test Result	Simulator Temperature
1	0.180 %	34.01 degrees centigrade
2	0.180 %	34.01 degrees centigrade
3	0.180 %	34.01 degrees centigrade
4	0.180 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 107808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA  
by Jonathan Mascolo  
on 04/28/2025 12:50 PM

Reviewed by:

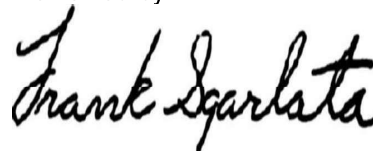

Digitally signed under ESRA  
by Frank Sgarlata  
on 04/28/2025 01:14 PM

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #45339**

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**

**BREATH TEST INSTRUMENT  
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

**Name of Submitting Agency: Cicero Town Police Department**  
**Manufacturer: NATL PATENT ANALYTICAL SYSTEM**  
**Model: DATAMASTER DMT**  
**Serial Number: 107808**  
**Date: April 28, 2025**

**1. General appearance and condition of this device -----: OK**

**2. Check controls and indicators -----: OK**

**3. Check breath flow system -----: OK**

**4. Check printer operation -----: OK**

**5. System cycles through all modes -----: OK**

**6. Record any repairs made to this instrument and list services provided : INSPECTED  
INSTRUMENT, CHECKED SETUP VOLTAGES, PRINT AND REMOTE OPERATION.  
PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT,  
TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.**

**THIS CERTIFICATE EXPIRES 365 DAYS FROM THE DATE AT THE TOP OF THIS  
PAGE.**

Performed by:




Digitally signed under ESRA  
by Jonathan Mascolo  
on 04/28/2025 12:50 PM

---

**Jonathan Mascolo**  
**Highway Safety Equipment Technician**  
**Breath Analysis Operator Permit #45339**

Reviewed by:

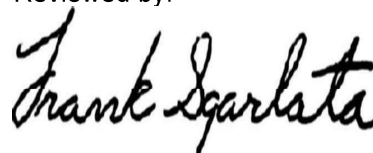

Digitally signed under ESRA  
by Frank Sgarlata  
on 04/28/2025 01:14 PM

---

**Frank Sgarlata**  
**Breath Analysis Technical Supervisor**



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 04/28/2025

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 24421

Nominal = 0.080 g/210L

BLANK TEST	0.000	11:52
INTERNAL STANDARD	VERIFIED	11:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	11:53
BLANK TEST	0.000	11:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	11:54
BLANK TEST	0.000	11:55
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.079	11:55
BLANK TEST	0.000	11:56
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.080	11:56
BLANK TEST	0.000	11:57

Average = 0.0795  
Std Dev = 0.0006



# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 04/28/2025

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 24371

Nominal = 0.100 g/210L

BLANK TEST	0.000	12:00
INTERNAL STANDARD	VERIFIED	12:00
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.099	12:01
BLANK TEST	0.000	12:01
REFERENCE STANDARD TEMP	34.03c	
REFERENCE STANDARD	0.098	12:02
BLANK TEST	0.000	12:02
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.098	12:03
BLANK TEST	0.000	12:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.098	12:04
BLANK TEST	0.000	12:05

Average = 0.0982  
Std Dev = 0.0005





# TECHNICIAN TEST

CICERO TOWN  
POLICE DEPT  
DATAMASTER dmt: 107808


Date: 04/28/2025

OPERATOR NAME:  
JONATHAN M MASCOLO  
Permit #: 45339  
Operator Agency/Dept: CICERO TOWN PD  
Reference Standard #: 24290

Nominal = 0.180 g/210L

BLANK TEST	0.000	12:07
INTERNAL STANDARD	VERIFIED	12:08
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:08
BLANK TEST	0.000	12:09
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:09
BLANK TEST	0.000	12:10
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:10
BLANK TEST	0.000	12:11
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.180	12:12
BLANK TEST	0.000	12:12

Average = 0.1800  
Std Dev = 0.0000






**SERVICE AUTHORIZATION FORM**  
Highway Safety Technology Unit  
80 South Swan Street  
Albany, NY 12210  
Ph: 518-485-7636 / 518-402-0689  
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

## SECTION I - AGENCY INFORMATION

Name of Agency		Today's Date	
Town of Cicero Police Dept.		04/28/2025	
Address		City, State, ZIP	
6200 Rte 31		Cicero, NY 13039	
Contact Person		Contact Telephone	
Kyle Harrington		315-699-3677 ext 247	
Contact Email		Best Way to Reach You During Appointment Period	
kharrington@ciceronypd.gov		315-447-3514	

## SECTION II—INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle)			
NPAS DMT	GUTH	Applied Concepts (Stalker)	Decatur (Genesis)
Kustom (Eagle/Falcon)		MPH	Alco-Sensor
Other:			
Model Number		Instrument Serial Number	
DMT		107808	
Antenna Serial Number (if applicable)		Type of maintenance (check appropriate)	
Antenna 1 -- / Antenna 2 --		<input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair	
Brief Description of Malfunction			
calibration			
List all parts, cables and/or accessories being submitted. <b>Tuning forks must accompany all radar units (if applicable).</b> (Please Circle)			
DMT/SIM:		Radar:	
DMT	SIM	Control Unit	Antenna(s)
Keyboard	Other:	Power Cord	Forks
Tubes Simulator take		Other:	
I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. <b>PLEASE SIGN AND DATE.</b>			
Signature		Date	
		04/27/2025	

DCJS USE ONLY

Inspected instrument, checked setup voltages, print and remote operation.  
Performed calibration/adjustment procedure, ran subject, technician & diagnostic tests, verified calibration. \* @ 4-28-25