SUPERVISOR TEST


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808

Date: 08/24/2026


OPERATOR NAME:
KYLE A HARRINGTON
Permit #: 48283
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	10:45
INTERNAL STANDARD	VERIFIED	10:45
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	10:45
BLANK TEST	0.00	10:46
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	10:46
BLANK TEST	0.00	10:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	10:47
BLANK TEST	0.00	10:48

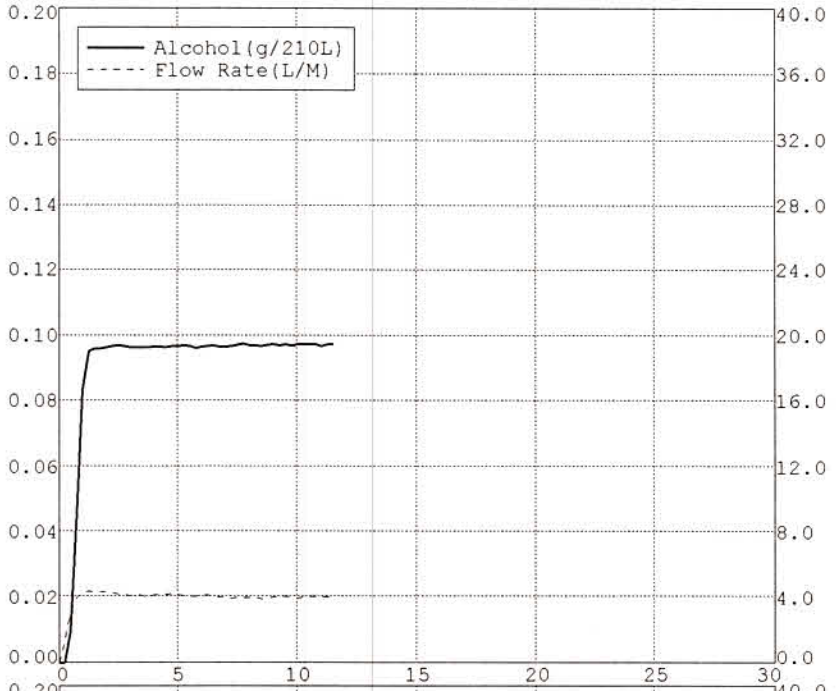



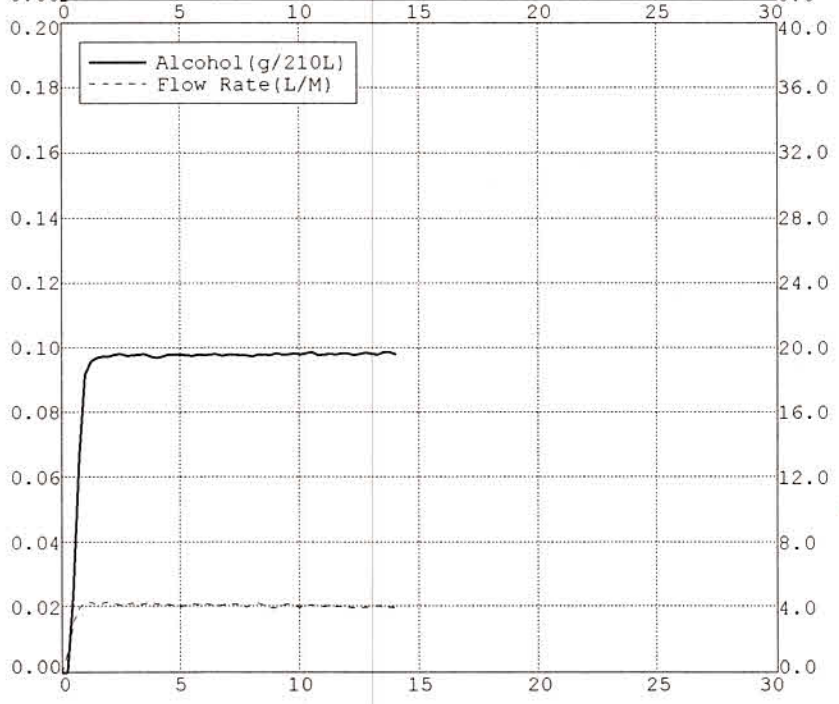

SOLUTION CHANGE


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 09/03/2026


OPERATOR NAME:
KYLE A HARRINGTON
Permit #: 48283
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:53
INTERNAL STANDARD	VERIFIED	23:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:53
BLANK TEST	0.00	23:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:55
BLANK TEST	0.00	23:55
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:56
BLANK TEST	0.00	23:57

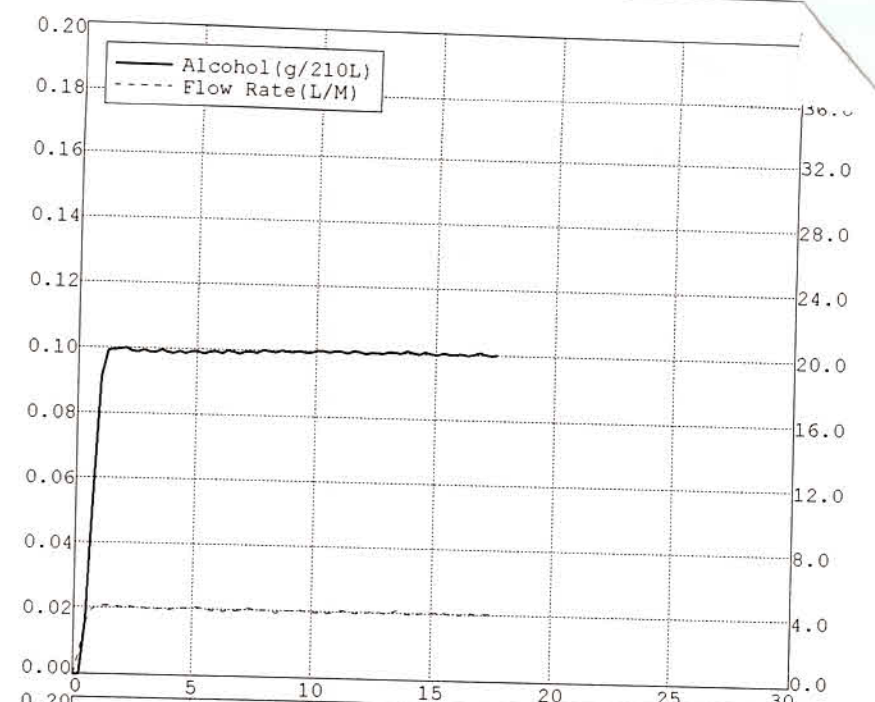

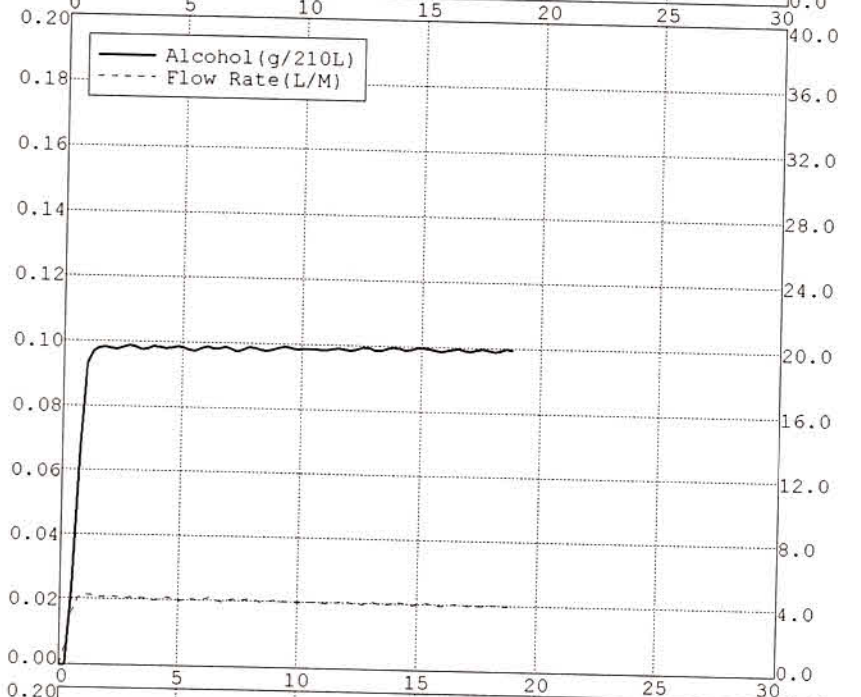

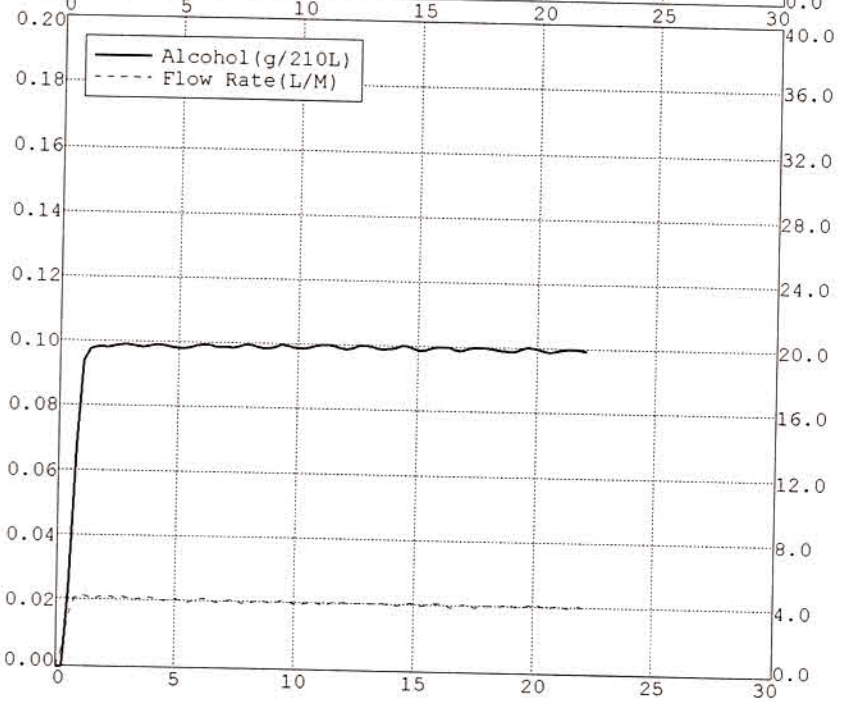

SUPERVISOR TEST

CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 09/09/2026


OPERATOR NAME:
KYLE A HARRINGTON
Permit #: 48283
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	05:53
INTERNAL STANDARD	VERIFIED	05:53
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	05:54
BLANK TEST	0.00	05:54
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	05:55
BLANK TEST	0.00	05:56
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	05:56
BLANK TEST	0.00	05:57



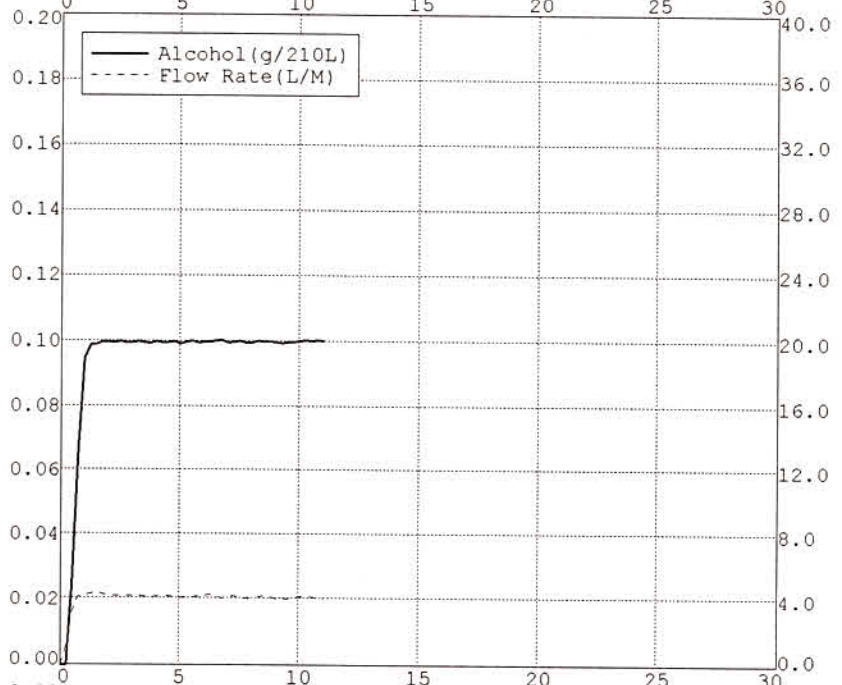

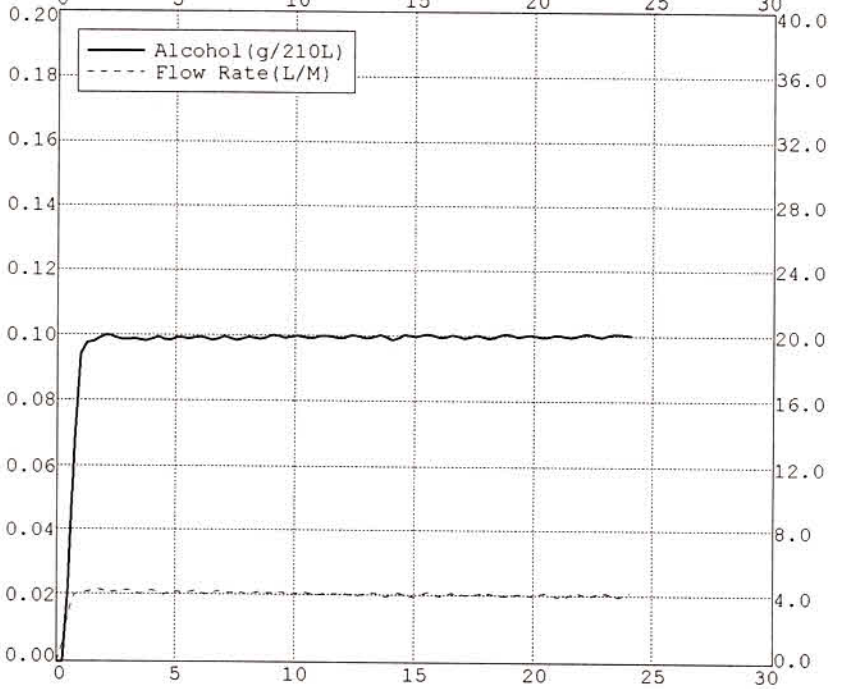

SUPERVISOR TEST


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 09/14/2026


OPERATOR NAME:
KYLE A HARRINGTON
Permit #: 48283
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:07
INTERNAL STANDARD	VERIFIED	22:07
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	22:07
BLANK TEST	0.00	22:08
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:08
BLANK TEST	0.00	22:09
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:10
BLANK TEST	0.00	22:10

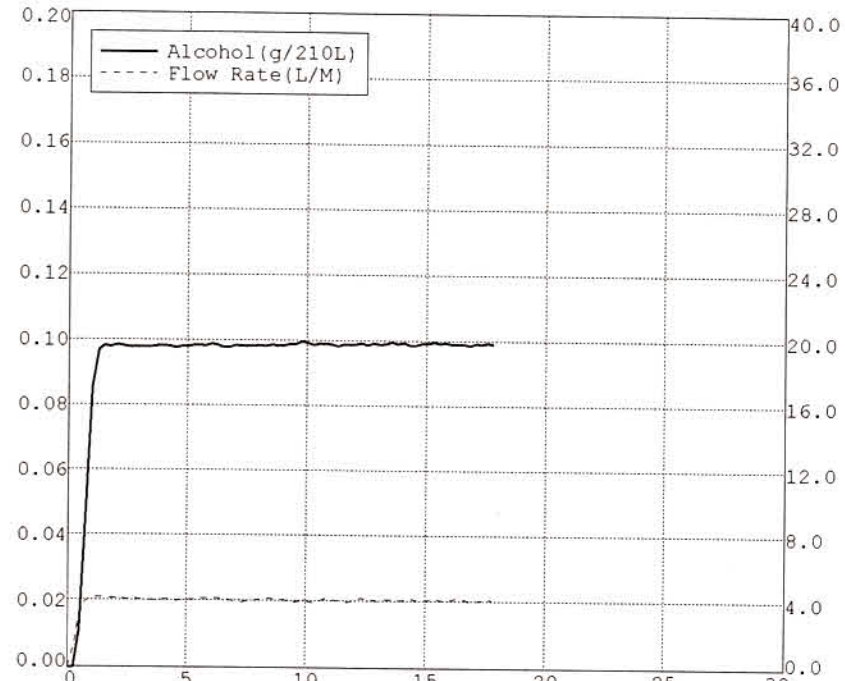

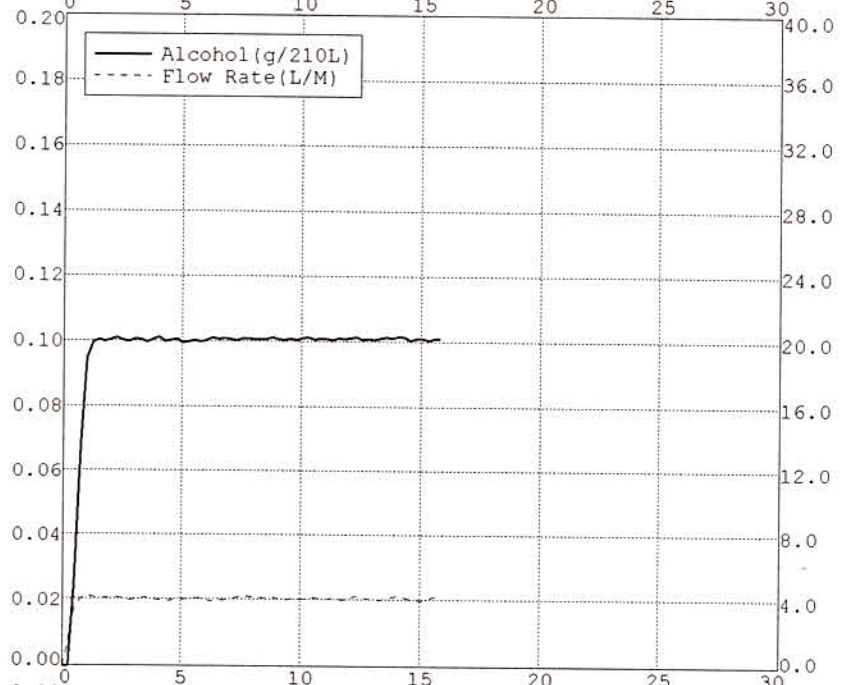

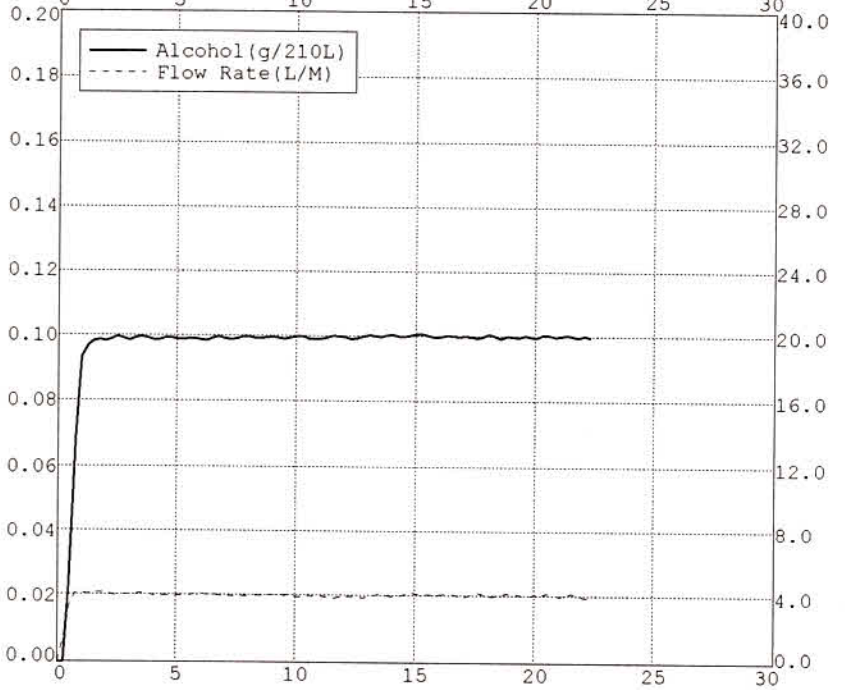

SUPERVISOR TEST


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 09/25/2026


OPERATOR NAME:
CASEY PLACITO
Permit #: 47415
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:04
INTERNAL STANDARD	VERIFIED	14:04
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:04
BLANK TEST	0.00	14:05
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:06
BLANK TEST	0.00	14:06
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:07
BLANK TEST	0.00	14:08

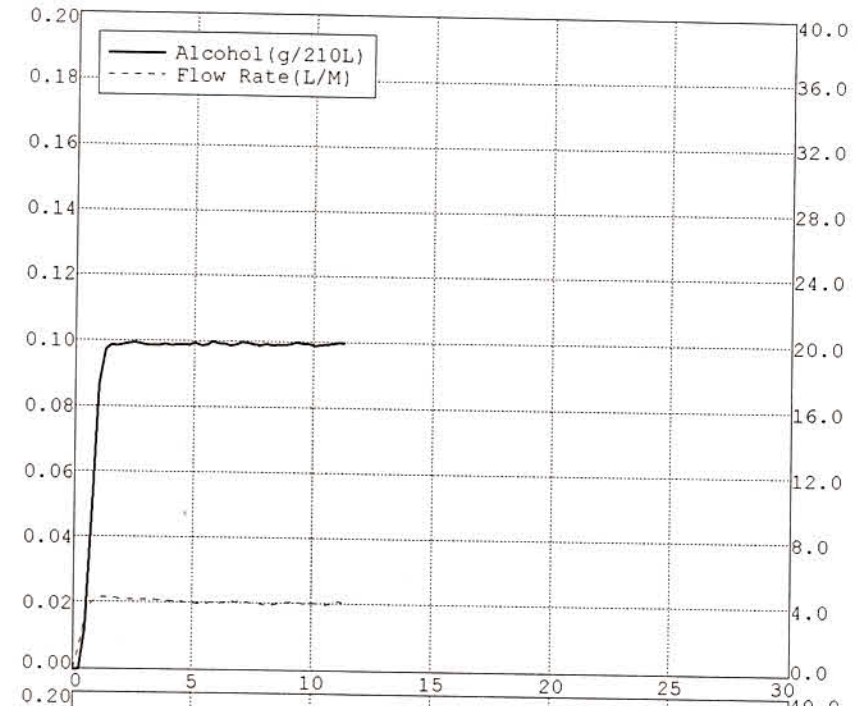

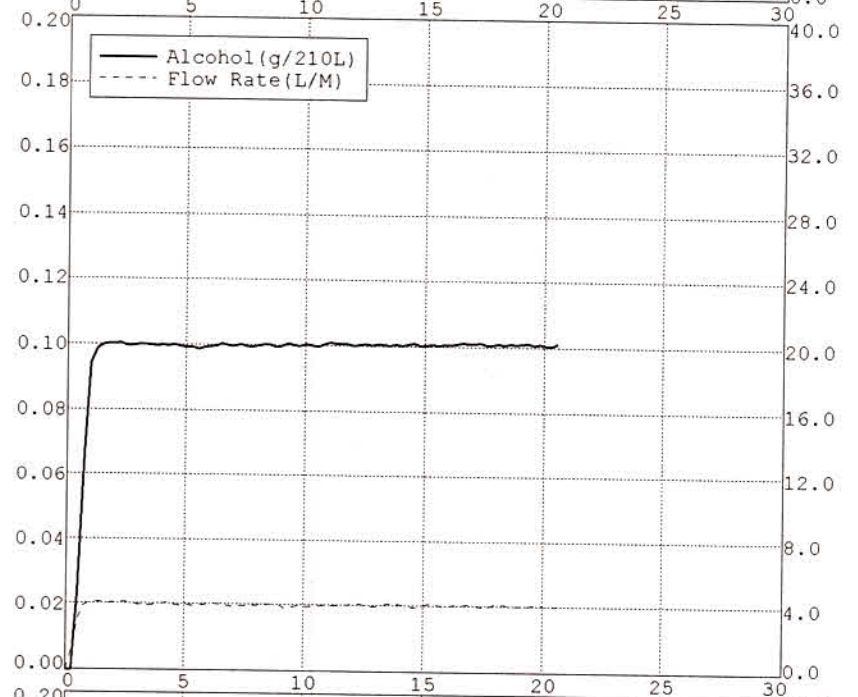

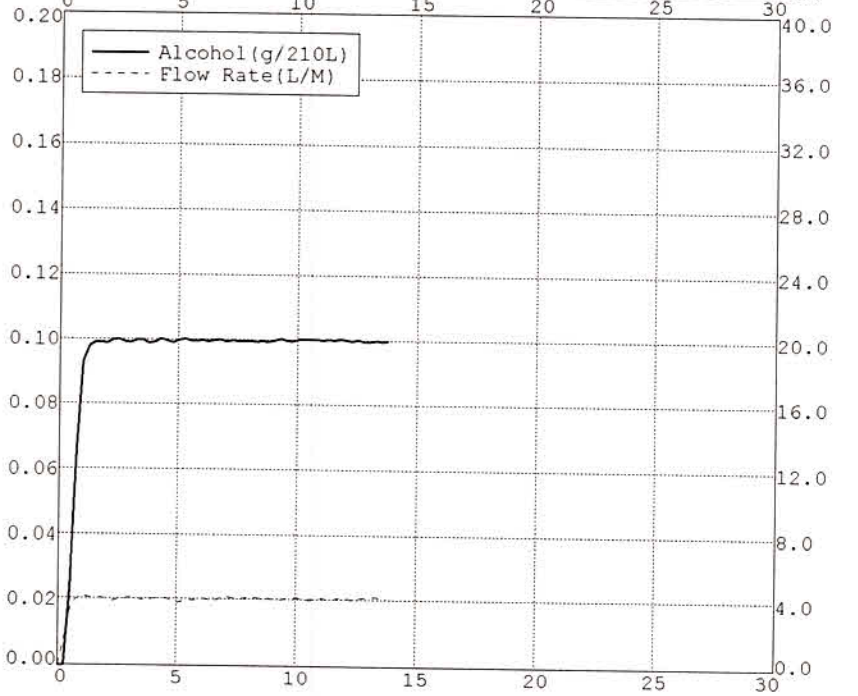

SUPERVISOR TEST


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 10/04/2026


OPERATOR NAME:
KYLE A HARRINGTON
Permit #: 48283
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	23:49
INTERNAL STANDARD	VERIFIED	23:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:50
BLANK TEST	0.00	23:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	23:51
BLANK TEST	0.00	23:52
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	23:52
BLANK TEST	0.00	23:53

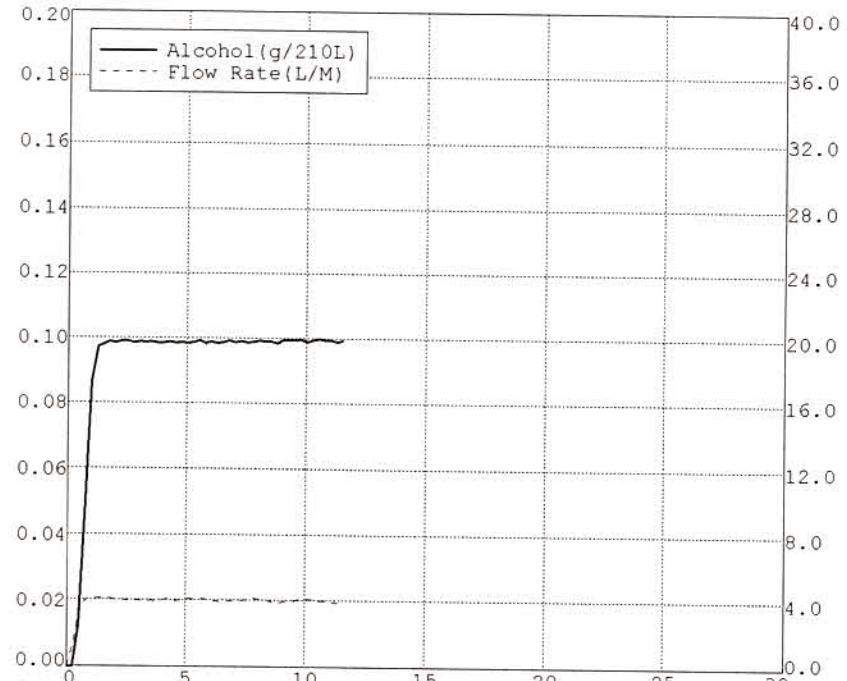

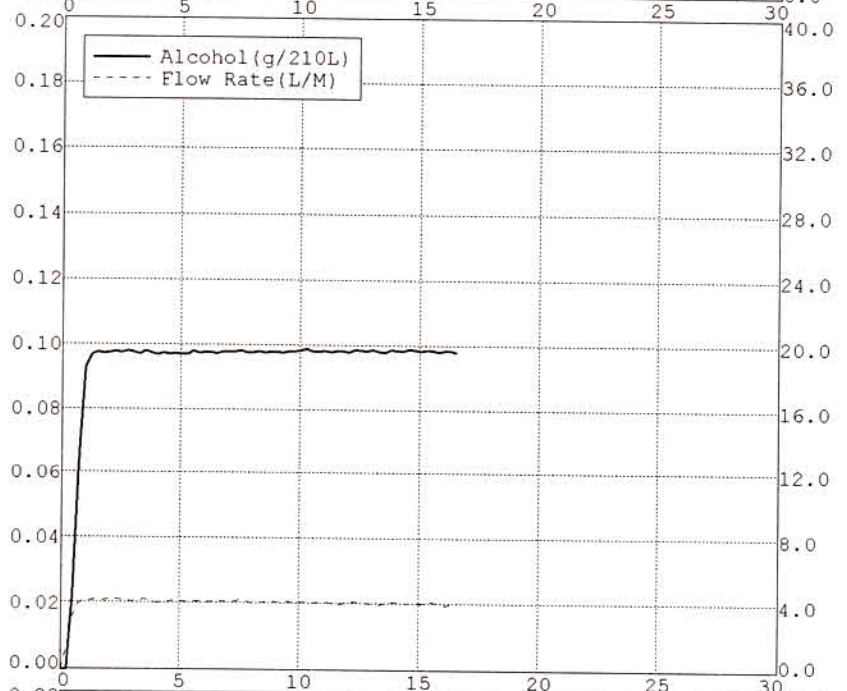

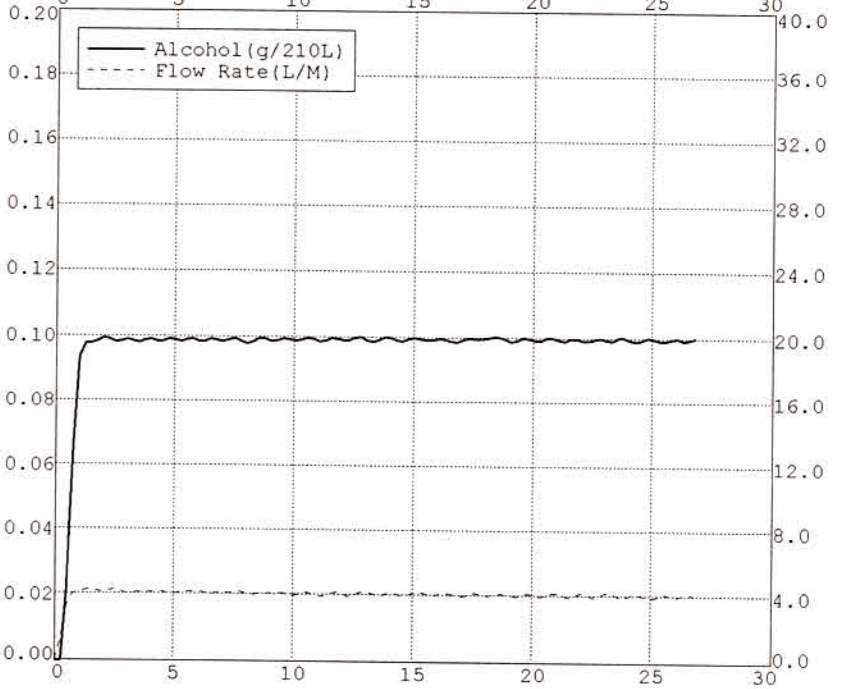

SUPERVISOR TEST


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 10/15/2026


OPERATOR NAME:
KYLE A HARRINGTON
Permit #: 48283
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	00:47
INTERNAL STANDARD	VERIFIED	00:47
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	00:48
BLANK TEST	0.00	00:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:49
BLANK TEST	0.00	00:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	00:50
BLANK TEST	0.00	00:51

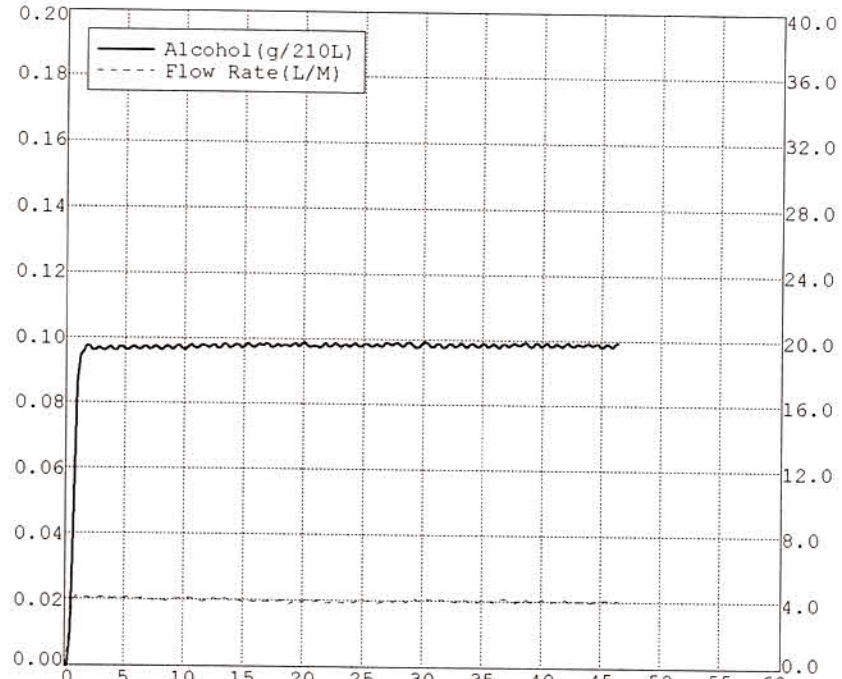

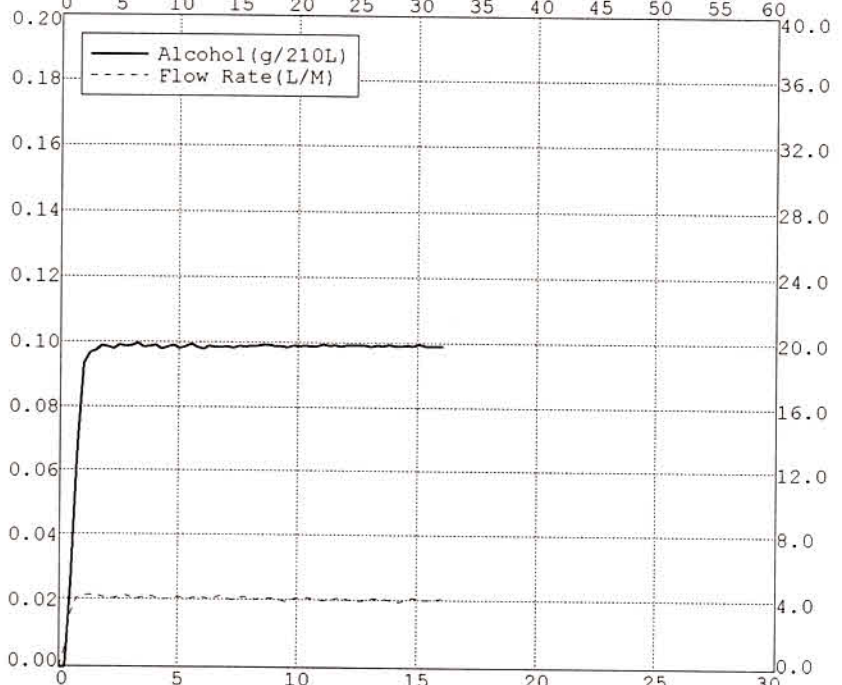

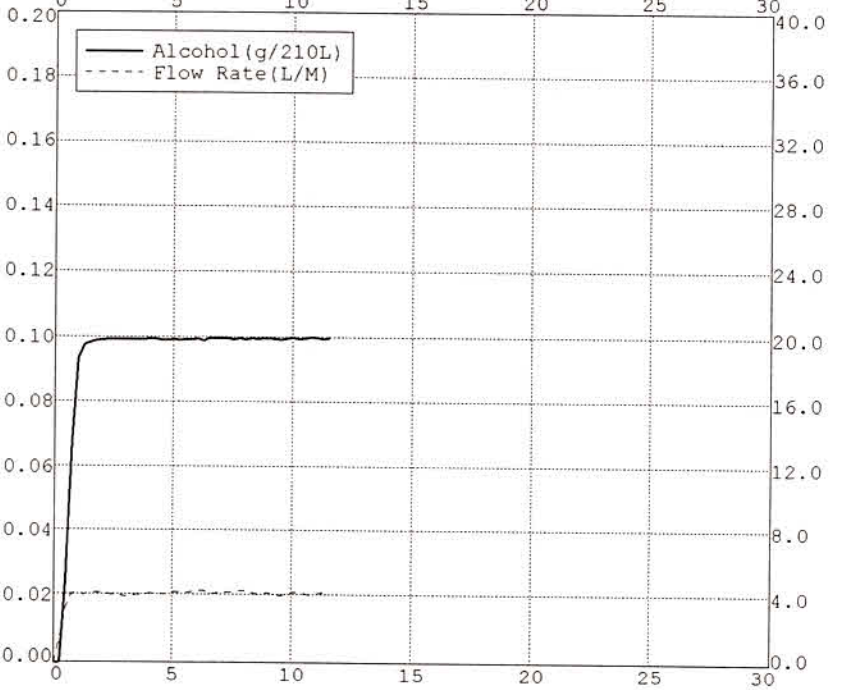

SOLUTION CHANGE


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808


Date: 11/02/2026


OPERATOR NAME:
CASEY PLACITO
Permit #: 47415
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26270

Nominal = 0.10 g/210L

BLANK TEST	0.00	22:27
INTERNAL STANDARD	VERIFIED	22:27
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:27
BLANK TEST	0.00	22:28
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:28
BLANK TEST	0.00	22:29
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	22:29
BLANK TEST	0.00	22:30

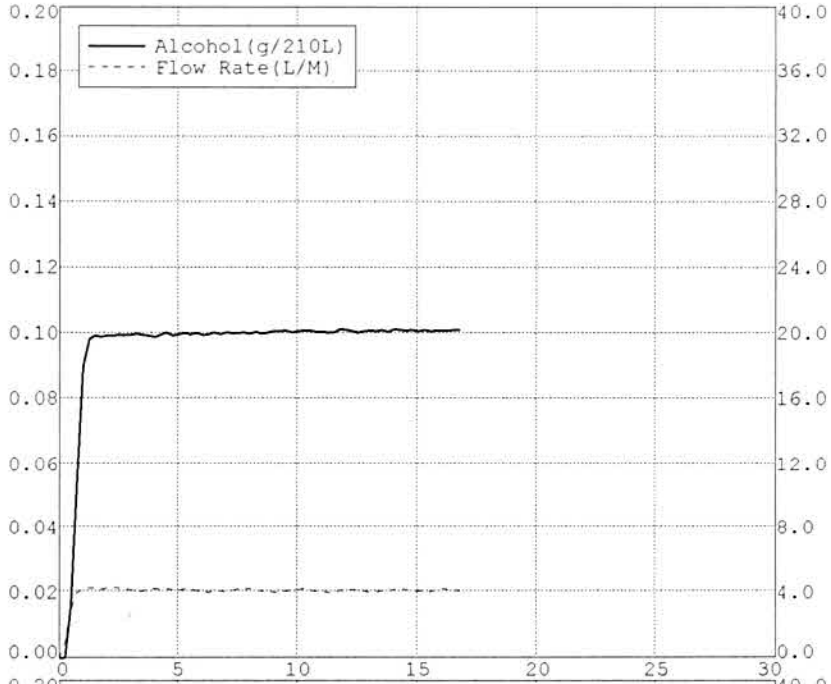

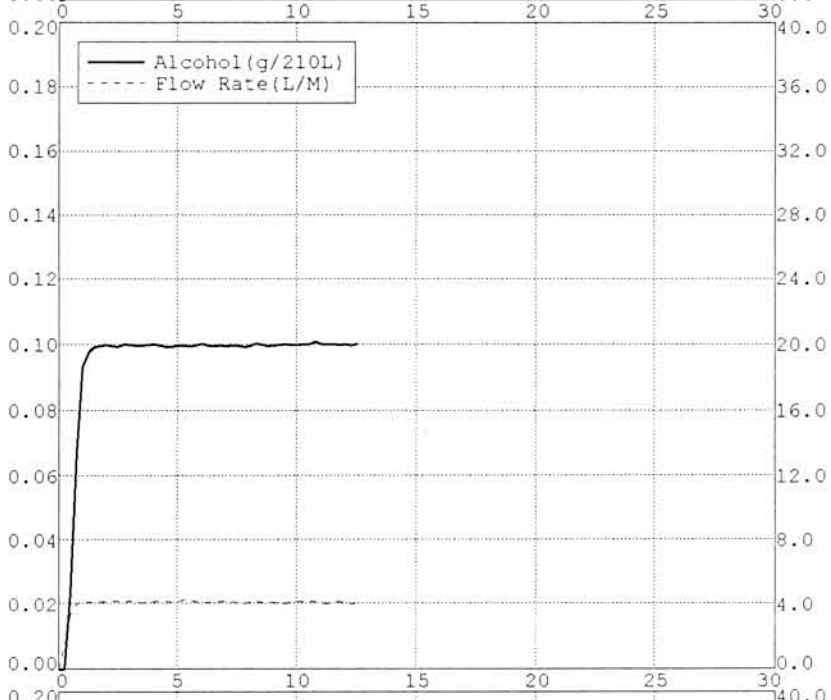

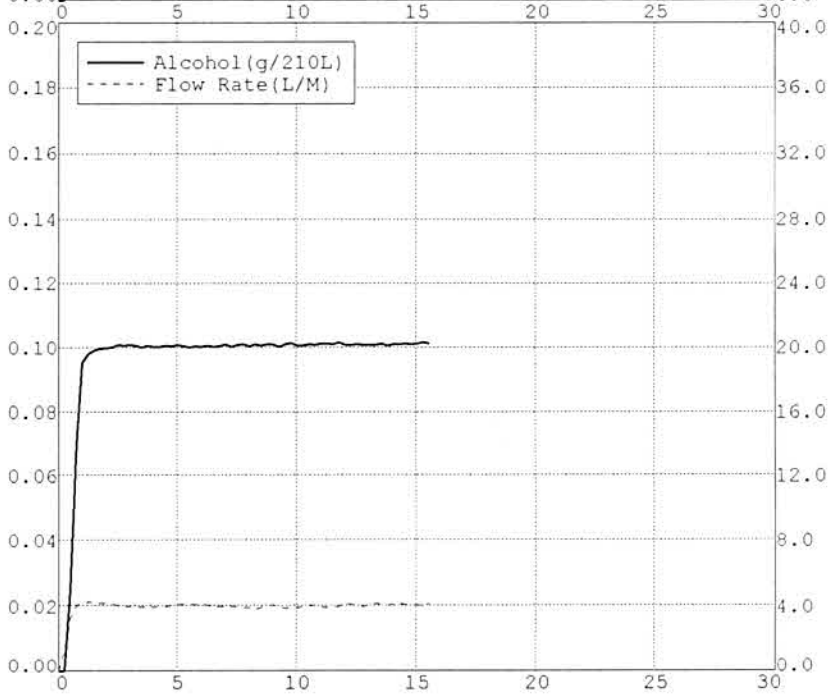

SUPERVISOR TEST


CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808

Date: 11/02/2026

OPERATOR NAME:
CASEY PLACITO
Permit #: 47415
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26190

Nominal = 0.10 g/210L

BLANK TEST	0.00	17:36
INTERNAL STANDARD	VERIFIED	17:36
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	17:36
BLANK TEST	0.00	17:37
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	17:37
BLANK TEST	0.00	17:38
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.09	17:38
BLANK TEST	0.00	17:39

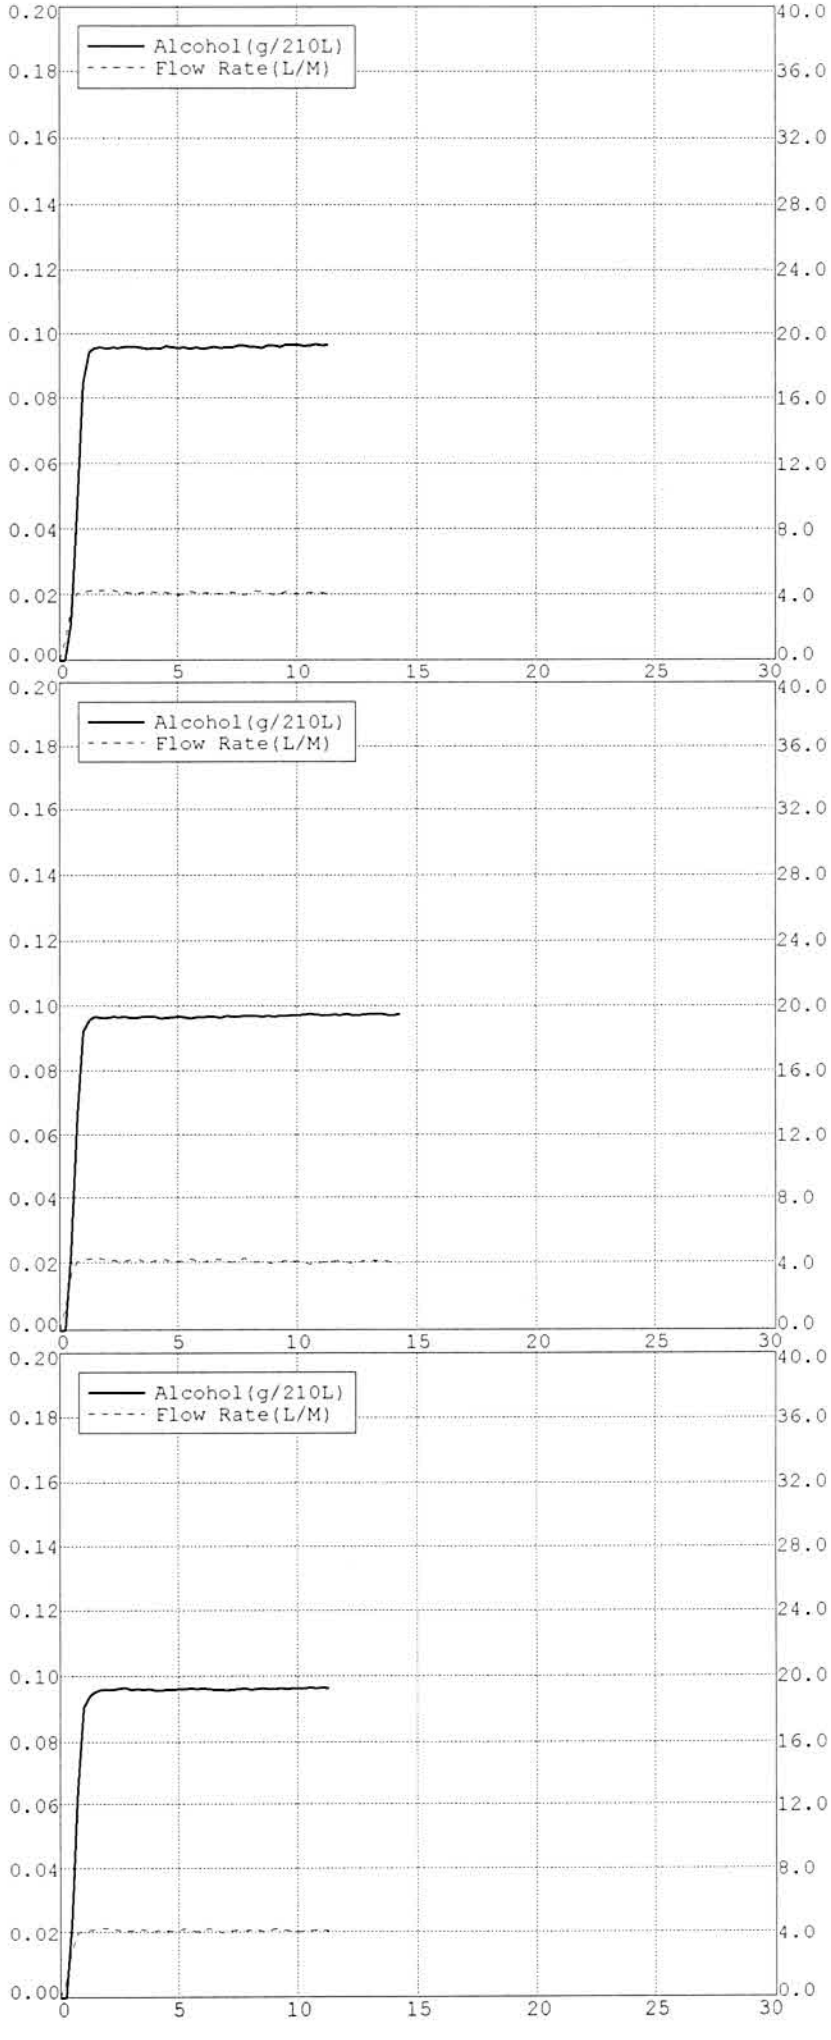

SUPERVISOR TEST

CICERO TOWN
POLICE DEPT
DATAMASTER dmt: 107808

Date: 11/16/2026

OPERATOR NAME:
JAMES J SNELL
Permit #: 38312
Operator Agency/Dept: CICERO TOWN PD
Reference Standard #: 26270

Nominal = 0.10 g/210L

BLANK TEST	0.00	14:48
INTERNAL STANDARD	VERIFIED	14:48
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:48
BLANK TEST	0.00	14:49
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:50
BLANK TEST	0.00	14:50
REFERENCE STANDARD TEMP	34.02c	
REFERENCE STANDARD	0.10	14:51
BLANK TEST	0.00	14:52

