
Neodent[®] Grand Morse[™] Single-Unit Restorations



Step 3 Take impression using open-tray or closed-tray impression copings and send to lab

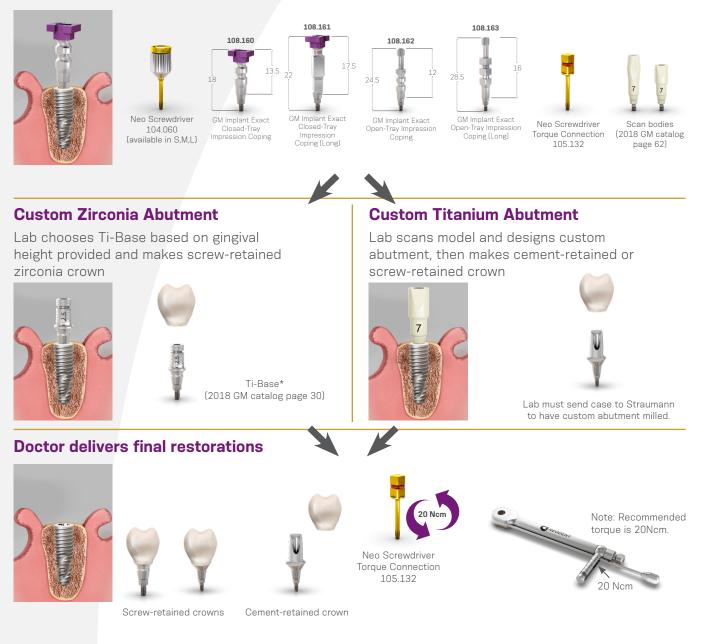

*The designed custom titanium abutment must be sent to Straumann for manufacture.

ifu.neodent.com.br/en



7

10/18

JSLIT.2020