

CATALOG • 2021



NEODENT® PRODUCT CATALOG 2021





NEW SMILES EVERY DAY

Neodent® provides you a complete range of products and services that are designed and produced by a team of professionals who truly love what they do. Just like you, we live to give people new reasons to smile. New ways to enjoy everything life has to offer. Every day.



Table of Contents

Technical Guidelines	5
Grand Morse®	10
Grand Morse Kits	47
Grand Morse Instruments	55
Neodent NeoArch Kits	69
Neodent NeoArch Instruments	71
Neodent Guided Surgery Kit	77
Neodent Guided Surgery Instruments	79
Neodent Techniques	83
Digital Solutions	89
General Instruments	91
Neodent Biomaterials	95

Technical Guidelines

Innovative and ease to use

Neodent® Packaging

Neodent® implant packaging has been updated to a concept that provides convenience through all steps of the procedure, from storage to the placement of the implant.

The new packaging aids in identification of both the implant model as well as its diameter and length, regardless of its storage position.



Package instruction of use



After breaking the sterility seal on the blister, hold the primary package (vial) and twist the lid to open it.



To remove the implant from the vial lift the cap up, which has the stand and implant attached to it.




To secure the implant, grip both sides of the implant carrier.



While gripping the implant carrier, remove the lid.



To capture the implant with the contra-angle handpiece attachment, grip the implant carrier while placing the attachment into the implant chamber.

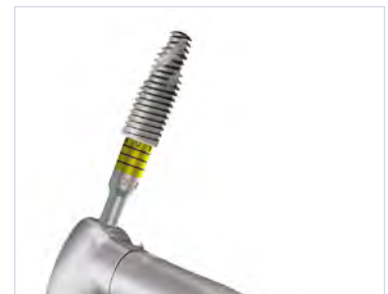

The implant can now be transported to the surgical site.

e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalog or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en



ifu.neodent.com.br/en

1 To access the IFU website, type the above address in your browser.

2 Enter in the field search the article number.

Search IFU

Type the product or IFU

We found 1 valid IFUs for your search

140.682.____

IFU

CM Drive Implant
Valid for all countries

3 The search result is presented below search field, informing the IFU code, the name of the product and countries where the IFU is valid.

download ▾

4 Click the "download" button to open the file.

NEODENT

330.252.19

Implante Drive CM
CA Drive Implant
Implante Drive CM
Implante Drive CM
CM Drive Implantat
Implant CA Drive

5 The IFU will automatically open in a new window. In case you want to download it, click the save as icon to download in your browser.



NeoPoros

Constant evolution.

Based on the abrasive sandblasting concept followed by acid etching, the **NeoPoros** surface promotes, by using controlled grain oxides, cavities on the implant surface that then are uniformed with the acid etching technique.

The whole process of obtaining this surface is guaranteed due to automated time, speed, pressure and particle size control.

Several scientific studies continue to be performed so that the **NeoPoros** surface may be always evolving and promoting much more reliability for you.

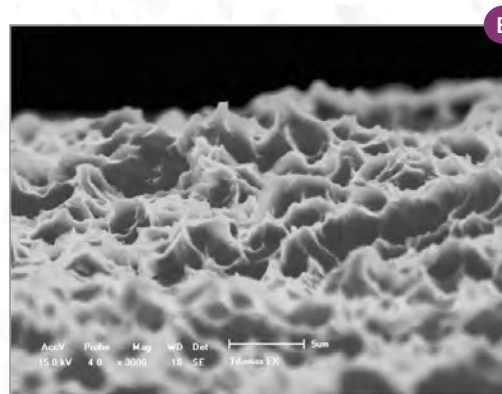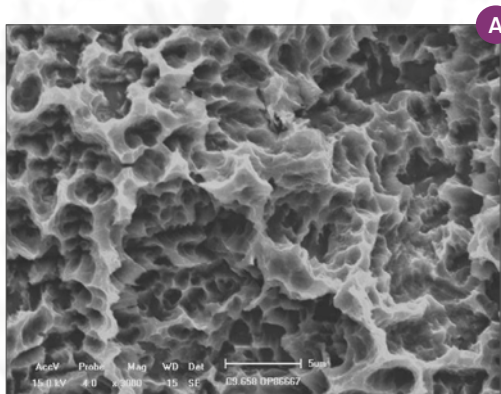

Controlled roughness on all implant surface. Scanning electron microscopy (A) shows macro (15-30 μ m) and (B) microtopography (0,3 - 1,3 μ m).

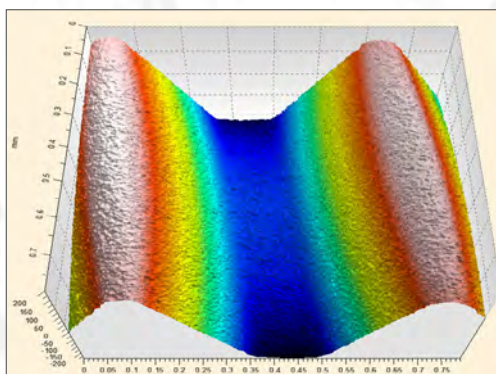


Image taken by confocal microscopy.
Roughness and Microtopography.
(S_a = 0,3 - 1,3 μ m; S_z = 6,0 - 15,5 μ m).

acqua®

Acqua Hydrophilic Surface designed for high treatment predictability.


The Neodent® Acqua hydrophilic surface is the next level of the highly successful S.L.A. type of surface developed to achieve successful outcomes even in challenging situations, such as soft bone or immediate protocols.⁽¹⁻⁴⁾

Hydrophilicity


The hydrophilic surface presents a smaller contact angle when in contact with hydrophilic liquids. This provides greater accessibility of organic fluids to Acqua implant surface.⁽²⁾

Surface comparison

Lab generated images.

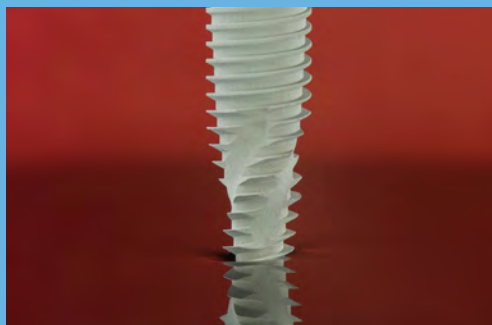

NeoPoros surface.

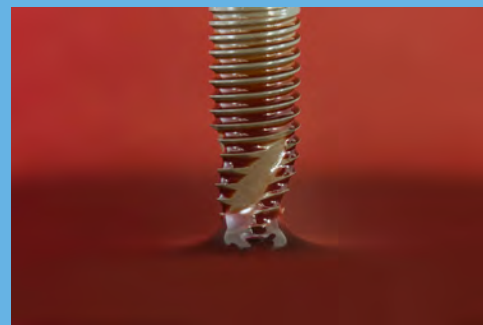

*Acqua Hydrophilic
Surface.*

Grand Morse®

GREATNESS IS AN ACHIEVEMENT



GRAND RELIABILITY


STABLE AND STRONG FOUNDATION
DESIGNED FOR LONG TERM SUCCESS

The implant-abutment interface is crucial for a successful long term functional and esthetic result. The Neodent® Grand Morse® connection offers a combination based on proven concepts: a platform switching associated with a deep 16° Morse Taper including an internal indexation for a strong and stable connection designed to achieve long-lasting results.



1 Platform Switching

Abutment design with a narrower diameter than the implant coronal area, enabling the platform switching concept⁽⁵⁻⁹⁾.




2 Internal Indexation

Precise abutment positioning, protection against rotation and easy handling.




3 Deep Connection

Allowing a large contact area between the abutment and the implant for an optimal load distribution.



4 16° Morse Taper Connection

Designed to ensure tight fit for an optimal connection sealing.






GRAND SIMPLICITY

EASE OF USE AT ITS BEST

Implant therapy has become an integral part of clinical dentistry, with ever increasing numbers of patients seeking such treatment. The Neodent® Grand Morse® Implant System is smartly engineered providing efficiency and simplicity within the dental treatment network for both surgical to restoratives steps.

ONE PROSTHETIC PLATFORM

All Neodent® Grand Morse® implants feature the unique Grand Morse® connection regardless of the implant diameter.

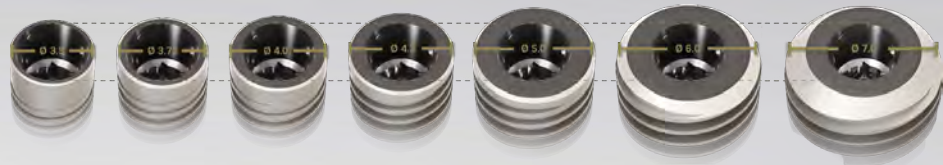

ONE SCREWDRIVER

The Neo Screwdriver has a star attachment offering reliability and durability compatible with all Neodent® Grand Morse® healing abutments and cover screws and most of the restorative screws.



ONE IMPLANT DRIVER

The Neodent® implant driver allows an easy and reliable implant pick up and placement.



ONE SURGICAL KIT

Intuitive and functional compact surgical kit, that allows the place of Helix GM® implants in all bone types.





GRAND STABILITY

STABLE AND STRONG FOUNDATION DESIGNED FOR LONG TERM SUCCESS

The increasing expectations for shortened treatment duration represent a significant challenge for dental professionals. The Neodent® Grand Morse® system offers an implant design featuring the Acqua hydrophilic surface designed to maximize primary stability and predictability in immediate protocols.



HELIX® - OPTIMAL IMPLANT DESIGNED TO ACHIEVE HIGH PRIMARY STABILITY

Helix® Grand Morse® is a hybrid implant design maximizing treatment options and efficiency in all bone types.

Fully tapered body design

- Coronal: 2° - 12°
- Apex: 16°
- » Allowing under-osteotomy




Hybrid contour

- Coronal: Cylindrical
- Apex: Conical
- » For stability with vertical placement flexibility



Active apex

- Soft rounded small tip
- Helical flutes
- » Enabling immediate loading




Dynamic progressive thread design

- Coronal: Trapezoidal > compressing
- Apex: V-Shape > Self-tapping
- » Achieving high primary stability in all bone types



Acqua hydrophilic surface

Designed for high treatment predictability



Titamax®

Vertical placement flexibility.
Bone types I & II.



Drive®

High primary stability in
challenging bone types.
Bone types III & IV.



GRAND ESTHETICS

DELIVER IMMEDIATE NATURAL ESTHETICS

Nowadays, patients expect both short treatment times and esthetic results. The Neodent® Grand Morse® restorative portfolio offers flexibility to simplify soft tissue management respecting the biological distances for achieving immediate function and esthetics.



Titanium Temporary Abutment



Pro-Peek Abutment



Titanium Base



Titanium Base C



Titanium Base for Bridge



Titanium Block (AG or Medentika Holder)



CoCr Abutment



Anatomic Abutment (straight and angled)



Universal Abutment (straight and angled)



Abutment



Angled Mini Conical Abutment



Attachment (straight and angled)



Titanium Base AS



Straight Mini Conical Abutment



Micro Abutment



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Overdenture



Multiple-unit screw-retained prosthesis



Multiple-unit cement-retained prosthesis



Temporary

Neodent easypack

GROW WITH PEACE OF MIND

Neodent® has developed EasyPack to simplify your daily practice. An all-in-one set that offers everything you need to grow while performing dental implant therapy with confidence, convenience and guidance.



GROW WITH CONFIDENCE

Choose a brand and products you can rely on



GROW WITH CONVENIENCE

The certainty of having everything in one package




GROW WITH GUIDANCE

All workflows in simple steps

THE NEODENT® EASYPACK INCLUDES

- 1 Grand Morse® Helix Implant
- 2 Grand Morse® Cover Screw
- 3 Grand Morse® Healing Abutment
- 4 Grand Morse® Hybrid Implant Analog
- 5 Grand Morse® 3-in-1 Neodent Smart Abutment™

NEW

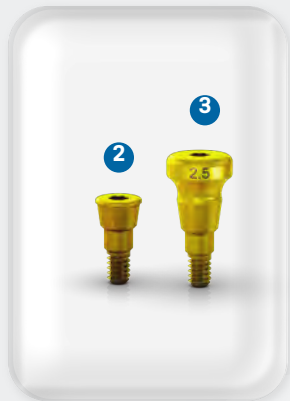



CONVENTIONAL
WORKFLOW




DIGITAL
WORKFLOW

Reliable guided workflow with the 3-in-1 GM Smart Abutment




The combination of the GM Smart Abutment, a solution combining a closed tray impression coping, a digital scanbody and a temporary abutment in a single piece, with healing components and the analog allows you to choose a restorative path guided for achieving predictable results.

IMPLANT PLACEMENT — HEALING PHASE — IMPRESSION PHASE — TEMPORARY RESTORATION — FINAL RESTORATION

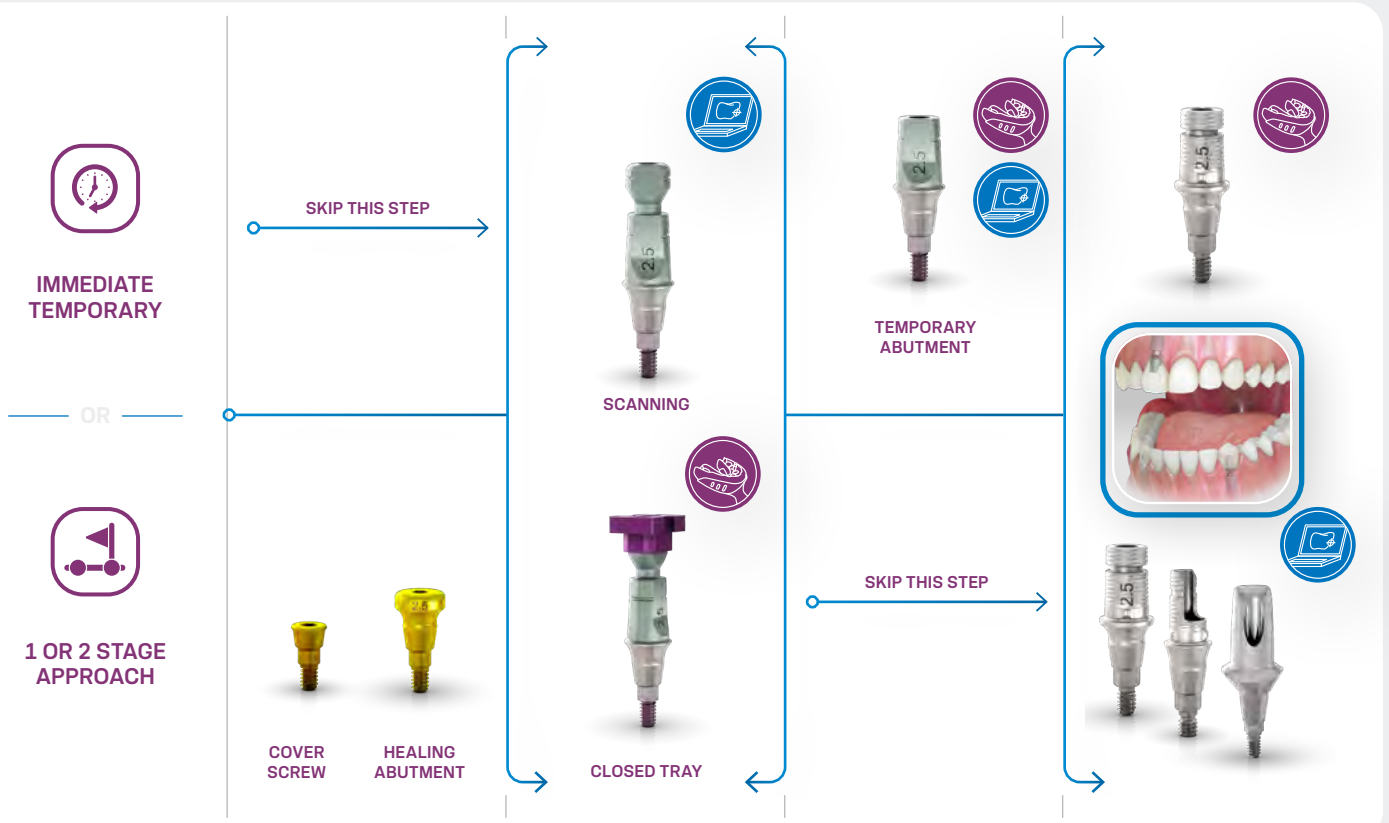

NEODENT® EASYPACK PRODUCT OPTIONS

	Ø 3.5		Ø 3.75		Ø 4.0		Ø 4.3	
	Acqua	NeoPoros	Acqua	NeoPoros	Acqua	NeoPoros	Acqua	NeoPoros
8.0	138.089	138.005	138.113	138.029	138.137	138.053	138.158	138.074
10.0	138.095	138.011	138.119	138.035	138.143	138.059	138.161	138.077
11.5	138.101	138.017	138.125	138.041	138.149	138.065	138.164	138.080
13.0	138.107	138.023	138.131	138.047	138.155	138.071	138.167	138.083



Helix GM[®]

PRODUCT FEATURES:

Implants Description:

- Full dual tapered implant;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex including a soft rounded small tip and helicoidal flutes;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-tapping V-shape threads on the apical part;
- Double threaded implant;
- Grand Morse[®] connection.

Indications:

- Indicated for all types of bone density and implant immediate placement post extraction.

Drilling features:

- Contour drill is required in bone types I and II;
- Final pilot drills are highly recommended in bone types I and II;
- Implant should be positioned 1 or 2 mm below bone level;
- Drilling speed: 800-1200 rpm for bone type I and II;
- Drilling speed: 500-800 rpm for bone type III and IV;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.



Available with:

NeoPoros or 

Drill Sequence



	Initial	Ø 2.0	Ø 3.5	Ø 3.5+	Ø 2.8/3.5	Ø 3.75	Ø 3.75+	Ø 3.0/3.75	Ø 4.0	Ø 4.0+	Ø 3.3/4.0	Ø 4.3	Ø 4.3+	Ø 3.6/4.3	Ø 5.0	Ø 5.0+	Ø 4.3/5.0	Ø 6.0	Ø 7.0	
	103.170	103.425	103.399	103.419	103.414	103.402	103.420	103.415	103.405	103.421	103.416	103.408	103.422	103.417	103.411	103.423	103.418	103.427	103.487	
Ø 3.5	Optional	✓		✓	✓															
Ø 3.75	Optional	✓	✓				✓	✓												
Ø 4.0	Optional	✓	✓			✓			✓	✓										
Ø 4.3	Optional	✓	✓			✓			✓				✓	✓						
Ø 5.0	Optional	✓	✓			✓			Optional			✓			✓	✓				

Bone types I and II

Ø 3.5	Optional	✓	✓																	
Ø 3.75	Optional	✓	✓			Optional														
Ø 4.0	Optional	✓	✓					Optional												
Ø 4.3	Optional	✓	✓			✓						Optional								
Ø 5.0	Optional	✓	✓									✓			Optional					
Ø 6.0	Optional	✓	✓			✓						✓			✓				✓	
Ø 7.0	Optional	✓	✓									✓			✓				✓	Optional

Bone types III and IV

Drill Sequence with Neodent® Control System

	Initial	Ø 2.0	Ø 3.5	Ø 3.5+	Ø 2.8/3.5	Ø 3.75	Ø 3.75+	Ø 3.0/3.75	Ø 4.0	Ø 4.0+	Ø 3.3/4.0	Ø 4.3	Ø 4.3+	Ø 3.6/4.3	Ø 5.0	Ø 5.0+	Ø 4.3/5.0	Ø 6.0	Ø 7.0	
	103.170	103.492	103.493	103.500	103.513	103.494	103.501	103.514	103.495	103.502	103.515	103.496	103.503	103.516	103.497	103.504	103.517	103.498	103.499	
Ø 3.5																				
Ø 3.75																				
Ø 4.0																				
Ø 4.3																				
Ø 5.0																				

*Optional Bone types I and II

Ø 3.5																				
Ø 3.75																				
Ø 4.0																				
Ø 4.3																				
Ø 5.0																				
Ø 6.0																				
Ø 7.0																				

*Optional Bone types III and IV

Helix GM® Implants

Ø 3.5	Acqua	NeoPoros	Ø 3.75	Acqua	NeoPoros	Ø 4.0	Acqua	NeoPoros	Ø 4.3	Acqua	NeoPoros
8.0	140.943	109.943	8.0	140.976	109.976	8.0	140.982	109.982	8.0	140.948	109.948
10.0	140.944	109.944	10.0	140.977	109.977	10.0	140.983	109.983	10.0	140.949	109.949
11.5	140.945	109.945	11.5	140.978	109.978	11.5	140.984	109.984	11.5	140.950	109.950
13.0	140.946	109.946	13.0	140.979	109.979	13.0	140.985	109.985	13.0	140.951	109.951
16.0	140.947	109.947	16.0	140.980	109.980	16.0	140.986	109.986	16.0	140.952	109.952
18.0	140.988	109.988	18.0	140.981	109.981	18.0	140.987	109.987	18.0	140.989	109.989

Ø 5.0	Acqua	NeoPoros	Ø 6.0	Acqua	NeoPoros	Ø 7.0	Acqua	NeoPoros
8.0	140.953	109.953	8.0	140.1009	109.1009	8.0	140.1059	109.1059
10.0	140.954	109.954	10.0	140.1010	109.1010	10.0	140.1060	109.1060
11.5	140.955	109.955	11.5	140.1011	109.1011	11.5	140.1061	109.1061
13.0	140.956	109.956	13.0	140.1012	109.1012	13.0	140.1062	109.1062
16.0	140.957	109.957						
18.0	140.990	109.990						

GM Cover Screw
 0 mm 2 mm
 117.021 117.022



Use the manual Neo Screwdriver (104.060);
 Do not exceed the insertion torque of 10 N.cm.

GM Healing Abutment

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218

Use the manual Neo Screwdriver (104.060);
 Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutment

	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

Use the manual Neo Screwdriver (104.060);
 Do not exceed the insertion torque of 10 N.cm.

Drive GM[®]

PRODUCT FEATURES:

Implants Description:

- Tapered implant;
- Square shape threads;
- Double threaded implant;
- Reverse cutting chambers distributed across the implant body;
- Rounded apex with a sharp edge;
- Grand Morse[®] connection.

Indications:

- Indicated for bone types III and IV and implant immediate placement post-extraction;

Drilling features:

- Final pilot drill is optional in bone types III and IV;
- Implant should be positioned 1 or 2 mm below bone level;
- Drilling speed: 500-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.



Available with:

NeoPoros[®] or 

Drill Sequence

	Initial	Ø 2.0	Ø 3.5	Ø 2.8/3.5	Ø 4.3	Ø 3.6/4.3	Ø 5.0	Ø 4.3/5.0
	103.170	103.425	103.399	103.414	103.408	103.417	103.411	103.418
Ø 3.5 mm	✓	✓	✓	Optional				
Ø 4.3 mm	✓	✓	✓		✓	Optional		
Ø 5.0 mm	✓	✓	✓		✓		✓	Optional

Bone types III and IV

Drill Sequence with Neodent® Control System

	Initial	Ø 2.0	Ø 3.5	Ø 2.8/3.5	Ø 4.3	Ø 3.6/4.3	Ø 5.0	Ø 4.3/5.0
	103.170	103.492	103.493	103.513	103.496	103.516	103.497	103.517
Ø 3.5				*				
Ø 4.3						*		
Ø 5.0								*

*Optional Bone types III and IV

Drive GM® Implants

	8.0 mm	10.0 mm	11.5 mm	13.0 mm	16.0 mm	18.0 mm	
Ø 3.5	Acqua	140.958	140.959	140.960	140.961	140.962	140.963
	NeoPoros	109.958	109.959	109.960	109.961	109.962	109.963
Ø 4.3	Acqua	140.964	140.965	140.966	140.967	140.968	140.969
	NeoPoros	109.964	109.965	109.966	109.967	109.968	109.969
Ø 5.0	Acqua	140.970	140.971	140.972	140.973	140.974	140.975
	NeoPoros	109.970	109.971	109.972	109.973	109.974	109.975

GM Healing Abutment



Profile	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Cover Screw



	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

Titamax GM[®]

PRODUCT FEATURES:

Implants Description:

- Cylindrical implant (parallel walls);
- V-shape threads;
- Double threaded implant;
- Self tapping apex;
- Grand Morse[®] connection.

Indications:

- Indicated for bone types I and II or grafted areas such as bone block.

Drilling features:

- Final pilot drill is highly recommended in bone types I and II;
- Implant should be positioned 1 or 2 mm below bone level;
- Self tapping implant which doesn't require the use of bone tap or contour drill;
- Drilling speed: 800-1200 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.



Available with:

NeoPoros[®] or 

Drill Sequence

	Initial	Ø 2.0	Ø 2/3	Ø 2.8	Ø 3.0	Ø 2.8/3.5	Ø 3.3	Ø 3.0/3.75	Ø 3.3/4.0	Ø 3.8	Ø 4.3	Ø 4.3/5.0
	103.170	103.162	103.213	103.163	103.164	103.414	103.166	103.415	103.416	103.167	103.168	103.418
Ø 3.5 mm	✓	✓		✓		✓						
Ø 3.75 mm	✓	✓	✓		✓			✓				
Ø 4.0 mm	✓	✓	✓		✓		✓		✓			
Ø 5.0 mm	✓	✓	✓		✓			✓		✓	✓	✓

Bone types I and II



Titamax GM® Implants

		7.0 mm	8.0 mm	9.0 mm	11.0 mm	13.0 mm	15.0 mm	17.0 mm
Ø 3.5								
	Acqua	140.906	140.907	140.908	140.909	140.910	140.911	140.912
	NeoPoros	109.906	109.907	109.908	109.909	109.910	109.911	109.912
Ø 3.75								
	Acqua	140.899	140.900	140.901	140.902	140.903	140.904	140.905
	NeoPoros	109.899	109.900	109.901	109.902	109.903	109.904	109.905
Ø 4.0								
	Acqua	140.913	140.914	140.915	140.916	140.917	140.918	140.919
	NeoPoros	109.913	109.914	109.915	109.916	109.917	109.918	109.919
Ø 5.0								
	Acqua	140.920	140.921	140.922	140.923	140.924		
	NeoPoros	109.920	109.921	109.922	109.923	109.924		

GM Healing Abutment



Profile	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

GM Cover Screw



0 mm	2 mm
117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.



GM Abutment

Consider in addition 1.5 - 2.0 mm for the restorative material

Minimum interocclusal space of 4.9 mm from the mucosa level

Single-unit screw-retained prosthesis

Ø 4.8 mm

Recommended for posterior region.

Exact
Unlocking feature



Installation Sequence


0.8 mm	1.5 mm	2.5 mm
115.237	115.238	115.239
3.5 mm	4.5 mm	5.5 mm
115.240	115.241	115.242





Intraoral



Model Scanning



Conventional

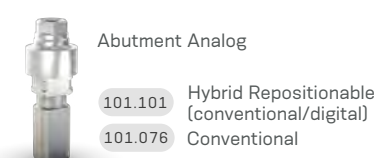


22

Drivers



Accessories




GM Abutment with Neo Removable Screw

Single-unit screw-retained prosthesis

Ø 4.8 mm

Recommended for posterior region.

Consider in addition 1.5 - 2.0 mm for the restorative material
 Minimum interocclusal space of 4.9 mm from the mucosa level
 With internal threads for secure engagement of the screw

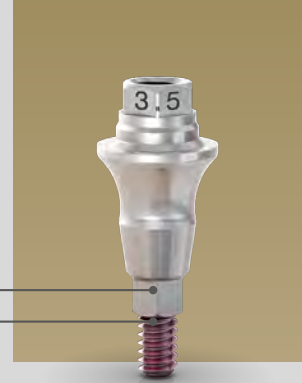

Installation Sequence

0.8 mm	1.5 mm	2.5 mm
115.269	115.270	115.271
3.5 mm	4.5 mm	5.5 mm
115.272	115.273	115.274



Drivers



Accessories

Replacement Abutment Screw

- 116.290 Neo GM Screw (Short) - for abutment with 0.8 GH
- 116.291 Neo GM Screw - for abutments with 1.5-2.5 GH
- 116.292 Neo GM Screw (Long) - for abutments with 3.5-5.5 GH

Mini Conical Abutment Polishing Protector 123.008

Replacement Coping Screw 116.266

GM Mini Conical Abutment

Consider in addition 1.5 - 2.0 mm for the restorative material

Minimum interocclusal space of 4.5 mm from the mucosa level for straight abutments



Multiple-unit screw-retained prosthesis



Ø 4.8 mm



Exact

Installation Sequence


0.8 mm	1.5 mm	2.5 mm	GM Mini Conical Abutment	or	GM Exact Mini Conical Abutment 17°/30°	1.5 mm	2.5 mm	3.5 mm	
115.243	115.244	115.245	 32 N.cm		 20 N.cm	17°	115.249	115.250	115.251
115.246	115.247	115.248		30°		115.252	115.253	115.254	

Intraoral

Model Scanning

Conventional

24

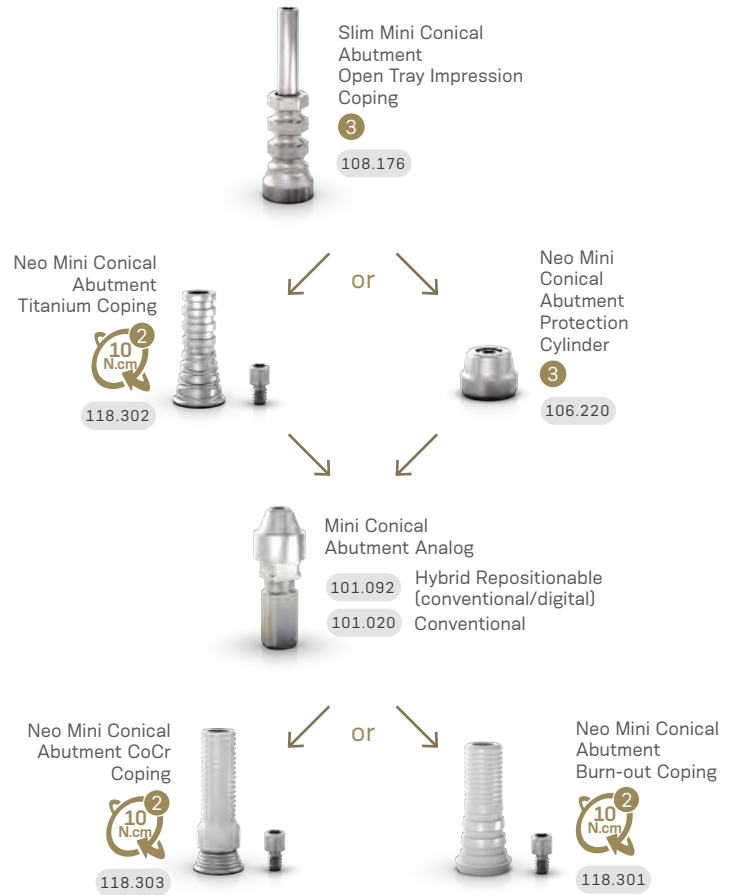

Drivers

- 1 Hexagonal Prosthetic Driver + Torque Wrench
- 2 Neo Screwdriver Torque Connection + Torque Wrench
- 3 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

- Mini Conical Abutment Polishing Protector (123.008)
- Replacement Coping Screw (116.269) Titanium

GM Micro Abutment



Single-unit screw-retained prosthesis




Multiple-unit screw-retained prosthesis



Ø 3.5 mm

Consider in addition 1.5 - 2.0 mm for the restorative material
Minimum interocclusal space of 3.5 mm from the mucosa level

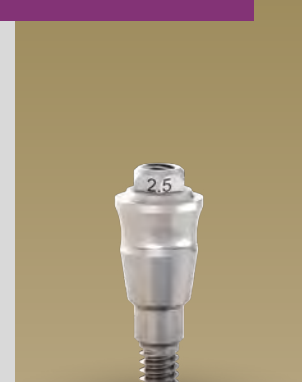

Recommended for limited spaces and narrow inter-dental spaces.

Installation Sequence

0.8 mm	1.5 mm	2.5 mm	GM Micro Abutment
115.255	115.256	115.257	
3.5 mm	4.5 mm	5.5 mm	

115.258 115.259 115.260



32 N.cm





Intraoral



Model Scanning

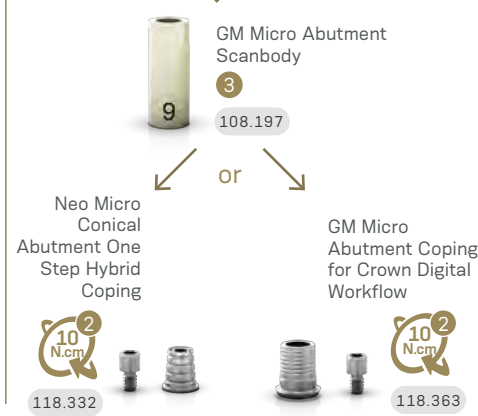

Conventional

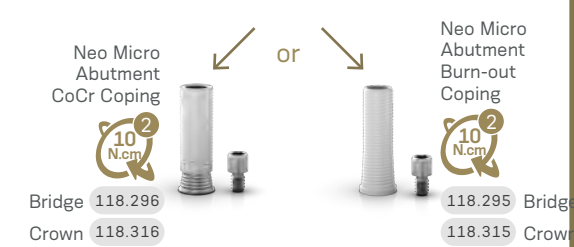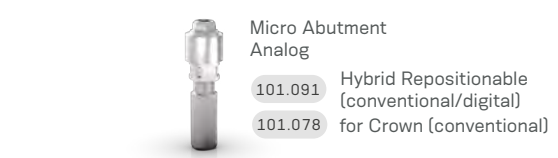

Drivers

- 1 Hexagonal Prosthetic Driver + Torque Wrench
- 2 Neo Screwdriver Torque Connection + Torque Wrench
- 3 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

- Micro Abutment Polishing Protector (123.015) Bridge
- Replacement Coping Screw (116.269)


GM Anatomic Abutment



Single-unit cement-retained prosthesis

Recommended for anterior region.

Gingiva color for esthetic outcomes
 Click retention for provisional copings
 Exact
 Unlocking feature

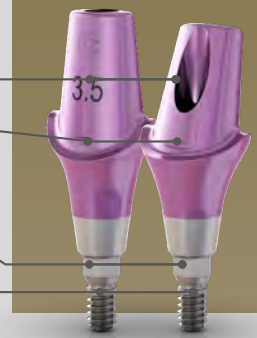


Installation Sequence

In Mouth

GM Exact Click Anatomic Abutment			or			GM Exact Click Narrow Anatomic Abutment					
1.5 mm	2.5 mm	3.5 mm		1.5 mm	2.5 mm	3.5 mm		1.5 mm	2.5 mm	3.5 mm	
114.752	114.753	114.754		114.758	114.759	114.760		114.761	114.762	114.763	
17°	114.755	114.756	114.757		17°	114.761	114.762	114.763			

GM Exact Click Anatomic Abutment Provisional Coping

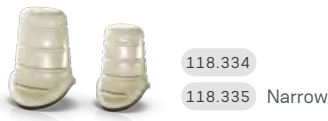

Impression of the GM Exact Click Anatomic Abutment

Lab stage

Finalized prosthesis

In Lab



GM Implant Exact Impression Coping Closed and Open Tray ²


Regular	108.160	108.162
Long	108.161	108.163



GM Implant Analog

Ø 3.5/3.75	Ø 4.0/4.3	Ø 5.0/6.0	Hybrid Repositionable (conventional/digital)
101.103	101.089	101.090	
	101.074	101.075	Conventional

GM Exact Click Anatomic Abutment Provisional Coping

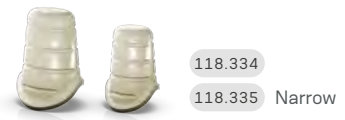

GM Exact Click Anatomic Abutment			or			GM Exact Click Narrow Anatomic Abutment					
1.5 mm	2.5 mm	3.5 mm		1.5 mm	2.5 mm	3.5 mm		1.5 mm	2.5 mm	3.5 mm	
114.752	114.753	114.754		114.758	114.759	114.760		114.761	114.762	114.763	
17°	114.755	114.756	114.757		17°	114.761	114.762	114.763			

Drivers




GM Anatomic Abutment with Neo Removable Screw



Single-unit
cement-retained
prosthesis

Recommended for anterior region.

Gingiva color for esthetic outcomes
Click retention for provisional copings
With internal threads for secure engagement of the screw
Exact
Neo Removable Screw

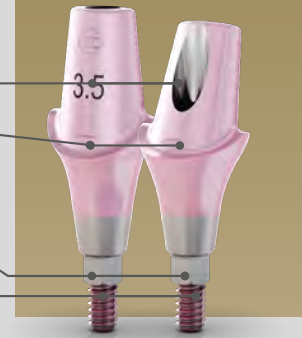

Installation Sequence

In Mouth

GM Exact Click Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.862	114.863	114.864
17° 114.865	114.866	114.867

OR

GM Exact Click Narrow Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.868	114.869	114.870
17° 114.871	114.872	114.873

GM Exact Click Anatomic Abutment Provisional Coping



Impression of the GM Exact Click Anatomic Abutment

Lab stage

Finalized prosthesis

In Lab

GM Implant Exact Impression Coping Closed and Open Tray

Regular	108.160	108.162
Long	108.161	108.163

GM Implant Analog

Ø 3.5/3.75	Ø 4.0/4.3	Ø 5.0/6.0	Hybrid Repositionable (conventional/digital)
101.103	101.089	101.090	Conventional
	101.074	101.075	

GM Exact Click Anatomic Abutment Provisional Coping



GM Exact Click Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.862	114.863	114.864
17° 114.865	114.866	114.867

OR

GM Exact Click Narrow Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.868	114.869	114.870
17° 114.871	114.872	114.873

Drivers

1 Neo Screwdriver Torque Connection + Torque Wrench

2 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

Replacement Abutment Screw

116.291 Neo GM Screw - for abutments with 1.5-2.5 GH

116.292 Neo GM Screw (Long) - for abutments with 3.5 GH



GM Universal Abutment




Single-unit cement-retained prosthesis



Ø 3.3/4.5 mm

Cementable area: 4.0 or 6.0 mm
Click retention for provisional copings

Exact
Unlocking feature

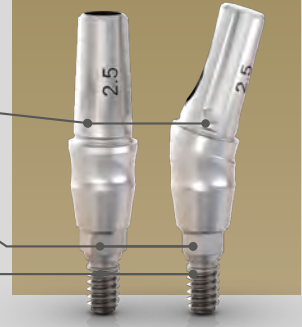

Installation Sequence

GM Exact Click Universal Abutment



or

GM Exact Click Universal Abutment 17°



or

GM Exact Click Universal Abutment 30°



	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
4 mm Ø 3.3	114.566	114.567	114.568	114.569	114.570	114.571
4 mm Ø 4.5	114.578	114.579	114.580	114.581	114.582	114.583
6 mm Ø 3.3	114.572	114.573	114.574	114.575	114.576	114.577
6 mm Ø 4.5	114.584	114.585	114.586	114.587	114.588	114.589

	1.5 mm	2.5 mm	3.5 mm
4 mm Ø 3.3	114.542	114.543	114.544
4 mm Ø 4.5	114.548	114.549	114.550
6 mm Ø 3.3	114.545	114.546	114.547
6 mm Ø 4.5	114.551	114.552	114.553

	1.5 mm	2.5 mm	3.5 mm
4 mm Ø 3.3	114.554	114.555	114.556
4 mm Ø 4.5	114.560	114.561	114.562
6 mm Ø 3.3	114.557	114.558	114.559
6 mm Ø 4.5	114.563	114.564	114.565

Intraoral



Universal Abutment Intraoral Scanbody

4 mm Ø 3.3	108.143	6 mm Ø 3.3	108.144
4 mm Ø 4.5	108.145	6 mm Ø 4.5	108.146



Universal abutment Hybrid Repositionable analog

4 mm Ø 3.3	101.097	6 mm Ø 3.3	101.098
4 mm Ø 4.5	101.099	6 mm Ø 4.5	101.100

Milled crown

Conventional



Click Universal Abutment Impression Coping

4 mm Ø 3.3	108.172	6 mm Ø 3.3	108.173
4 mm Ø 4.5	108.174	6 mm Ø 4.5	108.175



Click Universal Abutment Provisional Coping

4 mm Ø 3.3	118.304	6 mm Ø 3.3	118.305
4 mm Ø 4.5	118.306	6 mm Ø 4.5	118.307



Universal Abutment Analog

4 mm Ø 3.3	101.097	6 mm Ø 3.3	101.098	Hybrid Repositionable (conventional/digital)
4 mm Ø 4.5	101.099	6 mm Ø 4.5	101.100	

4 mm Ø 3.3	101.070	6 mm Ø 3.3	101.071	Click (conventional)
4 mm Ø 4.5	101.072	6 mm Ø 4.5	101.073	



Universal Abutment Burn-out Coping

4 mm Ø 3.3	118.181	6 mm Ø 3.3	118.182
4 mm Ø 4.5	118.183	6 mm Ø 4.5	118.184

Drivers



+



Torque Wrench

GM Titanium Base

Single-unit screw-retained prosthesis


Single-unit cement-retained prosthesis

Ø 3.5/4.5/
5.5/6.5 mm

With removable screw.



Installation Sequence

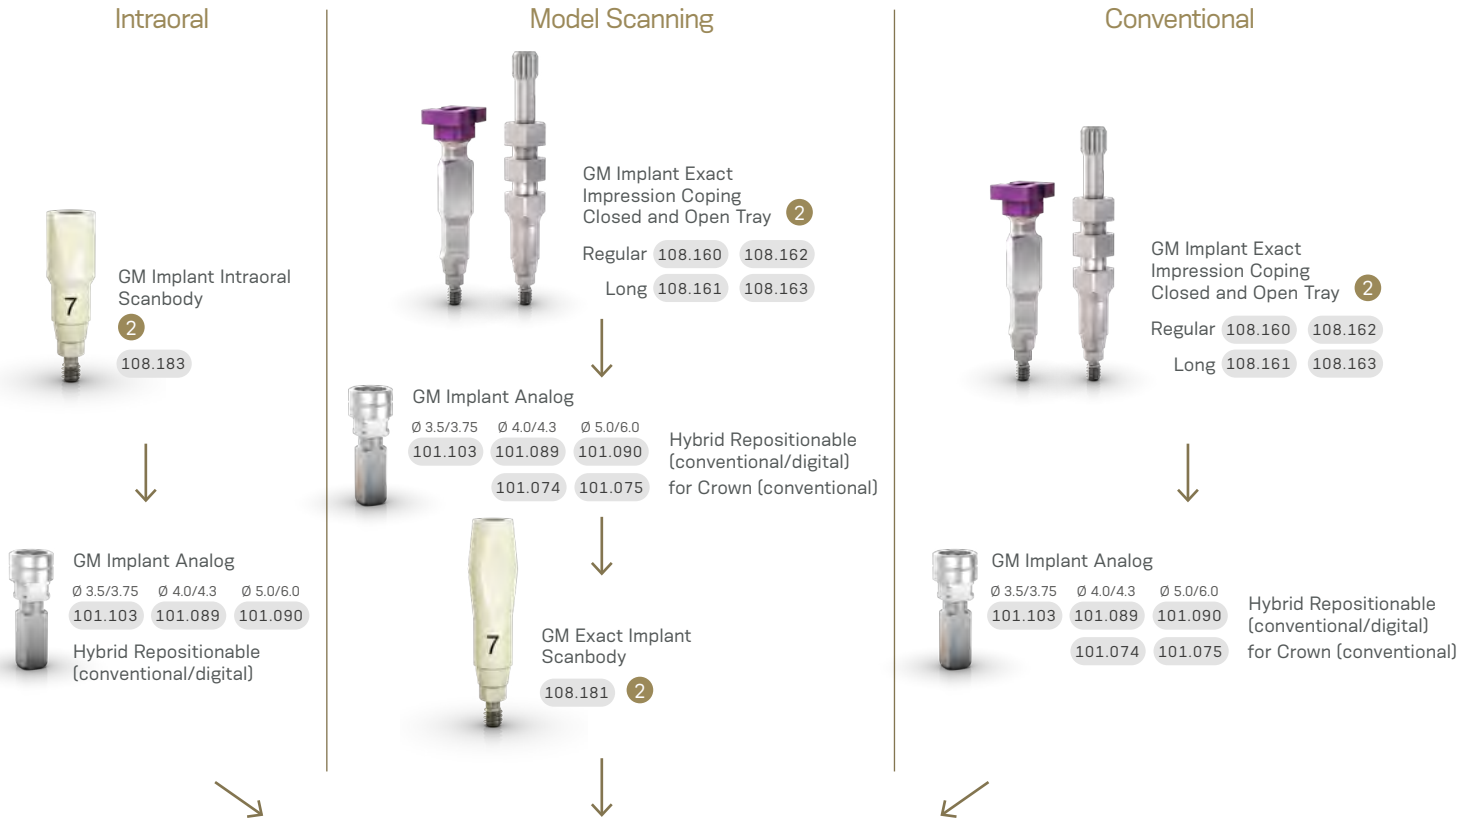

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	GM Exact Titanium Base 4mm	or	GM Exact Titanium Base 6mm		0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.260	135.261	135.262	135.263	135.264				Ø 3.5	135.266	135.267	135.268	135.269	135.270
Ø 4.5	135.272	135.273	135.274	135.275	135.276				Ø 4.5	135.278	135.279	135.280	135.281	135.282
Ø 5.5	135.284	135.285	135.286	135.287	135.288				Ø 5.5	135.290	135.291	135.292	135.293	135.294
Ø 6.5		135.319	135.320	135.321	135.322				Ø 6.5	135.323	135.324	135.325	135.326	

↓

GM Titanium Base Burn-out Coping

Ø 3.5	Ø 4.5	Ø 5.5
118.322	118.325	118.329
118.323	118.327	118.342

Drivers

1 Neo Screwdriver Torque Connection + Torque Wrench

2 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories


Replacement Sterile Screws
116.286

GM Titanium Base with Neo Removable Screw

Single-unit screw-retained prosthesis


Single-unit cement-retained prosthesis

Ø 3.5/4.5/5.5/6.5 mm

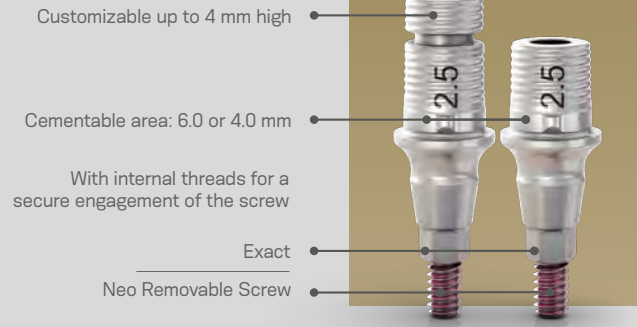


Installation Sequence


Intraoral

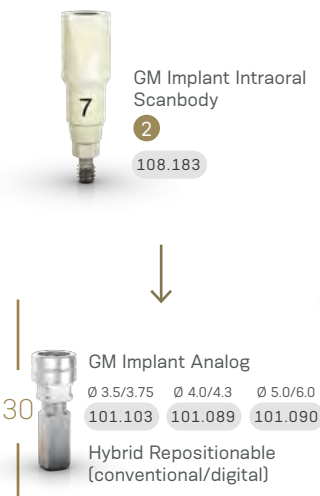

Model Scanning

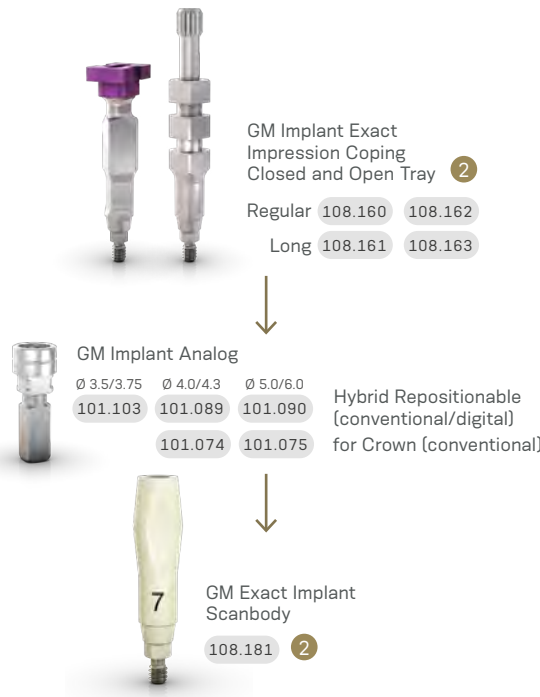

Conventional

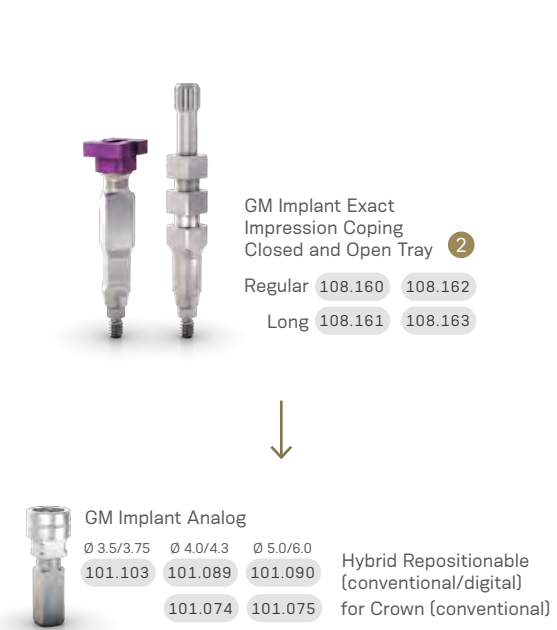


	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	GM Exact Titanium Base 4mm	Or	GM Exact Titanium Base 6mm		0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.355	135.356	135.357	135.358	135.359			Ø 3.5	135.361	135.362	135.363	135.364	135.365	
Ø 4.5	135.367	135.368	135.369	135.370	135.371			Ø 4.5	135.373	135.374	135.375	135.376	135.377	
Ø 5.5	135.379	135.380	135.381	135.382	135.383			Ø 5.5	135.385	135.386	135.387	135.388	135.389	
Ø 6.5	135.391	135.392	135.393	135.394				Ø 6.5	135.395	135.396	135.397	135.398		


GM Titanium Base Burn-out Coping

Ø 3.5	Ø 4.5	Ø 5.5	
118.322	118.325	118.329	4.0 mm
118.323	118.327	118.342	6.0 mm

Drivers

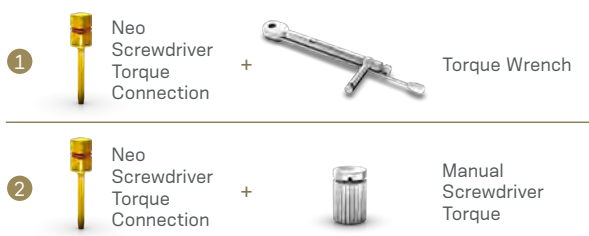

Accessories

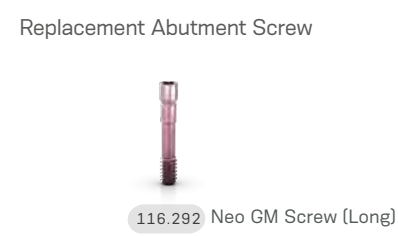

GM Titanium Base for Bridge



Multiple-unit
screw-
retained
prosthesis



Multiple-unit
cement-
retained
prosthesis



Ø 3.5/4.5/
5.5 mm

Cementable area:
4.0 mm for Ø 3.5
4.5 mm for Ø 4.5
and Ø 5.5



With removable screw.

Installation Sequence

Intraoral



GM Implant Intraoral
Scanbody
2
108.183



GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
Hybrid Repositionable
(conventional/digital)

Model Scanning



GM Implant Exact
Impression Coping
Open Tray
2
Regular 108.158
Long 108.159



GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
101.074 101.075
Hybrid Repositionable
(conventional/digital)
for Crown (conventional)




GM Exact Implant
Scanbody
108.181 2



GM Titanium
Base for
Bridge
20
Ncm
1

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.304	135.305	135.306	135.307	135.308
Ø 4.5	135.309	135.310	135.311	135.312	135.313
Ø 5.5	135.314	135.315	135.316	135.317	135.318


Drivers



+



Torque Wrench



+



Manual
Screwdriver
Torque

Accessories



Replacement
Sterile Screws

116.286



GM Titanium Base for Bridge with Neo Removable Screw



Multiple-unit screw-retained prosthesis



Multiple-unit cement-retained prosthesis



Ø 3.5/4.5/
5.5 mm

Cementable area:
4.0 mm for Ø 3.5
4.5 mm for Ø 4.5
and Ø 5.5.

With internal threads for secure engagement of the screw

Neo Removable Screw



Installation Sequence

Intraoral



GM Implant Intraoral Scanbody
2
108.183



GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
Hybrid Repositionable (conventional/digital)

Model Scanning



GM Implant Exact Impression Coping Open Tray
2
Regular 108.158
Long 108.159




GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
101.074 101.075
Hybrid Repositionable (conventional/digital) for Crown (conventional)



GM Exact Implant Scanbody
108.181 2





GM Titanium Base for Bridge	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø 3.5	135.399	135.400	135.401	135.402	135.403
Ø 4.5	135.404	135.405	135.406	135.407	135.408
Ø 5.5	135.409	135.410	135.411	135.412	135.413

Drivers

1



Neo Screwdriver Torque Connection

+



Torque Wrench

2



Neo Screwdriver Torque Connection

+



Manual Screwdriver Torque

Accessories


Replacement Abutment Screw




116.292 Neo GM Screw (Long)

GM Titanium Base Angled Solution (AS)






Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 4.0/4.5/5.5 mm

With removable screw.

Cementable area:
6.0 or 4.0 mm

Exact.



Installation Sequence

Intraoral



GM Implant Intraoral Scanbody
②
108.183



GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
Hybrid Repositionable (conventional/digital)

Model Scanning



GM Implant Exact Impression Coping Closed and Open Tray ②
Regular 108.160 108.162
Long 108.161 108.163




GM Implant Analog
Ø 3.5/3.75 Ø 4.0/4.3 Ø 5.0/6.0
101.103 101.089 101.090
101.074 101.075
Hybrid Repositionable (conventional/digital) for Crown (conventional)



GM Exact Implant Scanbody
②
108.181



			GM Titanium Base Angled Solution (AS) 4mm			GM Titanium Base Angled Solution (AS) 6mm		
	0.8 mm	1.5 mm	2.5 mm		0.8 mm	1.5 mm	2.5 mm	
Ø 4.0	135.327	135.328	135.329	 20 N.cm	Ø 4.0	135.330	135.331	135.332
Ø 4.5	135.333	135.334	135.335		Ø 4.5	135.336	135.337	135.338
Ø 5.5	135.339	135.340	135.341		Ø 5.5	135.342	135.343	135.344

Drivers

Accessories

①

Angled Solution Screwdriver for Torque Wrench


105.150 Short
105.151 Regular
105.152 Long

or

Angled Solution Screwdriver for Contra-angle


105.147 Short
105.148 Regular
105.149 Long

Torque Wrench



+

Contra-angle



②

Neo Screwdriver Torque Connection


+

Manual Screwdriver Torque




Replacement Sterile Screw


116.288 Screw for GM Titanium Base AS




Titanium Base C for GM

Cementable area: 4.7 mm

Exact



Single-unit screw-retained prosthesis




Single-unit cement-retained prosthesis



Ø 4.65 mm

With removable screw.

Installation Sequence

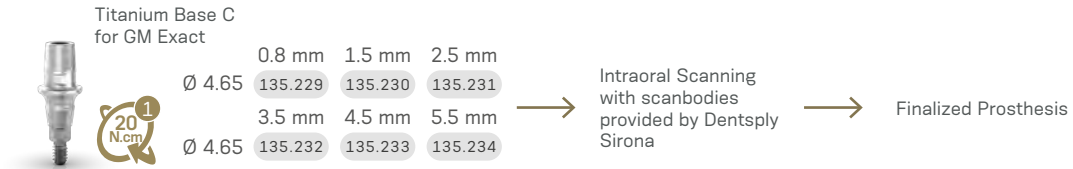

Workflow

Step 1

Gingiva height selection and ordering.



Select the Titanium Base C for GM Exact gingival height.



Order the Titanium Base C for GM Exact.

Please note that the scanbody has to be purchased directly from equipment manufacturer.

Step 2

Intra-oral scanning.



Insert the Titanium Base C for GM Exact in the Neodent® implant.



Insert scanbody on the Titanium Base C for GM Exact.

Step 3

Design and milling.



Select in the CAD software the comparable third-party Ti-base and perform the digital design.



Mill the digital design.

Step 4

Finalization and fixation.




- Check the fit of milled restoration in the patient's mouth and adapt it, if needed.
- Cement the restoration on the Titanium Base C for GM Exact and insert it into the patient's mouth.

CEREC® digital library compatibility

Library	Sirona's Products				Compatible with implant System	
Ti-base	Scanbody	REF Scanbody Omnicam	REF Scanbody Bluecam / Ineos	Grinding block	Implant manufacturer	Implant system
NBB 3.4 L						
NB A 4.5 L						
SSO 3.5 L						
S BL 3.3 L	L	6431329	6431303	inCoris ZI meso L	Neodent®	GM, CM, HE, IIPlus
S BL 4.1 L						
BO 3.4 L						

Drivers



+



Torque Wrench

Accessories



Replacement Sterile Screws

116.286 Titanium

Titanium Base C for GM with Neo Removable Screw



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø 4.65 mm

With internal threads for secure engagement of the screw


Cementable area: 4.7 mm

Exact

Neo Removable Screw



Installation Sequence

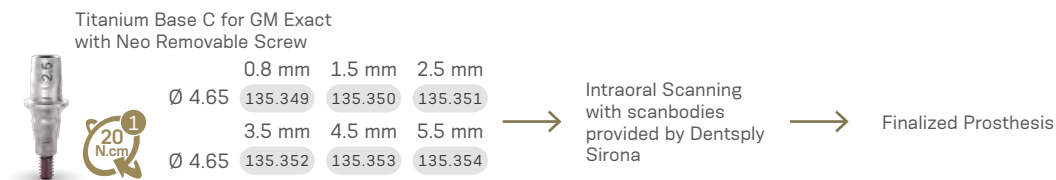

Workflow

Step 1

Gingiva height selection and ordering.




Select the Titanium Base C for GM Exact gingival height.



Order the Titanium Base C for GM Exact. Please note that the scanbody has to be purchased directly from equipment manufacturer.

Step 2

Intra-oral scanning.



Insert the Titanium Base C for GM Exact in the Neodent® implant.



Insert scanbody on the Titanium Base C for GM Exact.

Step 3

Design and milling.



Select in the CAD software the comparable third-party Ti-base and perform the digital design.



Mill the digital design.

Step 4

Finalization and fixation.




- Check the fit of milled restoration in the patient's mouth and adapt it, if needed.
- Cement the restoration on the Titanium Base C for GM Exact and insert it into the patient's mouth.

CEREC® digital library compatibility

Library	Sirona's Products			Compatible with implant System		
Ti-base	Scanbody	REF Scanbody Omnicam	REF Scanbody Bluecam / Ineos	Grinding block	Implant manufacturer	Implant system
NBB 3.4 L						
NB A 4.5 L						
SSO 3.5 L						
S BL 3.3 L	L	6431329	6431303	inCoris ZI meso L	Neodent®	GM, CM, HE, IIPlus
S BL 4.1 L						
BO 3.4 L						

Drivers



+



Torque Wrench

Accessories

Replacement Abutment Screw



116.292 Neo GM Screw (Long)

GM Titanium Block for MEDENTiKA Holder



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis




Multiple-unit cement-retained prosthesis



Ø 11.5/
15.8 mm

Screw sold separately.

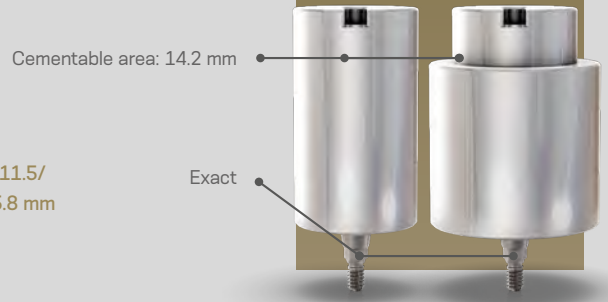

Installation Sequence

Complete Digital Workflow



GM Implant Intraoral Scanbody
2
108.183



GM Implant Analog
Ø 4.0/4.3
101.089
Hybrid Repositionable (conventional/digital)



GM Exact Titanium Block for MEDENTiKA Holder Ø 11.5mm



135.252

USK135.252-1



GM Exact Titanium Block for MEDENTiKA Holder Ø 15.8mm



135.253

USK135.253-1



Finalized Prosthesis with CAD/CAM process

Semi Digital Workflow



GM Implant Exact Impression Coping Closed and Open Tray 2
Regular 108.160 108.162
Long 108.161 108.163



GM Implant Analog
Ø 4.0/4.3
101.089 Hybrid Repositionable (conventional/digital)
101.074 Conventional



GM Exact Implant Scanbody
108.181 2



GM Exact Titanium Block for MEDENTiKA Holder Ø 11.5mm



135.252

USK135.252-1



135.253

USK135.253-1



Finalized Prosthesis with CAD/CAM process

Drivers



Neo Screwdriver Torque Connection



Torque Wrench



Neo Screwdriver Torque Connection



Manual Screwdriver Torque

Accessories



Sterile Screws sold separately

116.286 Titanium

GM Titanium Block for AG Holder



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Multiple-unit cement-retained prosthesis




Ø 12.0 mm

Screw sold separately.


Installation Sequence

Complete Digital Workflow



Finalized Prosthesis with CAD/CAM process

Semi Digital Workflow

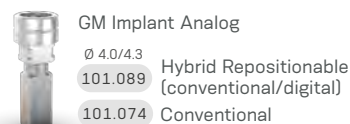


Finalized Prosthesis with CAD/CAM process

Drivers



Accessories



GM CoCr Abutment

Single-unit screw-retained prosthesis

Single-unit cement-retained prosthesis

Ø 4.1/4.5/
5.0 mm

Consider in addition 1.5 - 2.0 mm for the restorative material
Interocclusal height of 12 mm (can be customized up to 5.0 mm)



For implants placed at bone level.

Exact

Installation Sequence

GM Implant Exact Impression Coping Closed and Open Tray ²

Regular	108.160	108.162
Long	108.161	108.163

or

GM Temporary Abutment for Crown or GM Pro Peek Abutment

¹ 20 N.cm

GM Healing for CoCr Abutment ²

106.237	Ø 3.5 / 3.75
106.238	Ø 4.0 / 4.3
106.239	Ø 5.0 / 6.0

or

GM Implant Analog

↓

GM Exact CoCr Abutment Set

Ø 3.5 / 3.75	Ø 4.5 / 4.3	Ø 5.0 / 6.0
118.309	118.310	118.311

¹ 20 N.cm

The set includes one GM CoCr Abutment, one Screw and one GM Implant Analog.

38

Drivers

¹ Neo Screwdriver Torque Connection + Torque Wrench



² Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

Replacement Sterile Screws

116.283

GM Temporary Abutment




Consider in addition 1.5 - 2.0 mm for the restorative material

Channels for customization


Interocclusal height of 10 mm (can be customized up to 4.0 mm)

Exact

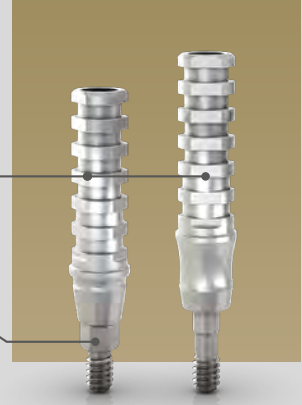

Customizable area made of titanium.
A minimum height of 4 mm of the customizable area must be kept.
With retentive grooves for acrylic material.


Installation Sequence

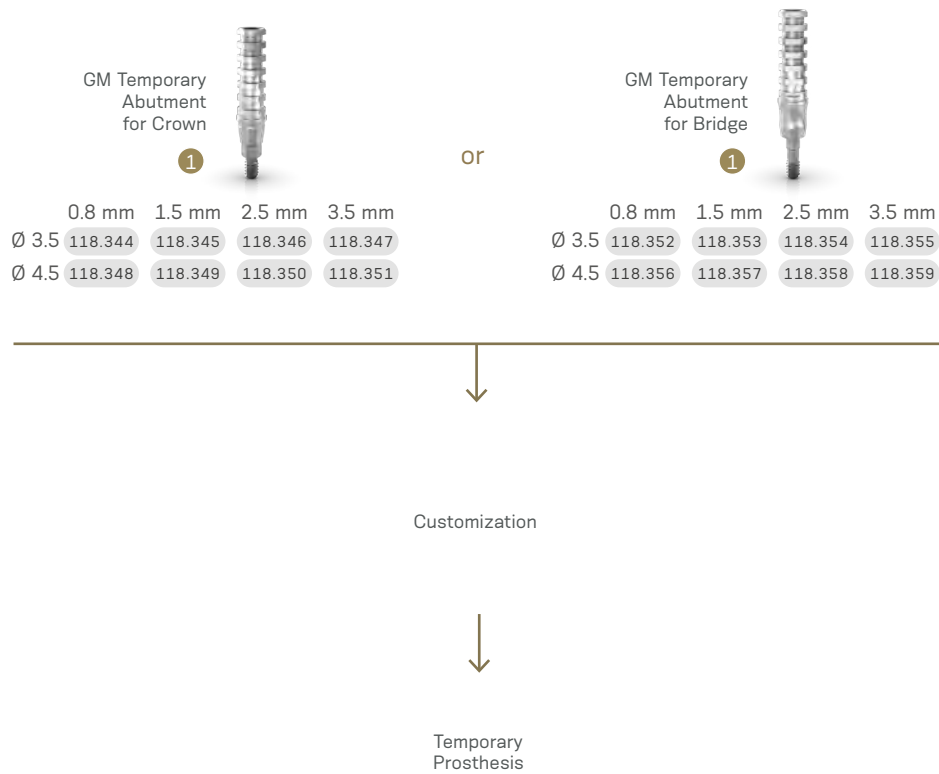

Drivers



Accessories





GM Pro Peek Abutment



Single-unit cement-retained temporary prosthesis



Ø 4.5/
6.0 mm

Biocompatible Peek for easy customization.

Consider in addition 1.5 - 2.0 mm for the restorative material


Interocclusal height of 9.2 mm (can be customized up to 5.0 mm)

Exact

Unlocking feature



Installation Sequence

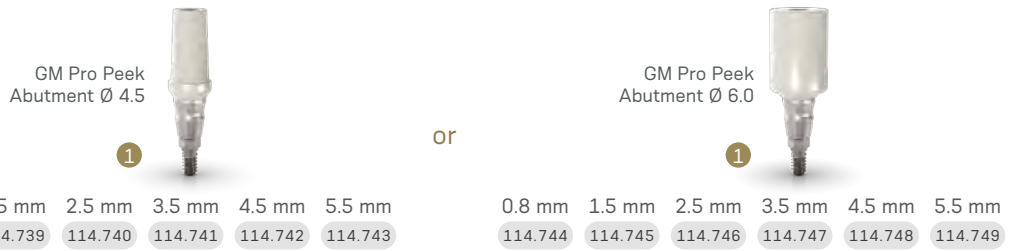

In mouth customization

40

Drivers



GM Pro Peek Abutment with Neo Removable Screw



Consider in addition 1.5 - 2.0 mm for the restorative material

Interocclusal height of 9.2 mm (can be customized up to 5.0 mm)

With internal threads for secure engagement of the screw


Exact

Neo Removable Screw

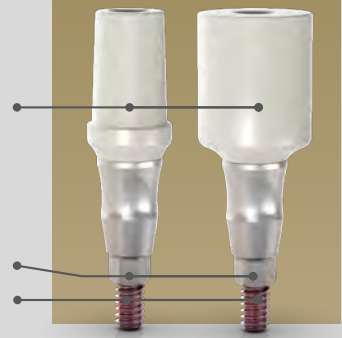

Biocompatible Peek for easy customization.

Installation Sequence

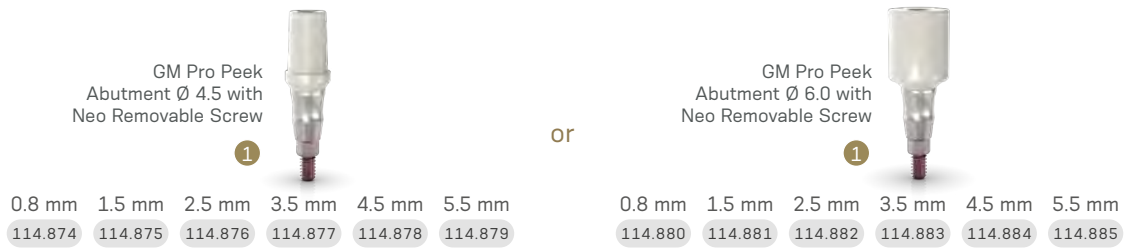

In mouth customization

Drivers




Accessories

Replacement Abutment Screw



GM Attachment TiN




Overdenture

Angled version with removable screw.




Installation Sequence

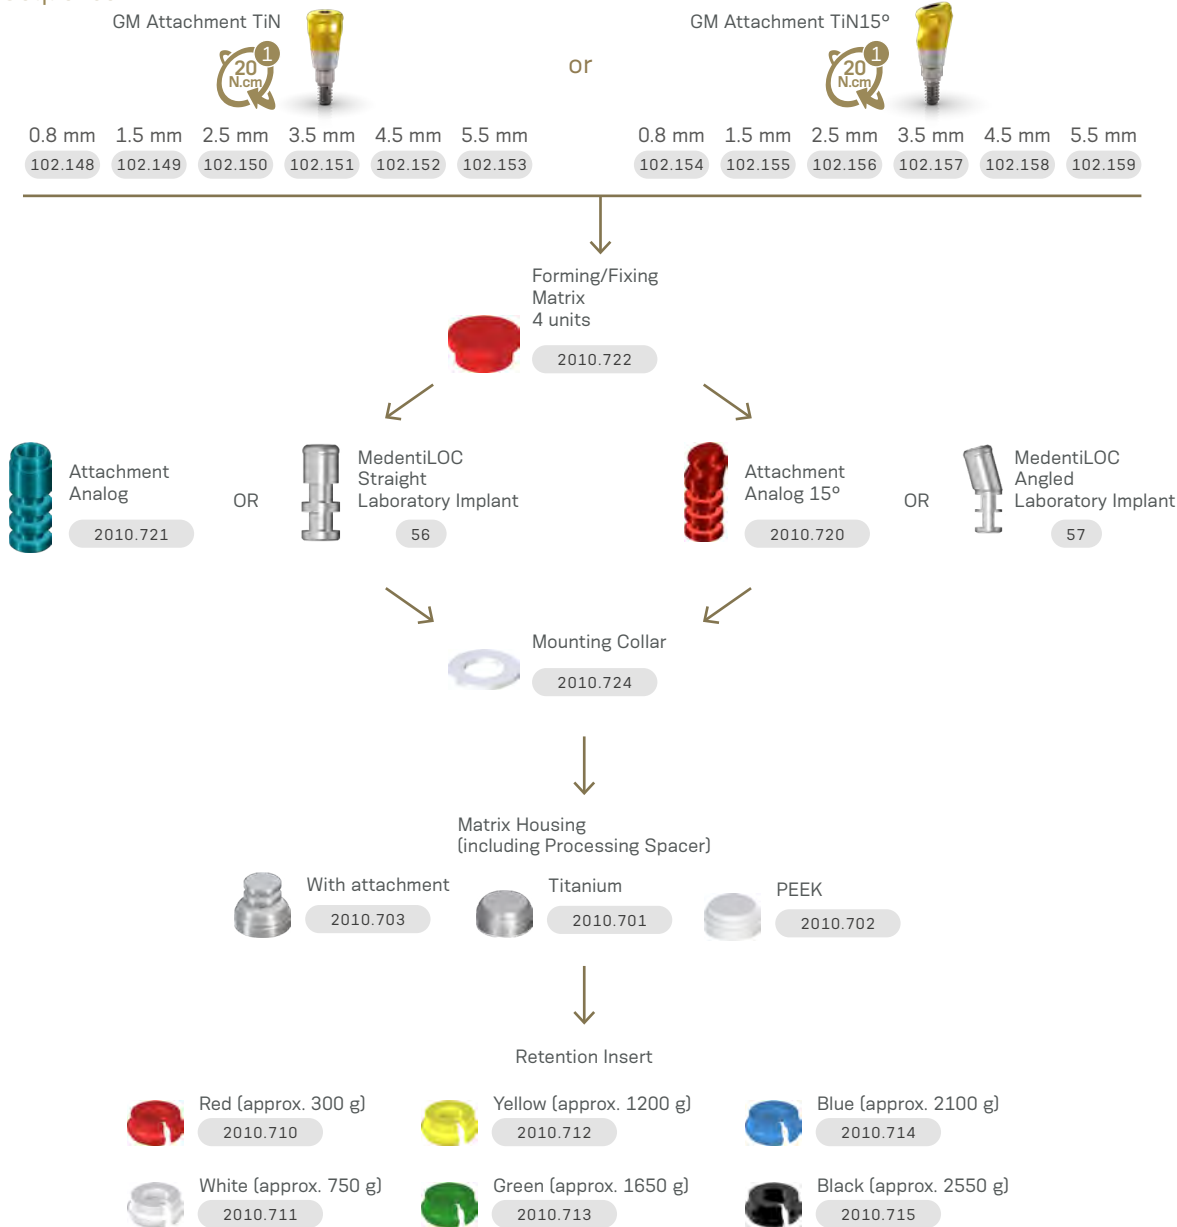

42

Drivers



Accessories





Measurements GM Mini Conical Abutment

17°




30°




Measurements GM Anatomic Abutment


Narrow Anatomic Abutment

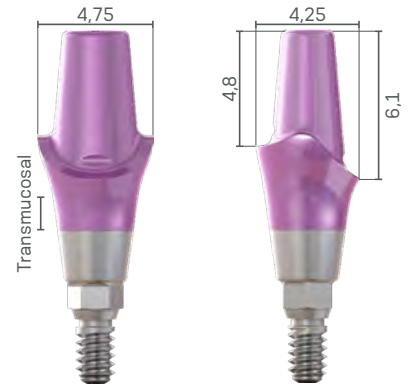

Anatomic Abutment

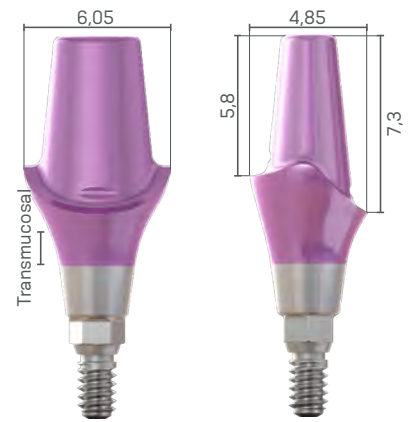

Narrow Anatomic Abutment 17°

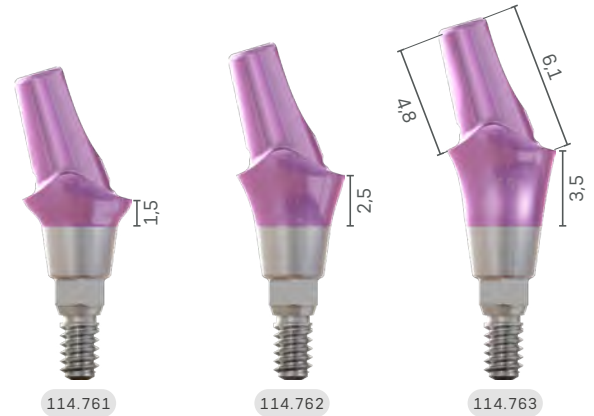

Anatomic Abutment 17°



Measurements GM Universal Abutment




4 mm chimney height / Ø 3.3 / 17°



4 mm chimney height / Ø 3.3 / 30°



4 mm chimney height / Ø 4.5 / 17°

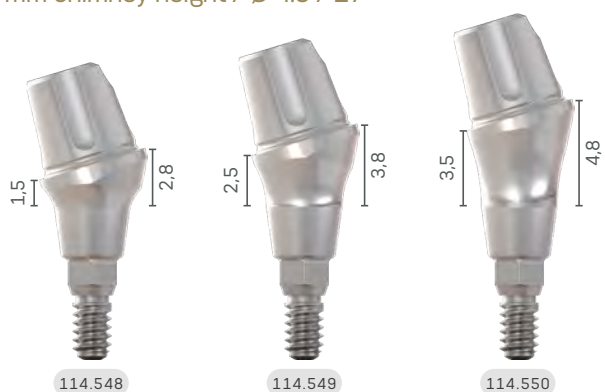

4 mm chimney height / Ø 4.5 / 30°



6 mm chimney height / Ø 3.3 / 17°



6 mm chimney height / Ø 3.3 / 30°



6 mm chimney height / Ø 4.5 / 17°



6 mm chimney height / Ø 4.5 / 30°





Grand Morse® Kits

Grand Morse[®] Surgical Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.302](#).



Articles

- 110.288 GM Surgical Kit Case
- 103.162 Twist Drill 2.0 Plus
- 103.213 Pilot Drill 2.0/3.0 Plus
- 103.164 Twist Drill 3.0 Plus
- 103.166 Twist Drill 3.3 Plus
- 103.167 Twist Drill 3.8 Plus
- 103.168 Twist Drill 4.3 Plus
- 103.163 Twist Drill 2.8 Plus
- 103.170 Initial Drill Plus
- 103.414 Pilot Drill GM 2.8/3.5
- 103.415 Pilot Drill GM 3.0/3.75
- 103.416 Pilot Drill GM 3.3/4.0
- 103.417 Pilot Drill GM 4.3
- 103.418 Pilot Drill GM 4.3/5.0

- 103.419 Tapered Contour Drill 3.5
- 103.420 Tapered Contour Drill 3.75
- 103.421 Tapered Contour Drill 4.0
- 103.422 Tapered Contour Drill 4.3
- 103.423 Tapered Contour Drill 5.0
- 103.425 Tapered Drill 2.0
- 103.399 Tapered Drill 3.5
- 103.402 Tapered Drill 3.75
- 103.405 Tapered Drill 4.0
- 103.408 Tapered Drill 4.3
- 103.411 Tapered Drill 5.0
- 103.427 Tapered Drill 6.0
- 105.131 GM Implant Driver - Contra-Angle
- 104.060 Neo Screwdriver (Medium)

- 105.130 GM Implant Driver - Torque Wrench (Long)
- 104.028 Manual Implant Driver - Contra-Angle
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 128.028 Height Measurer GM
- 129.004 Depth Probe
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench
- 103.426 Drill Extension

Note: Items that compose Neodent[®] Kits are sold separately.

Grand Morse[®] and WS Surgical Kit

Autoclavable polymer case.



Articles

- 110.287 GM/WS Surgical Kit Case
- 103.162 Twist Drill 2.0 Plus
- 103.213 Pilot Drill 2.0/3.0 Plus
- 103.164 Twist Drill 3.0 Plus
- 103.166 Twist Drill 3.3 Plus
- 103.415 GM Pilot Drill 3.0/3.75
- 103.167 Twist Drill 3.8 Plus
- 103.168 Twist Drill 4.3 Plus
- 103.215 Pilot Drill 4.3/5.3 Plus
- 103.163 Twist Drill 2.8 Plus
- 103.169 Twist Drill 5.3 Plus
- 103.170 Initial Drill Plus
- 103.414 Pilot Drill GM 2.8/3.5
- 103.416 Pilot Drill GM 3.3/4.0
- 103.417 Pilot Drill GM 4.3
- 103.418 Pilot Drill GM 4.3/5.0
- 103.221 Pilot Drill GM 5.3/6.0 Plus

- 103.419 Tapered Contour Drill 3.5
- 103.420 Tapered Contour Drill 3.75
- 103.421 Tapered Contour Drill 4.0
- 103.422 Tapered Contour Drill 4.3
- 103.423 Tapered Contour Drill 5.0
- 103.425 Tapered Drill 2.0
- 103.399 Tapered Drill 3.5
- 128.029 WS Height Measurer
- 103.402 Tapered Drill 3.75
- 103.405 Tapered Drill 4.0
- 103.408 Tapered Drill 4.3
- 103.411 Tapered Drill 5.0
- 103.427 Tapered Drill 6.0
- 105.131 GM Implant Driver - Contra-Angle
- 105.002 Smart/WS Implant Driver - Contra-Angle
- 104.060 Neo Screwdriver (Medium)
- 105.130 GM Implant Driver GM - Torque Wrench

- 105.018 Hex Connection - Torque Wrench (Long)
- 104.028 Manual Implant Driver - Contra-Angle
- 104.012 Manual Screwdriver (Medium)
- 105.129 GM Implant Driver GM - Torque Wrench
- 105.001 Smart/WS Implant Driver - Torque Wrench (Short)
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 128.024 WS Direction Indicator 4.3/5.0
- 128.025 WS Direction Indicator 5.3/6.0
- 128.028 GM Height Measurer
- 129.004 Depth Probe
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench
- 103.426 Drill Extension

Note: Items that compose Neodent[®] Kits are sold separately.

Helix GM[®] Compact Surgical Kit

Autoclavable polymer case.

The Kit allows the installation of Helix GM[®] Implants in all bone types.

To order the pre-mounted version of the kit, with its complete composition, use code [110.303](#).



Articles

- 110.297 Helix GM[®] Compact Surgical Kit Case
- 103.170 Initial Drill
- 103.425 Tapered Drill 2.0
- 103.399 Tapered Drill 3.5
- 103.402 Tapered Drill 3.75
- 103.405 Tapered Drill 4.0
- 103.408 Tapered Drill 4.3
- 103.411 Tapered Drill 5.0
- 103.427 Tapered Drill 6.0
- 103.487 Tapered Drill 7.0 (Short)*
- 104.060 Neo Manual Screwdriver (Medium)
- 104.028 Manual Implant Driver - Contra-angle

- 103.426 Drill Extension
- 103.419 Tapered Contour Drill 3.5
- 103.420 Tapered Contour Drill 3.75
- 103.421 Tapered Contour Drill 4.0
- 103.422 Tapered Contour Drill 4.3
- 103.423 Tapered Contour Drill 5.0
- 105.131 GM Implant Driver - Contra-angle GM
- 105.130 Implant Driver - Torque Wrench (Long)
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 103.414 GM Pilot Drill 2.8/3.5
- 103.415 GM Pilot Drill 3.0/3.75
- 103.416 GM Pilot Drill 3.3/4.0

- 103.417 GM Pilot Drill 4.3
- 103.418 GM Pilot Drill 4.3/5.0
- 128.028 GM Height Measurer
- 128.030 Angle Measurer for Drill 2.0 17°
- 128.031 Angle Measurer for Drill 2.0 30°
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 129.004 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent[®] Kits are sold separately.

*Tapered Drill 7.0 is not included in the pre-mounted kit composition.



Neodent controlsystem



TRUST YOURSELF


The surgical procedure for implant placement can be perceived as complex, especially when performed in the posterior regions with limited visibility, or in proximity with anatomical structures such as nerve canals. The Neodent® Control System brings confidence and efficiency building trust during the surgical procedure.

Protect anatomical structures

The placement of implants requires accuracy, and the Neodent® Control System has been designed to reduce the risk against overdrilling and protecting anatomical structures such as nerves, the sinus or adjacent roots by securing the final depth.

Master limited visibility

The Neodent® Control System helps to provide confidence during situations with reduced visibility due to adjacent teeth, limited mouth opening, blood, saliva, making it difficult to read the lines on a twisting drill by reaching the planned depth.

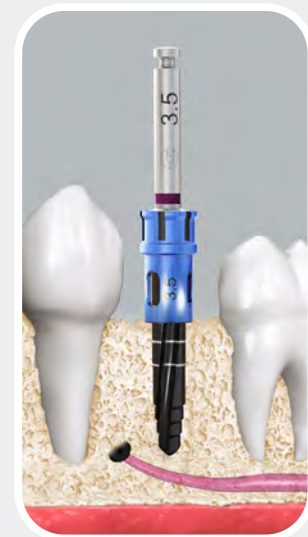

Intuitive solution

The Neodent® Control System is a color coded solution facilitating the identification of the drill sequence, the diameter and length of the implant and the combination of drill stop and drill.



Secure drill stop locking system

The Neodent® Control Drill Stop features a modern drill locking system enabling an easy and secure engaging into the drill, offering a peace-of-mind surgical experience.



Multiple use solution

The Neodent® Control Drill Stops are made of titanium for professional cleaning and autoclaving allowing multiple use.

User friendly kit retentive system

The Neodent® Control Drill Stop Kit includes an innovative retentive system.



A convenient and time-saving pick and drop mechanism during the surgical procedure.

Neodent® Color Code overview



Color code according to implant length



Compatible portfolio of Helix GM® Implants*



Length	Diameter						
	3.5	3.75	4.0	4.3	5.0	6.0	7.0
8	✓	✓	✓	✓	✓	✓	✓
10	✓	✓	✓	✓	✓	✓	✓
11.5	✓	✓	✓	✓	✓	✓	✓
13	✓	✓	✓	✓	✓	✓	✓

*Note that this system can be used with GM Drive and Helix implants.



Helix GM[®] Compact Kit Control Stop Drills

Autoclavable polymer case.

The Kit allows the installation of Helix GM[®] Implants in all bone types, using the Neodent[®] Control Stop Drills.

To order the pre-mounted version of the kit, with its complete composition, use code [110.308](#).



Articles

- 110.297 Helix GM[®] Compact Surgical Kit Case
- 103.170 Initial Drill
- 103.492 Tapered Control Stop Drill 2.0
- 103.493 Tapered Control Stop Drill 3.5
- 103.494 Tapered Control Stop Drill 3.75
- 103.495 Tapered Control Stop Drill 4.0
- 103.496 Tapered Control Stop Drill 4.3
- 103.497 Tapered Control Stop Drill 5.0
- 103.498 Tapered Control Stop Drill 6.0 (Short)
- 103.499 Tapered Control Stop Drill 7.0 (Short)*
- 104.060 Neo Manual Screwdriver (Medium)
- 104.028 Manual Implant Driver - Contra-angle

- 103.426 Drill Extension
- 103.500 Tapered Control Stop Drill 3.5+
- 103.501 Tapered Control Stop Drill 3.75+
- 103.502 Tapered Control Stop Drill 4.0+
- 103.503 Tapered Control Stop Drill 4.3+
- 103.504 Tapered Control Stop Drill 5.0+
- 105.131 GM Implant Driver - Contra-angle GM
- 105.130 Implant Driver - Torque Wrench (Long)
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 103.513 Pilot Drill 3.5
- 103.514 Pilot Drill 3.75
- 103.515 Pilot Drill 4.0

- 103.516 Pilot Drill 4.3
- 103.517 Pilot Drill 5.0
- 128.028 GM Height Measurer
- 128.030 Angle Measurer for Drill 2.0 17°
- 128.031 Angle Measurer for Drill 2.0 30°
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 129.004 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent[®] Kits are sold separately.

*Tapered Control Stop Drill 7.0 is not included in the pre-mounted kit composition (110.308).

Control Drill Stop Kit

Autoclavable polymer case.

The Kit allows the sterilization and engagement of Neodent[®] Control Drill Stops on the drills.

To order the pre-mounted version of the kit, with its complete composition, use code [110.306](#).



Articles

- 110.307 Control Drill Stop Kit Case
- 125.144 8.0 Control Drill Stop D2.0
- 125.145 10.0 Control Drill Stop D2.0
- 125.146 11.5 Control Drill Stop D2.0
- 125.147 13.0 Control Drill Stop D2.0
- 125.148 8.0 Control Drill Stop D3.5
- 125.149 10.0 Control Drill Stop D3.5
- 125.150 11.5 Control Drill Stop D3.5
- 125.151 13.0 Control Drill Stop D3.5
- 125.152 8.0 Control Drill Stop D3.75/4.0
- 125.153 10.0 Control Drill Stop D3.75/4.0
- 125.154 11.5 Control Drill Stop D3.75/4.0


- 125.155 13.0 Control Drill Stop D3.75/4.0
- 125.156 8.0 Control Drill Stop D4.3/5.0
- 125.157 10.0 Control Drill Stop D4.3/5.0
- 125.158 11.5 Control Drill Stop D4.3/5.0
- 125.159 13.0 Control Drill Stop D4.3/5.0
- 125.160 8.0 Control Drill Stop D6.0/7.0
- 125.161 10.0 Control Drill Stop D6.0/7.0
- 125.162 11.5 Control Drill Stop D6.0/7.0
- 125.163 13.0 Control Drill Stop D6.0/7.0

Note: Items that compose Neodent[®] Kits are sold separately.

Grand Morse® Prosthetic Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.304](#).

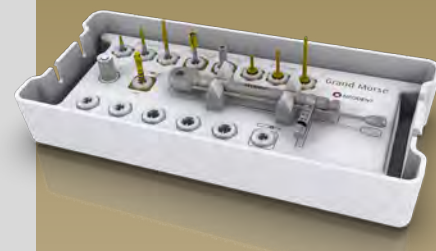

Articles

- 110.294 GM Prosthetic Kit Case
- 105.146 Neo Screwdriver Torque Connection - Contra-angle (Extra-short)
- 105.135 Neo Screwdriver Torque Connection - Contra-angle (Short)
- 105.136 Neo Screwdriver Torque Connection - Contra-angle (Medium)
- 105.138 Hexagonal Prosthetic Driver - Contra-angle
- 105.137 Hexagonal Prosthetic Driver - Torque Wrench
- 105.133 Neo Screwdriver Torque Connection (Short) - Torque Wrench
- 105.132 Neo Screwdriver Torque Connection (Medium) - Torque Wrench
- 105.134 Neo Screwdriver Torque Connection (Long) - Torque Wrench
- 104.005 Manual Screwdriver Torque
- 128.028 GM Height Measurer
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse® Try-In Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.305](#).



Articles

- | | | |
|--------------------------------------|--|---|
| 110.295 GM Try-In Kit Case | 114.782 GM Abutment Try-In 4.5X6X4.5 | 114.793 GM Abutment Try-In 30° 4.5X6X1.5 |
| 114.772 GM Abutment Try-In 3.3X6X0.8 | 114.783 GM Abutment Try-In 4.5X6X5.5 | 114.794 GM Abutment Try-In 30° 4.5X6X2.5 |
| 114.773 GM Abutment Try-In 3.3X6X1.5 | 114.784 GM Abutment Try-In 17° 3.3X6X1.5 | 114.795 GM Abutment Try-In 30° 4.5X6X3.5 |
| 114.774 GM Abutment Try-In 3.3X6X2.5 | 114.785 GM Abutment Try-In 17° 3.3X6X2.5 | 114.796 GM Anatomic Abutment Try-In 1.5 |
| 114.775 GM Abutment Try-In 3.3X6X3.5 | 114.786 GM Abutment Try-In 17° 3.3X6X3.5 | 114.797 GM Anatomic Abutment Try-In 2.5 |
| 114.776 GM Abutment Try-In 3.3X6X4.5 | 114.787 GM Abutment Try-In 17° 4.5X6X1.5 | 114.798 GM Anatomic Abutment Try-In 3.5 |
| 114.777 GM Abutment Try-In 3.3X6X5.5 | 114.788 GM Abutment Try-In 17° 4.5X6X2.5 | 114.799 GM Lateral Anatomic Abutment Try-In 1.5 |
| 114.778 GM Abutment Try-In 4.5X6X0.8 | 114.789 GM Abutment Try-In 17° 4.5X6X3.5 | 114.800 GM Lateral Anatomic Abutment Try-In 2.5 |
| 114.779 GM Abutment Try-In 4.5X6X1.5 | 114.790 GM Abutment Try-In 30° 3.3X6X1.5 | 114.801 GM Lateral Anatomic Abutment Try-In 3.5 |
| 114.780 GM Abutment Try-In 4.5X6X2.5 | 114.791 GM Abutment Try-In 30° 3.3X6X2.5 | 104.058 Neo Manual Screwdriver (Short) |
| 114.781 GM Abutment Try-In 4.5X6X3.5 | 114.792 GM Abutment Try-In 30° 3.3X6X3.5 | 128.028 GM Height Measurer |

Note: Items that compose Neodent® Kits are sold separately.



Grand Morse® Instruments



Initial Drill

- :: Available in surgical steel;
- :: 2.0mm diameter.

103.170

Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® and Drive GM® Implants.



	Short 31 mm	Regular 35 mm	Long 43 mm
Ø 2.0	103.559	103.425	103.560
Ø 3.5	103.400	103.399	103.401
Ø 3.75	103.403	103.402	103.404
Ø 4.0	103.406	103.405	103.407
Ø 4.3	103.409	103.408	103.410
Ø 5.0	103.412	103.411	103.413
Ø 6.0	103.427		

Tapered Contour Drills

- :: For preparing the implant bed in bone types I and II for Helix GM® Implants.



Ø 3.5+	103.419
Ø 3.75+	103.420
Ø 4.0+	103.421
Ø 4.3+	103.422
Ø 5.0+	103.423

Pilot Drills

- :: Available in surgical steel;
- :: Increasing the surgical alveolus diameter ridge, easing the penetration of the next drill or the implant.



Ø 2/3	103.213		
Ø 2.8/3.5	103.414	Ø 4.3/5	103.418
Ø 3/3.75	103.415	Ø 3.8/4.3	103.214
Ø 3.3/4	103.416	Ø 4.3/5.3	103.215
Ø 3.6/4.3	103.417	Ø 5.3/6	103.221

Twist Drills

- :: Available in surgical steel;
- :: Drill sequence for Titamax GM® Implants.



	Short 31 mm	Regular 35 mm	Long 43 mm
Ø 2.0	103.222	103.162	103.228
Ø 2.8	103.223	103.163	103.229
Ø 3.0	103.224	103.164	103.230
Ø 3.3	103.225	103.166	103.231
Ø 3.8	103.226	103.167	
Ø 4.3	103.227	103.168	

Tapered Control Stop Drills



- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Implants;
- :: Attachment to engage drill stops;
- :: With a color code according to the drill diameter.

Ø 2.0	103.492	Ø 4.3	103.496
Ø 3.5	103.493	Ø 5.0	103.497
Ø 3.75	103.494	Ø 6.0	103.498
Ø 4.0	103.495	Ø 7.0	103.499

Tapered+ Control Stop Drills



- :: Available in surgical steel;
- :: For preparing the implant bed in bone types I and II for Helix GM® Implants;
- :: Attachment to engage drill stops;
- :: With a color code according to the drill diameter and 2 stripes of color for identification.

Ø 3.5+	103.500	Ø 4.3+	103.503
Ø 3.75+	103.501	Ø 5.0+	103.504
Ø 4.0+	103.502		

Control Drill Stops


- :: Available in titanium;
- :: To be used in association with the Control Stop Drills;
- :: Physical control for drilling depth.

	8 mm	10 mm	11.5 mm	13 mm
Ø 2.0	125.144	125.145	125.146	125.147
Ø 3.5	125.148	125.149	125.150	125.151
Ø 3.75/4.0	125.152	125.153	125.154	125.155
Ø 4.3/5.0	125.156	125.157	125.158	125.159
Ø 6.0/7.0	125.160	125.161	125.162	125.163



Direction Indicators

- :: Available in titanium;
- :: Instrument to guide the implant position;
- :: Diameter of central band corresponds to GM Implant diameter;
- :: Smaller side to be used after Ø2.0mm drill;
- :: Larger side to be used after the last drill before implant installation.



2.8/3.5	128.019	3.6/4.3	128.022
3.0/3.75	128.020	4.3/5.0	128.023
3.3/4.0	128.021		

Drill Extension


- :: Available in surgical steel;
- :: Fit the drill directly into the Drill Extension.



103.426

GM Height Measurer

- :: Available in titanium;
- :: For selecting GM prosthetic abutments;
- :: Marks corresponding to transmucosa heights.
- :: Can be used as X-Ray Positioner.



128.028

GM Implant Driver - Contra-Angle



- :: To capture the implant directly from the packaging;
- :: To place GM Implants with contra-angle, or attached to a manual driver for contra-angle connections (104.028) for hand placement;
- :: With six dimples to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque 35 N.cm.

105.131

GM Implant Driver - Torque Wrench



- :: To place GM Implants with the Torque Wrench (104.050);
- :: With six marks to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque: 60 N.cm.

Short	Long
22 mm	30 mm
105.129	105.130

Angled Solution Screwdriver for Torque Wrench



- :: To place GM Titanium Bases for Angled Solution with torque wrench;
- :: Maximum torque of 20 N.cm.

Short	Medium	Long
16.5 mm	22.5 mm	28.5 mm
105.150	105.151	105.152

Angled Solution Screwdriver for Contra-angle



- :: To place GM Titanium Bases for Angled Solution with contra-angle;
- :: Maximum torque of 20 N.cm.

Short	Medium	Long
20 mm	26 mm	32 mm
105.147	105.148	105.149

Neo Screwdriver Torque Connection - Torque Wrench



- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
16.5 mm	22 mm	32 mm
105.133	105.132	105.157

GM Bone Profile Drill with Guide



- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.424

Neo Manual Screwdriver



- :: Available in surgical steel;
- :: Yellow color for line identification

Short	Medium	Long
21 mm	25 mm	37 mm
104.058	104.060	104.072

Angle Measurer for Drill 2.0



- :: Available in titanium;
- :: Angles: 17° and 30°;
- :: To select and plan the abutments angulation during surgical procedures;
- :: Suggested use: after Twist Drill 2.0.

17°	30°
128.030	128.031

Neo Screwdriver Torque Connection - Contra-angle



- :: Available in surgical steel;
- :: Yellow color for line identification;
- :: Extra Short Neo Screwdriver Torque Connection - Contra-angle (105.146) recommended for Impression Copings, Cover Screws and Healing Abutments.

Extra Short	Short	Long
16.5 mm	24 mm	31 mm
105.146	105.135	105.160

GM Angle Measurer



- :: Available in titanium;
- :: Angles: 17° and 30°;
- :: To a more accurate selection and planning of the abutments angulation during the prosthetic phase.

17°	30°
128.032	128.033

Hexagonal Prosthetic Driver



- :: Available in surgical steel;
- :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;

Contra-angle	Torque Wrench
105.138	105.137

Control Stop Kit Holder



- :: Available in polymer;
- :: Replacement piece;
- :: To keep the stops organized and to engage and remove them from the drills.

110.310

Manual Implant Drivers



- :: Available in surgical steel;
- :: For Contra-angle connections: connected to GM Implant Driver, it becomes a manual driver for implant placement.
- :: For Torque Wrench connections: connected to screwdrivers, it provides manual torque.

Contra-angle
Connections
104.028

Torque Wrench
Connections
104.005

Remover for Abutments with internal threads



- :: Available in surgical steel;
- :: To remove abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws

Short
130.118

Long
130.114

Remover for Neo Screws



- :: Available in surgical steel;
- :: Compatible with Neo removable screws for abutments

Short
130.119

Long
130.115

Torque Wrench



- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050

Removal Sets for Abutments with internal threads and Neo Screws

- :: Available in surgical steel;
- :: To remove Neo Removable Screws and abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws



Short
130.117

Long
130.116




A SMILE FOR EVERYONE

NEODENT® NEOARCH®

IMMEDIATE FIXED FULL-ARCH SOLUTION

Increasing expectations for shortened treatment duration represent a significant challenge for dental professionals especially in patients with anatomical deficiencies. The Neodent® Implant System offers an optimized solution for immediate fixed treatment protocols in edentulous patients even with severe atrophic maxilla. Neodent® NeoArch® allows to significantly improve patient satisfaction and quality of life by immediately restoring function and esthetics ⁽¹⁰⁾.

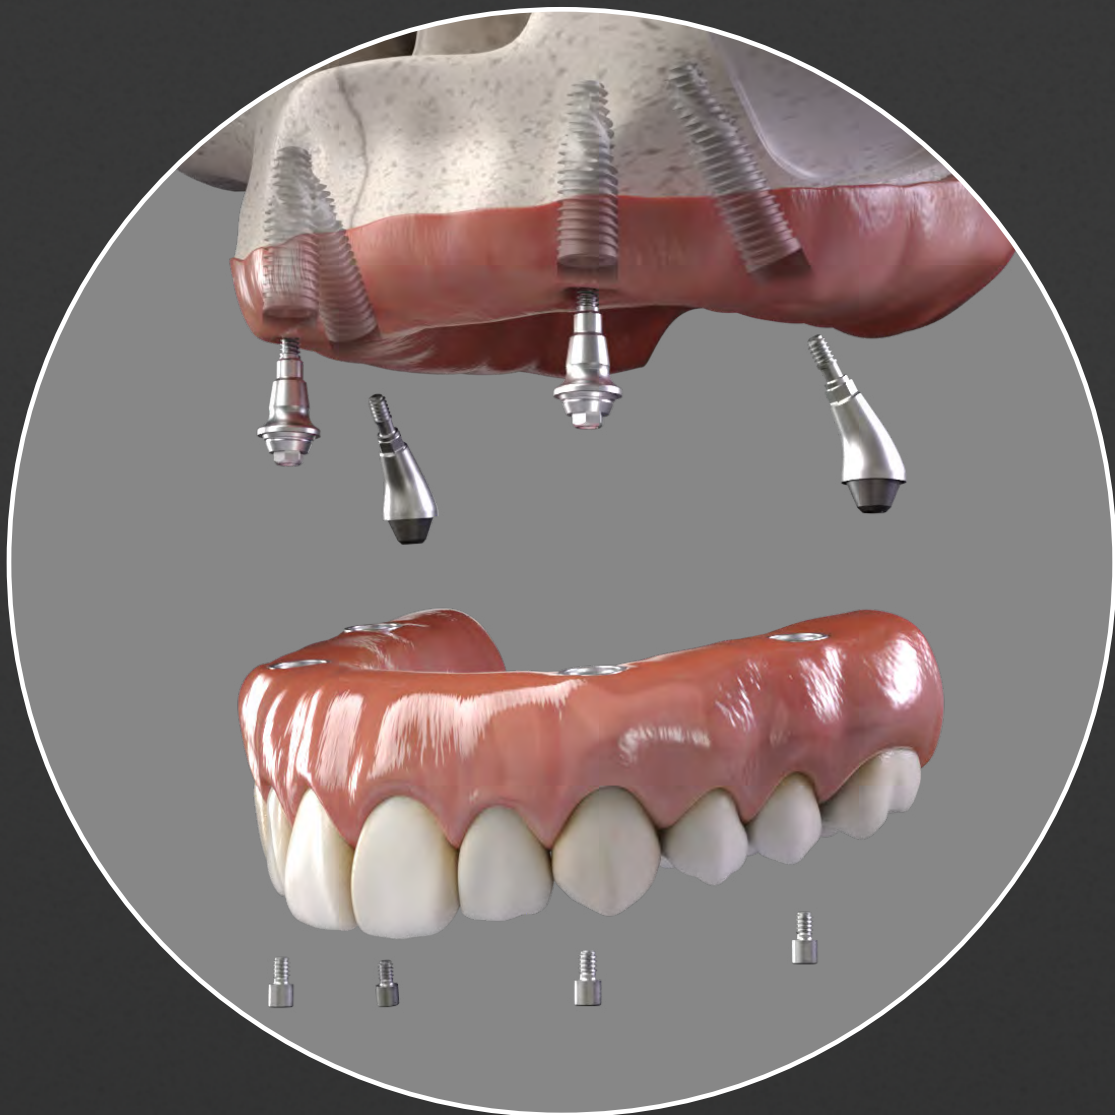



Immediate function resulting in shorter treatment times.

- Different implant techniques to minimize the use of a grafting procedure^(1,1).
- Optimized implant design to achieve high primary stability in all bone types^(1,2).



Immediate natural-looking esthetics with versatile restorative options.

- A broad range of abutment heights to cater the patient's needs.
- Options of straight and angled abutments (17°, 30° and 45°).



Immediate peace of mind thanks to a stable foundation.

- One connection regardless of the implant diameter.
- Unique connection combining Platform Switching associated with a deep 16° Morse taper including an internal indexation.

SOLUTIONS FOR ALL CLINICAL NEEDS

A implant system designed for predictable immediate treatments in all bone types even with different conditions of the residual alveolar bone.

60



Helix GM®



Helix GM® Long



Zygoma GM™



BONE RESORPTION

Helix GM[®] Long

PRODUCT FEATURES:

Implants Description:

- Full dual tapered implant;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex including a soft rounded small tip and helicoidal flutes;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-tapping threads on the apical part;
- Double lead threaded implant;
- Holder integrated to the implant body, which adapt in the packaging;
- Neoporos surface;
- Grand Morse[®] connection.

Indications:


- Indicated for surgical intraoral installation, in bone types III/IV for cases of total or partial edentulism and for multiple-unit prostheses.

Drilling features:

- For infraosseous positioning it is recommended to add 1 to 2 mm in length to the implant during surgical instrumentation.
- Drilling speed: 500-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.

Available with:

NeoPoros[®]

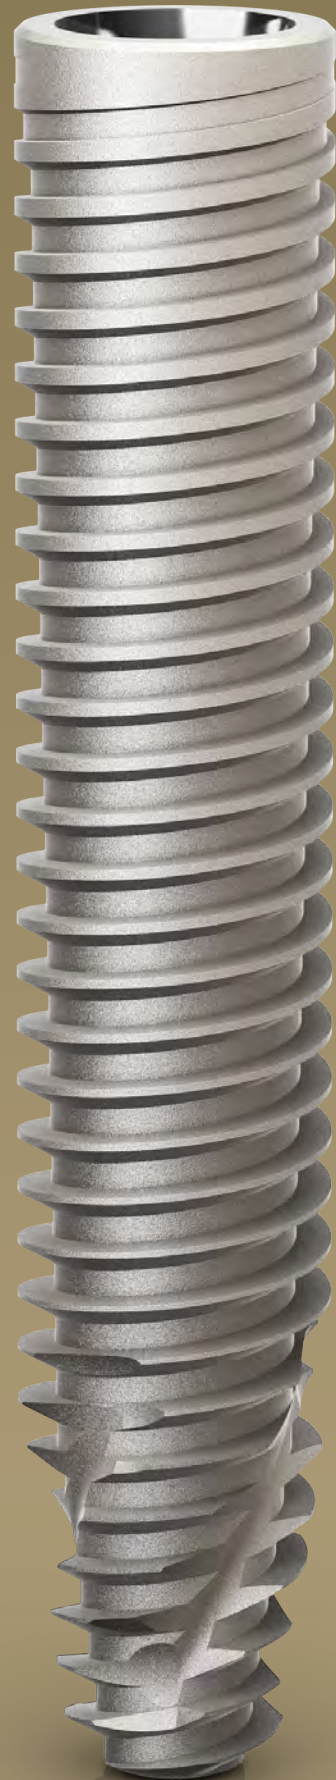

Drill Sequence

	Initial	Ø 2.35	Ø 3.75	Ø 4.0
	103.453	103.462	103.463	103.464
Ø 3.75 mm	Optional	✓	✓	
Ø 4.0 mm	Optional	✓	✓	✓

Bone types III and IV

The procedure can be with Guided Surgery. Check the instruments for more information.

Helix GM® Long implants

		20.0 mm	22.5 mm	25.0 mm
Ø 3.75	NeoPoros			
		109.1043	109.1044	109.1045
Ø 4.0	NeoPoros			
		109.1046	109.1047	109.1048

GM Healing Abutment



Profile	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø 3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø 4.5	106.213	106.214	106.215	106.216	106.217	106.218

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø 5.5	106.223	106.224	106.225	106.226	106.227	
Ø 7.0		106.228	106.229	106.230	106.231	106.232

GM Cover Screw



	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

Zygoma GM™

PRODUCT FEATURES:

Implants Description:

- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- The apex has a conical profile with a spherical tip and three equally spaced helical flutes;
- Trapezoidal thread and progressive increase of the thread depth at the apical portion;
- Tissue Protect: portion without threads, near the cervical region, indexed to the hexagon face;
- Holder integrated to the implant body, which adapt in the packaging;
- Neoporos surface;
- Grand Morse® connection.

Indications:

- Indicated for surgical procedures in the the posterior region of the maxilla and in the zygoma, in cases of severe maxilla resorption. Zygomatic Implants may be used in immediate loading procedures when there is good primary stability and appropriate occlusal loading.

Drilling features:

- Drilling speed: 800-1200 rpm;
- Lateral Direction Drill speed: 600-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 N.cm.



Available with:

NeoPoros®

Drill Sequence

	Ø 2.35	Lateral Direction Ø 4.0	Pilot Ø 2.3/3.2	Ø 3.75	Ø 4.0
	103.455	103.458	103.465	103.456	103.457
Ø 4.0 mm	✓	Optional	Optional	✓	✓

The procedure can start guided. Check the instruments for more information.

Zygoma GM™ Implants

30.0 mm 35.0 mm 37.5 mm 40.0 mm 42.5 mm 45.0 mm 47.5 mm 50.0 mm 52.5 mm 55.0 mm

Ø 4.0

NeoPoros 109.1049 109.1050 109.1051 109.1052 109.1053 109.1054 109.1055 109.1056 109.1057 109.1058

GM Cover Screw

0 mm	2 mm
117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 N.cm.

GM Mini Conical Abutment




Multiple-unit screw-retained prosthesis



Ø 4.8 mm

Consider in addition 1.5 - 2.0 mm for the restorative material
Minimum interocclusal space of 4.5 mm from the mucosa level for straight abutments

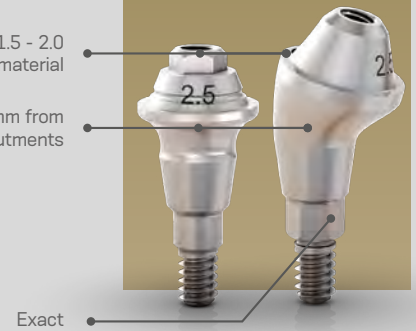

Installation Sequence

0.8 mm	1.5 mm	2.5 mm
115.243	115.244	115.245
3.5 mm	4.5 mm	5.5 mm
115.246	115.247	115.248



or



	1.5 mm	2.5 mm	3.5 mm
17°	115.249	115.250	115.251
30°	115.252	115.253	115.254
45°	115.267	115.268	

*The 45° Mini Conical Abutment is indicated for use only with Helix GM® Long and Zygoma GM™.

Intraoral



GM Mini Conical Abutment Scanbody
10 108.196



Mini Conical Abutment Hybrid Repositionable Analog
101.092



Neo Mini Conical Abutment One Step Hybrid Coping
10 118.330

Model Scanning



Slim Mini Conical Abutment Open Tray Impression Coping
3 108.176



Mini Conical Abutment Hybrid Repositionable Analog
101.092



GM Mini Conical Abutment Scanbody
3 108.196




Neo Mini Conical Abutment One Step Hybrid Coping
10 118.330

Conventional




Slim Mini Conical Abutment Open Tray Impression Coping
3 108.176




Neo Mini Conical Abutment Titanium Coping
10 118.302



Neo Mini Conical Abutment Protection Cylinder
3 106.220

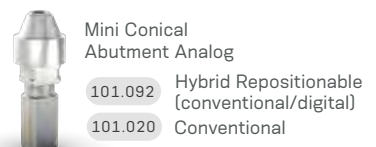

Mini Conical Abutment Analog
101.092
Hybrid Repositionable (conventional/digital)
Conventional
101.020



Neo Mini Conical Abutment CoCr Coping
10 118.303




Neo Mini Conical Abutment Burn-out Coping
10 118.301

Drivers



Accessories



Measurements GM Mini Conical Abutment

17°



30°



45°*



*The 45° Mini Conical Abutment is indicated for use only with Helix GM® Long and Zygoma GM™.




Neo Arch[®] Kits



Helix GM[®] Long Compact Surgical Kit

Autoclavable polymer case.

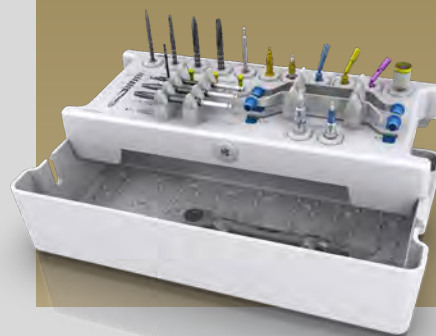

Articles

- 110.300 Helix GM[®] Long Compact Surgical Kit Case
- 103.395 Guided Surgery Drill 1.3mm
- 125.100 Guided Surgery Guide Clamp
- 125.140 Drill Guide For NGS Helix GM[®] Long 2.0/2.35mm
- 125.141 Drill Guide For NGS Helix GM[®] Long 3.75/4.0mm
- 103.459 Twist Drill For NGS Helix GM[®] Long 2.35mm
- 103.460 Twist Drill For NGS Helix GM[®] Long 3.75mm
- 103.461 Twist Drill For NGS Helix GM[®] Long 4.0mm


- 103.453 Helix GM[®] Long Initial Drill 2.0mm
- 103.462 Twist Drill For Helix GM[®] Long 2.35mm
- 103.463 Twist Drill For Helix GM[®] Long 3.75mm
- 103.464 Twist Drill For Helix GM[®] Long 4.0mm
- 129.021 Helix GM[®] Long X-ray Positioner
- 128.032 GM Angle Measurer 17°
- 128.033 GM Angle Measurer 30°
- 128.034 GM Angle Measurer 45°

- 105.143 Regular Guided Surgery GM Connection for Torque Wrench
- 105.140 Regular Guided Surgery GM Connection - Contra-angle
- 104.060 Neo Manual Screwdriver (medium)
- 105.129 GM Implant Driver - Torque Wrench (short)
- 105.131 GM Implant Driver - Contra-angle
- 104.050 Torque Wrench

Note: Items that compose Neodent[®] Kits are sold separately.

Zygoma GM[™] Surgical Kit

Autoclavable polymer case.

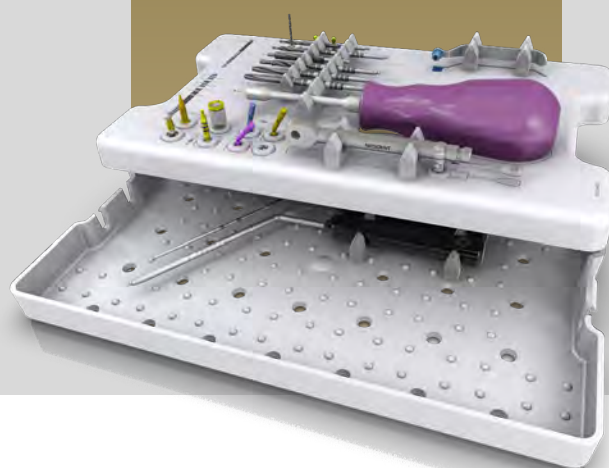

Articles

- 110.299 Zygoma GM[™] Surgical Kit Case
- 103.395 Guided Surgery Drill 1.3mm
- 125.100 Guided Surgery Guide Clamp
- 125.139 Drill Guide For Ngs Zygoma GM[™] 2.35mm
- 103.454 Twist Drill For Ngs Zygoma GM[™] 2.35mm
- 103.455 Twist Drill For Zygoma GM[™] 2.35mm
- 103.456 Twist Drill For Zygoma GM[™] 3.75mm

- 103.457 Twist Drill For Zygoma GM[™] 4.0mm
- 103.458 Lateral Direction Drill For Zygoma GM[™] 4.0mm
- 103.465 Pilot Twist Drill For Zygoma GM[™] 2.3/3.2mm
- 104.063 Zygoma GM[™] Installation Driver
- 129.022 Zygoma GM[™] Probe 2.35mm
- 129.023 Zygoma GM[™] Probe 4.0mm
- 128.032 GM Angle Measurer 17°

- 128.033 GM Angle Measurer 30°
- 128.034 GM Angle Measurer 45°
- 128.028 GM Height Measurer
- 104.060 Neo Manual Screwdriver (medium)
- 105.129 GM Implant Driver - Torque Wrench (short)
- 105.131 GM Implant Driver - Contra-angle
- 104.050 Torque Wrench

Note: Items that compose Neodent[®] Kits are sold separately.



Neo Arch[®] Instruments



Helix GM® Long Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Long implants.

Initial	Ø 2.35	Ø 3.75	Ø 4.0
103.453	103.462	103.463	103.464



Helix GM® Long Drills for Guided Surgery

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Long implants on Guided Surgery.

Ø 2.35	Ø 3.75	Ø 4.0
103.459	103.460	103.461



Zygoma GM™ Drills

- :: Available in surgical steel;
- :: Drill sequence for Zygoma GM™ implants.

	Pilot			
Ø 2.35	Ø 2.3/3.2	Ø 3.75	Ø 4.0	
103.455	103.465	103.456	103.457	



Zygoma GM™ Lateral Direction Drill

- :: Available in surgical steel;
- :: Spherical tip with guide pin and helical blades for preparing the site for the implant placement in the exteriorized technique.

Ø 4.0
103.458



Zygoma GM™ Drill for Guided Surgery

- :: Available in surgical steel;
- :: After using the first drill, the surgical guide must be removed and the conventional protocol must be started.

Ø 2.35
103.454



GM Height Measurer

- :: Available in titanium;
- :: For selecting GM prosthetic abutments;
- :: Marks corresponding to transmucosa heights.
- :: Can be used as X-Ray Positioner.

128.028

GM Implant Driver - Contra-Angle



- :: To capture the implant directly from the packaging;
- :: To place GM Implants with contra-angle, or attached to a manual driver for contra-angle connections (104.028) for hand placement;
- :: With six dimples to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque 35 N.cm.

105.131

GM Implant Driver - Torque Wrench



- :: To place GM Implants with the Torque Wrench (104.050);
- :: With six marks to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque: 60 N.cm.

Short	Long
22 mm	30 mm
105.129	105.130

Neo Screwdriver Torque Connection - Torque Wrench



- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
16.5 mm	22 mm	32 mm
105.133	105.132	105.157



Neo Manual Screwdriver

- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
21 mm	25 mm	37 mm
104.058	104.060	104.072

Neo Screwdriver Torque Connection - Contra-angle



- :: Available in surgical steel;
- :: Yellow color for line identification;
- :: Medium Neo Screwdriver Torque Connection
- :: Extra Short Neo Screwdriver Torque Connection - Contra-angle (105.146) recommended for Impression Copings, Cover Screws and Healing Abutments.

Extra Short	Short	Long
16.5 mm	24 mm	31 mm
105.146	105.135	105.160



Hexagonal Prosthetic Driver

- :: Available in surgical steel;
- :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;
- :: Yellow color for line identification.

Contra-angle Torque Wrench
 105.138 105.137



GM Bone Profile Drill with Guide

- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.424



GM Angle Measurer

- :: Available in titanium;
- :: Angles: 17°, 30° and 45°;
- :: To a more accurate selection and planning of the abutments angulation during the prosthetic phase.

17° 30° 45°
 128.032 128.033 128.034



Helix GM® Long Drill Guide for Guided Surgery

- :: Instrument with the purpose of guiding the drills during the bone bed preparation according to the guided surgery technique.

Ø 2.0/2.35 Ø 3.75/4.0
 125.140 125.141



Zygoma GM™ Drill Guide for Guided Surgery

- :: Instrument with the purpose of starting the Zygomatic Surgery guided.

Ø 2.35
 125.139



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in surgical steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø 1.3 Guide Clamp
 103.395 125.100



Guided Surgery GM Connection - Contra-Angle

- :: Available in stainless steel;
- :: To start the implant placement through the surgical guide.

Regular
 105.140



Guided Surgery GM Connection - Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide.

Regular
 105.143



Helix GM® Long X-ray Positioner

- :: Indicated for evaluation of the osteotomy depth in the implant placement procedure.

129.021



Zygoma GM™ Probes

- :: Available in Stainless Steel;
- :: The probe for the drill Ø2.35 mm has a tip design in L;
- :: The probe for the drill Ø4.0 mm has a tip with a design similar to the apex of the drill that allows identifying the correct drilling depth for implant anchorage.

Ø 2.35 Ø 4.0
 129.022 129.023



Zygoma GM™ Installation Driver

- :: Instrument for application of manual torque.

104.063



Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning;
- :: For full instructions see page 80.

104.050



Remover for Abutments with internal threads

- :: Available in surgical steel;
- :: To remove abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws

Short Long
 130.118 130.114



Remover for Neo Screws

- :: Available in surgical steel;
- :: Compatible with Neo removable screws for abutments

Short Long
 130.119 130.115

Removal Sets for Abutments with internal threads and Neo Screws

- :: Available in surgical steel;
- :: To remove Neo Removable Screws and abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws



Short
 130.117

Long
 130.116

GRAND MORSE® NEODENT® GUIDED SURGERY.

GRAND POSSIBILITIES WITH A LIMITLESS SOLUTION

Patients' expectations regarding tooth replacement are increasing and are even higher when it comes to treatment duration and esthetic outcomes. The Neodent® Guided Surgery helps clinicians to provide prosthetically driven treatments, enabling them to perform immediate protocols with peace of mind, fulfilling patients' expectations.



DIFFERENTIATE YOUR PRACTICE WITH GUIDED SURGERY.



Improve patient quality of life.

- Functional with an immediate fixed restoration.
- Esthetics with a personalized restoration and less bone remodeling ⁽¹³⁾.
- Comfort by the reduction of operative and postoperative discomfort (e.g. reduced patient chair time).



Access to more treatment options.

- Reliable access to flapless surgery ⁽¹⁴⁻¹⁶⁾.
- Designed to reduce bone grafting procedures.
- Predictable immediate protocols.



Increase patient acceptance.

- Better communication building trust with patients.
- Reliable treatment estimates from root to tooth including components and procedures.

SURGICAL PREDICTABILITY AND EFFICIENCY WITH A LIMITLESS SOLUTION.

Guided surgery is designed to reduce chair time and postoperative discomfort. It helps increasing implant positioning accuracy ⁽¹⁷⁾.



Complete
Helix® and Drive GM®
Implants portfolio



Convenient
Color-coded instruments
and symbol-marked



Flexible
2 sleeve height positions




Guided implant
insertion



Guided bed
preparation

Neodent® Guided Surgery Kit for Grand Morse®

Compatible with major guided
surgery software

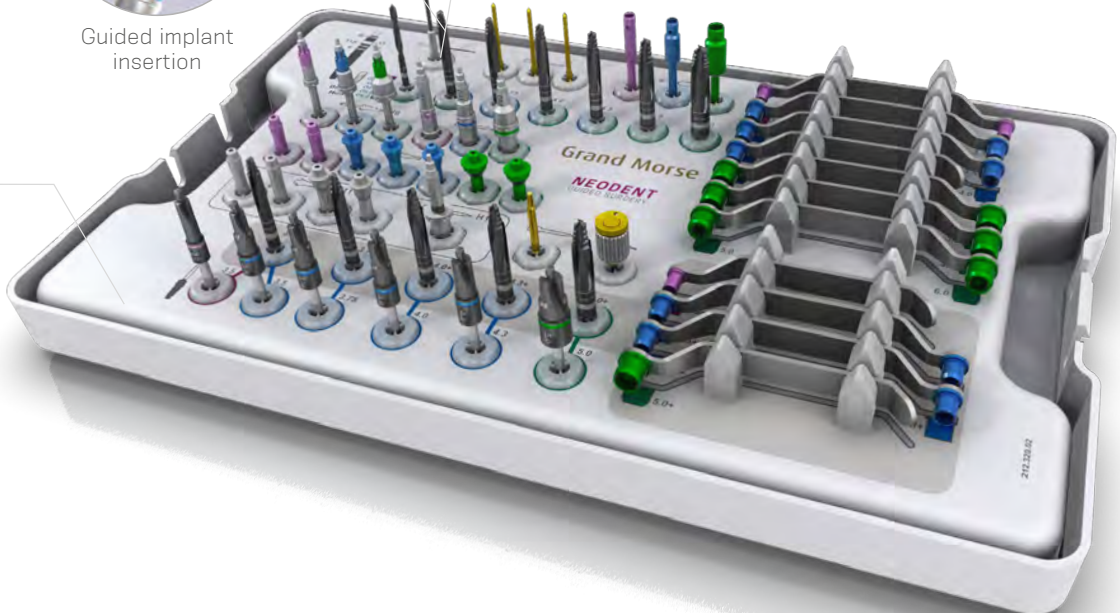




Neodent[®] Guided Surgery Kit

Grand Morse® Guided Surgery Surgical Kit

Autoclavable polymer case.
The Kit allows the use of Helix GM® and Drive GM® Implants in the Guided Surgery technique.

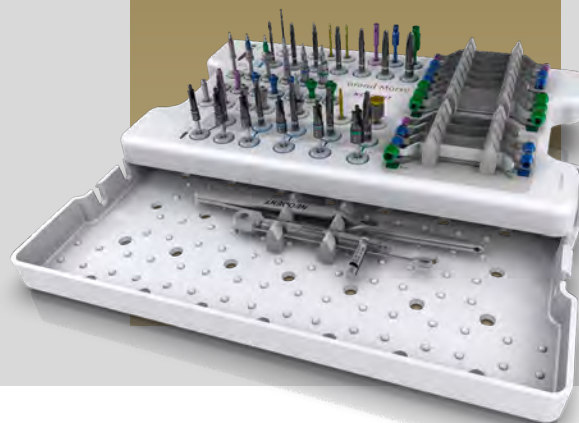

Articles

- 110.296 GM Guided Surgery Surgical Kit Case
- 103.395 Guided Surgery 1.3
- 125.100 Guided Surgery Guide Clamp
- 103.429 Narrow Guided Surgery Punch - Contra-Angle
- 103.430 Regular Guided Surgery Punch - Contra-Angle
- 103.431 Wide Guided Surgery Punch - Contra-Angle
- 103.432 Guided Surgery Drill 2.0
- 103.433 Tapered Guided Surgery Drill 3.5*
- 103.434 Tapered Guided Surgery Drill 3.75*
- 103.435 Tapered Guided Surgery Drill 4.0*
- 103.436 Tapered Guided Surgery Drill 4.3*
- 103.437 Tapered Guided Surgery Drill 5.0*
- 103.438 Tapered Guided Surgery Drill 6.0*
- 105.139 Narrow Guided Surgery GM Connection - Contra-angle
- 105.140 Regular Guided Surgery GM Connection - Contra-angle
- 105.141 Wide Guided Surgery GM Connection - Contra-angle
- 105.142 Narrow Guided Surgery GM Connection for Torque Wrench
- 105.143 Regular Guided Surgery GM Connection for Torque Wrench
- 105.144 Wide Guided Surgery GM Connection for Torque Wrench
- 125.130 Narrow Guided Surgery GM Guide Stabilizer
- 125.131 Regular Guided Surgery GM Guide Stabilizer
- 125.132 Wide Guided Surgery GM Guide Stabilizer
- 125.133 Narrow Guided Surgery GM Guide Stabilizer (Long)
- 125.134 Regular Guided Surgery GM Guide Stabilizer (Long)
- 105.145 Guided Surgery GM H11 Connection for Torque Wrench
- 105.136 Neo Screwdriver Torque Connection - Contra-angle (Medium)

- 104.060 Neo Manual Screwdriver (Medium)
- 103.439 Tapered Contour Guided Surgery Drill 3.5*
- 103.440 Tapered Contour Guided Surgery Drill 3.75*
- 103.441 Tapered Contour Guided Surgery Drill 4.0*
- 103.442 Tapered Contour Guided Surgery Drill 4.3*
- 103.443 Tapered Contour Guided Surgery Drill 5.0*
- 103.444 Narrow Guided Surgery GM Pilot Drill 3.5
- 103.445 Regular Guided Surgery GM Pilot Drill 3.5
- 103.446 Guided Surgery GM Pilot Drill 3.75
- 103.447 Guided Surgery GM Pilot Drill 4.0
- 103.448 Guided Surgery GM Pilot Drill 4.3
- 103.449 Guided Surgery GM Pilot Drill 5.0
- 125.119 Narrow Guided Surgery Drill Guide 2.0/3.5
- 125.121 Regular Guided Surgery Drill Guide 2.0/3.5
- 125.122 Regular Guided Surgery Drill Guide 3.75/4.0
- 125.123 Regular Guided Surgery Drill Guide 4.3
- 125.126 Wide Guided Surgery Drill Guide 2.0/3.5
- 125.127 Wide Guided Surgery Drill Guide 4.0/4.3
- 125.128 Wide Guided Surgery Drill Guide 5.0/6.0
- 125.120 Narrow Tapered Contour Guided Surgery Drill Guide 3.5
- 125.124 Regular Tapered Contour Guided Surgery Drill Guide 3.5/3.75
- 125.125 Regular Tapered Contour Guided Surgery Drill Guide 4.0/4.3
- 125.129 Wide Tapered Contour Guided Surgery Drill Guide 5.0
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

*Conventional guided surgery drills that can be replaced by the respective short version.



Neodent® Guided Surgery Instruments



Guided Surgery Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® and Drive GM® Implants in the guided surgery technique;
- :: Fully guided technique with Short Drills indicated for 8, 10 or 11.5 mm long implants.

Short 36.5 mm	Ø 2.0 103.475	Ø 3.5 103.476	Ø 3.75 103.477	Ø 4.0 103.478	Ø 4.3 103.479	Ø 5.0 103.480	Ø 6.0 103.481
Regular 41 mm	103.432	103.433	103.434	103.435	103.436	103.437	103.438



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in surgical steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø 1.3	Guide Clamp
103.395	125.100



Guided Surgery Tapered Contour Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM® Implants in the guided surgery technique for bone types I or II;
- :: Fully guided technique with Short Drills indicated for 8, 10 or 11.5 mm long implants.

Short 36.5 mm	Ø 3.5+ 103.482	Ø 3.75+ 103.483	Ø 4.0+ 103.484	Ø 4.3+ 103.485	Ø 5.0+ 103.486
Regular 41 mm	103.439	103.440	103.441	103.442	103.443



Guided Surgery Punch - Contra-Angle

- :: Available in titanium;
- :: Color-coded according to the sleeve diameter;
- :: To remove the mucosa before beginning the osteotomy.

Narrow	Regular	Wide
103.429	103.430	103.431



Guided Surgery GM Pilot Drills

- :: Available in surgical steel;
- :: Color-coded according to the sleeve diameter;
- :: Recommended for Helix GM® in bone types I or II;
- :: Optional Drive GM® in bone types III or IV.

	Narrow	Regular	Wide
Ø 3.5	103.444	Ø 3.5 103.445	Ø 5.0 103.449
		Ø 3.75 103.446	
		Ø 4.0 103.447	
		Ø 4.3 103.448	



Guided Surgery Drill Guides

- :: Available in titanium and stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To fit in the sleeve in the surgical guide;
- :: To be used with correspondent drill diameter and type.

	Narrow	Regular	Wide
Ø 2.0/3.5	125.119	Ø 2.0/3.5 125.121	Ø 2.0/3.5 125.126
Ø 3.5+	125.120	Ø 3.75/4.0 125.122	Ø 4.0/4.3 125.127
		Ø 4.3 125.123	Ø 5.0/6.0 125.128
		Ø 3.5+/3.75+ 125.124	Ø 5.0+ 125.129
		Ø 4.0+/4.3+ 125.125	



Guided Surgery GM Connection - Contra-Angle

- :: Available in stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To start the implant placement through the surgical guide.

Narrow 105.139 Regular 105.140 Wide 105.141



Guided Surgery Guide Stabilizers

- :: Available in titanium;
- :: Color-coded according to the sleeve diameter;
- :: Additional fixation of the surgical guide.

Narrow 125.130 Regular 125.131 Wide 125.132



Guided Surgery GM Connection - Torque Wrench

- :: Available in stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To finish the implant placement through the surgical guide.

Narrow 105.142 Regular 105.143 Wide 105.144



Guided Surgery Guide Stabilizers - Long

- :: Available in titanium;
- :: Additional fixation of the surgical guide;
- :: To be used when the H11 sleeve height is chosen.

Narrow 125.133 Regular 125.134



Guided Surgery GM H 11 Connection - Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide;
- :: To be used when the H11 sleeve height is chosen.

105.145

Sleeves for Neodent® Guided Surgery System

- :: Available in titanium;
- :: Sold in bags with 10 units each.



125.135 Sleeve for Narrow Guided Surgery System



125.136 Sleeve for Regular Guided Surgery System



125.137 Sleeve for Wide Guided Surgery System




125.138 Sleeve of Setter for Guided Surgery System



Neodent® Techniques

One Step Hybrid Technique

Technique that allows passive fitting, with no need for welding as the titanium coping is cemented to the substructure. Used for multiple prostheses and reduces laboratory work times.

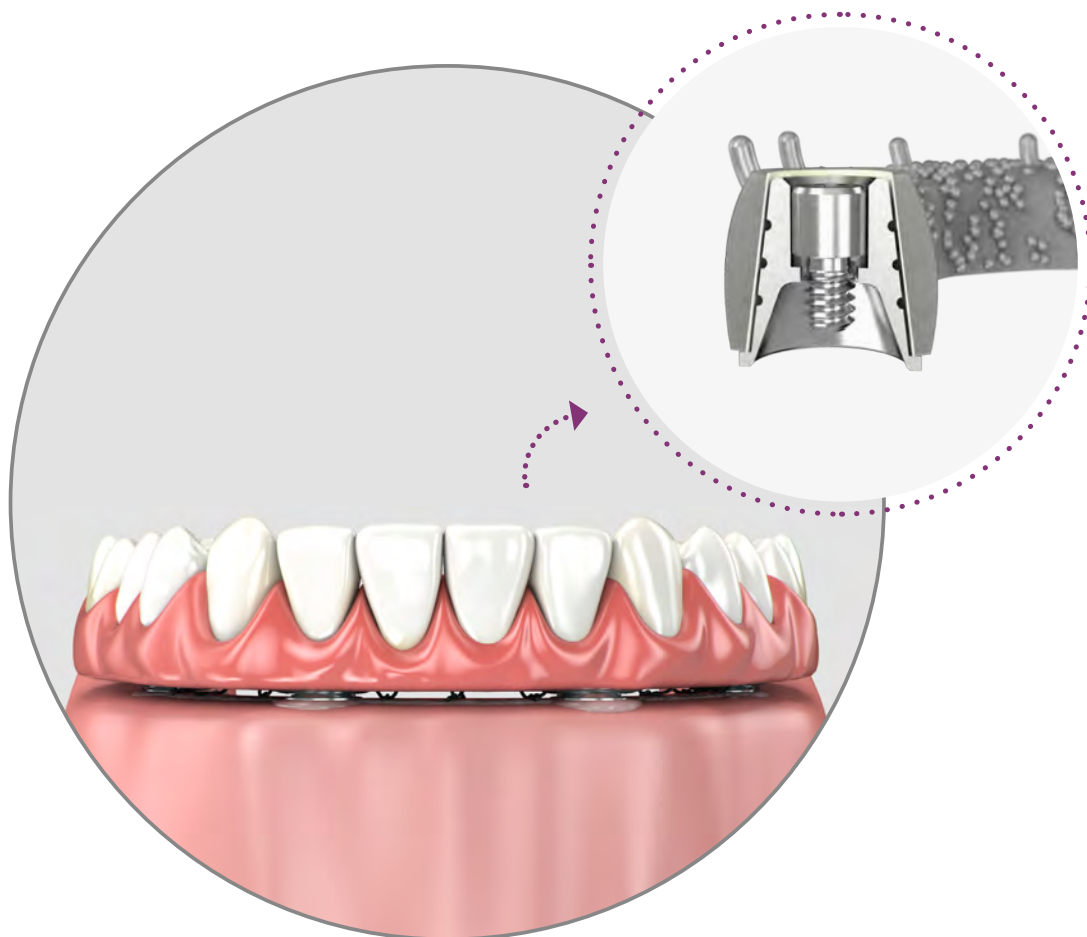

Neo Mini Conical Abutment One Step Hybrid Copings

:: For installation, use the Neo Torque Connection (105.132);
 :: For torque control, use Torque Wrench (104.050).

Burn-out	Brass	Titanium
118.340	118.331	118.330



Neo Micro Conical Abutment One Step Hybrid Copings

:: For installation, use the Neo Torque Connection (105.132);
 :: For torque control, use Torque Wrench (104.050).

Burn-out	Brass	Titanium
118.341	118.333	118.332



Neo Working Screw One Step Hybrid

:: For laboratory use.

116.271


Demonstration Sequence



1
Regularize the alveolar ridge.



2
Surgical drilling completed, obtaining adequate distance from distal implant in relation to the mental foramen with 7 mm Space Planning Instrument.

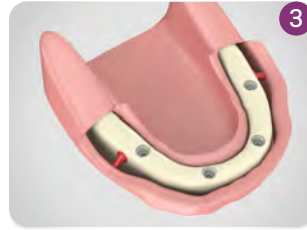

3
Placement of 4 Neodent® implants, according to their indication.



4
Placement of corresponding Neodent® Abutments.



5
Placement of Impression Copings, splinted with acrylic resin.



6
Positioning of Multifunctional Guide to obtain intermaxillary correlation. Soft silicone is injected to take the soft tissue impression.



7
Removal of Multi-Functional Guide and placement of Analogs to the impression copings.



8
Working model with artificial gum.



9
Burn-out One Step Hybrid Coping, Brass One Step Hybrid Coping, grooved Titanium One Step Hybrid Coping. The last one with lower dimensions than the brass one, which compensates using the mill.



10
Brass Copings are placed over analogs, then Burn-out Copings are fixed by working screws.



11
Castable ring with waxed framework.



12
Cast framework.



13
Place the framework over the stone model.



14
Please note cementing area.



15
Cementing with Panavia the structure over the titanium copings.



16
Final inside-mouth view.

Distal Bar Technique

Technique used to ease mandible rehabilitation, through a provisional hybrid type prostheses supported by implants.



Neo Distal Bar Coping

- :: Available in titanium;
- :: Retainers to ease joining with acrylic resin;
- :: Recommended torque: 10 N.cm;
- :: For torque, use Neo Screwdriver (105.132)

118.308



Neo Distal Bar

- :: Recommended for distal Implants to reinforce the cantilever.

125.116



Polishing Protector

- :: Available in surgical steel;
- :: Protection for the lab polishing.

123.008

Demonstration Sequence




1 Neodent® Abutments placed.



2 Prosthesis wearing, keeping posterior region integrity.




3 Place the copings into the central Implants and Distal Bar to distal Implants.

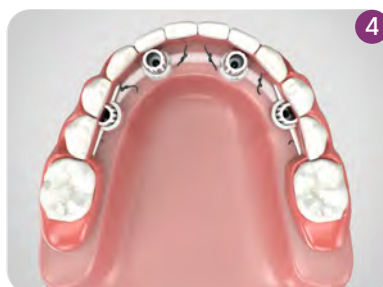

4 Proof of inferior prostheses wearing (centered occlusion position, no interference on copings).



5 Placement of rubber dam over copings to protect soft tissues.

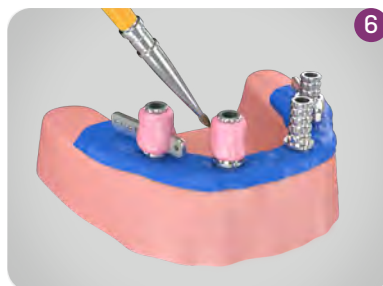

6 Apply self polymerizing acrylic resin on and between the copings.



7 Apply to worn area in lower prosthesis, repositioning inside mouth. Keep patient in occlusion until total polymerization.



8 Remove the inferior prosthesis after resin is polymerized. Copings are already captured.



9 Adjustments, finishing and polishing procedures of inferior prosthesis with polishing protectors.




10 Placed provisional implant supported prosthesis.



11 Final inside-mouth posterior view.



Digital Solutions

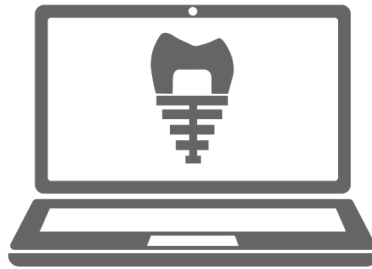

Visit www.neodent.com/cadcam to download the digital files to work with Neodent® Titanium Bases, Titanium Blocks, Abutments, Mini Conical Abutments, Micro Abutments, Universal Abutments, One Step Hybrid Copings, Scanbodies and Hybrid Repositionable Analogs. Libraries are available for the following companies: exocad GmbH, Amann Girrbach AG Inc, Dental Wings Inc and 3Shape A/S.

Scanbody

Neodent® Scanbodies can be used for scanning and digitalization of the patient or model providing accuracy in determining the analog position.



- 108.183 GM Exact Implant Intraoral Scanbody
- 108.181 GM Exact Implant Scanbody (for model)
- 108.196 GM Mini Conical Abutment Scanbody (intraoral and model)
- 108.197 GM Micro Abutment (intraoral and model)
- 108.198 GM Abutment (intraoral and model)




Hybrid Repositionable Analog

Neodent® Hybrid Repositionable Analogs can be used in prototyped models, produced by 3D printers, or conventional plaster models.



- 101.103 GM Hybrid Repositionable Analog 3.5/3.75
- 101.089 GM Hybrid Repositionable Analog 4.0/4.3
- 101.090 GM Hybrid Repositionable Analog 5.0/6.0
- 101.091 Micro Abutment Hybrid Repositionable Analog
- 101.092 Mini Conical Abutment Hybrid Repositionable Analog
- 101.097 Universal Abutment Hybrid Repositionable Analog 3.3X4
- 101.098 Universal Abutment Hybrid Repositionable Analog 3.3X6
- 101.099 Universal Abutment Hybrid Repositionable Analog 4.5X4
- 101.100 Universal Abutment Hybrid Repositionable Analog 4.5X6
- 101.101 GM Abutment Hybrid Repositionable Analog

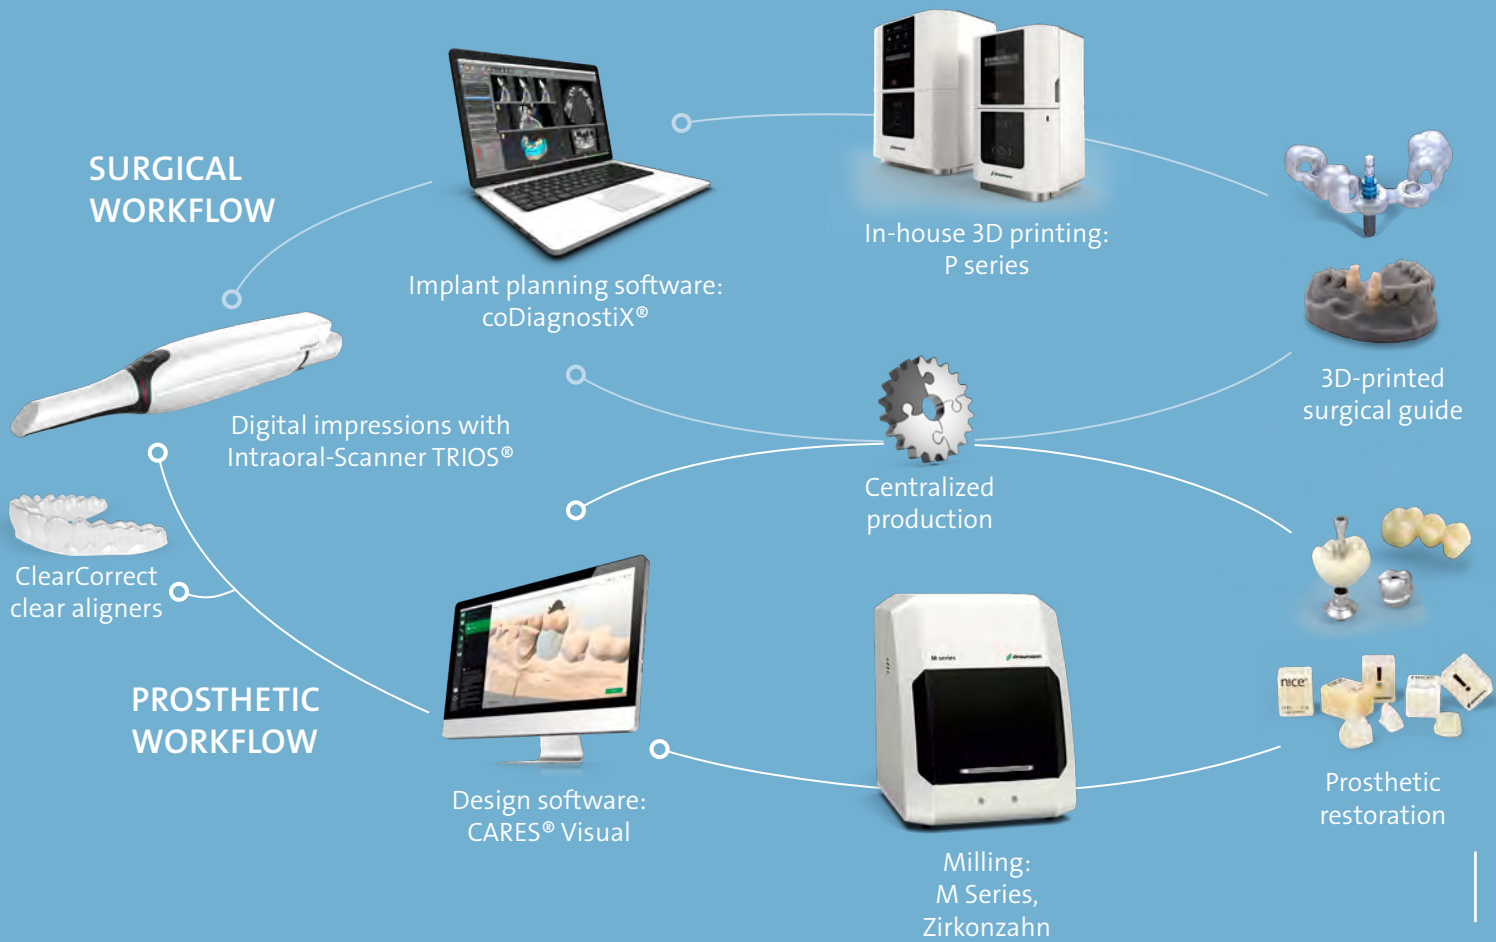

Straumann Group Digital Solutions

The path to succeed in the new standard of excellence in dentistry.

Straumann Group Digital Solutions supports your journey in digital dentistry from scanning and planning to design and production of the final restoration. Whether you are new to digital dentistry or advanced, our integrated, flexible workflows and a choice of in-house or out-sourced solutions put you on the leading edge of patient care.

For more information, contact your Straumann Group representative for the Straumann Group Digital Solutions Catalog or visit our website at straumann.us/digitaldentistry.

Our digital solutions also integrate with ClearCorrect clear aligners for more predictable treatment and beautiful outcomes. To learn more, contact ClearCorrect at 888-331-3323 or support@clearcorrect.com.

Note:

** Straumann® CARES® solutions are available in selected countries. Please contact your local Straumann Group sales representative for further information.*

General Instruments

Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050



Operational Instructions

The Neodent® Torque Wrench was designed to allow the necessary torque to be applied and simultaneous verification of that torque with the same Instrument.

All that is needed is to apply force to the wrench handle **1** (never the wrench body) until the value marked on the LATERAL SCALE **2** corresponds to the desired torque.



The wrench function works in both directions, by simply pulling and turning the driver's pin 180°. However, the torque measurements work only clockwise.

•WARNING: When inverting the torque direction, the gear may come loose from the driver body and fall. Therefore, this inversion should only be done with the driver connected to a part or outside the patient's mouth.



The Neodent® Torque Wrench comes with pre-calibrated torques

Titanium Tweezers



- :: To handle implants;
- :: New Tweezer system that prevents deviation in the active bit;
- :: Millimeter scale for checking during procedures;
- :: Self-locking implant.

129.001

Depth Probe



- :: Available in titanium;
- :: To probe preparations and analyze depth;
- :: Millimeter scale for checking during procedures.

129.004

7 and 9 mm Space Planning Instrument



- :: Available in surgical steel;
- :: Recommended for prosthetic/surgical planning.
- :: 7 and 9 mm marks.

128.026

Surgical Labial Retractor



- :: Available in surgical steel;
- :: Rounded edges to minimize surgical trauma.

124.001

Columbia Retractor



- :: Available in surgical steel;
- :: Rounded edges to minimize surgical trauma.

124.003

Scapel Handle



- :: Available in surgical steel;
- :: For standard scalpel blade use;
- :: Blade not included.

129.008


Bivers Handle



- :: Available in surgical steel;
- :: Non-traumatic extraction for implant placement;
- :: Similar to a periosteal elevator.

129.002


Concave Osteotome



- :: Available in surgical steel;
- :: Concave active cutting bit for nontraumatic lifting the floor of the maxillary sinus;
- :: Used to prepare the surgical alveolus for Implant placement in the posterior maxillary region with low bone height;
- :: Marks from 7 to 17mm.
- :: Marks from 7 to 17mm.

1.8 mm	2.5 mm	3.0 mm	3.5 mm	4.0 mm	4.5 mm
110.154	110.155	110.156	110.157	110.158	110.159

Convex Osteotome



- :: Available in surgical steel;
- :: Convex active bit;
- :: Used when the bone width is insufficient, demanding bone compression and expansion before placing the implant;
- :: Marks from 7 to 17mm.

1.8 mm	2.5 mm	3.0 mm	3.5 mm
110.160	110.161	110.162	110.163

Osteotomes Kit Case

- :: Available in polymer;
- :: Autoclavable;
- :: Osteotomes sold separately.

110.262



Surgical Hammer


- :: Available in surgical steel;
- :: Polymer active bit;
- :: Used in compactors and expanders;
- :: Weight: 130g.

126.001



Trepine Bur

- :: Available in surgical steel;
- :: Collecting bone cylinder;
- :: Implant removal.



Ø 3.3	Ø 3.5	Ø 3.75	Ø 4.1
103.051	103.490	103.491	103.026
Ø 4.3	Ø 5.0	Ø 8.0	
103.087	103.027	103.028	

Sinus Lift Curette

- :: Available in surgical steel;
- :: Used to displace the Sinusal Membrane.



Complement Case

- :: Available in autoclavable polymer;
- :: Used to organize drills and auxilliary connections.

110.270



Handle Implant Driver

- :: Available in stainless steel;
- :: Manual implant placement.

104.047



Analog Handle

- :: Used for tightening analogs and milling prosthetic abutments.

104.036



Prosthetic Surgical Guide

- :: Available in titanium;
- :: Abutments to prepare the surgical guide;
- :: Prosthetic guide inner diameter 2 mm
- :: Heights 6 and 10 mm;
- :: Surgical Guide: package with 10 units (5 units of 10 mm and 5 units of 6 mm);
- :: Surgical Guide Pin: package with 5 units



Guide	Pin
103.092	103.093



Neodent[®] Biomaterials



Everything you need for GBR

Neodent offers a wide assortment of biomaterials including bovine bone, allograft, and collagen barriers. Created to regenerate hard tissues in a predictable and reliable way, this range of flexible solutions is designed to provide patients with the functional and aesthetic results they seek, elevating their overall experience.

► Neodent AlloGraft granules



AlloGraft Mineralized Cortical

	Granule size	Content
NAMND070206	250-710 µm	0.5 cc
NAMND070207	250-710 µm	1.0 cc
NAMND070208	250-710 µm	2.0 cc
NAMND070218	250-1000 µm	0.25 cc
NAMND070219	250-1000 µm	0.5 cc
NAMND070220	250-1000 µm	1.0 cc
NAMND070221	250-1000 µm	2.0 cc
NAMND070230	250-1000 µm	2.5 cc



AlloGraft Mineralized Cancellous

	Granule size	Content
NAMND070229	250-1000 µm	0.25 cc
NAMND070212	250-1000 µm	0.5 cc
NAMND070213	250-1000 µm	1.0 cc
NAMND070214	250-1000 µm	2.0 cc
NAMND070231	250-1000 µm	2.5 cc



AlloGraft Mineralized Cortical Cancellous Mix

	Granule size	Content
NAMND070226	250-1000 µm	0.5 cc
NAMND070227	250-1000 µm	1.0 cc
NAMND070228	250-1000 µm	2.0 cc
NAMND070232	250-1000 µm	2.5 cc

► Neodent Membrane Flex™



	Description
NAMND070.008	15 × 20 mm Neodent® Membrane Flex™
NAMND070.009	20 × 30 mm Neodent® Membrane Flex™
NAMND070.010	30 × 40 mm Neodent® Membrane Flex™

eShop

At Neodent® we understand that time is money, and being efficient in every activity is important to your business.

We are committed to helping you achieve this goal by providing a secure online portal with our eShop.

The **Neodent eShop** goes beyond convenient online product shopping. It is a complete online service that helps you:

- Manage your account
- Track order history
- View order status
- Return product
- Pay invoices online
- Review payment history



Discover how you can save time and money today by visiting neodent.us/eShop



References

- (1) Novellino MM, Sesma N, Zanardi PR, Laganá DC. Resonance frequency analysis of dental implants placed at the posterior maxilla varying the surface treatment only: A randomized clinical trial. *Clin Implant Dent Relat Res*. 2017 Jun 20. doi: 10.1111/cid.12510. [Epub ahead of print]
- (2) Sartoretto SC, Alves AT, Resende RF, et al. Early osseointegration driven by the surface chemistry and wettability of dental implants. *J Appl Oral Sci*. 2015 May-Jun;23(3):279-87.
- (3) Sartoretto SC, Alves AT, Zarranz L, et al. Hydrophilic surface of Ti6Al4V-ELI alloy improves the early bone apposition of sheep tibia. *Clin Oral Implants Res*. 2016 Jun 17. doi: 10.1111/clr.12894. [Epub ahead of print]
- (4) Val JE, Gómez-Moreno G, Ruiz-Linares M, et al. Effects of Surface Treatment Modification and Implant Design in Implants Placed Crestal and Subcrestally Applying Delayed Loading Protocol. *J Craniofac Surg*. 2017 Mar;28(2):552-558.
- (5) Al-Nsour MM, Chan HL, Wang HL. Effect of the platform- switching technique on preservation of peri-implant marginal bone: a systematic review. *Int J Oral Maxillofac Implants*. 2012 Jan-Feb;27(1):138-45.
- (6) Annibaldi S, Bignozzi I, Cristalli MP, et al. Peri-implant marginal bone level: a systematic review and meta-analysis of studies comparing platform switching versus conventionally restored implants. *J Clin Periodontol*. 2012 Nov;39(11):1097-113.
- (7) Hsu YT, Lin GH, Wang HL. Effects of Platform-Switching on Peri-implant Soft and Hard Tissue Outcomes: A Systematic Review and Meta-analysis. *Int J Oral Maxillofac Implants*. 2017;32(1):e9-e24.
- (8) Lazzara RJ, Porter SS. Platform switching: a new concept in implant dentistry for controlling postrestorative crestal bone levels. *Int J Periodontics Restorative Dentistry*. 2006 Feb;26(1):9-17.
- (9) Rocha S, Wagner W, Wiltfang J, Nicolau P, Moergel M, Messias A, Behrens E, Guerra F. Effect of platform switching on crestal bone levels around implants in the posterior mandible: 3 years results from a multicentre randomized clinical trial. *J Clin Periodontol*. 2016 Apr;43(4):374-82.
- (10) Babbush CA. Post treatment quantification of patient experiences with full-arch implant treatment using a modification of the OHIP-14 questionnaire. *J Oral Implantol*. 2012 Jun;38(3):251-60.
- (11) Block MS, Haggerty CJ, Fisher GR. Nongrafting implant options for restoration of the edentulous maxilla. *J Oral Maxillofac Surg* 2009;67:872-881.
- (12) Steigenga J, Al-Shammari K, Misch C, Nociti FH Jr, Wang HL. Effects of implant thread geometry on percentage of osseointegration and resistance to reverse torque in the tibia of rabbits. *J Periodontol*. 2004;75(9):1233-41.
- (13) Carvajal Mejía JB, Wakabayashi K, Nakano T, Yatani H. Marginal Bone Loss Around Dental Implants Inserted with Static Computer Assistance in Healed Sites: A Systematic Review and Metaanalysis. *Int J Oral Maxillofac Implants*. 2016 Jul-Aug;31(4):761-75.1.
- (14) Pozzi A, Tallarico M, Marchetti M, Scarfò B, Esposito M. Computer-guided versus free-hand placement of immediately loaded dental implants: 1-year post-loading results of a multicentre randomized controlled trial. *Eur J Oral Implantol*. 2014 Autumn;7(3):229-42.
- (15) Hultin M, Svensson KG, Trulsson M. Clinical advantages of computer-guided implant placement: a systematic review. *Clin Oral Implants Res*. 2012 Oct;23 Suppl 6:124-35.
- (16) Soares MM, Harari ND, Cardoso ES, et al. An in vitro model to evaluate the accuracy of guided surgery systems. *Int J Oral Maxillofac Implants*. 2012 Jul-Aug;27(4):824-31.
- (17) Pozzi A, Polizzi G, Moy PK. Guided surgery with tooth-supported templates for single missing teeth: a critical review. *Eur J Oral Implantol*. 2016;9(1):135-53.

Neodent®, NeoPoros, Acqua, Helix®, Drive®, Titamax®, Grand Morse®, Helix GM®, Drive GM®, Titamax GM®, Neotorque, NeoArch®, Zygomax GM™ are trademarks or registered trademarks of JIGC Indústria e Comércio de Materiais Dentários S.A.

CEREC® is a trademark or registered trademark of Sirona Dental Systems GmbH (DE).

Dentsply Sirona is a trademark or registered trademark of Dentsply Sirona, Inc.

MEDENTiKA is a trademark or registered trademark of Medentika GmbH.

Novaloc is a trademark or registered trademark of Valoc AG.

Panavia is a trademark or registered trademark of Kuraray Co. Ltd.

Amann Girrbach is a trademark or registered trademark of Amann Girrbach AG.

exocad is a trademark or registered trademark of exocad GmbH.

Dental Wings is a trademark or registered trademark of Dental Wings Inc.

3Shape is a trademark or registered trademark of 3Shape A/S.

© Neodent® 2021. All rights reserved.
Neodent® and/or other trademarks and logos
from Neodent® that are mentioned herein are
the trademarks or registered trademarks of
Straumann Holding AG and/or its affiliates.
All rights reserved.

ifu.neodent.com.br/en
www.neodent.us • www.neodent.ca



Straumann North American Headquarters
Straumann USA, LLC
60 Minuteman Road
Andover, MA 01810
Phone 800/448 8168 (US) • 800/363 4024 (CA)
Fax 978/747 2490
www.straumann.us • www.straumann.ca

USLIT.2040 4/21 V1 PMR

