


CATALOG • 2022

VOLUME 02



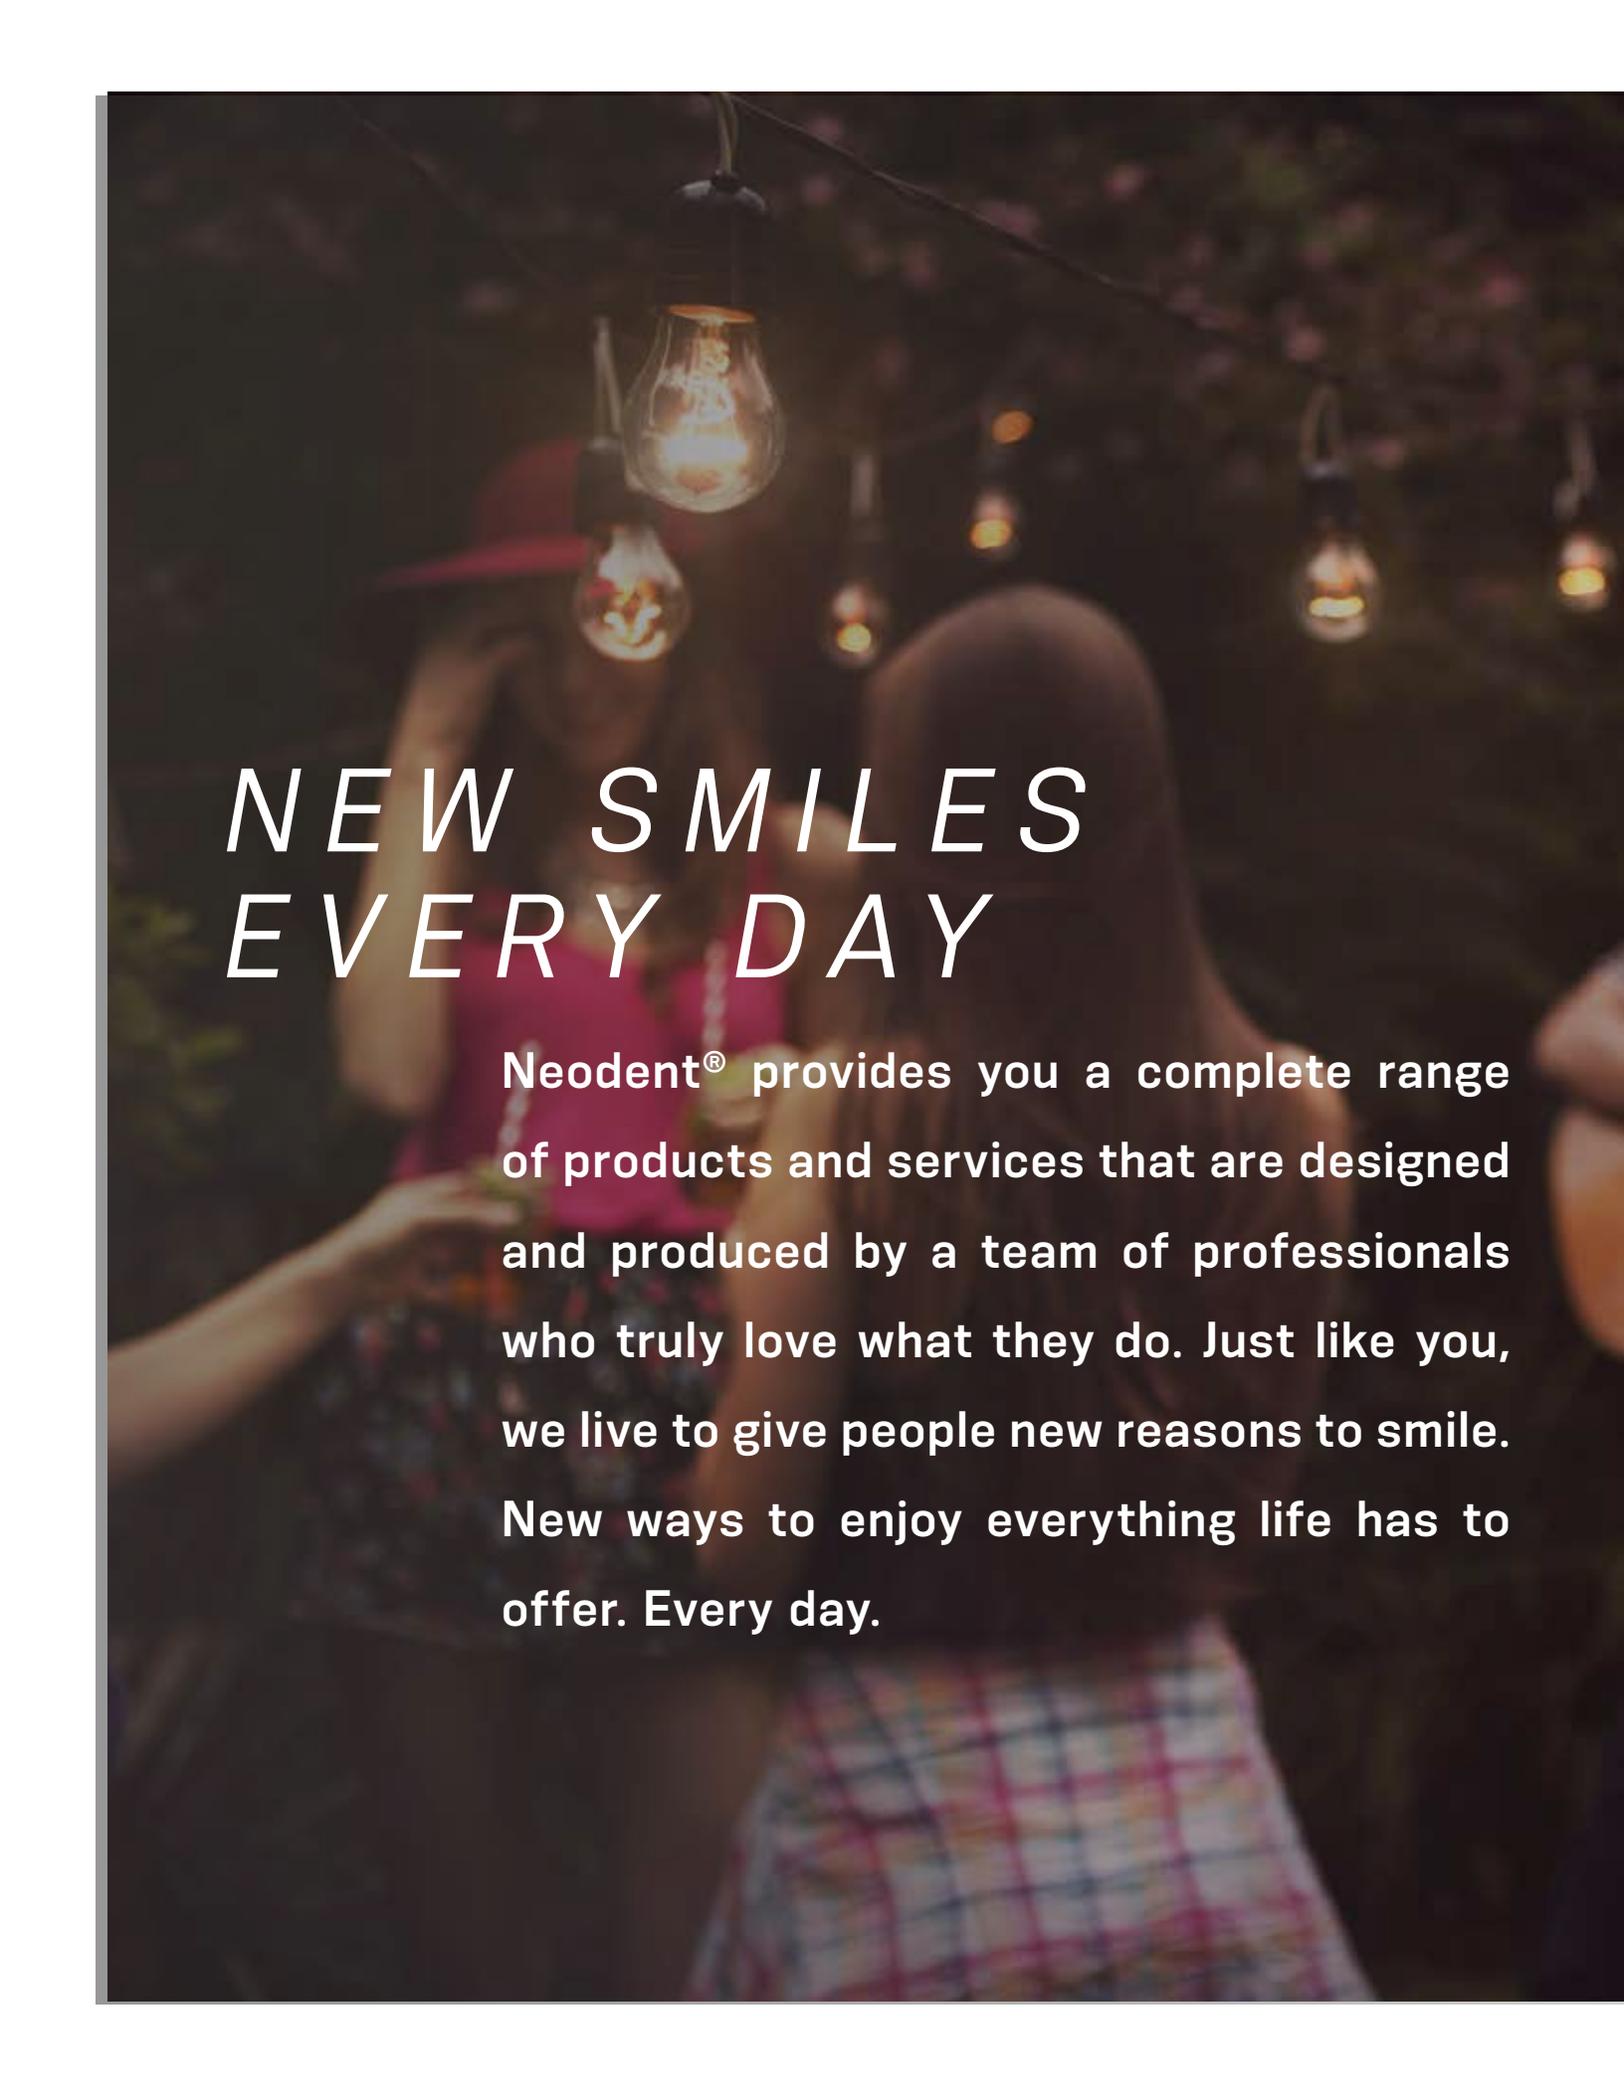

NEW SMILES EVERY DAY

Neodent® provides you a complete range of products and services that are designed and produced by a team of professionals who truly love what they do. Just like you, we live to give people new reasons to smile. New ways to enjoy everything life has to offer. Every day.



Grand Morse™

GREATNESS IS AN ACHIEVEMENT



GRAND RELIABILITY


STABLE AND STRONG FOUNDATION
DESIGNED FOR LONG TERM SUCCESS

The implant-abutment interface is crucial for a successful long term functional and esthetic result. The Neodent® Grand Morse™ connection offers a combination based on proven concepts: a platform switching associated with a deep 16° Morse Taper including an internal indexation for a strong and stable connection designed to achieve long-lasting results.



1 Platform Switching

Abutment design with a narrower diameter than the implant coronal area, enabling the platform switching concept⁽⁵⁻⁹⁾.



2 Internal Indexation

Precise abutment positioning, protection against rotation and easy handling.



3 Deep Connection

Allowing a large contact area between the abutment and the implant for an optimal load distribution.



4 16° Morse Taper Connection

Designed to ensure tight fit for an optimal connection sealing.





GRAND SIMPLICITY

EASE OF USE AT ITS BEST

Implant therapy has become an integral part of clinical dentistry, with ever increasing numbers of patients seeking such treatment. The Neodent® Grand Morse™ Implant System is smartly engineered providing efficiency and simplicity within the dental treatment network for both surgical to restoratives steps.

ONE PROSTHETIC PLATFORM

All Neodent® Grand Morse™ implants feature the Grand Morse™ connection regardless of the implant diameter.



ONE SCREWDRIVER

The Neo Screwdriver has a star attachment offering reliability and durability compatible with all Neodent® Grand Morse™ healing abutments and cover screws and most of the restorative screws.



ONE IMPLANT DRIVER

The Neodent® implant driver allows an easy and reliable implant pick up and placement.



ONE SURGICAL KIT

Intuitive and functional compact surgical kit, that allows the place of Helix GM™ implants in all bone types.





GRAND STABILITY

STABLE AND STRONG FOUNDATION DESIGNED FOR LONG TERM SUCCESS

The increasing expectations for shortened treatment duration represent a significant challenge for dental professionals. The Neodent® Grand Morse™ system offers an implant design featuring the ACQUA hydrophilic surface designed to maximize primary stability and predictability in immediate protocols.



HELIX® - OPTIMAL IMPLANT DESIGNED TO ACHIEVE HIGH PRIMARY STABILITY

Helix® Grand Morse™ is an innovative hybrid implant design maximizing treatment options and efficiency in all bone types.

Fully tapered body design

- Coronal: 2° - 12°
- Apex: 16°
- » Allowing under-osteotomy



Hybrid contour

- Coronal: Cylindrical
- Apex: Conical
- » For stability with vertical placement flexibility



Active apex

- Soft rounded small tip
- Helical flutes
- » Enabling immediate loading



Dynamic progressive thread design

- Coronal: Trapezoidal > compressing
- Apex: V-Shape > Self-tapping
- » Achieving high primary stability in all bone types



ACQUA hydrophilic surface

Designed for high treatment predictability



Titamax®

Vertical placement flexibility.
Bone types I & II.



Drive®

High primary stability in challenging
bone types.
Bone types III & IV.



GRAND ESTHETICS

DELIVER IMMEDIATE NATURAL-LOOKING ESTHETICS

Nowadays, patients expect both short treatment times and esthetic results. The Neodent® Grand Morse™ restorative portfolio offers flexibility to simplify soft tissue management respecting the biological distances for achieving immediate function and esthetics.



Titanium Temporary Abutment



Pro-Peek Abutment



Titanium Base



Titanium Base C



Titanium Base for Bridge



Titanium Block (AG or Medentika Holder)



CoCr Abutment



Anatomic Abutment (straight and angled)



Universal Abutment (straight and angled)



Abutment



Angled Mini Conical Abutment



Attachment TiN* for Removable Prosthesis (straight and angled)



Titanium Base AS



Straight Mini Conical Abutment



Micro Abutment



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Overdenture



Multiple-unit screw-retained prosthesis



Multiple-unit cement-retained prosthesis



Temporary

*TiN - Titanium nitride

Neodent® Grand Morse™ Implant Packaging

Neodent® implant packaging has been updated to a concept that provides convenience through all steps of the procedure, from storage to the placement of the implant.

The new packaging aids in identification of both the implant model as well as its diameter and length, regardless of its storage position.



Package instruction of use



1. After breaking the sterility seal on the blister, hold the primary package (vial) and twist the lid to open it.



2. To remove the implant from the vial lift the cap up, which has the stand and implant attached to it.



3. To secure the implant, grip both sides of the implant carrier.



4. While gripping the implant carrier, remove the lid.



5. To capture the implant with the contra-angle handpiece attachment, grip the implant carrier while placing the attachment into the implant chamber.




6. The implant can now be transported to the surgical site.

e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalogue or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en

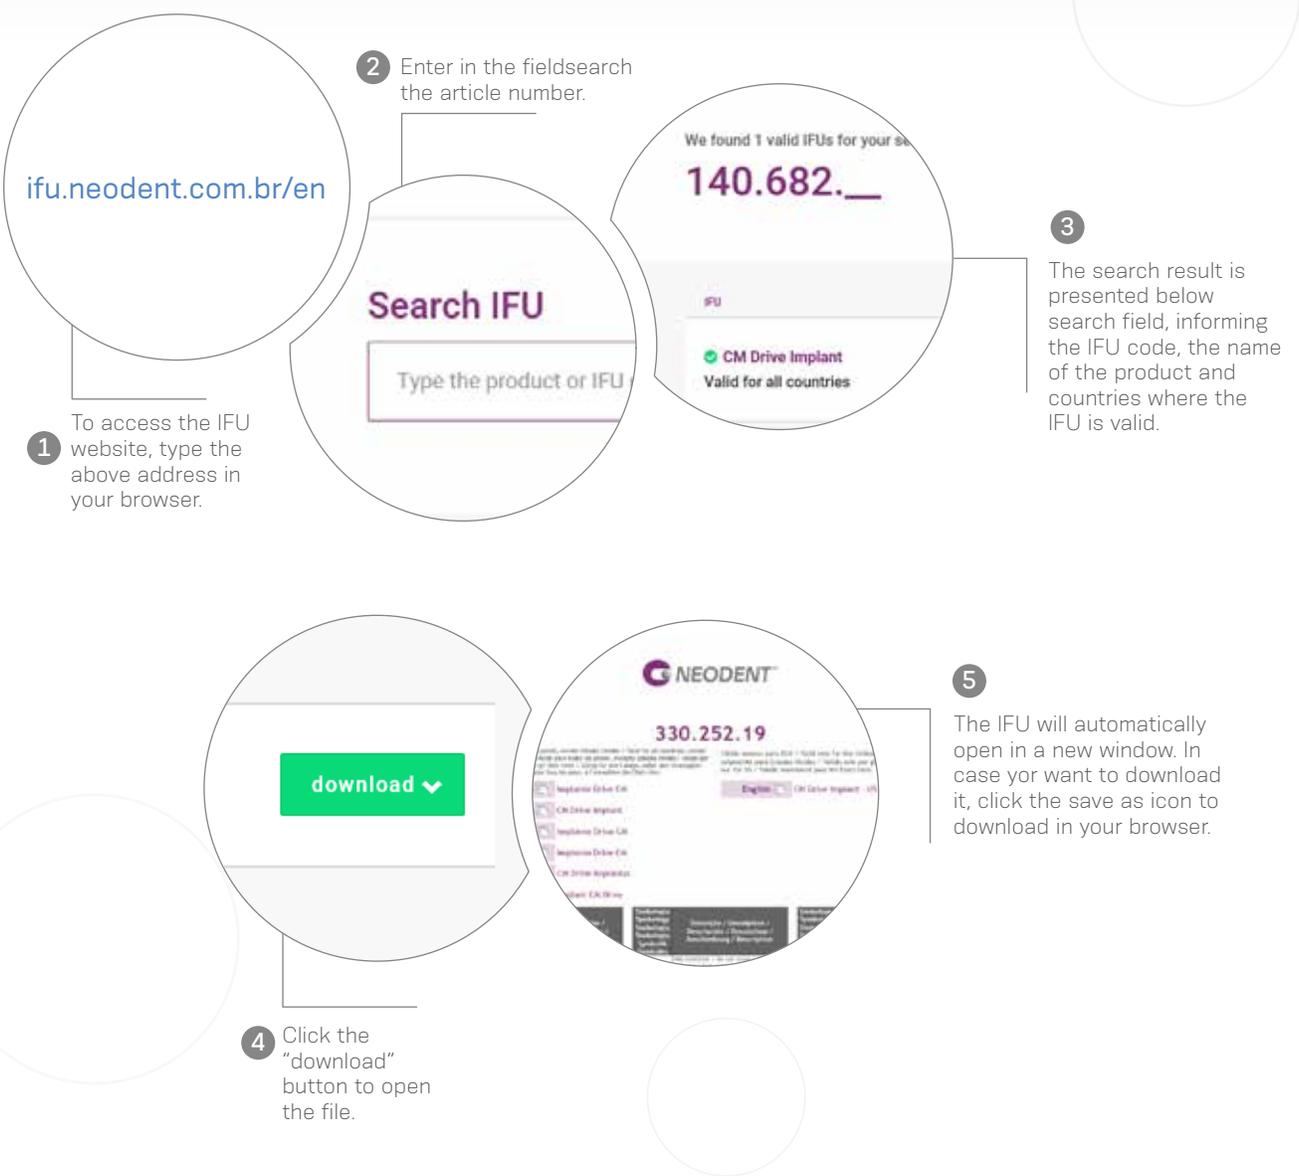



NeoPoros

Constant Evolution.

Based on the abrasive sandblasting concept followed by acid etching, the **NeoPoros** surface promotes, by using controlled grain oxides, cavities on the implant surface that then are uniformed with the acid etching technique.

The whole process of obtaining this surface is guaranteed due to automated time, speed, pressure and particle size control.

Several scientific studies continue to be performed so that the **NeoPoros** surface may be always evolving and promoting much more reliability for you.

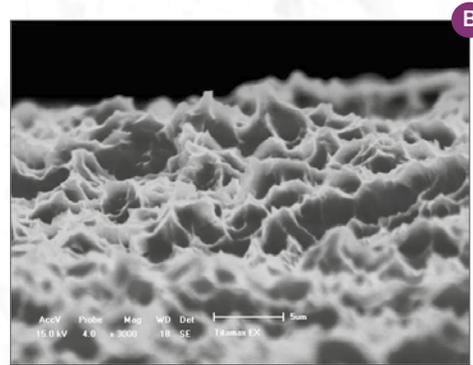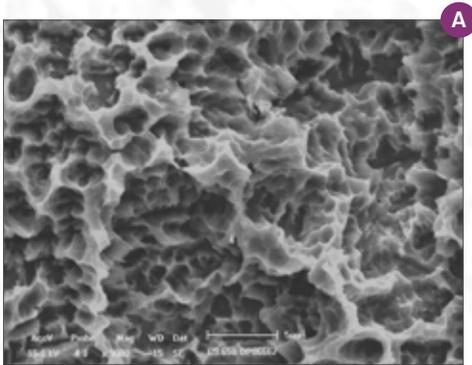

Controlled roughness on all implant surface. Scanning electron microscopy (A) shows macro (15-30 μ m) and (B) microtopography (0.3 - 1.3 μ m).

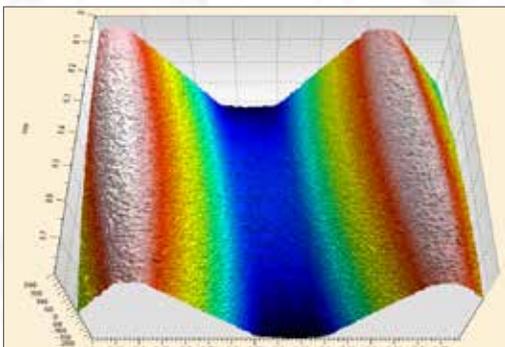


Image taken by confocal microscopy.
Roughness and Microtopography.
(S_a = 0.3 - 1.3 μ m; S_z = 6.0 - 15.5 μ m).

acqua®

ACQUA Hydrophilic Surface designed for high treatment predictability.

The Neodent® ACQUA hydrophilic surface is the next level of the highly successful S.L.A. type of surface developed to achieve successful outcomes even in challenging situations, such as soft bone or immediate protocols.⁽¹⁻⁴⁾

Hydrophilicity

The hydrophilic surface presents a smaller contact angle when in contact with hydrophilic liquids. This provides greater accessibility of organic fluids to ACQUA implant surface.⁽²⁾

Surface comparison

Lab generated images.



NeoPoros surface.



*ACQUA Hydrophilic
Surface.*

Neodent easypack

GROW WITH PEACE OF MIND

Neodent® has developed EasyPack to simplify your daily practice. An all-in-one set that offers everything you need to grow while performing dental implant therapy with confidence, convenience and guidance.



GROW WITH CONFIDENCE

Choose a brand and products you can rely on



GROW WITH CONVENIENCE

The certainty of having everything in one package




GROW WITH GUIDANCE

All workflows in simple steps



THE NEODENT® EASYPACK INCLUDES


- 1 Grand Morse™ Helix™ Implant
- 2 Grand Morse™ Cover Screw
- 3 Grand Morse™ Healing Abutment
- 4 Grand Morse™ Hybrid Implant Analog
- 5 Grand Morse™ 3-in-1 Neodent Smart Abutment™

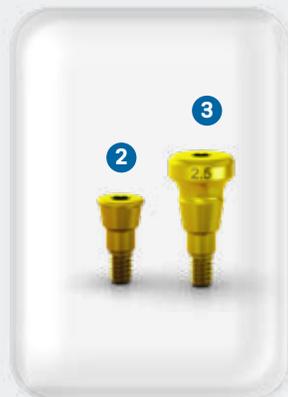



Reliable guided workflow with the 3-in-1 GM Smart Abutment

The combination of the GM™ Smart Abutment, a unique patent-pending solution combining a closed tray impression coping, a digital scanbody and a temporary abutment in a single piece, with healing components and the analog allows you to choose a restorative path guided for achieving predictable results.

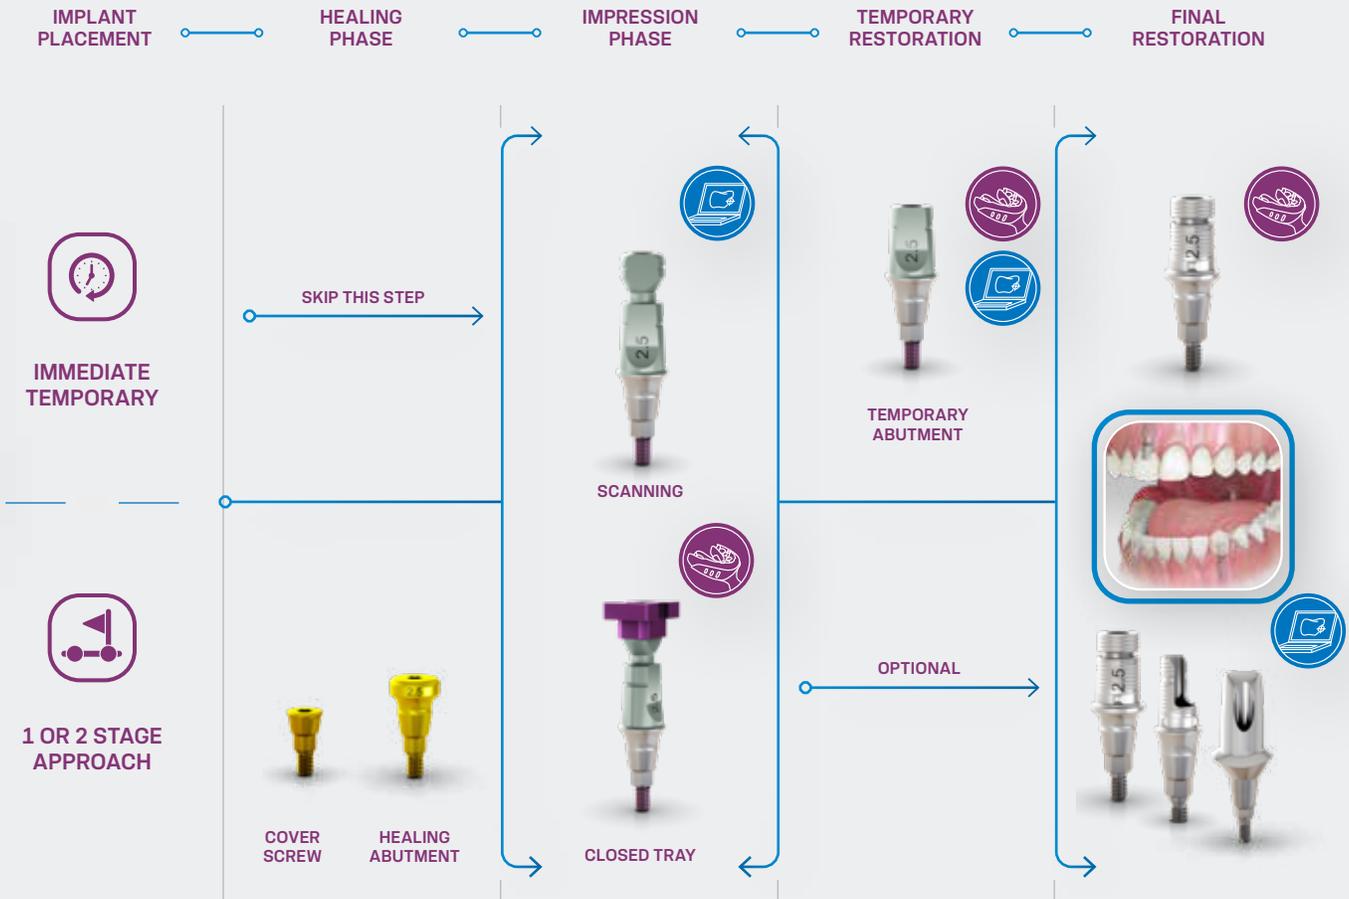

NEODENT® EASYPACK PRODUCT OPTIONS

	Ø3.5		Ø3.75		Ø4.0		Ø4.3	
	ACQUA	NeoPoros	ACQUA	NeoPoros	ACQUA	NeoPoros	ACQUA	NeoPoros
8.0	138.089	138.005	138.113	138.029	138.137	138.053	138.158	138.074
10.0	138.095	138.011	138.119	138.035	138.143	138.059	138.161	138.077
11.5	138.101	138.017	138.125	138.041	138.149	138.065	138.164	138.080
13.0	138.107	138.023	138.131	138.047	138.155	138.071	138.167	138.083

GM Cover Screw
0 mm

GM Healing Abutment
Ø4.5 X 2.5 mm

GM Hybrid Repositionable Analog*
Ø3.5/3.75 Ø4.0/4.3
*according to implant diameter

GM Smart Abutment
Ø4.5 X 2.5 mm

Helix GM™

PRODUCT FEATURES:

Implants Description:

- Full dual tapered implant;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex including a soft rounded small tip and helicoidal flutes;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-tapping V-shape threads on the apical part;
- Double threaded implant;
- Grand Morse™ connection.

Indications:

- Indicated for all types of bone density and implant immediate placement post extraction.

Drilling features:

- Contour drill is required in bone types I and II;
- Final pilot drills are highly recommended in bone types I and II;
- Implant should be positioned 1 or 2 mm below bone level;
- Drilling speed: 800-1200 rpm for bone type I and II;
- Drilling speed: 500-800 rpm for bone type III and IV;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 Ncm.



Available with:

NeoPoros

or

acqua®

Drill Sequence

	103.170	103.425	103.561	103.578	103.513	103.564	103.579	103.514	103.567	103.580	103.515	103.570	103.581	103.516	103.573	103.582	103.517	103.576	103.577	
Ø3.5	□*	□	■	■	■															
Ø3.75	□*	□	■			■	■	■												
Ø4.0	□*	□	■			■			■	■	■									
Ø4.3	□*	□	■			■			■			■	■	■						
Ø5.0	□*	□	■			■			■			■	■			■	■			

*Optional / Bone types I and II

Ø3.5	□*	□	■																	
Ø3.75	□*	□	■			■*														
Ø4.0	□*	□	■					■*												
Ø4.3	□*	□	■			■						■*								
Ø5.0	□*	□	■			■						■	■			■*				
Ø6.0	□*	□	■			■						■				■			■	
Ø7.0	□*	□	■			■						■				■			■	■*

*Optional / Bone types III and IV

Drill Sequence with Neodent® Control System

	103.170	103.492	103.493	103.500	103.513	103.494	103.501	103.514	103.495	103.502	103.515	103.496	103.503	103.516	103.497	103.504	103.517	103.498	103.499	
Ø3.5	□*	□	■	■	■															
Ø3.75	□*	□	■			■	■	■												
Ø4.0	□*	□	■			■			■	■	■									
Ø4.3	□*	□	■			■			■			■	■	■						
Ø5.0	□*	□	■			■			■			■	■			■	■			

*Optional / Bone types I and II

Ø3.5	□*	□	■																	
Ø3.75	□*	□	■			■*														
Ø4.0	□*	□	■					■*												
Ø4.3	□*	□	■			■						■*								
Ø5.0	□*	□	■			■						■	■			■*				
Ø6.0	□*	□	■			■						■				■			■	
Ø7.0	□*	□	■			■						■				■			■	■*

*Optional / Bone types III and IV

Helix GM™ Implants

Ø3.5	ACQUA	NeoPoros	Ø3.75	ACQUA	NeoPoros	Ø4.0	ACQUA	NeoPoros	Ø4.3	ACQUA	NeoPoros
	8.0 140.943	109.943		8.0 140.976	109.976		8.0 140.982	109.982		8.0 140.948	109.948
	10.0 140.944	109.944		10.0 140.977	109.977		10.0 140.983	109.983		10.0 140.949	109.949
	11.5 140.945	109.945		11.5 140.978	109.978		11.5 140.984	109.984		11.5 140.950	109.950
	13.0 140.946	109.946		13.0 140.979	109.979		13.0 140.985	109.985		13.0 140.951	109.951
	16.0 140.947	109.947		16.0 140.980	109.980		16.0 140.986	109.986		16.0 140.952	109.952
	18.0 140.988	109.988		18.0 140.981	109.981		18.0 140.987	109.987		18.0 140.989	109.989

Ø5.0	ACQUA	NeoPoros	Ø6.0	ACQUA	NeoPoros	Ø7.0	ACQUA	NeoPoros
	8.0 140.953	109.953		8.0 140.1009	109.1009		8.0 140.1059	109.1059
	10.0 140.954	109.954		10.0 140.1010	109.1010		10.0 140.1060	109.1060
	11.5 140.955	109.955		11.5 140.1011	109.1011		11.5 140.1061	109.1061
	13.0 140.956	109.956		13.0 140.1012	109.1012		13.0 140.1062	109.1062

GM Cover Screw

0 mm	2 mm
117.021	117.022

Use the manual Neo Screwdriver (104.060).
Do not exceed the insertion torque of 10 Ncm.

GM Healing Abutment

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
	Ø3.3 106.207	106.208	106.209	106.210	106.211	106.212
	Ø4.5 106.213	106.214	106.215	106.216	106.217	106.218
	Ø5.5	106.250	106.251	106.252	106.253	
	Ø6.5	106.254	106.255	106.256	106.257	

Use the manual Neo Screwdriver (104.060).
Do not exceed the insertion torque of 10 Ncm.

GM Customizable Healing Abutment

	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
	Ø5.5 106.223	106.224	106.225	106.226	106.227	
	Ø7.0	106.228	106.229	106.230	106.231	106.232

Use the manual Neo Screwdriver (104.060).
Do not exceed the insertion torque of 10 Ncm.

Drive GM™

PRODUCT FEATURES:

Implants Description:

- Tapered implant;
- Square shape threads;
- Double threaded implant;
- Reverse cutting chambers distributed across the implant body;
- Rounded apex with a sharp edge;
- Grand Morse™ connection.

Indications:

- Indicated for bone types III and IV and implant immediate placement post-extraction;

Drilling features:

- Final pilot drill is optional in bone types III and IV;
- Implant should be positioned 1 or 2 mm below bone level;
- Drilling speed: 500-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 Ncm.



Available with:

NeoPoros or

acqua®

Drill Sequence

								
	Initial	Ø2.0	Ø3.5	Ø3.5	Ø4.3	Ø4.3	Ø5.0	Ø5.0
	103.170	103.425	103.561	103.513	103.570	103.516	103.573	103.517
Ø3.5 mm				 *				
Ø4.3 mm						 *		
Ø5.0 mm								 *

*Optional / Bone types III and IV 

Drill Sequence with Neodent® Control System

								
	Initial	Ø2.0	Ø3.5	Ø2.8/3.5	Ø4.3	Ø3.6/4.3	Ø5.0	Ø4.3/5.0
	103.170	103.492	103.493	103.513	103.496	103.516	103.497	103.517
Ø3.5								
Ø4.3								
Ø5.0								

*Optional Bone types III and IV 

Drive GM™ Implants

		8.0 mm	10.0 mm	11.5 mm	13.0 mm	16.0 mm	18.0 mm
Ø3.5							
	ACQUA	140.958	140.959	140.960	140.961	140.962	140.963
	NeoPoros	109.958	109.959	109.960	109.961	109.962	109.963
Ø4.3							
	ACQUA	140.964	140.965	140.966	140.967	140.968	140.969
	NeoPoros	109.964	109.965	109.966	109.967	109.968	109.969
Ø5.0							
	ACQUA	140.970	140.971	140.972	140.973	140.974	140.975
	NeoPoros	109.970	109.971	109.972	109.973	109.974	109.975

GM Healing Abutment

	Profile	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
	Ø3.3	106.207	106.208	106.209	106.210	106.211	106.212
	Ø4.5	106.213	106.214	106.215	106.216	106.217	106.218
	Ø5.5	106.250	106.251	106.252	106.253		
	Ø6.5	106.254	106.255	106.256	106.257		

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 Ncm.

GM Cover Screw

	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 Ncm.

GM Customizable Healing Abutments

	Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
	Ø5.5	106.223	106.224	106.225	106.226	106.227	
	Ø7.0	106.228	106.229	106.230	106.231	106.232	

Titamax GM™

PRODUCT FEATURES:

Implants Description:

- Cylindrical implant (parallel walls);
- V-shape threads;
- Double threaded implant;
- Self tapping apex;
- Grand Morse™ connection.

Indications:

- Indicated for bone types I and II or grafted areas such as bone block.

Drilling features:

- Final pilot drill is highly recommended in bone types I and II;
- Implant should be positioned 1 or 2 mm below bone level;
- Self tapping implant which doesn't require the use of bone tap or contour drill;
- Drilling speed: 800-1200 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 Ncm.



Available with:

NeoPoros

or

acqua®

Drill Sequence



	Initial 103.170	Ø2.0 103.162	Ø2/3 103.213	Ø2.8 103.163	Ø3.0 103.164	Ø3.5 103.513	Ø3.3 103.166	Ø3.75 103.514	Ø4.0 103.515	Ø3.8 103.167	Ø4.3 103.168	Ø5.0 103.517
Ø3.5 mm	✓	✓		✓		✓						
Ø3.75 mm	✓	✓	✓		✓			✓				
Ø4.0 mm	✓	✓	✓		✓		✓		✓			
Ø5.0 mm	✓	✓	✓		✓			✓		✓	✓	✓

Bone types I and II



Titamax GM™ Implants

		7.0 mm	8.0 mm	9.0 mm	11.0 mm	13.0 mm	15.0 mm	17.0 mm
Ø3.5	ACQUA	140.906	140.907	140.908	140.909	140.910	140.911	140.912
	NeoPoros	109.906	109.907	109.908	109.909	109.910	109.911	109.912
Ø3.75	ACQUA	140.899	140.900	140.901	140.902	140.903	140.904	140.905
	NeoPoros	109.899	109.900	109.901	109.902	109.903	109.904	109.905
Ø4.0	ACQUA	140.913	140.914	140.915	140.916	140.917	140.918	140.919
	NeoPoros	109.913	109.914	109.915	109.916	109.917	109.918	109.919
Ø5.0	ACQUA	140.920	140.921	140.922	140.923	140.924		
	NeoPoros	109.920	109.921	109.922	109.923	109.924		

GM Healing Abutment



Profile	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø4.5	106.213	106.214	106.215	106.216	106.217	106.218
Ø5.5		106.250	106.251	106.252	106.253	
Ø6.5		106.254	106.255	106.256	106.257	

:: Use the manual Neo Screwdriver (104.060);
:: Do not exceed the insertion torque of 10 Ncm.

GM Cover Screw



	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
:: Do not exceed the insertion torque of 10 Ncm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø5.5	106.223	106.224	106.225	106.226	106.227	
Ø7.0		106.228	106.229	106.230	106.231	106.232

GM™ Abutment



Single-unit
screw-retained
prosthesis



Ø4.8 mm

Recommended for posterior region.

Consider in addition 1.5 - 2.0 mm
for the restorative material;
Minimum interocclusal space of 4.9
mm from the mucosa level;
With internal threads for a secure
engagement of the screw;
Exact;
Neo Removable Screw;



Installation Sequence

0.8 mm	1.5 mm	2.5 mm
115.269	115.270	115.271
3.5 mm	4.5 mm	5.5 mm
115.272	115.273	115.274



Intraoral



Abutment
Scanbody
2
108.220



GM Abutment Hybrid
Repositionable Analog
101.101



GM Abutment Coping
for Crown - Digital
Workflow
10
118.362

Model Scanning



GM Abutment
Impression Coping
Closed Tray
2
108.179



GM Abutment Hybrid
Repositionable Analog
101.101



Abutment
Scanbody
2
108.220



GM Abutment Coping
for Crown - Digital
Workflow
10
118.362

Conventional



GM Abutment
Impression Coping
Closed Tray
2
108.179



Neo Abutment
Titanium Coping
10
118.300



Neo Abutment
Protection
Cylinder
2
106.221



101.101 Hybrid Repositionable
(conventional/digital)
101.076 Conventional



Neo Abutment
CoCr Coping
10
118.299



Neo Abutment
Burn-out
Coping
10
118.298

Drivers



1 Neo
Screwdriver
Torque
Connection

Torque Wrench



2 Neo
Screwdriver
Torque
Connection

Manual
Screwdriver
Torque

Accessories



Replacement Abutment Screw

116.290 Neo GM Screw (Short) - for abutment with 0.8 GH

116.291 Neo GM Screw - for abutments with 1.5-2.5 GH

116.292 Neo GM Screw (Long) - for abutments with 3.5-5.5 GH



Mini Conical Abutment
Polishing Protector
123.008



Replacement Coping Screw
116.266 Titanium

GM™ Mini Conical Abutment



Multiple-unit
screw-retained
prosthesis



Ø4.8 mm

Consider in addition 1.5 - 2.0 mm for the restorative material;

Minimum interocclusal space of 4.5 mm from the mucosa level for straight abutments;

Exact;

Neo Removable Screw.



Installation Sequence



Intraoral



Mini Conical Abutment Scanbody
3
108.218



Mini Conical Abutment Hybrid Repositionable Analog
101.092



Neo Mini Conical Abutment One Step Hybrid Coping
10
118.382

Model Scanning



Slim Mini Conical Abutment Open Tray Impression Coping
3
108.176



Mini Conical Abutment Hybrid Repositionable Analog
101.092



Mini Conical Abutment Scanbody
3
108.218



Neo Mini Conical Abutment One Step Hybrid Coping
10
118.382

Conventional



Slim Mini Conical Abutment Open Tray Impression Coping
3
108.176



Neo Mini Conical Abutment Titanium Coping
10
118.302



Mini Conical Abutment Analog
101.092
Hybrid Repositionable (conventional/digital)
101.020
Conventional



Neo Mini Conical Abutment CoCr Coping
10
118.303





Neo Mini Conical Abutment Burn-out Coping
10
118.301

21

Drivers



Accessories



GM™ Micro Abutment

Consider in addition
1.5 - 2.0 mm for the
restorative material;
Minimum interocclusal
space of 3.5 mm from the
mucosa level.



**Single-unit
screw-retained
prosthesis**

**Multiple-unit
screw-retained
prosthesis**

Ø3.5 mm

Recommended for limited spaces and narrow inter-dental spaces.

Installation Sequence

0.8 mm 115.255	1.5 mm 115.256	2.5 mm 115.257	GM Micro Abutment
3.5 mm 115.258	4.5 mm 115.259	5.5 mm 115.260	



Intraoral



3

108.219



101.091



Neo Micro
Conical
Abutment One
Step Hybrid
Coping



118.381

GM Micro
Abutment Coping
for Crown Digital
Workflow



118.363

Model Scanning



108.182



108.178

3



101.091



108.219



Neo Micro
Conical
Abutment One
Step Hybrid
Coping



118.381

GM Micro
Abutment Coping
for Crown Digital
Workflow



118.363

Conventional



108.182



108.178

3




118.297
118.317



3

106.267



101.091
101.078 Hybrid Repositionable
(conventional/digital)
for Crown (conventional)



118.296
118.316



118.295
118.315

22

Drivers

1 Hexagonal Prosthetic Driver + Torque Wrench

2 Neo Screwdriver Torque Connection + Torque Wrench

3 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

Micro Abutment Polishing Protector
123.015 Bridge

Replacement Coping Screw
116.269 Titanium

GM™ Anatomic Abutment with Neo Removable Screw



Single-unit
cement-retained
prosthesis

Recommended for anterior region.

Gingiva color for esthetic outcomes
Click retention for provisional copings
With internal threads for a secure engagement of the screw
Exact
Neo Removable Screw



Installation Sequence

In Mouth

GM Exact Click Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.862	114.863	114.864
17° 114.865	114.866	114.867

or

GM Exact Click Narrow Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.868	114.869	114.870
17° 114.871	114.872	114.873

GM Exact Click Anatomic Abutment Provisional Coping

118.334
118.335 Narrow

Impression of the GM Exact Click Anatomic Abutment

Lab stage

Finalized prosthesis

In Lab

GM Implant Exact Impression Coping Closed and Open Tray

Regular	108.160	108.162
Long	108.161	108.163

GM Implant Analog

Ø3.5/3.75	Ø4.0/4.3	Ø5.0/6.0	Hybrid Repositionable (conventional/digital) Conventional
101.103	101.089	101.090	
	101.074	101.075	

GM Exact Click Anatomic Abutment Provisional Coping

118.334
118.335 Narrow

GM Exact Click Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.862	114.863	114.864
17° 114.865	114.866	114.867

or

GM Exact Click Narrow Anatomic Abutment with Neo Removable Screw

1.5 mm	2.5 mm	3.5 mm
114.868	114.869	114.870
17° 114.871	114.872	114.873

Drivers

1 Neo Screwdriver Torque Connection + Torque Wrench

2 Neo Screwdriver Torque Connection + Manual Screwdriver Torque

Accessories

Replacement Abutment Screw

116.291	Neo GM Screw - for abutments with 1.5-2.5 GH
116.292	Neo GM Screw (Long) - for abutments with 3.5 GH

GM™ Universal Abutment with Neo Removable Screw



Single-unit cement-retained prosthesis



Ø3.3/4.5 mm

Cementable area: 4.0 or 6.0 mm;
Click retention for provisional copings;
With internal threads for a secure engagement of the screw;
Exact;
Neo Removable Screw.



Installation Sequence

Height	Diameter	GM Exact Click Universal Abutment with Removable Screw						or	Height	Diameter	GM Exact Click Universal Abutment 17° with Removable Screw			or	Height	Diameter	GM Exact Click Universal Abutment 30° with Removable Screw		
		0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm				1.5 mm	2.5 mm	3.5 mm				1.5 mm	2.5 mm	3.5 mm
4 mm	Ø3.3	114.826	114.827	114.828	114.829	114.830	114.831	4 mm	Ø3.3	114.802	114.803	114.804	4 mm	Ø3.3	114.814	114.815	114.816		
	Ø4.5	114.838	114.839	114.840	114.841	114.842	114.843		Ø4.5	114.808	114.809	114.810		Ø4.5	114.820	114.821	114.822		
6 mm	Ø3.3	114.832	114.833	114.834	114.835	114.836	114.837	6 mm	Ø3.3	114.805	114.806	114.807	6 mm	Ø3.3	114.817	114.818	114.819		
	Ø4.5	114.844	114.845	114.846	114.847	114.848	114.849		Ø4.5	114.811	114.812	114.813		Ø4.5	114.823	114.824	114.825		

Intraoral

Height	Diameter	Part No.	Height	Diameter	Part No.
4 mm	Ø3.3	108.143	6 mm	Ø3.3	108.144
	Ø4.5	108.145		Ø4.5	108.146

Universal abutment Hybrid Repositionable analog

4 mm Ø3.3	101.097	6 mm Ø3.3	101.098
4 mm Ø4.5	101.099	6 mm Ø4.5	101.100

Milled crown

Conventional

Click Universal Abutment Impression Coping

4 mm Ø3.3	108.172	6 mm Ø3.3	108.173
4 mm Ø4.5	108.174	6 mm Ø4.5	108.175

Click Universal Abutment Provisional Coping

4 mm Ø3.3	118.304	6 mm Ø3.3	118.305
4 mm Ø4.5	118.306	6 mm Ø4.5	118.307

Universal Abutment Analog

4 mm Ø3.3	101.097	6 mm Ø3.3	101.098	Hybrid Repositionable (conventional/digital)
4 mm Ø4.5	101.099	6 mm Ø4.5	101.100	

4 mm Ø3.3	101.070	6 mm Ø3.3	101.071	Click (conventional)
4 mm Ø4.5	101.072	6 mm Ø4.5	101.073	

Universal Abutment Burn-out Coping


4 mm Ø3.3	118.181	6 mm Ø3.3	118.182
4 mm Ø4.5	118.183	6 mm Ø4.5	118.184

24

Drivers



Accessories

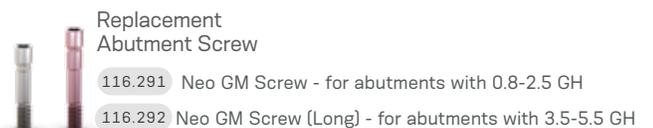

GM™ Titanium Base with Neo Removable Screw

Customizable up to 4 mm high;

Cementable area: 6.0 or 4.0 mm;

With internal threads for a secure engagement of the screw


Exact;

Neo Removable screw;



Installation Sequence

Intraoral

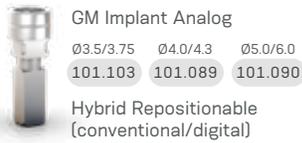

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø3.5	135.355	135.356	135.357	135.358	135.359
Ø4.5	135.367	135.368	135.369	135.370	135.371
Ø5.5	135.379	135.380	135.381	135.382	135.383
Ø6.5		135.391	135.392	135.393	135.394

GM Exact Titanium Base with Removable Screw 4mm

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø3.5	135.355	135.356	135.357	135.358	135.359
Ø4.5	135.367	135.368	135.369	135.370	135.371
Ø5.5	135.379	135.380	135.381	135.382	135.383
Ø6.5		135.391	135.392	135.393	135.394



GM Exact Titanium Base with Removable Screw 6mm


	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø3.5	135.361	135.362	135.363	135.364	135.365
Ø4.5	135.373	135.374	135.375	135.376	135.377
Ø5.5	135.385	135.386	135.387	135.388	135.389
Ø6.5		135.395	135.396	135.397	135.398



Model Scanning




GM Implant Exact Impression Coping Closed and Open Tray 2
Regular 108.160 108.162
Long 108.161 108.163

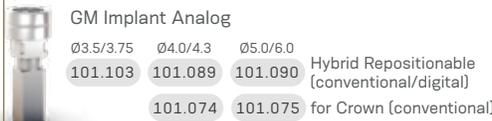

Conventional



GM Implant Exact Impression Coping Closed and Open Tray 2
Regular 108.160 108.162
Long 108.161 108.163

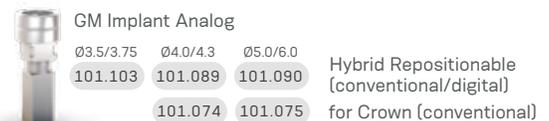

GM Exact Titanium Base with Removable Screw 4mm

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø3.5	135.355	135.356	135.357	135.358	135.359
Ø4.5	135.367	135.368	135.369	135.370	135.371
Ø5.5	135.379	135.380	135.381	135.382	135.383
Ø6.5		135.391	135.392	135.393	135.394



GM Exact Titanium Base with Removable Screw 6mm

	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø3.5	135.361	135.362	135.363	135.364	135.365
Ø4.5	135.373	135.374	135.375	135.376	135.377
Ø5.5	135.385	135.386	135.387	135.388	135.389
Ø6.5		135.395	135.396	135.397	135.398




GM Titanium Base Burn-out Coping

	Ø3.5	Ø4.5	Ø5.5	
	118.322	118.325	118.329	4.0 mm
	118.323	118.327	118.342	6.0 mm

Drivers



Accessories



GM™ Titanium Base for Bridge with Neo Removable Screw



Multiple-unit screw-retained prosthesis



Multiple-unit cement-retained prosthesis



Ø3.5/4.5/
5.5 mm

Cementable area:
4.0 mm for Ø3.5
4.5 mm for Ø4.5
and Ø5.5.


With internal threads for a secure engagement of the screw;

Neo Removable Screw.



Installation Sequence

Intraoral

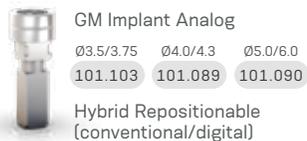

Model Scanning



GM Implant Exact Impression Coping Open Tray

Regular 108.158
Long 108.159



GM Implant Analog

Ø3.5/3.75 101.103 Ø4.0/4.3 101.089 Ø5.0/6.0 101.090
101.074 101.075

Hybrid Repositionable (conventional/digital)

for Crown (conventional)



GM Implant Intraoral Scanbody

108.207



GM Titanium Base for Bridge	Diameter					
	Ø3.5	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm
Ø3.5	135.399	135.400	135.401	135.402	135.403	135.403
Ø4.5	135.404	135.405	135.406	135.407	135.408	135.408
Ø5.5	135.409	135.410	135.411	135.412	135.413	135.413

Drivers

1



+



Torque Wrench

2



+



Manual Screwdriver Torque

Accessories



Replacement Abutment Screw

116.292 Neo GM Screw (Long)

GM™ Titanium Base Angled Solution (AS)



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø4.0/4.5/5.5 mm

With removable screw.


Cementable area:
6.0 or 4.0 mm;

Exact.



Installation Sequence


Intraoral

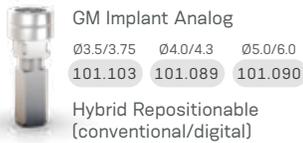

Model Scanning



GM Implant Exact Impression Coping Closed and Open Tray ²
 Regular 108.160 108.162
 Long 108.161 108.163

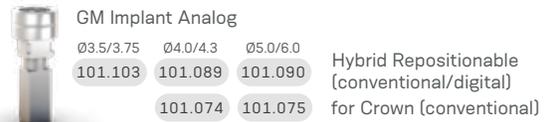

	0.8 mm	1.5 mm	2.5 mm			0.8 mm	1.5 mm	2.5 mm	
Ø4.0	135.327	135.328	135.329	GM Titanium Base Angled Solution (AS) 4mm 	or	Ø4.0	135.330	135.331	
Ø4.5	135.333	135.334	135.335			Ø4.5	135.336	135.337	135.338
Ø5.5	135.339	135.340	135.341			Ø5.5	135.342	135.343	135.344

Drivers

1

 Angled Solution Screwdriver for Torque Wrench 105.150 Short 105.151 Regular 105.152 Long	+	 Torque Wrench
or		
 Angled Solution Screwdriver for Contra-angle 105.147 Short 105.148 Regular 105.149 Long	+	 Contra-angle

Accessories

2

 Neo Screwdriver Torque Connection + Manual Screwdriver Torque	+	 Replacement Sterile Screw 116.288 Screw for GM Titanium Base AS
---	---	---

Titanium Base C for GM™ with Neo Removable Screw



Cementable area: 4.7 mm;


With internal threads for a secure engagement of the screw;

Exact;

Neo Removable Screw.



Installation Sequence

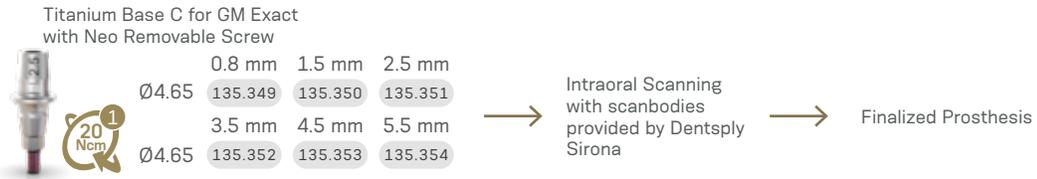

Workflow

Step 1

Gingiva height selection and ordering.



Select the Titanium Base C for GM Exact gingival height.



Order the Titanium Base C for GM Exact. Please note that the scanbody has to be purchased directly from equipment manufacturer.

Step 2

Intra-oral scanning.



Insert the Titanium Base C for GM Exact in the Neodent® implant.



Insert scanbody on the Titanium Base C for GM Exact.

Step 3

Design and milling.



Select in the CAD software the comparable third-party Ti-base and perform the digital design.



Mill the digital design.

Step 4

Finalization and fixation.



- Check the fit of milled restoration in the patient's mouth and adapt it, if needed.
- Cement the restoration on the Titanium Base C for GM Exact and insert it into the patient's mouth.

CEREC digital library compatibility

Library	Sirona's Products				Compatible with implant System	
Ti-base	Scanbody	REF Scanbody Omnicam	REF Scanbody Bluecam / Ineos	Grinding block	Implant manufacturer	Implant system
NBB 3.4 L						
NB A 4.5 L						
SSO 3.5 L						
S BL 3.3 L	L	6431329	6431303	inCoris Zi meso L	Neodent®	GM, CM, HE, IIPlus
S BL 4.1 L						
BO 3.4 L						

Drivers

1

Neo Screwdriver Torque Connection



+

Torque Wrench

Accessories



Replacement Abutment Screw


116.292 Neo GM Screw (Long)

GM™ Titanium Block for MEDENTiKA Holder

 Single-unit screw-retained prosthesis	 Single-unit cement-retained prosthesis	 Multiple-unit cement-retained prosthesis
--	---	---




Ø11.5/
15.8 mm

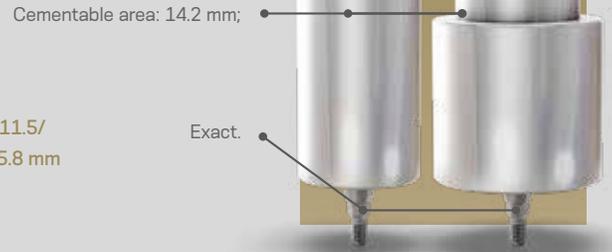

Screw sold separately.

Installation Sequence

Complete Digital Workflow

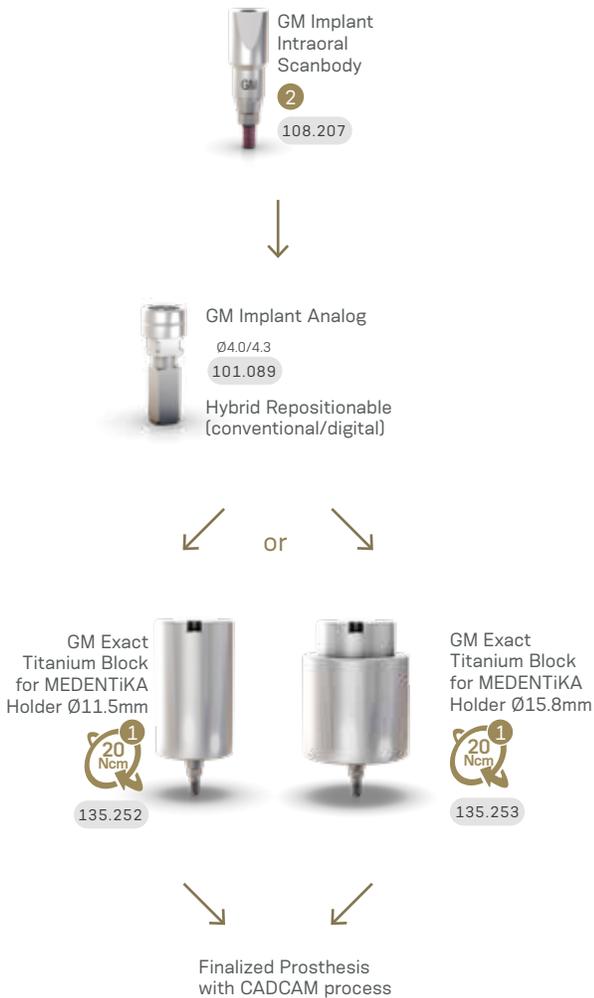

Semi Digital Workflow



Drivers

1 	+		Torque Wrench
2 	+		Manual Screwdriver Torque

Accessories



Sterile Screws
sold separately
116.286 Titanium

GM™ Titanium Block for AG Holder



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Multiple-unit cement-retained prosthesis



Ø12.0 mm



Screw sold separately.

Installation Sequence

Complete Digital Workflow



Finalized Prosthesis with CAD/CAM process

Semi Digital Workflow



Finalized Prosthesis with CAD/CAM process

30

Drivers



Accessories



GM™ CoCr Abutment



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



Ø4.1/4.5/
5.0 mm


Consider in addition 1.5 - 2.0 mm for the restorative material;
Interocclusal height of 12 mm (can be customized up to 5.0 mm);



Exact.

For implants placed at bone level.

Installation Sequence

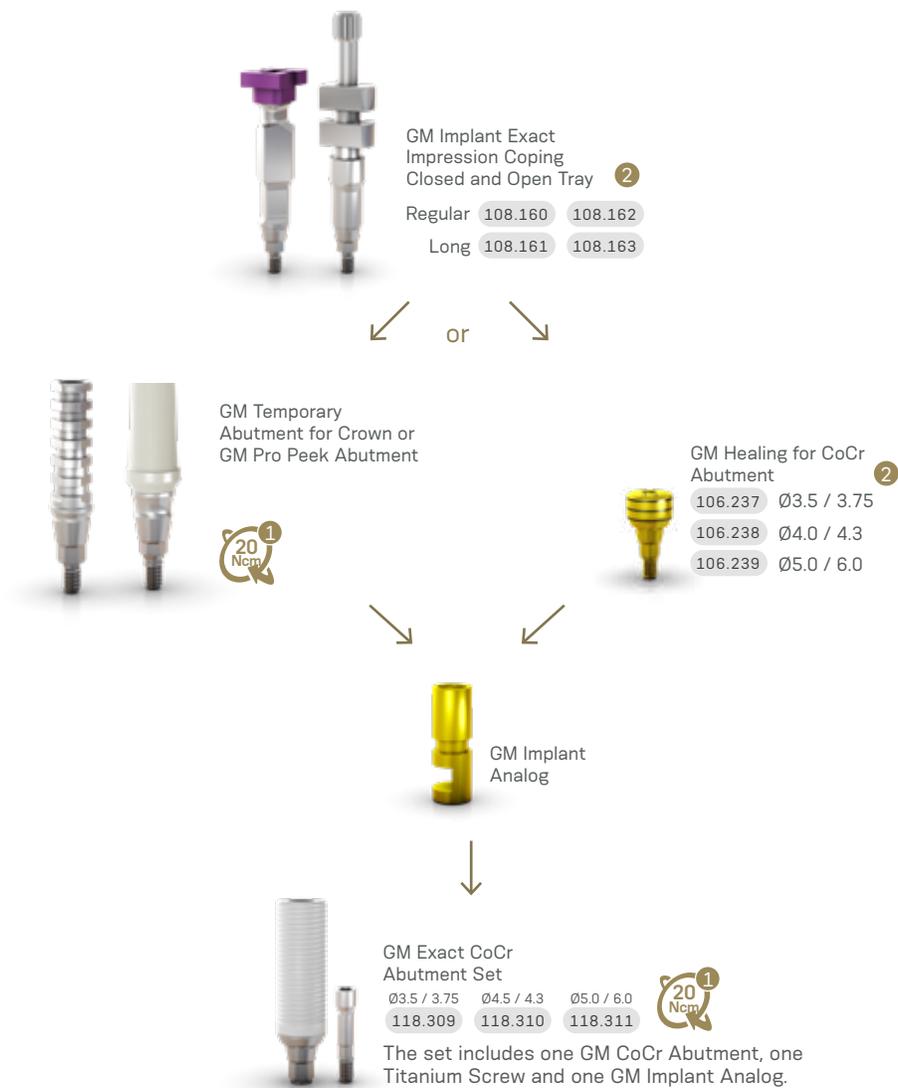

Drivers



Accessories



GM™ Temporary Abutment



Single-unit screw-retained temporary prosthesis



Multiple-unit screw-retained temporary prosthesis



Ø3.5/
4.5 mm

Consider in addition 1.5 - 2.0 mm for the restorative material;

Channels of customizations;

Interocclusal height of 10 mm (can be customized up to 4.0 mm);

Exact.




Customizable area made of titanium.

A minimum height of 4 mm of the customizable area must be kept.

With retentive grooves for acrylic material and allows customization.


Installation Sequence

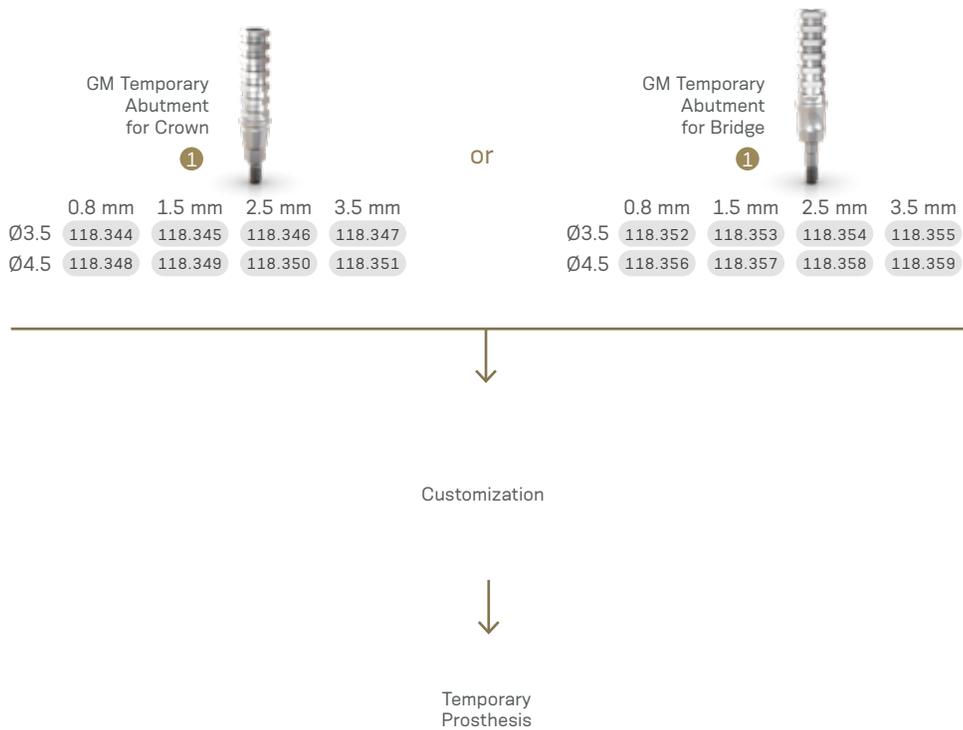

Drivers



Accessories



GM™ Pro Peek Abutment with Neo Removable Screw

Consider in addition 1.5 - 2.0 mm for the restorative material

Interocclusal height of 9.2 mm (can be customized up to 5.0 mm)

With internal threads for a secure engagement of the screw

Exact

Neo Removable Screw




Single-unit cement-retained temporary prosthesis



Ø4.5/
6.0 mm

Biocompatible Peek of easy customization.

Installation Sequence

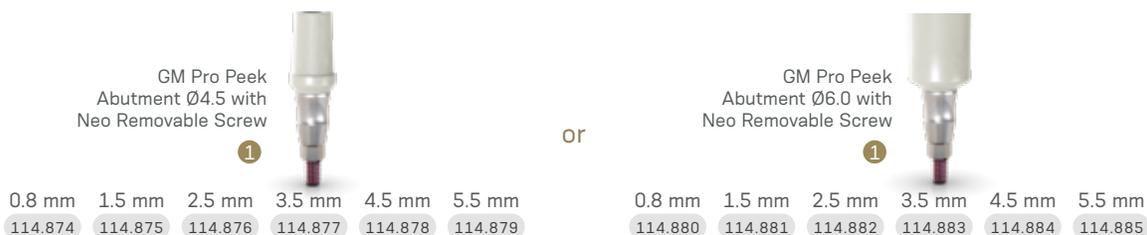

In mouth customization

Drivers



Accessories

Replacement Abutment Screw




GM™ Attachment TiN* for Removable Prosthesis



Overdenture

Angled version with removable screw.

Installation Sequence

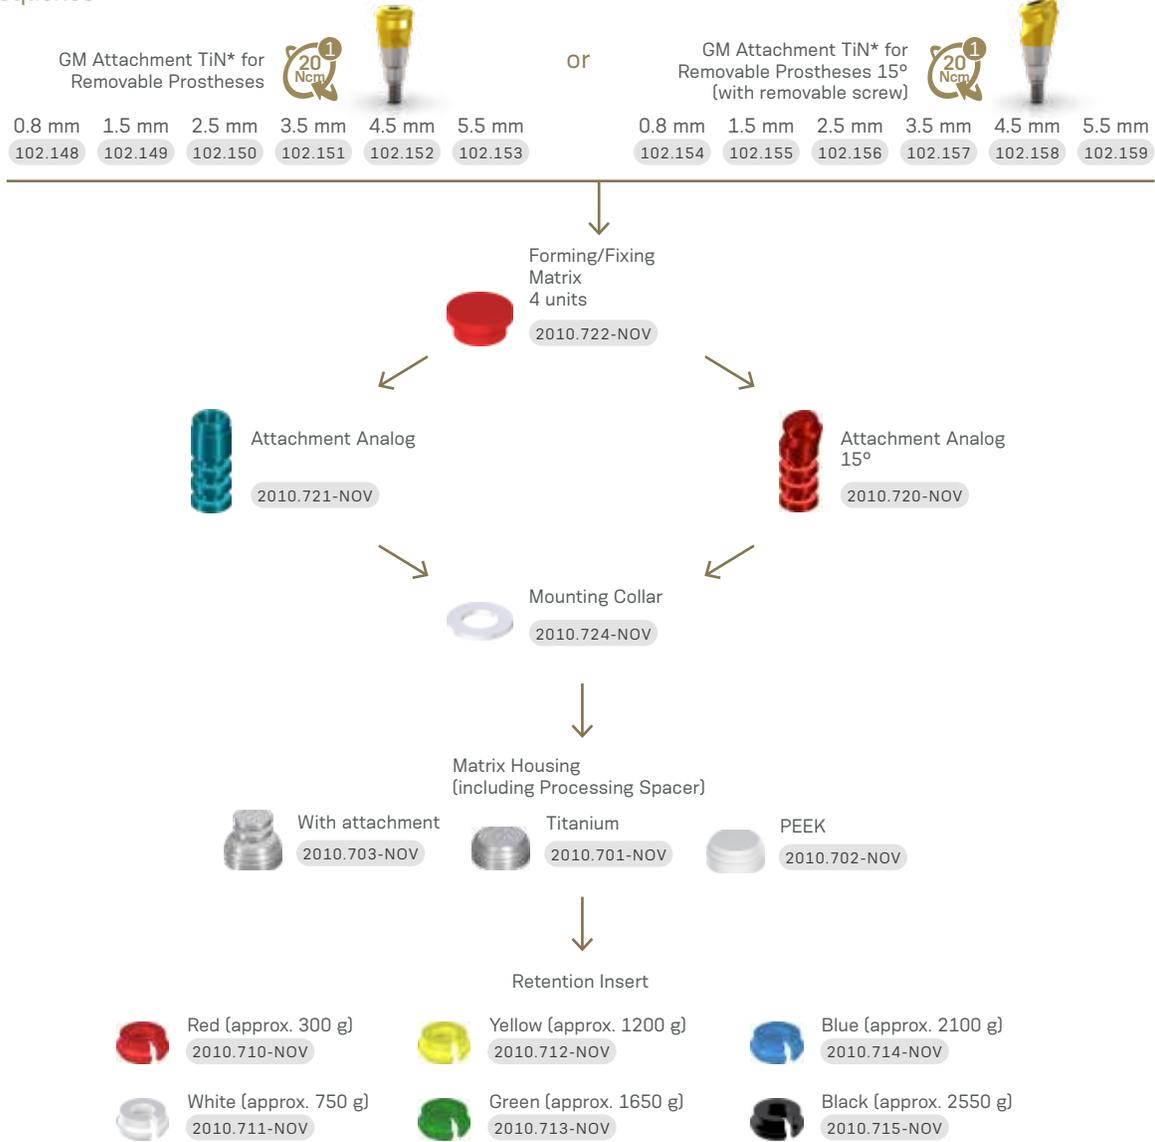

*TiN - Titanium nitride

34

Drivers



Accessories



Measurements GM™ Mini Conical Abutment with Neo Removable Screw

17°




30°



Measurements GM™ Anatomic Abutment with Neo Removable Screw

Narrow Anatomic
Abutment

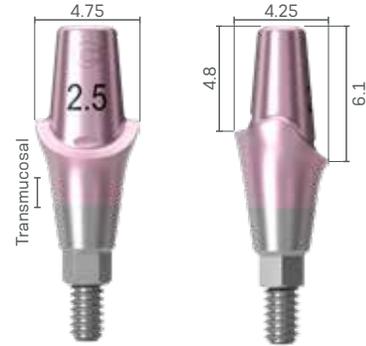

Anatomic
Abutment



Narrow Anatomic Abutment 17°




Anatomic Abutment 17°




Measurements GM™ Universal Abutment with Neo Removable Screw


4 mm chimney height / Ø3.3 / 17°

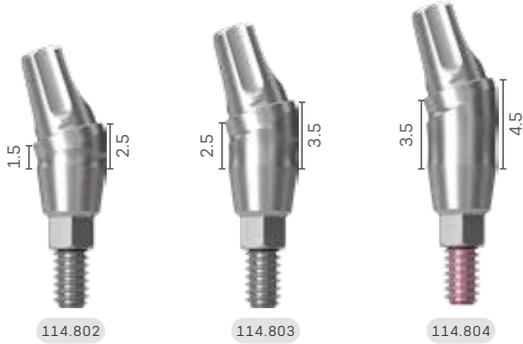


4 mm chimney height / Ø3.3 / 30°

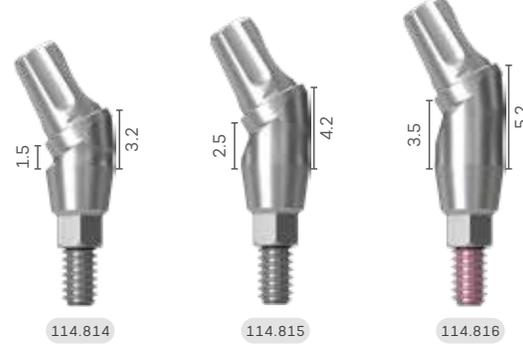


4 mm chimney height / Ø4.5 / 17°

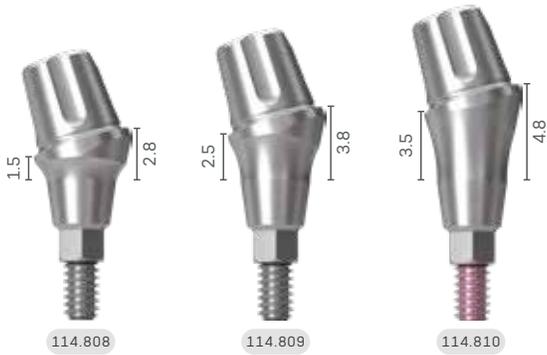

4 mm chimney height / Ø4.5 / 30°

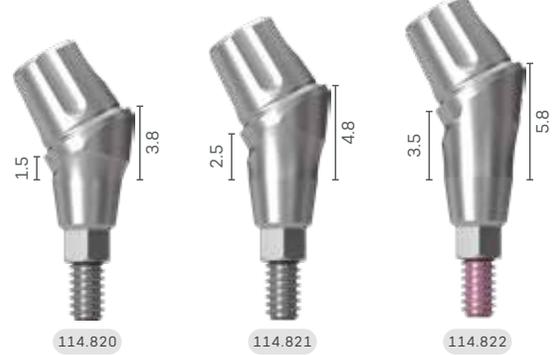

6 mm chimney height / Ø3.3 / 17°

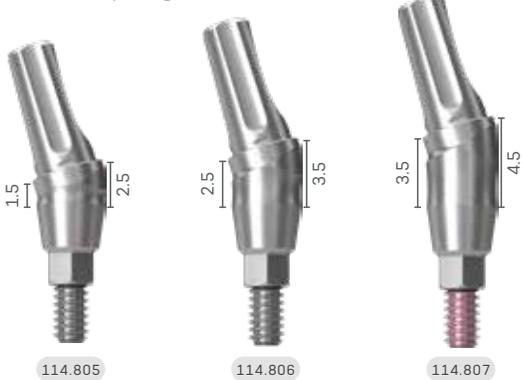


6 mm chimney height / Ø3.3 / 30°



6 mm chimney height / Ø4.5 / 17°



6 mm chimney height / Ø4.5 / 30°

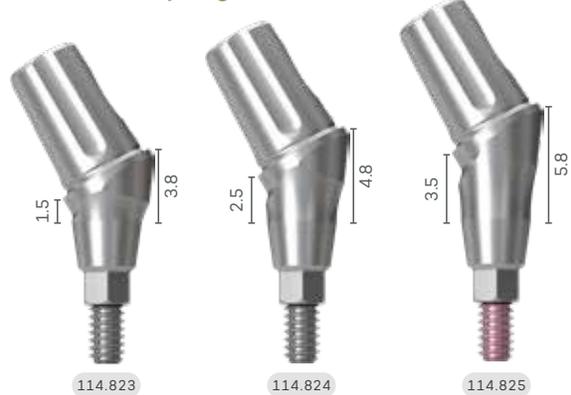

Grand Morse™ Kits

Grand Morse™ Surgical Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.302](#).



Articles

- 110.288 GM Surgical Kit Case
- 103.162 Twist Drill 2.0 Plus
- 103.213 Pilot Drill 2.0/3.0 Plus
- 103.164 Twist Drill 3.0 Plus
- 103.166 Twist Drill 3.3 Plus
- 103.167 Twist Drill 3.8 Plus
- 103.168 Twist Drill 4.3 Plus
- 103.163 Twist Drill 2.8 Plus
- 103.170 Initial Drill Plus
- 103.513 Pilot Drill GM 2.8/3.5
- 103.514 Pilot Drill GM 3.0/3.75
- 103.515 Pilot Drill GM 3.3/4.0
- 103.516 Pilot Drill GM 4.3
- 103.517 Pilot Drill GM 4.3/5.0

- 103.578 Tapered Contour Drill 3.5
- 103.579 Tapered Contour Drill 3.75
- 103.580 Tapered Contour Drill 4.0
- 103.581 Tapered Contour Drill 4.3
- 103.582 Tapered Contour Drill 5.0
- 103.425 Tapered Drill 2.0
- 103.561 Tapered Drill 3.5
- 103.564 Tapered Drill 3.75
- 103.567 Tapered Drill 4.0
- 103.570 Tapered Drill 4.3
- 103.573 Tapered Drill 5.0
- 103.576 Tapered Drill 6.0
- 105.131 GM Implant Driver - Contra-Angle
- 104.060 Neo Screwdriver (Medium)


- 105.130 GM Implant Driver - Torque Wrench (Long)
- 104.028 Manual Implant Driver - Contra-Angle
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 128.028 Height Measurer GM
- 129.004 Depth Probe
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench
- 103.426 Drill Extension

Note: Items that compose Neodent® Kits are sold separately.

40

Grand Morse™ and WS Surgical Kit

Autoclavable polymer case.

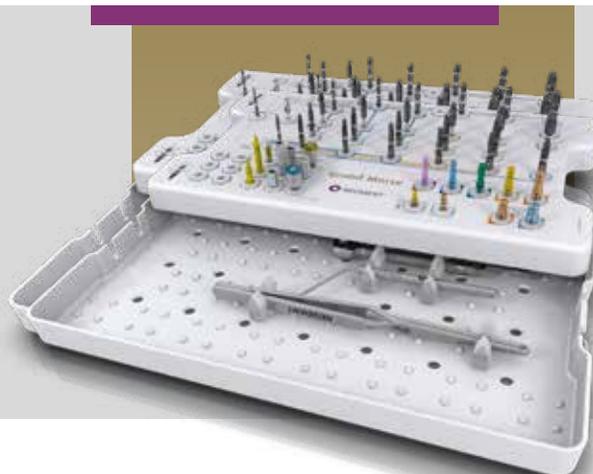

Articles

- 110.287 GM/WS Surgical Kit Case
- 103.162 Twist Drill 2.0 Plus
- 103.213 Pilot Drill 2.0/3.0 Plus
- 103.164 Twist Drill 3.0 Plus
- 103.166 Twist Drill 3.3 Plus
- 103.415 GM Pilot Drill 3.0/3.75
- 103.167 Twist Drill 3.8 Plus
- 103.168 Twist Drill 4.3 Plus
- 103.215 Pilot Drill 4.3/5.3 Plus
- 103.163 Twist Drill 2.8 Plus
- 103.169 Twist Drill 5.3 Plus
- 103.170 Initial Drill Plus
- 103.513 Pilot Drill GM 2.8/3.5
- 103.515 Pilot Drill GM 3.3/4.0
- 103.516 Pilot Drill GM 4.3
- 103.517 Pilot Drill GM 4.3/5.0
- 103.221 Pilot Drill CM 5.3/6.0 Plus

- 103.578 Tapered Contour Drill 3.5
- 103.579 Tapered Contour Drill 3.75
- 103.580 Tapered Contour Drill 4.0
- 103.581 Tapered Contour Drill 4.3
- 103.582 Tapered Contour Drill 5.0
- 103.425 Tapered Drill 2.0
- 103.561 Tapered Drill 3.5
- 128.029 WS Height Measurer
- 103.564 Tapered Drill 3.75
- 103.567 Tapered Drill 4.0
- 103.570 Tapered Drill 4.3
- 103.573 Tapered Drill 5.0
- 103.576 Tapered Drill 6.0
- 105.131 GM Implant Driver - Contra-Angle
- 105.002 Smart/WS Implant Driver - Contra-Angle
- 104.060 Neo Screwdriver (Medium)
- 105.130 GM Implant Driver GM - Torque Wrench

- 105.018 Hex Connection - Torque Wrench (Long)
- 104.028 Manual Implant Driver - Contra-Angle
- 104.012 Manual Screwdriver (Medium)
- 105.129 GM Implant Driver GM - Torque Wrench
- 105.001 Smart/WS Implant Driver - Torque Wrench (Short)
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 128.024 WS Direction Indicator 4.3/5.0
- 128.025 WS Direction Indicator 5.3/6.0
- 128.028 GM Height Measurer
- 129.004 Depth Probe
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench
- 103.426 Drill Extension

Note: Items that compose Neodent® Kits are sold separately.

Helix GM™ Compact Surgical Kit

Autoclavable polymer case.

The Kit allows the installation of Helix GM™ Implants in all bone types.

To order the pre-mounted version of the kit, with its complete composition, use code [110.303](#).



Articles

110.297 Helix GM™ Compact Surgical Kit Case
103.170 Initial Drill
103.425 Tapered Drill 2.0
103.561 Tapered Drill 3.5
103.564 Tapered Drill 3.75
103.567 Tapered Drill 4.0
103.570 Tapered Drill 4.3
103.573 Tapered Drill 5.0
103.576 Tapered Drill 6.0
103.577 Tapered Drill 7.0 (Short)*
104.060 Neo Manual Screwdriver (Medium)
104.028 Manual Implant Driver - Contra-angle

103.426 Drill Extension
103.578 Tapered Contour Drill 3.5
103.579 Tapered Contour Drill 3.75
103.580 Tapered Contour Drill 4.0
103.581 Tapered Contour Drill 4.3
103.582 Tapered Contour Drill 5.0
105.131 GM Implant Driver - Contra-angle GM
105.130 Implant Driver - Torque Wrench (Long)
105.129 GM Implant Driver - Torque Wrench (Short)
103.513 GM Pilot Drill 2.8/3.5
103.514 GM Pilot Drill 3.0/3.75
103.515 GM Pilot Drill 3.3/4.0

103.516 GM Pilot Drill 4.3
103.517 GM Pilot Drill 4.3/5.0
128.028 GM Height Measurer
128.030 Angle Measurer for Drill 2.0 17°
128.031 Angle Measurer for Drill 2.0 30°
128.019 Direction Indicator 2.8/3.5
128.020 Direction Indicator 3.0/3.75
128.021 Direction Indicator 3.3/4.0
128.022 Direction Indicator 3.6/4.3
128.023 Direction Indicator 4.3/5.0
129.004 Depth Probe
104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

*Tapered Drill 7.0 is not included in the pre-mounted kit composition (110.303).



Neodent controlsystem



TRUST YOURSELF

The surgical procedure for implant placement can be perceived as complex, especially when performed in the posterior regions with limited visibility, or in proximity with anatomical structures such as nerve canals. The Neodent® Control System brings confidence and efficiency building trust during the surgical procedure.

Protect anatomical structures

The placement of implants requires accuracy, and the Neodent® Control System has been designed to reduce the risk against overdrilling and protecting anatomical structures such as nerves, the sinus or adjacent roots by securing the final depth.

Master limited visibility

The Neodent® Control System helps to provide confidence during situations with reduced visibility due to adjacent teeth, limited mouth opening, blood, saliva, making it difficult to read the lines on a twisting drill by reaching the planned depth.



Intuitive solution

The Neodent® Control System is a color coded solution facilitating the identification of the drill sequence, the diameter and length of the implant and the combination of drill stop and drill.



Secure drill stop locking system

The Neodent® Control Drill Stop features a modern drill locking system enabling an easy and secure engaging into the drill, offering a peace-of-mind surgical experience.



Multiple use solution

The Neodent® Control Drill Stops are made of titanium for professional cleaning and autoclaving allowing multiple use.

User friendly kit retentive system

The Neodent® Control Drill Stop Kit includes an innovative retentive system.



A convenient and time-saving pick and drop mechanism during the surgical procedure.

Neodent® Color Code overview



Color code according to implant length



Compatible portfolio of Helix GM™ Implants



Length	Diameter						
	3.5	3.75	4.0	4.3	5.0	6.0	7.0
8	✓	✓	✓	✓	✓	✓	✓
10	✓	✓	✓	✓	✓	✓	✓
11.5	✓	✓	✓	✓	✓	✓	✓
13	✓	✓	✓	✓	✓	✓	✓

Helix GM™ Compact Kit Control Stop Drills

Autoclavable polymer case.

The Kit allows the installation of Helix GM™ Implants in all bone types, using the Neodent® Control Stop Drills.

To order the pre-mounted version of the kit, with its complete composition, use code [110.308](#).



Articles

- 110.297 Helix GM™ Compact Surgical Kit Case
- 103.170 Initial Drill
- 103.492 Tapered Control Stop Drill 2.0
- 103.493 Tapered Control Stop Drill 3.5
- 103.494 Tapered Control Stop Drill 3.75
- 103.495 Tapered Control Stop Drill 4.0
- 103.496 Tapered Control Stop Drill 4.3
- 103.497 Tapered Control Stop Drill 5.0
- 103.498 Tapered Control Stop Drill 6.0 (Short)
- 103.499 Tapered Control Stop Drill 7.0 (Short)*
- 104.060 Neo Manual Screwdriver (Medium)
- 104.028 Manual Implant Driver - Contra-angle

- 103.426 Drill Extension
- 103.500 Tapered Control Stop Drill 3.5+
- 103.501 Tapered Control Stop Drill 3.75+
- 103.502 Tapered Control Stop Drill 4.0+
- 103.503 Tapered Control Stop Drill 4.3+
- 103.504 Tapered Control Stop Drill 5.0+
- 105.131 GM Implant Driver - Contra-angle GM
- 105.130 Implant Driver - Torque Wrench (Long)
- 105.129 GM Implant Driver - Torque Wrench (Short)
- 103.513 Pilot Drill 3.5
- 103.514 Pilot Drill 3.75
- 103.515 Pilot Drill 4.0

- 103.516 Pilot Drill 4.3
- 103.517 Pilot Drill 5.0
- 128.028 GM Height Measurer
- 128.030 Angle Measurer for Drill 2.0 17°
- 128.031 Angle Measurer for Drill 2.0 30°
- 128.019 Direction Indicator 2.8/3.5
- 128.020 Direction Indicator 3.0/3.75
- 128.021 Direction Indicator 3.3/4.0
- 128.022 Direction Indicator 3.6/4.3
- 128.023 Direction Indicator 4.3/5.0
- 129.004 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

*Tapered Control Stop Drill 7.0 is not included in the pre-mounted kit composition (110.308).

Control Drill Stop Kit

Autoclavable polymer case.

The Kit allows the sterilization and engagement of Neodent® Control Drill Stops on the drills.

To order the pre-mounted version of the kit, with its complete composition, use code [110.306](#).



Articles

- 110.307 Control Drill Stop Kit Case
- 125.144 8.0 Control Drill Stop D2.0
- 125.145 10.0 Control Drill Stop D2.0
- 125.146 11.5 Control Drill Stop D2.0
- 125.147 13.0 Control Drill Stop D2.0
- 125.148 8.0 Control Drill Stop D3.5
- 125.149 10.0 Control Drill Stop D3.5
- 125.150 11.5 Control Drill Stop D3.5
- 125.151 13.0 Control Drill Stop D3.5
- 125.152 8.0 Control Drill Stop D3.75/4.0
- 125.153 10.0 Control Drill Stop D3.75/4.0
- 125.154 11.5 Control Drill Stop D3.75/4.0


- 125.155 13.0 Control Drill Stop D3.75/4.0
- 125.156 8.0 Control Drill Stop D4.3/5.0
- 125.157 10.0 Control Drill Stop D4.3/5.0
- 125.158 11.5 Control Drill Stop D4.3/5.0
- 125.159 13.0 Control Drill Stop D4.3/5.0
- 125.160 8.0 Control Drill Stop D6.0/7.0
- 125.161 10.0 Control Drill Stop D6.0/7.0
- 125.162 11.5 Control Drill Stop D6.0/7.0
- 125.163 13.0 Control Drill Stop D6.0/7.0

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse™ Prosthetic Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.304](#).

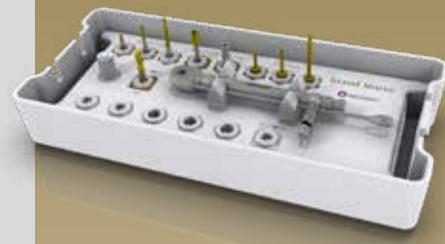

Articles

- 110.294 GM Prosthetic Kit Case
- 105.146 Neo Screwdriver Torque Connection - Contra-angle (Extra-short)
- 105.160 Neo Screwdriver Torque Connection - Contra-angle (Long)
- 105.136 Neo Screwdriver Torque Connection - Contra-angle (Medium)
- 105.138 Hexagonal Prosthetic Driver - Contra-angle
- 105.137 Hexagonal Prosthetic Driver - Torque Wrench
- 105.133 Neo Screwdriver Torque Connection (Short) - Torque Wrench
- 105.132 Neo Screwdriver Torque Connection (Medium) - Torque Wrench
- 105.157 Neo Screwdriver Torque Connection (Long) - Torque Wrench
- 104.005 Manual Screwdriver Torque
- 128.028 GM Height Measurer
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse™ Try-In Kit

Autoclavable polymer case.

To order the pre-mounted version of the kit, with its complete composition, use code [110.305](#).



Articles

- | | | |
|--------------------------------------|--|---|
| 110.295 GM Try-In Kit Case | 114.782 GM Abutment Try-In 4.5X6X4.5 | 114.793 GM Abutment Try-In 30° 4.5X6X1.5 |
| 114.772 GM Abutment Try-In 3.3X6X0.8 | 114.783 GM Abutment Try-In 4.5X6X5.5 | 114.794 GM Abutment Try-In 30° 4.5X6X2.5 |
| 114.773 GM Abutment Try-In 3.3X6X1.5 | 114.784 GM Abutment Try-In 17° 3.3X6X1.5 | 114.795 GM Abutment Try-In 30° 4.5X6X3.5 |
| 114.774 GM Abutment Try-In 3.3X6X2.5 | 114.785 GM Abutment Try-In 17° 3.3X6X2.5 | 114.796 GM Anatomic Abutment Try-In 1.5 |
| 114.775 GM Abutment Try-In 3.3X6X3.5 | 114.786 GM Abutment Try-In 17° 3.3X6X3.5 | 114.797 GM Anatomic Abutment Try-In 2.5 |
| 114.776 GM Abutment Try-In 3.3X6X4.5 | 114.787 GM Abutment Try-In 17° 4.5X6X1.5 | 114.798 GM Anatomic Abutment Try-In 3.5 |
| 114.777 GM Abutment Try-In 3.3X6X5.5 | 114.788 GM Abutment Try-In 17° 4.5X6X2.5 | 114.799 GM Lateral Anatomic Abutment Try-In 1.5 |
| 114.778 GM Abutment Try-In 4.5X6X0.8 | 114.789 GM Abutment Try-In 17° 4.5X6X3.5 | 114.800 GM Lateral Anatomic Abutment Try-In 2.5 |
| 114.779 GM Abutment Try-In 4.5X6X1.5 | 114.790 GM Abutment Try-In 30° 3.3X6X1.5 | 114.801 GM Lateral Anatomic Abutment Try-In 3.5 |
| 114.780 GM Abutment Try-In 4.5X6X2.5 | 114.791 GM Abutment Try-In 30° 3.3X6X2.5 | 104.058 Neo Manual Screwdriver (Short) |
| 114.781 GM Abutment Try-In 4.5X6X3.5 | 114.792 GM Abutment Try-In 30° 3.3X6X3.5 | 128.028 GM Height Measurer |

Note: Items that compose Neodent® Kits are sold separately.

Grand Morse™ Instruments



Initial Drill

- :: Available in surgical steel;
- :: 2.0mm diameter.

103.170

Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM™ and Drive GM™ Implants;
- :: With a color code according to the drill diameter.



	Short 31 mm	Regular 35 mm	Long 43 mm
Ø2.0	103.559	103.425	103.560
Ø3.5	103.562	103.561	103.563
Ø3.75	103.565	103.564	103.566
Ø4.0	103.568	103.567	103.569
Ø4.3	103.571	103.570	103.572
Ø5.0	103.574	103.573	103.575
Ø6.0	103.576		
Ø7.0	103.577		

Tapered+ Drills

- :: For preparing the implant bed in bone types I and II for Helix GM™ Implants;
- :: With a color code according to the drill diameter and 2 stripes of color for identification.



Ø3.5+	103.578
Ø3.75+	103.579
Ø4.0+	103.580
Ø4.3+	103.581
Ø5.0+	103.582

Pilot Drills

- :: Available in surgical steel;
- :: Increasing the surgical alveolus diameter ridge, easing the penetration of the next drill or the implant.



Ø2/3	103.213		
Ø3.5	103.513	Ø5.0	103.517
Ø3.75	103.514	Ø3.8/4.3	103.214
Ø4.0	103.515	Ø4.3/5.3	103.215
Ø4.3	103.516	Ø5.3/6	103.221

Twist Drills

- :: Available in surgical steel;
- :: Drill sequence for Titamax GM™ Implants.



	Short 31 mm	Regular 35 mm	Long 43 mm
Ø2.0	103.222	103.162	103.228
Ø2.8	103.223	103.163	103.229
Ø3.0	103.224	103.164	103.230
Ø3.3	103.225	103.166	103.231
Ø3.8	103.226	103.167	
Ø4.3	103.227	103.168	

Tapered Control Stop Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM™ Implants;
- :: Attachment to engage drill stops;
- :: With a color code according to the drill diameter.



Ø2.0	103.492	Ø4.3	103.496
Ø3.5	103.493	Ø5.0	103.497
Ø3.75	103.494	Ø6.0	103.498
Ø4.0	103.495	Ø7.0	103.499

Tapered+ Control Stop Drills

- :: Available in surgical steel;
- :: For preparing the implant bed in bone types I and II for Helix GM™ Implants;
- :: Attachment to engage drill stops;
- :: With a color code according to the drill diameter and 2 stripes of color for identification.



Ø3.5+	103.500	Ø4.3+	103.503
Ø3.75+	103.501	Ø5.0+	103.504
Ø4.0+	103.502		

Control Drill Stops


- :: Available in titanium;
- :: To be used in association with the Control Stop Drills;
- :: Physical control for drilling depth.



	8 mm	10 mm	11.5 mm	13 mm
Ø2.0	125.144	125.145	125.146	125.147
Ø3.5	125.148	125.149	125.150	125.151
Ø3.75/4.0	125.152	125.153	125.154	125.155
Ø4.3/5.0	125.156	125.157	125.158	125.159
Ø6.0/7.0	125.160	125.161	125.162	125.163

Direction Indicators

- :: Available in titanium;
- :: Instrument to guide the implant position;
- :: Diameter of central band corresponds to GM Implant diameter;
- :: Smaller side to be used after Ø2.0mm drill;
- :: Larger side to be used after the last drill before implant installation.



2.8/3.5	128.019	3.6/4.3	128.022
3.0/3.75	128.020	4.3/5.0	128.023
3.3/4.0	128.021		

Drill Extension

- :: Available in surgical steel;
- :: Fit the drill directly into the Drill Extension.



103.426

GM Height Measurer

- :: Available in titanium;
- :: For selecting GM prosthetic abutments;
- :: Marks corresponding to transmucosa heights.
- :: Can be used as X-Ray Positioner.



128.028

GM™ Implant Driver - Contra-Angle



- :: To capture the implant directly from the packaging;
- :: To place GM Implants with contra-angle, or attached to a manual driver for contra-angle connections (104.028) for hand placement;
- :: With six dimples to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque 35 Ncm.

105.131

GM Implant Driver - Torque Wrench



- :: To place GM Implants with the Torque Wrench (104.050);
- :: With six marks to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque: 60 Ncm..

Short	Long
22 mm	30 mm

105.129 105.130

Neo Screwdriver Torque Connection - Torque Wrench



- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
16.5 mm	22 mm	32 mm

105.133 105.132 105.157

Neo Manual Screwdriver



- :: Available in surgical steel;
- :: Yellow color for line identification

Short	Medium	Long
21 mm	25 mm	37 mm

104.058 104.060 104.072

Neo Screwdriver Torque Connection - Contra-angle



- :: Available in surgical steel;
- :: Yellow color for line identification;
- :: Extra Short Neo Screwdriver Torque Connection - Contra-angle (105.146) recommended for Impression Copings, Cover Screws and Healing Abutments.

Extra Short	Short	Long
16.5 mm	24 mm	31 mm

105.146 105.135 105.160

Hexagonal Prosthetic Driver



- :: Available in surgical steel;
- :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;

Contra-angle	Torque Wrench
105.138	105.137

105.138

105.137

Angled Solution Screwdriver for Torque Wrench



- :: To place GM Titanium Bases for Angled Solution with torque wrench;
- :: Maximum torque of 20 Ncm.

Short	Medium	Long
16.5 mm	22.5 mm	28.5 mm

105.150 105.151 105.152

Angled Solution Screwdriver for Contra-angle



- :: To place GM Titanium Bases for Angled Solution with contra-angle;
- :: Maximum torque of 20 Ncm.

Short	Medium	Long
20 mm	26 mm	32 mm

105.147 105.148 105.149

GM Bone Profile Drill with Guide



- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.424

Angle Measurer for Drill 2.0



- :: Available in titanium;
- :: Angles: 17° and 30°;
- :: To select and plan the abutments angulation during surgical procedures;
- :: Suggested use: after Twist Drill 2.0.

17°	30°
128.030	128.031

GM Angle Measurer



- :: Available in titanium;
- :: Angles: 17° and 30°;
- :: To a more accurate selection and planning of the abutments angulation during the prosthetic phase.

17°	30°
128.032	128.033

Control Stop Kit Holder



- :: Available in polymer;
- :: Replacement piece;
- :: To keep the stops organized and to engage and remove them from the drills.

110.310

Manual Implant Drivers



- :: Available in surgical steel;
- :: For Contra-angle connections: connected to GM Implant Driver, it becomes a manual driver for implant placement.
- :: For Torque Wrench connections: connected to screwdrivers, it provides manual torque.

Contra-angle
Connections
104.028

Torque Wrench
Connections
104.005

Remover for Abutments with internal threads



- :: Available in surgical steel;
- :: To remove abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws

130.118 Long
130.114

Remover for Neo Screws



- :: Available in surgical steel;
- :: Compatible with Neo removable screws for abutments

130.119 Long
130.115

Torque Wrench



- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050

Removal Sets for Abutments with internal threads and Neo Screws

- :: Available in surgical steel;
- :: To remove Neo Removable Screws and abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws



130.117

Long
130.116



Neodent easyguide

SIMPLICITY AT ONE HAND

Neodent® is designed to offer straightforward guided surgery techniques enabling predictable surgical results, efficient treatment protocols and patient treatment acceptance.



STRAIGHTFORWARD GUIDED SURGERY TECHNIQUE

Surgical convenience with one-hand procedures



EFFICIENT TREATMENT PROTOCOLS

Intuitive and simple technique



PREDICTABLE SURGICAL RESULTS

Confidence for accurate implant positioning



PATIENT TREATMENT ACCEPTANCE

Communication building trust and patient engagement



NEODENT® EASYGUIDE ENABLES ONE-HAND PROCEDURES WITH NO DRILL HANDLES

Simple technique

Reduced number of instruments

Surgeries can be performed without assistance

ONE DRILL DESIGN

The unique geometry of the Neodent® EasyGuide tapered drills is indicated for all bone types and dismisses the need for additional drill types or taps, simplifying the drilling sequence.

1



COLOR CODE ACCORDING TO IMPLANT DIAMETER

2



BUILT-IN TITANIUM STOP FOR PHYSICAL DEPTH CONTROL, WITH COLOR MATCHING THE SLEEVE IN THE SURGICAL GUIDE

3




LASER-MARKED LENGTH

4



ACTIVE PORTION MATCHING IMPLANT LENGTHS

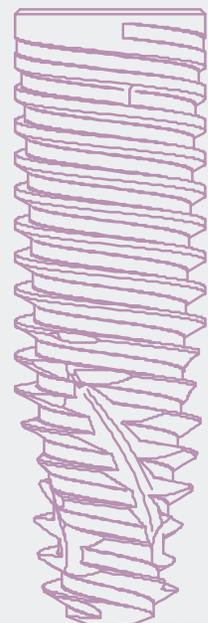

1

2

3

4





FULLY GUIDED BED PREPARATION

- Intimate contact between drill and sleeve for accuracy in angulation
- Depth control with stop drills

FULLY GUIDED IMPLANT INSERTION

- Implant driver fits the sleeve, for a fully guided insertion with physical depth control
- Offset: 10 mm



1. DATA ACQUISITION
3D (CB)CT scan (DICOM)
Intraoral or lab scanning
(STL images)




2. VIRTUAL PLANNING
Implant positioned respecting the patient's anatomy and prosthetic outcome. Neodent® **EasyGuide** is compatible with major software.

3. SURGICAL GUIDE PRODUCTION
The surgical guide must contain the sleeves that guide the instruments and the implants.




4. SURGICAL PROCEDURE
Neodent® **EasyGuide** presents two surgical kits, selected according to the implant diameter.


EASYGUIDE KIT NARROW/REGULAR • Ø3.5, Ø3.75

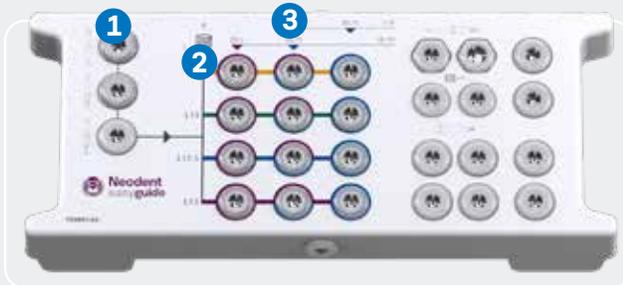

EASYGUIDE KIT REGULAR/WIDE • Ø4.0, Ø4.3, Ø5.0

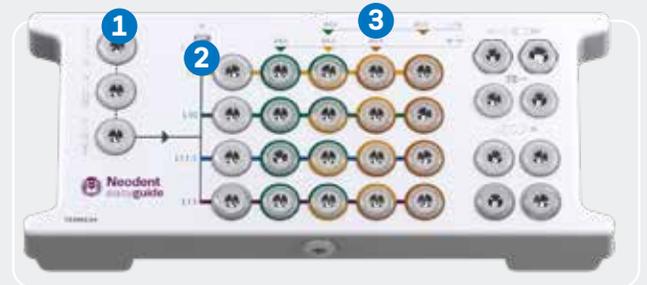

1. UNIQUE START REGARDLESS OF BONE TYPE



2. STRAIGHTFORWARD IMPLANT LENGTH IDENTIFICATION



3. COLOR CODED DRILL SEQUENCE FOR EACH IMPLANT DIAMETER



NARROW SLEEVE: Ø3.5/Ø3.75



REGULAR SLEEVE: Ø4.0/Ø4.3/Ø5.0

Neodent®
EasyGuide
Kits

Neodent® EasyGuide Kit for Narrow/Regular Diameter Implants

Autoclavable polymer case.

The kit allows the installation of Helix GM™ Implants of Ø3.5 and Ø3.75 in all bone types, using the Neodent® EasyGuide Guided Surgery Technique.



Articles

- 110.313 EasyGuide Kit Narrow/Reg. Diam. Tray
- 125.170 GM Narrow Stabilizer - 3 units per kit
- 105.161 GM Narrow Driver for Contra-angle
- 105.162 GM Narrow Driver for Torque Wrench
- 103.583 Narrow Mucosa Punch
- 103.519 Narrow Bone Leveling Drill
- 103.545 Narrow Initial Drill
- 103.546 Narrow Tapered Drill D3.5X8
- 103.547 Narrow Tapered Drill D3.5X10
- 103.548 Narrow Tapered Drill D3.5X11.5
- 103.549 Narrow Tapered Drill D3.5X13
- 103.550 Narrow Tapered Drill D3.5/3.75X8

- 103.551 Narrow Tapered Drill D3.5/3.75X10
- 103.552 Narrow Tapered Drill D3.5/3.75X11.5
- 103.553 Narrow Tapered Drill D3.5/3.75X13
- 103.554 Narrow Tapered Drill D3.75X8
- 103.555 Narrow Tapered Drill D3.75X10
- 103.556 Narrow Tapered Drill D3.75X11.5
- 103.557 Narrow Tapered Drill D3.75X13
- 105.160 Long Neo Screwdriver for Contra-angle
- 104.060 Neo Manual Screwdriver (Medium)
- 103.558 Drill for Palatal Setter
- 125.176 Palatal Setter
- 103.395 Guided Surgery Drill 1.3

- 125.142 Fixation Clamp - 3 units per kit
- 129.034 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

Neodent® EasyGuide Kit for Regular/Wide Diameter Implants

Autoclavable polymer case.

The kit allows the installation of Helix GM™ Implants of Ø4.0, Ø4.3 and Ø5.0 in all bone types, using the Neodent® EasyGuide Guided Surgery Technique.



Articles

- 110.314 EasyGuide Kit Reg./Wide Diam. Tray
- 125.171 GM Regular Stabilizer - 3 units per kit
- 105.163 GM Regular Driver for Contra-angle
- 105.164 GM Regular Driver for Torque Wrench
- 103.584 Regular Mucosa Punch
- 103.518 Regular Bone Leveling Drill
- 103.520 Regular Initial Drill
- 103.521 Regular Tapered Drill D2.7X8
- 103.522 Regular Tapered Drill D2.7X10
- 103.523 Regular Tapered Drill D2.7X11.5
- 103.524 Regular Tapered Drill D2.7X13
- 103.529 Regular Tapered Drill D4.0X8

- 103.530 Regular Tapered Drill D4.0X10
- 103.531 Regular Tapered Drill D4.0X11.5
- 103.532 Regular Tapered Drill D4.0X13
- 103.533 Regular Tapered Drill D4.0/4.3X8
- 103.534 Regular Tapered Drill D4.0/4.3X10
- 103.535 Regular Tapered Drill D4.0/4.3X11.5
- 103.536 Regular Tapered Drill D4.0/4.3X13
- 103.537 Regular Tapered Drill D4.3/5.0X8
- 103.538 Regular Tapered Drill D4.3/5.0X10
- 103.539 Regular Tapered Drill D4.3/5.0X11.5
- 103.540 Regular Tapered Drill D4.3/5.0X13
- 103.541 Regular Tapered Drill D5.0X8

- 103.542 Regular Tapered Drill D5.0X10
- 103.543 Regular Tapered Drill D5.0X11.5
- 103.544 Regular Tapered Drill D5.0X13
- 105.160 Long Neo Screwdriver for Contra-angle
- 104.060 Neo Manual Screwdriver (Medium)
- 103.558 Drill for Palatal Setter
- 125.176 Palatal Setter
- 103.395 Guided Surgery Drill 1.3
- 125.142 Fixation Clamp - 3 units per kit
- 129.034 Depth Probe
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

Neodent®
EasyGuide
Instruments



Narrow Tapered Drills

- :: Available in surgical steel;
- :: For Helix GM™ implants with Ø3.5 and Ø3.75 in diameter;
- :: Built-in titanium stops for a fully-guided procedure, matching the color of the sleeve of the surgical guide;
- :: Color code according to implant diameter;
- :: Laser-marked length.

	Ø3.5	Ø3.5/3.75	Ø3.75
8.0	103.546	103.550	103.554
10.0	103.547	103.551	103.555
11.5	103.548	103.552	103.556
13.0	103.549	103.553	103.557



Regular Tapered Drills

- :: Available in surgical steel;
- :: For Helix GM™ implants with Ø4.0, Ø4.3 and Ø5.0 in diameter;
- :: Built-in titanium stops for a fully-guided procedure matching the color of the sleeve of the surgical guide;
- :: Color code according to implant diameter;
- :: Laser-marked length.

	Ø2.7	Ø4.0	Ø4.0/4.3	Ø4.3/5.0	Ø5.0
8.0	103.521	103.529	103.533	103.537	103.541
10.0	103.522	103.530	103.534	103.538	103.542
11.5	103.523	103.531	103.535	103.539	103.543
13.0	103.524	103.532	103.536	103.540	103.544



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in stainless steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø1.3	Guide Clamp
103.395	125.142



Drill and Palatal Setter

- :: Drill and Palatal Setter available in stainless steel;
- :: Palatal Setter placed with the GM Implant Driver for Contra-angle;
- :: Maximum torque of 20 Ncm.

Drill	Palatal Setter
103.558	125.176



Mucosa Punches

- :: Available in stainless steel;
- :: To remove the mucosa before beginning the osteotomy.
- :: Rotation recommended: 60 rpm.

Narrow	Regular
103.583	103.584



Bone Leveling Drills

- :: Available in stainless steel;
- :: Built-in titanium stops matching the color of the sleeve of the surgical guide;
- :: For flattening bone surface before osteotomy.

Narrow	Regular
103.519	103.518



Initial Drills

- :: Available in stainless steel;
- :: Built-in titanium stops matching the color of the sleeve of the surgical guide;;
- :: For rupture of the cortical bone.

Narrow	Regular
103.545	103.520



GM Drivers for Contra-Angle

- :: Available in stainless steel;
- :: Color-coded according to the sleeve of the surgical guide;
- :: To start the implant placement through the surgical guide;
- :: Maximum torque 35 Ncm.

Narrow Regular
105.161 105.163

Neo Manual Screwdriver

- :: Available in surgical steel and titanium.



Medium
25 mm

104.060



GM Drivers for Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide;
- :: Maximum torque 60 Ncm.

Narrow Regular
105.162 105.164

Neo Screwdriver Torque Connection - Contra-angle

- :: Available in stainless steel;
- :: Maximum torque 20 Ncm.



105.160



Guide Stabilizers

- :: Available in titanium;
- :: Color-coded according to the sleeve of the surgical guide;
- :: Additional fixation of the surgical guide.

Narrow Regular
125.170 125.171

Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly and cleaning.



104.050

Depth Probe

- :: Available in titanium;
- :: With marks matching the Helix GM™ implant lengths.



129.034

Sleeves for Neodent® EasyGuide

- :: Available in titanium;
- :: Sold in bags with 10 units each.



125.165 Regular Sleeve D5.2



125.168 Narrow Sleeve D3.93



125.177 Sleeve for Palatal Setter



125.143 Sleeve for Fixation Clamp




A SMILE FOR EVERYONE

NEODENT® NEOARCH®

IMMEDIATE FIXED FULL-ARCH SOLUTION

Increasing expectations for shortened treatment duration represent a significant challenge for dental professionals especially in patients with anatomical deficiencies. The Neodent® Implant System offers an optimized solution for immediate fixed treatment protocols in edentulous patients even with severe atrophic maxilla. Neodent® NeoArch® allows to significantly improve patient satisfaction and quality of life by immediately restoring function and esthetics ^[10].

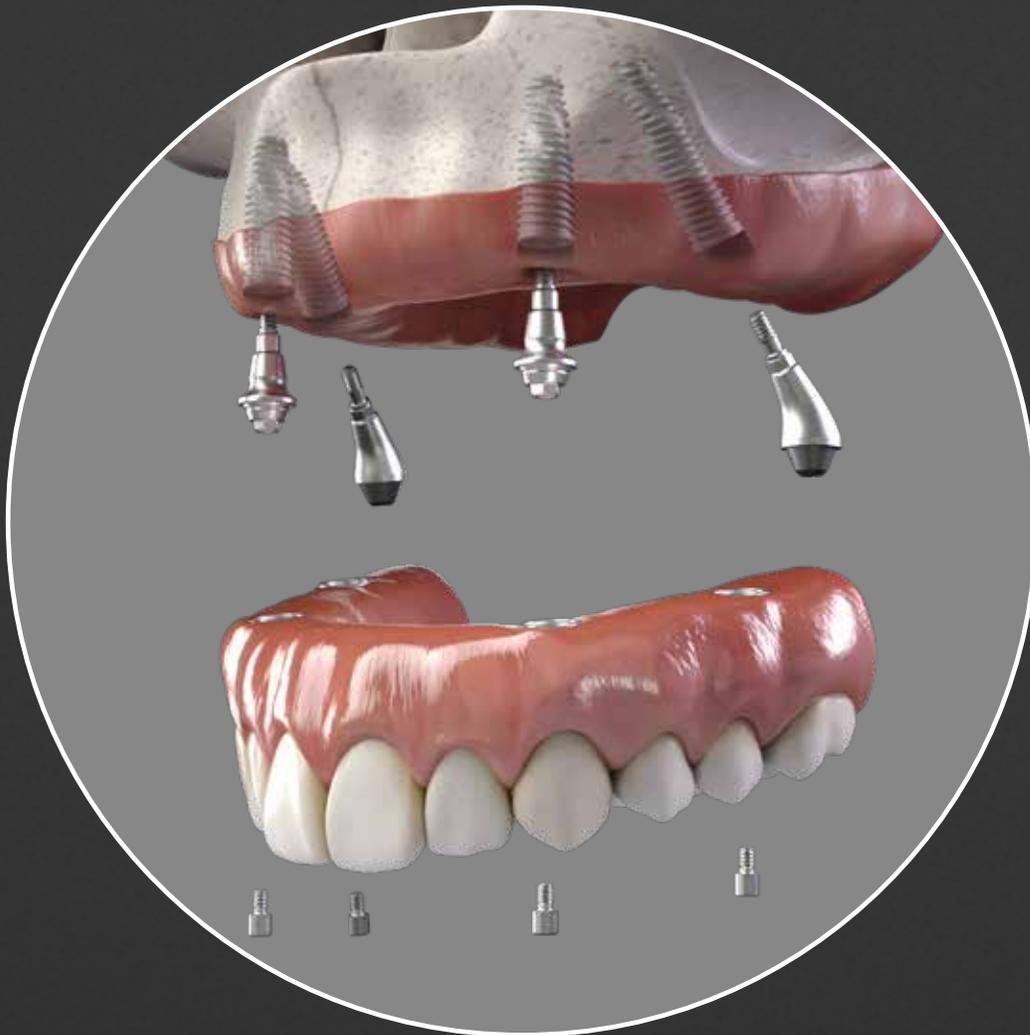



Immediate function resulting in shorter treatment times.

- Different implants techniques to minimize the use of grafting procedure⁽¹¹⁾.
- Optimized implant design to achieve high primary stability in all bone types⁽¹²⁾.



Immediate natural-looking esthetics with versatile restorative options.

- A broad gingival height abutment range to cater the patient's needs.
- Options of straight and angled abutments (17°, 30°, 45° and 60°).



Immediate peace of mind thanks to a stable foundation.

- One connection regardless of the diameters.
- Unique connection combining Platform Switching associated with a deep 16° Morse taper including an internal indexation.

SOLUTIONS FOR ALL CLINICAL NEEDS

An implant system designed for predictable immediate treatments in all bone types even with different conditions of the residual alveolar bone.



Helix GM™



Helix GM™ Long



Zygoma GM™



BONE RESORPTION

Helix GM™ Long

PRODUCT FEATURES:

Implants Description:

- Full dual tapered implant;
- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- Active apex including a soft rounded small tip and helicoidal flutes;
- Dynamic progressive thread design: from compressing trapezoidal threads on the coronal area to self-tapping threads on the apical part;
- Double lead threaded implant;
- Holder integrated to the implant body, which adapt in the packaging;
- Neoporos surface;
- Grand Morse™ connection.

Indications:

- Indicated for surgical intraoral installation, in bone types III/IV for cases of total or partial edentulism and for multiple-unit prostheses.

Drilling features:

- For infraosseous positioning it is recommended to add 1 to 2 mm in length to the implant during surgical instrumentation.
- Drilling speed: 500-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 Ncm.

Available with:

NeoPoros®



Drill Sequence



	Initial	Ø2.35	Ø3.75	Ø4.0
	103.453	103.462	103.463	103.464
Ø3.75 mm	Optional	✓	✓	
Ø4.0 mm	Optional	✓	✓	✓

Bone types III and IV 

The procedure can be with Guided Surgery. Check the instruments for more information.

Helix GM™ Long implants

	20.0 mm	22.5 mm	25.0 mm
Ø3.75			
NeoPoros	109.1043	109.1044	109.1045
Ø4.0			
NeoPoros	109.1046	109.1047	109.1048

GM Healing Abutment



Profile	0.8 mm	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm
Ø3.3	106.207	106.208	106.209	106.210	106.211	106.212
Ø4.5	106.213	106.214	106.215	106.216	106.217	106.218
Ø5.5		106.250	106.251	106.252	106.253	
Ø6.5		106.254	106.255	106.256	106.257	

:: Use the manual Neo Screwdriver (104.060);
:: Do not exceed the insertion torque of 10 Ncm.

GM Customizable Healing Abutments



Profile	1.5 mm	2.5 mm	3.5 mm	4.5 mm	5.5 mm	6.5 mm
Ø5.5	106.223	106.224	106.225	106.226	106.227	
Ø7.0		106.228	106.229	106.230	106.231	106.232

GM Cover Screw



	0 mm	2 mm
	117.021	117.022

:: Use the manual Neo Screwdriver (104.060);
:: Do not exceed the insertion torque of 10 Ncm.

Zygoma GM™

PRODUCT FEATURES:

Implants Description:

- Hybrid contour with a cylindrical coronal part and conical on the apical area;
- The apex has a conical profile with a spherical tip and three equally spaced helical flutes;
- Trapezoidal thread and progressive increase of the thread depth at the apical portion;
- Tissue Protect: portion without threads, near the cervical region, indexed to the hexagon face;
- Holder integrated to the implant body, which adapt in the packaging;
- Neoporos surface;
- Grand Morse™ connection.

Indications:

- Indicated for surgical procedures in the the posterior region of the maxilla and in the zygoma, in cases of severe maxilla resorption. Zygomatic Implants may be used in immediate loading procedures when there is good primary stability and appropriate occlusal loading.

Drilling features:

- Drilling speed: 800-1200 rpm;
- Lateral Direction Drill speed: 600-800 rpm;
- Implant insertion speed: 30 rpm;
- Maximum torque for implant placement: 60 Ncm.

Available with:

NeoPoros®




Drill Sequence



The procedure can start guided. Check the instruments for more information.

Zygoma GM™ Implants

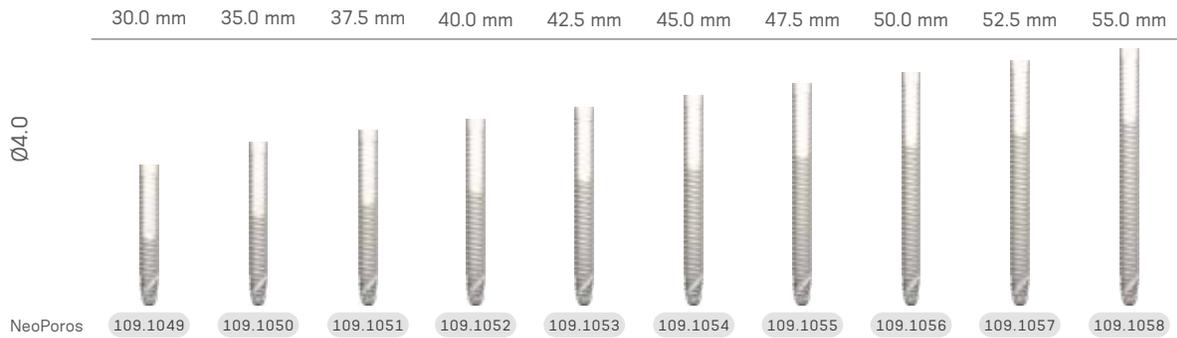

GM Cover Screw



0 mm 2 mm
117.021 117.022

:: Use the manual Neo Screwdriver (104.060);
:: Do not exceed the insertion torque of 10 Ncm.

GM™ Mini Conical Abutment

Consider in addition 1.5 - 2.0 mm for the restorative material;

Minimum interocclusal space of 4.5 mm from the mucosa level for straight abutments;



Multiple-unit screw-retained prosthesis



Ø4.8 mm

Exact;
Neo Removable Screw.



Installation Sequence

 1 32 Ncm GM Mini Conical Abutment 0.8 mm 1.5 mm 2.5 mm 115.243 115.244 115.245 3.5 mm 4.5 mm 5.5 mm 115.246 115.247 115.248	or	 2 20 Ncm GM Exact Mini Conical Abutment 17°/30°/45°/60° 1.5 mm 2.5 mm 3.5 mm 17° 115.275 115.276 115.277 30° 115.278 115.279 115.280 45° 115.281 115.282 60° 115.285 115.286
--	----	---

*The 45° Mini Conical Abutment is indicated for use only with Helix GM® Long and Zygoma GM™.

*The 60° Mini Conical Abutment is indicated for use only with Zygoma GM™.

Intraoral

Mini Conical Abutment Scanbody
3
108.218

↓

Mini Conical Abutment Hybrid Repositionable Analog
101.092

↓

Neo Mini Conical Abutment One Step Hybrid Coping
2
10 Ncm
118.382

Model Scanning

Slim Mini Conical Abutment Open Tray Impression Coping
3
108.176

↓

Mini Conical Abutment Hybrid Repositionable Analog
101.092

↓

Mini Conical Abutment Scanbody
3
108.218

↓

Neo Mini Conical Abutment One Step Hybrid Coping
2
10 Ncm
118.382

Conventional

Slim Mini Conical Abutment Open Tray Impression Coping
3
108.176

or

Neo Mini Conical Abutment Titanium Coping
2
10 Ncm
118.302

or

Neo Mini Conical Abutment Protection Cylinder
3
106.268

↓

Mini Conical Abutment Analog
101.092 Hybrid Repositionable (conventional/digital)
101.020 Conventional

or

Neo Mini Conical Abutment CoCr Coping
2
10 Ncm
118.303

or

Neo Mini Conical Abutment Burn-out Coping
2
10 Ncm
118.301

64

Drivers

1	 Hexagonal Prosthetic Driver	+	 Torque Wrench
2	 Neo Screwdriver Torque Connection	+	 Torque Wrench
3	 Neo Screwdriver Torque Connection	+	 Manual Screwdriver Torque

Accessories

 Replacement Abutment Screw 116.291 Neo GM Screw - for abutments with 1.5-2.5 GH 116.292 Neo GM Screw (Long) - for abutments with 3.5-5.5 GH	 Mini Conical Abutment Polishing Protector 123.008	 Replacement Coping Screw 116.269 Titanium
---	--	--

Measurements GM™ Mini Conical Abutment

17°



30°



45°*



*The 45° Mini Conical Abutment is indicated for use only with Helix GM® Long and Zygoma GM™.

60°**



**The 60° Mini Conical Abutment is indicated for use only with Zygoma GM™.

NeoArch[®] Kits

Helix GM™ Long Compact Surgical Kit

Autoclavable polymer case.



Articles

- | | | |
|---|---|--|
| 110.300 Helix GM™ Long Compact Surgical Kit Case | 103.453 Helix GM™ Long Initial Drill 2.0mm | 105.143 Regular Guided Surgery GM Connection for Torque Wrench |
| 103.395 Guided Surgery Drill 1.3mm | 103.462 Twist Drill For Helix GM™ Long 2.35mm | 105.140 Regular Guided Surgery GM Connection - Contra-angle |
| 125.100 Guided Surgery Guide Clamp | 103.463 Twist Drill For Helix GM™ Long 3.75mm | 104.060 Neo Manual Screwdriver (medium) |
| 125.140 Drill Guide For NGS Helix GM™ Long 2.0/2.35mm | 103.464 Twist Drill For Helix GM™ Long 4.0mm | 105.129 GM Implant Driver - Torque Wrench (short) |
| 125.141 Drill Guide For NGS Helix GM™ Long 3.75/4.0mm | 129.021 Helix GM™ Long X-ray Positioner | 105.131 GM Implant Driver - Contra-angle |
| 103.459 Twist Drill For NGS Helix GM™ Long 2.35mm | 128.032 GM Angle Measurer 17° | 104.050 Torque Wrench |
| 103.460 Twist Drill For NGS Helix GM™ Long 3.75mm | 128.033 GM Angle Measurer 30° | |
| 103.461 Twist Drill For NGS Helix GM™ Long 4.0mm | 128.034 GM Angle Measurer 45° | |

Note: Items that compose Neodent® Kits are sold separately.

Zygoma GM™ Surgical Kit

Autoclavable polymer case.



Articles

- | | | |
|---|--|---|
| 110.299 Zygoma GM™ Surgical Kit Case | 103.457 Twist Drill For Zygoma GM™ 4.0mm | 128.033 GM Angle Measurer 30° |
| 103.395 Guided Surgery Drill 1.3mm | 103.458 Lateral Direction Drill For Zygoma GM™ 4.0mm | 128.034 GM Angle Measurer 45° |
| 125.100 Guided Surgery Guide Clamp | 103.465 Pilot Twist Drill For Zygoma GM™ 2.3/3.2mm | 128.028 GM Height Measurer |
| 125.139 Drill Guide For Ngs Zygoma GM™ 2.35mm | 104.063 Zygoma GM™ Installation Driver | 104.060 Neo Manual Screwdriver (medium) |
| 103.454 Twist Drill For Ngs Zygoma GM™ 2.35mm | 129.022 Zygoma GM™ Probe 2.35mm | 105.129 GM Implant Driver - Torque Wrench (short) |
| 103.455 Twist Drill For Zygoma GM™ 2.35mm | 129.023 Zygoma GM™ Probe 4.0mm | 105.131 GM Implant Driver - Contra-angle |
| 103.456 Twist Drill For Zygoma GM™ 3.75mm | 128.032 GM Angle Measurer 17° | 104.050 Torque Wrench |

Note: Items that compose Neodent® Kits are sold separately.

NeoArch[®] Instruments



Helix GM™ Long Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM™ Long implants.

Initial	Ø2.35	Ø3.75	Ø4.0
103.453	103.462	103.463	103.464



Helix GM™ Long Drills for Guided Surgery

- :: Available in surgical steel;
- :: Drill sequence for Helix GM™ Long implants on Guided Surgery.

Ø2.35	Ø3.75	Ø4.0
103.459	103.460	103.461



Zygoma GM™ Drills

- :: Available in surgical steel;
- :: Drill sequence for Zygoma GM™ implants.

	Pilot		
Ø2.35	Ø2.3/3.2	Ø3.75	Ø4.0
103.455	103.465	103.466	103.457



Zygoma GM™ Lateral Direction Drill

- :: Available in surgical steel;
- :: Spherical tip with guide pin and helical blades for preparing the site for the implant placement in the exteriorized technique.

Ø4.0
103.458



Zygoma GM™ Drill for Guided Surgery

- :: Available in surgical steel;
- :: After using the first drill, the surgical guide must be removed and the conventional protocol must be started.

Ø2.35
103.454



GM Height Measurer

- :: Available in titanium;
- :: For selecting GM prosthetic abutments;
- :: Marks corresponding to transmucosa heights.
- :: Can be used as X-Ray Positioner.

128.028

GM Implant Driver - Contra-Angle



- :: To capture the implant directly from the packaging;
- :: To place GM Implants with contra-angle, or attached to a manual driver for contra-angle connections (104.028) for hand placement;
- :: With six dimples to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque 35 Ncm.

105.131

GM Implant Driver - Torque Wrench



- :: To place GM Implants with the Torque Wrench (104.050);
- :: With six marks to indicate the hex index face position;
- :: The laser marks indicate the depth of implant placement, bone level, 1 and 2mm infra-bone and last marking (3mm) biological space;
- :: Maximum torque: 60 Ncm.

Short	Long
22 mm	30 mm
105.129	105.130

Neo Screwdriver Torque Connection - Torque Wrench



- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
16.5 mm	22 mm	32 mm
105.133	105.132	105.157



Neo Manual Screwdriver

- :: Available in surgical steel;
- :: Yellow color for line identification.

Short	Medium	Long
21 mm	25 mm	37 mm
104.058	104.060	104.072

Neo Screwdriver Torque Connection - Contra-angle



- :: Available in surgical steel;
- :: Yellow color for line identification;
- :: Medium Neo Screwdriver Torque Connection
- :: Extra Short Neo Screwdriver Torque Connection - Contra-angle (105.146) recommended for Impression Copings, Cover Screws and Healing Abutments.

Extra Short	Short	Long
16.5 mm	24 mm	31 mm
105.146	105.135	105.160



Hexagonal Prosthetic Driver

- :: Available in surgical steel;
- :: To install and apply torque over straight GM Mini Conical Abutments and GM Micro Abutments;
- :: Yellow color for line identification.

Contra-angle Torque Wrench
 105.138 105.137



GM Bone Profile Drill with Guide

- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.

103.424



GM Angle Measurer

- :: Available in titanium;
- :: Angles: 17°, 30° and 45°;
- :: To a more accurate selection and planning of the abutments angulation during the prosthetic phase.

17° 30° 45° 60°
 128.032 128.033 128.034 128.035

72



Helix GM™ Long Drill Guide for Guided Surgery

- :: Instrument with the purpose of guiding the drills during the bone bed preparation according to the guided surgery technique.

Ø2.0/2.35 Ø3.75/4.0
 125.140 125.141



Zygoma GM™ Drill Guide for Guided Surgery

- :: Instrument with the purpose of starting the Zygomatic Surgery guided.

Ø2.35
 125.139



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in surgical steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø1.3 Guide Clamp
 103.395 125.100



Guided Surgery GM Connection - Contra-Angle

- :: Available in stainless steel;
- :: To start the implant placement through the surgical guide.

Regular
 105.140



Guided Surgery GM Connection - Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide.

Regular
 105.143



Helix GM™ Long X-ray Positioner

- :: Indicated for evaluation of the osteotomy depth in the implant placement procedure.

129.021



Zygoma GM™ Probes

- :: Available in Stainless Steel;
- :: The probe for the drill Ø2.35 mm has a tip design in L;
- :: The probe for the drill Ø4.0 mm has a tip with a design similar to the apex of the drill that allows identifying the correct drilling depth for implant anchorage.

Ø2.35 Ø4.0
 129.022 129.023



Zygoma GM™ Installation Driver

- :: Instrument for application of manual torque.

104.063



Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning;
- :: For full instructions see page 80.

104.050



Remover for Abutments with internal threads

- :: Available in surgical steel;
- :: To remove abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws

130.118 Long
130.114



Remover for Neo Screws

- :: Available in surgical steel;
- :: Compatible with Neo removable screws for abutments

130.119 Long
130.115

Removal Sets for Abutments with internal threads and Neo Screws

- :: Available in surgical steel;
- :: To remove Neo Removable Screws and abutments with internal threads from the implants, after removal of the screws;
- :: Compatible with abutments with Neo removable Screws



130.117

Long
130.116

GRAND MORSE™ NEODENT® GUIDED SURGERY.

GRAND POSSIBILITIES WITH A LIMITLESS SOLUTION

Patients' expectations regarding tooth replacement are increasing and are even higher when it comes to treatment duration and esthetic outcomes. The Neodent® Guided Surgery helps clinicians to provide prosthetically driven treatments, enabling them to perform immediate protocols with peace of mind, fulfilling patients' expectations.



DIFFERENTIATE YOUR PRACTICE WITH GUIDED SURGERY.



Improve patient quality of life.

- Functional with an immediate fixed restoration.
- Esthetical with a personalized restoration and less bone remodeling ⁽¹³⁾.
- Comfort by the reduction of operative and postoperative discomfort (e.g. reduced patient chair time).



Access to more treatment options.

- Reliable access to flapless surgery ⁽¹⁴⁻¹⁶⁾.
- Designed to reduce bone grafting procedures.
- Predictable immediate protocols.



Increase patient acceptance.

- Better communication building trust with patients.
- Reliable treatment estimates from root to tooth including components and procedures.

SURGICAL PREDICTABILITY AND EFFICIENCY WITH A LIMITLESS SOLUTION.

Guided surgery is designed to reduce chair time and postoperative discomfort. It helps increasing implant positioning accuracy ⁽¹⁷⁾.



Complete
Helix® and Drive GM™
Implants portfolio




Convenient
Color-coded instruments
and symbol-marked



Flexible
2 sleeve height positions




Guided implant
insertion



Guided bed
preparation

Neodent® Guided Surgery Kit for Grand Morse™

Compatible with major guided
surgery software

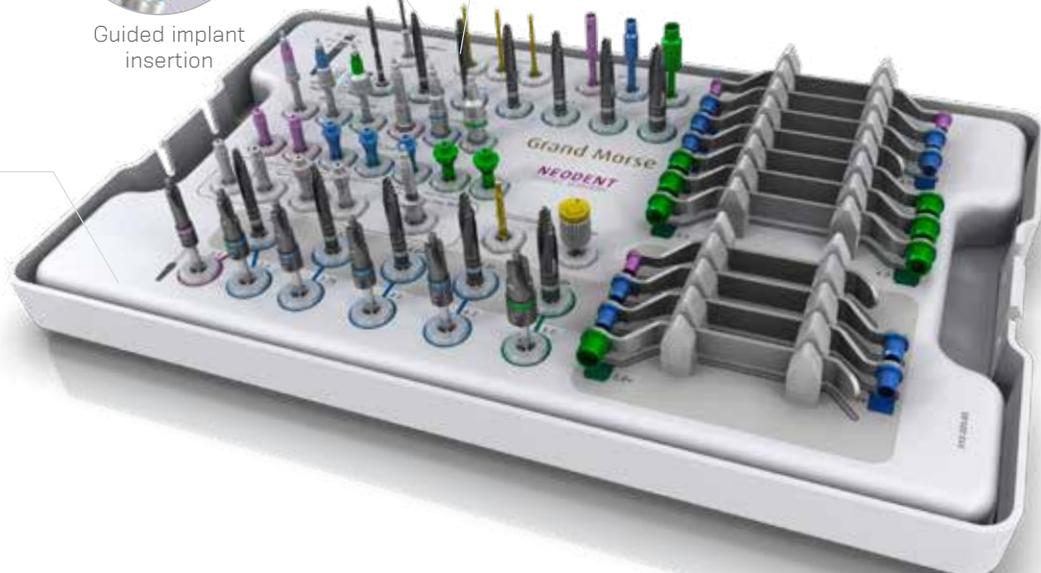

Neodent[®] Guided Surgery **Kit**

Grand Morse™ Guided Surgery Surgical Kit

Autoclavable polymer case.
The Kit allows the use of Helix GM™ and Drive GM™ Implants in the Guided Surgery technique.



Articles

- 110.296 GM Guided Surgery Surgical Kit Case
- 103.395 Guided Surgery 1.3
- 125.100 Guided Surgery Guide Clamp
- 103.429 Narrow Guided Surgery Punch - Contra-Angle
- 103.430 Regular Guided Surgery Punch - Contra-Angle
- 103.431 Wide Guided Surgery Punch - Contra-Angle
- 103.432 Guided Surgery Drill 2.0
- 103.433 Tapered Guided Surgery Drill 3.5*
- 103.434 Tapered Guided Surgery Drill 3.75*
- 103.435 Tapered Guided Surgery Drill 4.0*
- 103.436 Tapered Guided Surgery Drill 4.3*
- 103.437 Tapered Guided Surgery Drill 5.0*
- 103.438 Tapered Guided Surgery Drill 6.0*
- 105.139 Narrow Guided Surgery GM Connection - Contra-angle
- 105.140 Regular Guided Surgery GM Connection - Contra-angle
- 105.141 Wide Guided Surgery GM Connection - Contra-angle
- 105.142 Narrow Guided Surgery GM Connection for Torque Wrench
- 105.143 Regular Guided Surgery GM Connection for Torque Wrench
- 105.144 Wide Guided Surgery GM Connection for Torque Wrench
- 125.130 Narrow Guided Surgery GM Guide Stabilizer
- 125.131 Regular Guided Surgery GM Guide Stabilizer
- 125.132 Wide Guided Surgery GM Guide Stabilizer
- 125.133 Narrow Guided Surgery GM Guide Stabilizer (Long)
- 125.134 Regular Guided Surgery GM Guide Stabilizer (Long)
- 105.145 Guided Surgery GM H11 Connection for Torque Wrench
- 105.136 Neo Screwdriver Torque Connection - Contra-angle (Medium)
- 104.060 Neo Manual Screwdriver (Medium)
- 103.439 Tapered Contour Guided Surgery Drill 3.5*
- 103.440 Tapered Contour Guided Surgery Drill 3.75*
- 103.441 Tapered Contour Guided Surgery Drill 4.0*
- 103.442 Tapered Contour Guided Surgery Drill 4.3*
- 103.443 Tapered Contour Guided Surgery Drill 5.0*
- 103.444 Narrow Guided Surgery GM Pilot Drill 3.5
- 103.445 Regular Guided Surgery GM Pilot Drill 3.5
- 103.446 Guided Surgery GM Pilot Drill 3.75
- 103.447 Guided Surgery GM Pilot Drill 4.0
- 103.448 Guided Surgery GM Pilot Drill 4.3
- 103.449 Guided Surgery GM Pilot Drill 5.0
- 125.119 Narrow Guided Surgery Drill Guide 2.0/3.5
- 125.121 Regular Guided Surgery Drill Guide 2.0/3.5
- 125.122 Regular Guided Surgery Drill Guide 3.75/4.0
- 125.123 Regular Guided Surgery Drill Guide 4.3
- 125.126 Wide Guided Surgery Drill Guide 2.0/3.5
- 125.127 Wide Guided Surgery Drill Guide 4.0/4.3
- 125.128 Wide Guided Surgery Drill Guide 5.0/6.0
- 125.120 Narrow Tapered Contour Guided Surgery Drill Guide 3.5
- 125.124 Regular Tapered Contour Guided Surgery Drill Guide 3.5/3.75
- 125.125 Regular Tapered Contour Guided Surgery Drill Guide 4.0/4.3
- 125.129 Wide Tapered Contour Guided Surgery Drill Guide 5.0
- 129.001 Titanium Tweezers
- 104.050 Torque Wrench

Note: Items that compose Neodent® Kits are sold separately.

*Conventional guided surgery drills that can be replaced by the respective short version.

Neodent[®]
Guided Surgery
Instruments



Guided Surgery Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM™ and Drive GM™ Implants in the guided surgery technique;
- :: Fully guided technique with Short Drills indicated for 8, 10 or 11.5 mm long implants.

	Ø2.0	Ø3.5	Ø3.75	Ø4.0	Ø4.3	Ø5.0	Ø6.0
Short 36.5 mm	103.475	103.476	103.477	103.478	103.479	103.480	103.481
Regular 41 mm	103.432	103.433	103.434	103.435	103.436	103.437	103.438



Guided Surgery Drill 1.3 and Guide Clamp

- :: Drill available in surgical steel;
- :: Guide Clamp available in titanium;
- :: For initial fixation of the surgical guide.

Drill Ø1.3	Guide Clamp
103.395	125.100



Guided Surgery Tapered Contour Drills

- :: Available in surgical steel;
- :: Drill sequence for Helix GM™ Implants in the guided surgery technique for bone types I or II;
- :: Fully guided technique with Short Drills indicated for 8, 10 or 11.5 mm long implants.

	Ø3.5+	Ø3.75+	Ø4.0+	Ø4.3+	Ø5.0+
Short 36.5 mm	103.482	103.483	103.484	103.485	103.486
Regular 41 mm	103.439	103.440	103.441	103.442	103.443



Guided Surgery Punch - Contra-Angle

- :: Available in titanium;
- :: Color-coded according to the sleeve diameter;
- :: To remove the mucosa before beginning the osteotomy.

Narrow	Regular	Wide
103.429	103.430	103.431



Guided Surgery GM Pilot Drills

- :: Available in surgical steel;
- :: Color-coded according to the sleeve diameter;
- :: Recommended for Helix GM™ in bone types I or II;
- :: Optional Drive GM™ in bone types III or IV.

	Narrow	Regular	Wide
Ø3.5	103.444	Ø3.5 103.445	Ø5.0 103.449
		Ø3.75 103.446	
		Ø4.0 103.447	
		Ø4.3 103.448	



Guided Surgery Drill Guides

- :: Available in titanium and stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To fit in the sleeve in the surgical guide;
- :: To be used with correspondent drill diameter and type.

	Narrow	Regular	Wide
Ø2.0/3.5	125.119	Ø2.0/3.5 125.121	Ø2.0/3.5 125.126
Ø3.5+	125.120	Ø3.75/4.0 125.122	Ø4.0/4.3 125.127
		Ø4.3 125.123	Ø5.0/6.0 125.128
		Ø3.5+/3.75+ 125.124	Ø5.0+ 125.129
		Ø4.0+/4.3+ 125.125	



Guided Surgery GM™ Connection - Contra-Angle

- :: Available in stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To start the implant placement through the surgical guide.

Narrow	Regular	Wide
105.139	105.140	105.141



Guided Surgery Guide Stabilizers

- :: Available in titanium;
- :: Color-coded according to the sleeve diameter;
- :: Additional fixation of the surgical guide.

Narrow	Regular	Wide
125.130	125.131	125.132



Guided Surgery GM Connection - Torque Wrench

- :: Available in stainless steel;
- :: Color-coded according to the sleeve diameter;
- :: To finish the implant placement through the surgical guide.

Narrow	Regular	Wide
105.142	105.143	105.144



Guided Surgery Guide Stabilizers - Long

- :: Available in titanium;
- :: Additional fixation of the surgical guide;
- :: To be used when the H11 sleeve height is chosen.

Narrow	Regular
125.133	125.134



Guided Surgery GM H 11 Connection - Torque Wrench

- :: Available in stainless steel;
- :: To finish the implant placement through the surgical guide;
- :: To be used when the H11 sleeve height is chosen.

105.145

Sleeves for Neodent® Guided Surgery System

- :: Available in titanium;
- :: Sold in bags with 10 units each.



125.135	Sleeve for Narrow Guided Surgery System
125.136	Sleeve for Regular Guided Surgery System
125.137	Sleeve for Wide Guided Surgery System
125.138	Sleeve of Setter for Guided Surgery System



Ceramic Implant System

Increasing expectations for esthetic treatments, the Neodent® Ceramic Implant System combines the notions of flexibility, stability, and esthetics. The two-piece system with a Zi Ceramic implant and Zi Ceramic abutment solution retained with a titanium alloy screw, allows an immediate loading protocol when good primary stability is achieved along with physiological occlusal loading, thanks to the modern naturally tapered Ceramic implant design. The system features a comprehensive ceramic prosthetic portfolio to maximize stability and predictability in immediate treatments.

A new **mindset**

- A new flexibility mindset
- A new stability mindset
- A new esthetic mindset





A new flexibility mindset

Looking to treat several demanding treatments, the Zi Ceramic Implant System delivers the flexibility of a 2-piece connection combined with a strong screw-retained ceramic implant and ceramic abutment connection.



RELIABLE AND STRONG CERAMIC SYSTEM

The unique patent pending ZiLock™ connection is designed with a longer screw which provides a secure engagement between the ceramic implant and the ceramic abutment. Additionally, it improves the zirconia performance by optimizing the force distribution along the internal connection.



FRIENDLY ZILOCK™ CONNECTION

ZiLock™ is a ceramic straight internal connection with 6 lobes and 6 points. This indexation is designed for precise abutment positioning and protection against rotation. The outcome is a user-friendly system that provides higher treatment flexibility when compared to one-piece implants.




A new **stability mindset**

Aiming to achieve stable immediate protocols, Zi combines a naturally tapered implant design and implant treated surface. Both designed to maximize stability and predictability in immediate treatments.

TAPERED DESIGN FOR PRIMARY STABILITY

The Zi Ceramic Implant System exhibits a modern tapered implant geometry designed for predictable immediacy in all bone types. This feature was designed to mimic the tapered shape of a natural tooth root, driving to achieve high primary stability.

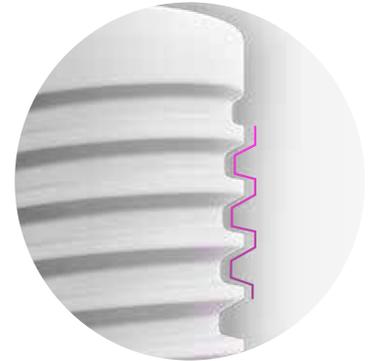

Double trapezoidal thread design.



Apically tapered with chamber flutes.

PREDICTABILITY WITH SAND-BLASTED AND ACID-ETCHED SURFACE

Zi features the sand-blasted and acid-etched surface treatment, presenting macro and micro roughness based on the highly successful Neoporos® treatment surface.





A new **esthetic mindset**

Zi offers a comprehensive portfolio to achieve an outstanding esthetic performance with a natural esthetic result using the ceramic material.

OUTSTANDING ESTHETIC PERFORMANCE

The Neodent Zi Ceramic Implant System seeks to offer outstanding natural-looking performance and outcome, featuring a ceramic material which supports the reconstruction due to its color that mimics natural teeth and benefits from a high translucency compared to metals for amazing esthetic results.

A PORTFOLIO TO ACHIEVE NATURAL ESTHETIC RESULTS

The Ceramic prosthetic portfolio allows for immediate protocol. In addition, preferable workflow can be applied, providing a natural-looking restoration.



ZI BASE

-  Single-unit screw-retained prosthesis
-  Single-unit cement-retained prosthesis
-  Ø3.75/4.5 mm

ZI CR ABUTMENT

-  Single-unit cement-retained prosthesis
-  Ø4.0/4.5 mm

Neodent Zi Implant Packaging

Neodent® packaging has been specially updated for easy handling and seeking to achieve a surgical procedure, providing practicality from implant stocking to the capture and transport and implant bed. The implant's features, such as type, diameter and length, are readily identifiable on the outside of the packaging.

Three self-adhesive labels are provided for recording in the patient's medical records and for reporting to the prosthesis team. They also allow traceability for all articles.



Package instruction of use



1. The cardboard and blister packagings must be opened, manually, without the use of sterile gloves. Break the seal of the cardboard packaging and remove the blister. Open the blister pack. Deposit the sterile flask over the surgical field.

NOTE: The clear tube and implant must be handled with a sterile surgical glove, in a surgical environment. Hold the bottle using the non-dominant hand and take the lid off.



2. The internal support containing the implant and transfer piece must come out attached to the lid. To do so, remove the lid and the clear tube's internal support in the axial direction without making any lateral movements.



3. Keep the support stable and remove the lid.



4. For installation, capture the implant transfer piece with the Hexagonal Connection, keeping it stable and slightly rotating the internal support, searching for the perfect fit between connection and transfer piece.




5. Take the transfer-implant assembly to the surgical cavity.

e-IFU – Electronic Instructions For Use

Neodent® innovates once more, providing an on-line platform designed to provide quick and practical use of its own products instructions: the e-IFU (Instructions For Use) website.

To facilitate access, have the article number, which can be found on the external packaging of the product, in this catalogue or with your local distributor. Once the article number is entered in the website, the professional will have access to relevant information to this product, such as description, indication for use, contraindications, handling, traceability and other features.

Access: ifu.neodent.com.br/en

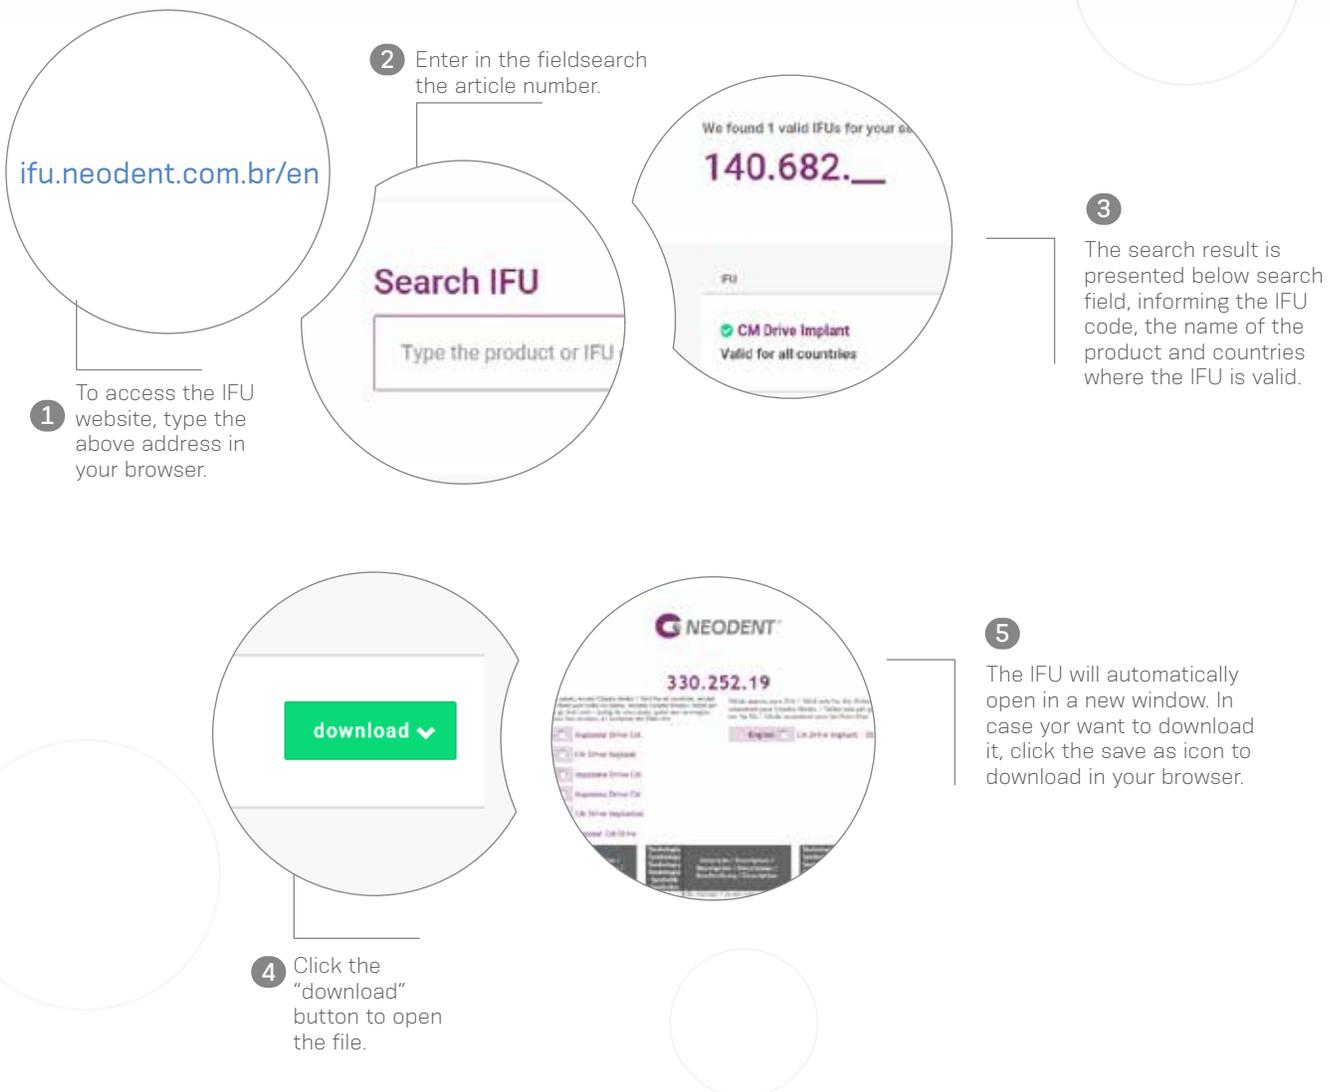

Zi Implant

PRODUCT FEATURES:

Implants Description:

- Naturally tapered design
 - Compacting trapezoidal threads
 - Double threaded implant
 - Apically tapered with chamber flutes
 - ZiLock™ connection
-

Indications:

- Indicated for all types of bone density
-

Drilling features:

- Drilling speed: 800-1200 rpm for bone types I and II
 - Drilling speed: 500-800 rpm for bone types III and IV.
 - Countersink is required if used in bone types I, II and III with 300rpm.
 - Bone tap is required if used in bone types I and II: contra angle: 30rpm/35 Ncm and torque wrench: maximum torque of 60Ncm
 - Maximum insertion torque: 60 Ncm
 - Maximum torque value for immediate loading: 35Ncm
-

Surface:

- Zi features the sand-blasted and acid-etched surface treatment, presenting macro and micro roughness based on the highly successful Neoporos® treatment surface.



Drill Sequence



Ø3.75 mm	✓*	✓	✓	✓	✓	✓			
Ø4.3 mm	✓*	✓	✓				✓	✓	✓

*Optional / Bone types I and II 


Ø3.75 mm	✓*	✓	✓	✓	✓				
Ø4.3 mm	✓*	✓	✓				✓	✓	

*Optional / Bone type III 

Ø3.75 mm	✓*	✓	✓	✓					
Ø4.3 mm	✓*	✓	✓				✓		

*Optional / Bone type IV 

Zi Implants

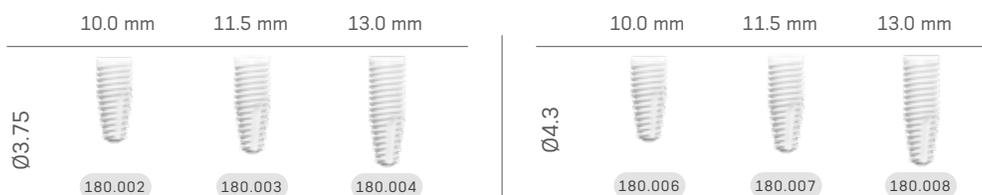

Zi Healing Abutments



Profile	1.5 mm	2.5 mm
Ø3.75	106.233	106.234
Ø4.5	106.235	106.236

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 Ncm.

Zi Cover Screw



117.023

:: Use the manual Neo Screwdriver (104.060);
 :: Do not exceed the insertion torque of 10 Ncm.

Peek CR Abutment



Single-unit
cement-retained
temporary
prosthesis



Ø4.0/4.5 mm

- Neo screwdriver connection;
- Cementable area height: 5.0 mm;
- Gingival height: 1.5 & 2.5 mm;
- ZiLock™ connection;
- Removable screw.



Installation Sequence

	1.5 mm	2.5 mm	Peek CR Abutment	
Ø4.0	114.888	114.889		
Ø4.5	114.886	114.887		

↓

	Impression Coping CR Abutment
Ø4.0	108.201
Ø4.5	108.202

↓

	Provisional Coping CR Abutment
Ø4.0	108.201
Ø4.5	108.202

↓

	Zi CR Abutment Analog
Ø4.0	101.105
Ø4.5	101.106

Hybrid use: can be used as an impression coping and a provisional abutment.

90

Drivers

① + Torque Wrench

Zi Base



Single-unit screw-retained prosthesis



Single-unit cement-retained prosthesis



- Neo screwdriver connection;
- Chimney height: 4.0 mm;
- Gingiva height: 1.5 & 2.5 mm;
- ZiLock™ connection;
- Removable screw.





Installation Sequence

Intraoral scanning



Model Scanning

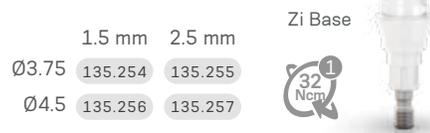

Drivers



Zi CR Abutment

Single-unit cement-retained prosthesis

Ø4.0/4.5 mm

- Neo screwdriver connection;
- Chimney height: 5.0 mm;
- Gingiva height: 1.5 & 2.5 mm;
- ZiLock™ Connection;
- Removable screw.



Installation Sequence

	1.5 mm	2.5 mm			1.5 mm	2.5 mm			
Ø4.0	114.854	114.855	 Zi CR Abutment Straight		Ø4.0	114.858	114.859	 Zi CR Abutment Angulated 17°	
Ø4.5	114.856	114.857		Ø4.5	114.860	114.861			

↓
Intraoral

		Zi CR Abutment Scanbody
Ø4.0	108.199	
Ø4.5	108.200	

↓

		Zi CR Abutment Analog
Ø4.0	101.105	
Ø5.0	101.106	

↓
Milled Crown

Drivers

Neo Screwdriver Torque Connection
 +

 Torque Wrench

Zi Implant System Kit

Zi Compact Surgical Kit

Autoclavable polymer case.

The Kit allows the installation of Zi® Implants in all bone types.



Articles

- 110.293 Compact Surgical Kit Zirconia Implant
- 103.488 Countersink Drill For Zirconia Implant 3.75
- 103.450 Countersink Drill For Zirconia Implant 4.3
- 104.050 Torque Wrench Driver
- 111.046 Bone Tap For Zirconia Implant 3.75
- 111.048 Bone Tap For Zirconia Implant 4.3
- 103.170 Initial drill Ø2.0 medium
- 103.425 Tapered Drill Ø2.0
- 103.561 Tapered Drill Ø3.5
- 103.564 Tapered Drill Ø3.75
- 103.570 Tapered Drill Ø4.3

- 103.426 Drill extender
- 104.060 Neo Manual Screwdriver (medium)
- 105.001 Smart/ws Implant Driver - Torque Wrench (short)
- 105.002 Smart/ws Implant Driver - Contra-angle
- 105.018 Hex Connection - Torque Wrench (long)
- 105.132 Neo Screwdriver Torque Connection
- 128.020 Direction indicator Ø3.75
- 128.022 Direction indicator Ø4.3
- 129.020 Tapered X-ray Positioner 3.75
- 129.013 Tapered X-ray Positioner 4.3
- 103.428 Zi Bone Profile Drill With Guide

Note: Items that compose Zi Neodent® Kit are sold separately.

Zi Ceramic Implant System Instruments



Initial Drill

- :: Available in surgical steel;
- :: 2.0mm diameter.

103.170

Neo Screwdriver Torque Connection - Torque Wrench

- :: Available in surgical steel;
- :: Yellow color for line identification.



Short	Medium	Long
16.5 mm	22 mm	32 mm

105.133 105.132 105.157

Tapered Drills

- :: Available in surgical steel;
- :: Drill sequence for Zi Implants.

- 103.425 Tapered Drill Ø2.0
- 103.561 Tapered Drill Ø3.5
- 103.564 Tapered Drill Ø3.75
- 103.570 Tapered Drill Ø4.3
- 103.562 Tapered Drill (short) Ø3.5
- 103.563 Tapered Drill (long) Ø3.5
- 103.565 Tapered Drill (short) Ø3.75
- 103.566 Tapered Drill (long) Ø3.75
- 103.571 Tapered Drill (short) Ø4.3
- 103.572 Tapered Drill (Long) Ø4.3
- 103.574 Tapered Drill (short) Ø5.0
- 103.575 Tapered Drill (Long) Ø5.0



Neo Manual Screwdriver

- :: Available in surgical steel;
- :: Yellow color for line identification



Short	Medium	Long
21 mm	25 mm	37 mm

104.058 104.060 104.072

Direction Indicators

- :: Available in titanium;
- :: Instrument to guide the implant position;
- :: Diameter of central band corresponds to GM and Zi Implant diameter;
- :: Smaller side to be used after Ø2.0mm drill;
- :: Larger side to be used after the last drill before implant installation.



3.0/3.75 128.020 3.6/4.3 128.022

Countersink Drills

- :: Available in surgical steel;

- 103.488 Countersink Drill For Zirconia Implant Ø3.75
- 103.450 Countersink Drill For Zirconia Implant Ø4.3



Drill Extension

- :: Available in surgical steel;
- :: Fit the drill directly into the Drill Extension.



103.426

Bone Tap

- :: Available in surgical steel;

- 111.046 Bone Tap For Zirconia Implant Ø3.75
- 111.048 Bone Tap For Zirconia Implant Ø4.3



Zi Bone Profile Drill with Guide

- :: Available in surgical steel;
- :: Used in the surgical second step;
- :: Conforms the bone around the implant platform, preparing the emergence profile to be suitable to prosthetic components.



103.428

Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.



104.050

Tapered X-Ray Positioner

- :: Check the axis in relation to adjacent roots using numbers identification.



Ø3.75	Ø4.3
129.020	129.013

Neodent[®]
Techniques

One Step Hybrid Technique

The One Step Hybrid technique allows the passive fitting of prosthesis, without the need for weld procedure, by cementing the neo micro/mini titanium abutment coping base into the metal structure. This technique allows as well through a digital workflow, milled dental structure to be cemented on top of this titanium abutment coping. It is indicated for multi-unit screw-retained prosthesis and results in reduced laboratory work times. It can be performed over GM™ Mini Conical Abutments or GM Micro Abutments. The sequence to perform the One Step Hybrid technique is described in the following pictures:



100



Neo Mini Conical Abutments Copings One Step Hybrid Technique

:: For installation, use the Neo Torque Connection (105.132);
 :: For torque control, use Torque Wrench (104.050).

Burn-out	Brass	Titanium
118.340	118.331	118.382



Neo Micro Conical Abutments Copings One Step Hybrid Technique

:: For installation, use the Neo Torque Connection (105.132);
 :: For torque control, use Torque Wrench (104.050).

Burn-out	Brass	Titanium
118.341	118.333	118.381



Neo Working Screw One Step Hybrid

:: For laboratory use.

116.271

Demonstration Sequence



Regularize the alveolar ridge.



Surgical drilling completed, obtaining adequate distance from distal implant in relation to the mental foramen with 7 mm Space Planning Instrument.



Placement of 4 Neodent® implants, according to their indication.



Placement of corresponding Neodent® Abutments.



Placement of Impression Copings, splinted with acrylic resin.



Positioning of Multifunctional Guide to obtain intermaxillary correlation. Soft silicone is injected to take the soft tissue impression.




Removal of Multi-Functional Guide and placement of Analogs to the impression copings.



Working model with artificial gum.

Option 1 -Conventional Workflow for cast framework


Neo Mini Abutments Copings
One Step Hybrid Technique

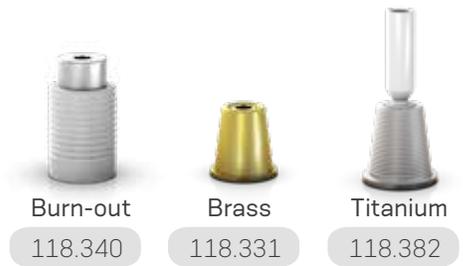

1 Working model with artificial gum.



2 Brass Copings are placed over analogs, then Burn-out Copings are fixed by working screws.

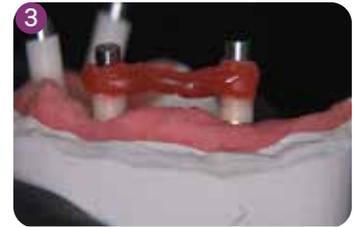


3 Wax-up the framework.



4 Cast framework. If necessary, provide internal wear in the regions corresponding to the castable copings.



5 Placement of both the Neo Mini Conical Abutment Coping Base and the sealing pin on top of the analog.

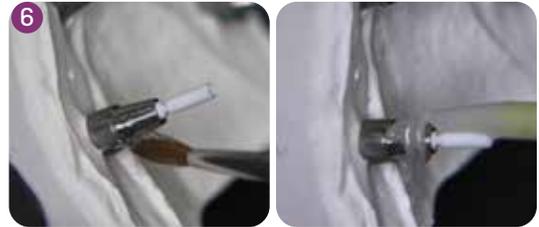

6 Apply a specific primer and proceed with the cementation according to the cement manufacturer.



7 Press the infrastructure over the coping base and immediately remove any overflowed cement excess as well as the sealing pin.



8 Unscrew the infrastructure from the model. Final framework with ensured passivity.

Option 2- Digital Workflow for milled Zirconia Bar

Neo Mini Conical Abutment Coping Base



1 Working model with artificial gum.



2 Install the GM Mini Conical Abutment Scanbody on the model and proceed with the scanning.



3 Design the zirconia bar in the CAD/CAM software.



4 Mill the zirconia bar.



5 Placement of both the Neo Mini Conical Abutment Coping Base and the sealing pin on top of the analog.



6 Apply a specific primer and proceed with the cementation according to the cement manufacturer.



7 Press the infrastructure over the coping base and immediately remove any overflown cement excess as well as the sealing pin.



8 Unscrew the infrastructure from the model. Final framework with ensured passivity.



9 Final framework.

Distal Bar Technique

Technique used to ease mandible rehabilitation, through a provisional hybrid type prostheses supported by implants.



104



Neo Distal Bar Copping

- :: Available in titanium;
- :: Retainers to ease joining with acrylic resin;
- :: Recommended torque: 10 Ncm;
- :: For torque, use Neo Screwdriver (105.132)

118.308



Neo Distal Bar

- :: Recommended for distal Implants to reinforce the cantilever.

125.116



Polishing Protector

- :: Available in surgical steel;
- :: Protection for the lab polishing.

123.008

Demonstration Sequence



1 Neodent®
Abutments
placed.




2 Prosthesis
wearing,
keeping
posterior
region
integrity.




3 Place the
copings into
the central
Implants and
Distal Bar to
distal Implants.



4 Proof of inferior
prostheses
wearing
(centered
occlusion
position, no
interference on
copings).

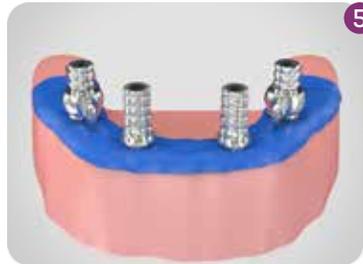

5 Placement of
rubber dam
over copings
to protect soft
tissues.

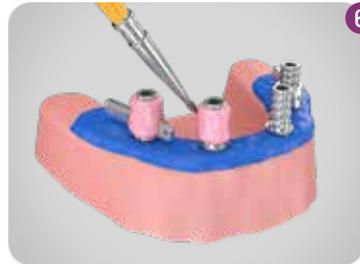

6 Apply
selfpolymerizing
acrylic resin on
and between the
copings.



7 Apply to worn area
in lower prosthesis,
repositioning
inside mouth.
Keep patient in
occlusion until total
polymerization.



8 Remove
the inferior
prosthesis
after resin is
polymerized.
Copings
already
captured.



9 Adjustments,
finishing and
polishing
procedures
of inferior
prosthesis
with polishing
protectors.



10 Placed provisional
implant supported
prosthesis.



11 Final inside-
mouth
posterior view.

Digital Solutions



Visit www.neodent.com/cadcam to download the digital files to work with Neodent® Titanium Bases, Titanium Blocks, Abutments, Mini Conical Abutments, Micro Abutments, Universal Abutments, One Step Hybrid Copings, Scanbodies and Hybrid Repositionable Analogs. Libraries are available for the following companies: exocad GmbH, Amann Girrbach AG Inc, Dental Wings Inc and 3Shape A/S.

Scanbody

Neodent® Scanbodies can be used for scanning and digitalization of the patient or model providing accuracy in determining the analog position.



- 108.207 GM Exact Implant Intraoral Scanbody
- 108.218 GM Mini Conical Abutment Scanbody (intraoral and model)
- 108.219 GM Micro Abutment (intraoral and model)
- 108.220 GM Abutment (intraoral and model)
- 108.222 Zi Implant Scanbody



Hybrid Repositionable Analog

Neodent® Hybrid Repositionable Analogs can be used in prototyped models, produced by 3D printers, or conventional plaster models.



- 101.103 GM Hybrid Repositionable Analog 3.5/3.75
- 101.089 GM Hybrid Repositionable Analog 4.0/4.3
- 101.090 GM Hybrid Repositionable Analog 5.0/6.0
- 101.091 Micro Abutment Hybrid Repositionable Analog
- 101.092 Mini Conical Abutment Hybrid Repositionable Analog
- 101.097 Universal Abutment Hybrid Repositionable Analog 3.3X4
- 101.098 Universal Abutment Hybrid Repositionable Analog 3.3X6
- 101.099 Universal Abutment Hybrid Repositionable Analog 4.5X4
- 101.100 Universal Abutment Hybrid Repositionable Analog 4.5X6
- 101.101 GM Abutment Hybrid Repositionable Analog

General Instruments

Torque Wrench

- :: Available in surgical steel;
- :: Fitting for square connections;
- :: Collapsible Wrench that allows for proper assembly cleaning.

104.050



Operational Instructions

The Neodent® Torque Wrench was designed to allow the necessary torque to be applied and simultaneous verification of that torque with the same Instrument.

All that is needed is to apply force to the wrench handle **1** (never the wrench body) until the value marked on the LATERAL SCALE **2** corresponds to the desired torque.



The wrench function works in both directions, by simply pulling and turning the driver's pin 180°. However, the torque measurements work only lockwise.

•WARNING: When inverting the torque direction, the gear may come loose from the driver body and fall. Therefore, this inversion should only be done with the driver connected to a part or outside the patient's mouth.



The Neodent® Torque Wrench comes with pre-calibrated torques

Titanium Tweezers

- :: To handle implants;
- :: New Tweezer system that prevents deviation in the active bit;
- :: Millimeter scale for checking during procedures;
- :: Self-locking implant.

129.001



Depth Probe

- :: Available in titanium;
- :: To probe preparations and analyze depth;
- :: Millimeter scale for checking during procedures.

129.004



7 and 9 mm Space Planning Instrument

- :: Available in surgical steel;
- :: Recommended for prosthetic/surgical planning.
- :: 7 and 9 mm marks.

128.026



Surgical Labial Retractor

- :: Available in surgical steel;
- :: Rounded edges to minimize surgical trauma.

124.001



Columbia Retractor

- :: Available in surgical steel;
- :: Rounded edges to minimize surgical trauma.

124.003



Scapel Handle

- :: Available in surgical steel;
- :: For standard scalpel blade use;
- :: Blade not included.

129.008



Bivers Handle

- :: Available in surgical steel;
- :: Non-traumatic extraction for implant placement;
- :: Similar to a periosteal.

129.002




Concave Osteotome



- :: Available in surgical steel;
- :: Concave active cutting bit for nontraumatic lifting the floor of the maxillary sinus;
- :: Used to prepare the surgical alveolus for Implant placement in the posterior maxillary region with low bone height;
- :: Marks from 7 to 17mm.
- :: Marks from 7 to 17mm.

1.8 mm	2.5 mm	3.0 mm	3.5 mm	4.0 mm	4.5 mm
110.154	110.155	110.156	110.157	110.158	110.159

Convex Osteotome



- :: Available in surgical steel;
- :: Convex active bit;
- :: Used when the bone width is insufficient, demanding bone compression and expansion before placing the implant;
- :: Marks from 7 to 17mm.

1.8 mm	2.5 mm	3.0 mm	3.5 mm
110.160	110.161	110.162	110.163

Osteotomes Kit Case

- :: Available in polymer;
- :: Autoclavable;
- :: Osteotomes sold separately.



110.262

Surgical Hammer




- :: Available in surgical steel;
- :: Polymer active bit;
- :: Used in compactors and expanders;
- :: Weight: 130g.

126.001

Trepine Bur



- :: Available in surgical steel;
- :: Collecting bone cylinder;
- :: Implant removal.



Ø3.3	Ø3.5	Ø3.75	Ø4.1
103.051	103.490	103.491	103.026
Ø4.3	Ø5.0	Ø8.0	
103.087	103.027	103.028	

Sinus Lift Curette

- :: Available in surgical steel;
- :: Used to displace the Sinusal Membrane.



Complement Case



- :: Available in autoclavable polymer;
- :: Used to organize drills and auxiliary connections.

110.270

Handle Implant Driver



- :: Available in stainless steel;
- :: Manual implant placement.

104.047

Analog Handle



- :: Used for tightening analogs and milling prosthetic abutments.

104.036

Prosthetic Surgical Guide



- :: Available in titanium;
- :: Abutments to prepare the surgical guide;
- :: Prosthetic guide inner diameter 2 mm
- :: Heights 6 and 10 mm;
- :: Surgical Guide: package with 10 units (5 units of 10 mm and 5 units of 6 mm);
- :: Surgical Guide Pin: package with 5 units

Guide	Pin
103.092	103.093



Neodent®
Biomaterials

Everything you need for GBR

Neodent offers a wide assortment of biomaterials including bovine bone, allograft, and collagen barriers. Created to regenerate hard tissues in a predictable and reliable way, this range of flexible solutions is designed to provide patients with the functional and aesthetic results they seek, elevating their overall experience.

► Neodent AlloGraft granules

AlloGraft Mineralized Cortical



	Granule size	Content
NAMND070206	250-710 μm	0.5 cc
NAMND070207	250-710 μm	1.0 cc
NAMND070208	250-710 μm	2.0 cc
NAMND070218	250-1000 μm	0.25 cc
NAMND070219	250-1000 μm	0.5 cc
NAMND070220	250-1000 μm	1.0 cc
NAMND070221	250-1000 μm	2.0 cc
NAMND070230	250-1000 μm	2.5 cc

AlloGraft Mineralized Cancellous



	Granule size	Content
NAMND070229	250-1000 μm	0.25 cc
NAMND070212	250-1000 μm	0.5 cc
NAMND070213	250-1000 μm	1.0 cc
NAMND070214	250-1000 μm	2.0 cc
NAMND070231	250-1000 μm	2.5 cc

AlloGraft Mineralized Cortical Cancellous Mix



	Granule size	Content
NAMND070226	250-1000 μm	0.5 cc
NAMND070227	250-1000 μm	1.0 cc
NAMND070228	250-1000 μm	2.0 cc
NAMND070232	250-1000 μm	2.5 cc

► Neodent Membrane Flex™



	Description
NAMND070.008	15 x 20 mm Neodent® Membrane Flex™
NAMND070.009	20 x 30 mm Neodent® Membrane Flex™
NAMND070.010	30 x 40 mm Neodent® Membrane Flex™

eShop

At Neodent® we understand that time is money, and being efficient in every activity is important to your business.

We are committed to helping you achieve this goal by providing a secure online portal with our eShop.

The **Neodent eShop** goes beyond convenient online product shopping. It is a complete online service that helps you:

- Manage your account
- Track order history
- View order status
- Return product
- Pay invoices online
- Review payment history



Discover how you can save time and money today by visiting neodent.us/eShop



References

- [1] Novellino MM, Sesma N, Zanardi PR, Laganá DC. Resonance frequency analysis of dental implants placed at the posterior maxilla varying the surface treatment only: A randomized clinical trial. *Clin Implant Dent Relat Res*. 2017 Jun 20. doi: 10.1111/cid.12510. [Epub ahead of print]
- [2] Sartoretto SC, Alves AT, Resende RF, et al. Early osseointegration driven by the surface chemistry and wettability of dental implants. *J Appl Oral Sci*. 2015 May-Jun;23(3):279-87.
- [3] Sartoretto SC, Alves AT, Zarranz L, et al. Hydrophilic surface of Ti6Al4V-ELI alloy improves the early bone apposition of sheep tibia. *Clin Oral Implants Res*. 2016 Jun 17. doi: 10.1111/clr.12894. [Epub ahead of print]
- [4] Val JE, Gómez-Moreno G, Ruiz-Linares M, et al. Effects of Surface Treatment Modification and Implant Design in Implants Placed Crestal and Subcrestally Applying Delayed Loading Protocol. *J Craniofac Surg*. 2017 Mar;28(2):552-558.
- [5] Al-Nsour MM, Chan HL, Wang HL. Effect of the platform-switching technique on preservation of peri-implant marginal bone: a systematic review. *Int J Oral Maxillofac Implants*. 2012 Jan-Feb;27(1):138-45.
- [6] Annibaldi S, Bignozzi I, Cristalli MP, et al. Peri-implant marginal bone level: a systematic review and meta-analysis of studies comparing platform switching versus conventionally restored implants. *J Clin Periodontol*. 2012 Nov;39(11):1097-1113.
- [7] Hsu YT, Lin GH, Wang HL. Effects of Platform-Switching on Peri-implant Soft and Hard Tissue Outcomes: A Systematic Review and Meta-analysis. *Int J Oral Maxillofac Implants*. 2017;32(1):e9-e24.
- [8] Lazzara RJ, Porter SS. Platform switching: a new concept in implant dentistry for controlling postrestorative crestal bone levels. *Int J Periodontics Restorative Dentistry*. 2006 Feb;26(1):9-17.
- [9] Rocha S, Wagner W, Wiltfang J, Nicolau P, Moergel M, Messias A, Behrens E, Guerra F. Effect of platform switching on crestal bone levels around implants in the posterior mandible: 3 years results from a multicentre randomized clinical trial. *J Clin Periodontol*. 2016 Apr;43(4):374-82.
- [10] Babbush CA. Post treatment quantification of patient experiences with full-arch implant treatment using a modification of the OHIP-14 questionnaire. *J Oral Implantol*. 2012 Jun;38(3):251-60.
- [11] Block MS, Haggerty CJ, Fisher GR. Nongrafting implant options for restoration of the edentulous maxilla. *J Oral Maxillofac Surg* 2009;67:872-881.
- [12] Steigenga J, Al-Shammari K, Misch C, Nociti FH Jr, Wang HL. Effects of implant thread geometry on percentage of osseointegration and resistance to reverse torque in the tibia of rabbits. *J Periodontol*. 2004;75(9):1233-41.
- [13] Carvajal Mejía JB, Wakabayashi K, Nakano T, Yatani H. Marginal Bone Loss Around Dental Implants Inserted with Static Computer Assistance in Healed Sites: A Systematic Review and Metaanalysis. *Int J Oral Maxillofac Implants*. 2016 Jul-Aug;31(4):761-75.1.
- [14] Pozzi A, Tallarico M, Marchetti M, Scarfò B, Esposito M. Computer-guided versus free-hand placement of immediately loaded dental implants: 1-year post-loading results of a multicentre randomized controlled trial. *Eur J Oral Implantol*. 2014 Autumn;7(3):229-42.
- [15] Hultin M, Svensson KG, Trulsson M. Clinical advantages of computer-guided implant placement: a systematic review. *Clin Oral Implants Res*. 2012 Oct;23 Suppl 6:124-35.
- [16] Soares MM, Harari ND, Cardoso ES, et al. An in vitro model to evaluate the accuracy of guided surgery systems. *Int J Oral Maxillofac Implants*. 2012 Jul-Aug;27(4):824-31.
- [17] Pozzi A, Polizzi G, Moy PK. Guided surgery with tooth-supported templates for single missing teeth: a critical review. *Eur J Oral Implantol*. 2016;9(1)135-53.

Neodent®, NeoPoros, ACQUA, Helix®, Drive®, Titamax®, Grand Morse™, Helix GM™, Drive GM™, Titamax GM™, NeoArch®, Zygomax GM™, Zi™, ZiLock™ are trademarks or registered trademarks of JIGC Indústria e Comércio de Materiais Dentários S.A.

CEREC® is a trademark or registered trademark of Sirona Dental Systems GmbH (DE).

Dentsply Sirona is a trademark or registered trademark of Dentsply Sirona, Inc.

MEDENTiKA is a trademark or registered trademark of Medentika GmbH.

Panavia is a trademark or registered trademark of Kuraray Co. Ltd.

Amann Girschbach is a trademark or registered trademark of Amann Girschbach AG.

exocad is a trademark or registered trademark of exocad GmbH.

Dental Wings is a trademark or registered trademark of Dental Wings Inc.

3Shape is a trademark or registered trademark of 3Shape A/S.

© Neodent® 2022. All rights reserved.
Neodent® and/or other trademarks and logos
from Neodent® that are mentioned herein are
the trademarks or registered trademarks of
Straumann Holding AG and/or its affiliates.
All rights reserved.

ifu.neodent.com.br/en
www.neodent.us • www.neodent.ca



Straumann North American Headquarters
Straumann USA, LLC
60 Minuteman Road
Andover, MA 01810
Phone 800/448 8168 (US) • 800/363 4024 (CA)

Fax 978/747 2490
www.straumann.us • www.straumann.ca

USLIT.2040 9/22 V2 PMR

