



# Certificate of Analysis

## COMPLIANCE FOR RETAIL

Laboratory Sample ID: DA50529015-001



Jun 03, 2025 | factoryfwd

2030 Stirling rd apt 102  
Hollywood, FL, 33020, US

**Production Method:** Other - Not Listed  
**Batch#:** NR26NR041525  
**Harvest Date:** 05/30/25  
**Sample Size Received:** 1 units  
**Total Amount:** 1 units  
**Retail Product Size:** 3.6945 gram  
**Retail Serving Size:** 1 gram  
**Servings:** 3.6945  
**Ordered:** 05/29/25  
**Sampled:** 05/29/25  
**Completed:** 06/03/25  
**Sampling Method:** SOP.T.20.010.FL

**TESTED**


Pages 1 of 1

### SAFETY RESULTS

								
Pesticides <b>NOT TESTED</b>	Heavy Metals <b>NOT TESTED</b>	Microbials <b>NOT TESTED</b>	Mycotoxins <b>NOT TESTED</b>	Residuals Solvents <b>NOT TESTED</b>	Filtth <b>NOT TESTED</b>	Water Activity <b>NOT TESTED</b>	Moisture <b>NOT TESTED</b>	Terpenes <b>NOT TESTED</b>

### MISC.

## Cannabinoid **TESTED**

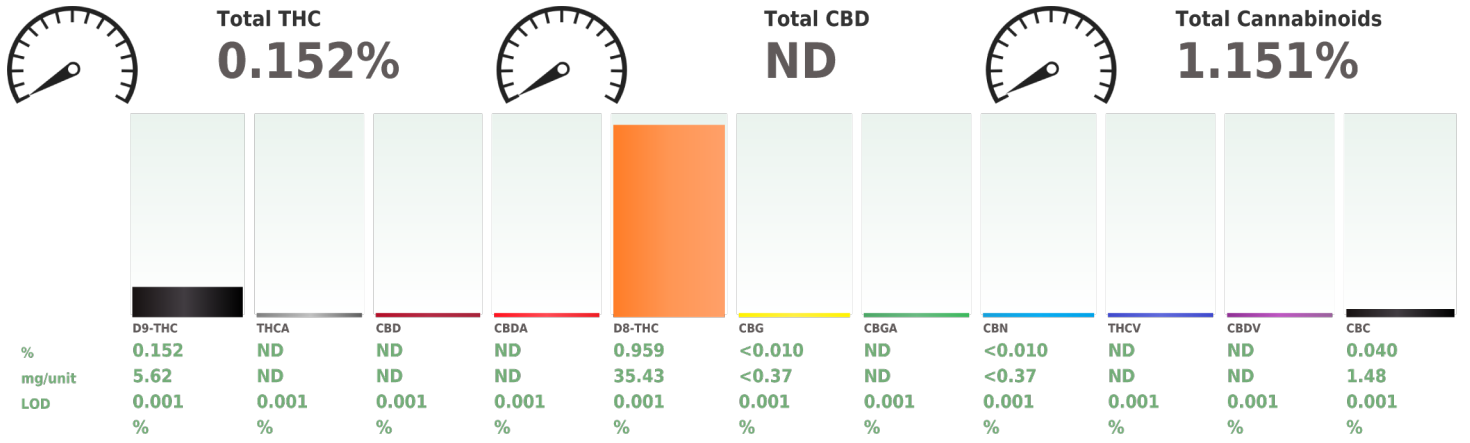

Analyzed by: 3335, 1665, 585, 1440      Weight: 3.6945g      Extraction date: 05/30/25 12:43:44      Extracted by: 3335

Analysis Method : SOP.T.40.031, SOP.T.30.031      Analytical Batch : DA087007POT      Batch Date : 05/30/25 09:57:01  
 Instrument Used : DA-LC-008  
 Analyzed Date : 06/02/25 23:03:00

Dilution : 400  
 Reagent : 120324.07; 053025.R03; 090924.05; 021125.07; 053025.R04  
 Consumables : 947.110; 04312111; 062224CH01; 0000355309  
 Pipette : DA-079; DA-108; DA-078

Full Spectrum cannabinoid analysis utilizing High Performance Liquid Chromatography with UV detection in accordance with F.S. Rule 64ER20-39.

This Kaycha Labs Certification shall not be reproduced, unless in its entirety, without written approval from Kaycha Labs. The results relate only to the material or product analyzed. ND=Not Detected, ppm=Parts Per Million, ppb=Parts Per Billion, RSD=Relative Standard Deviation. Limit of Detection (LOD) and Limit Of Quantitation (LOQ) are terms used to describe the smallest concentration that can be detected and reliably measured by an analytical procedure, respectively. Action Levels are State determined thresholds based on F.S. Rule 64ER20-39 and F.S. Rule 5K-4. The Measurement of Uncertainty (MU) error is available from the lab upon request. The "Decision Rule" for pass/fail does not include the MU. Any calculated totals may contain rounding errors.

**Vivian Celestino**  
Lab Director

State License # CMTL-0002  
ISO 17025 Accreditation # ISO/IEC  
17025:2017 Accreditation PJA-  
Testing 97164



Signature  
06/03/25