


Masimo® sensor selection guide for SpO₂ and rainbow® (SpO₂, SpCO, SpMet)

For use with LIFEPAK® 15 monitor/defibrillators

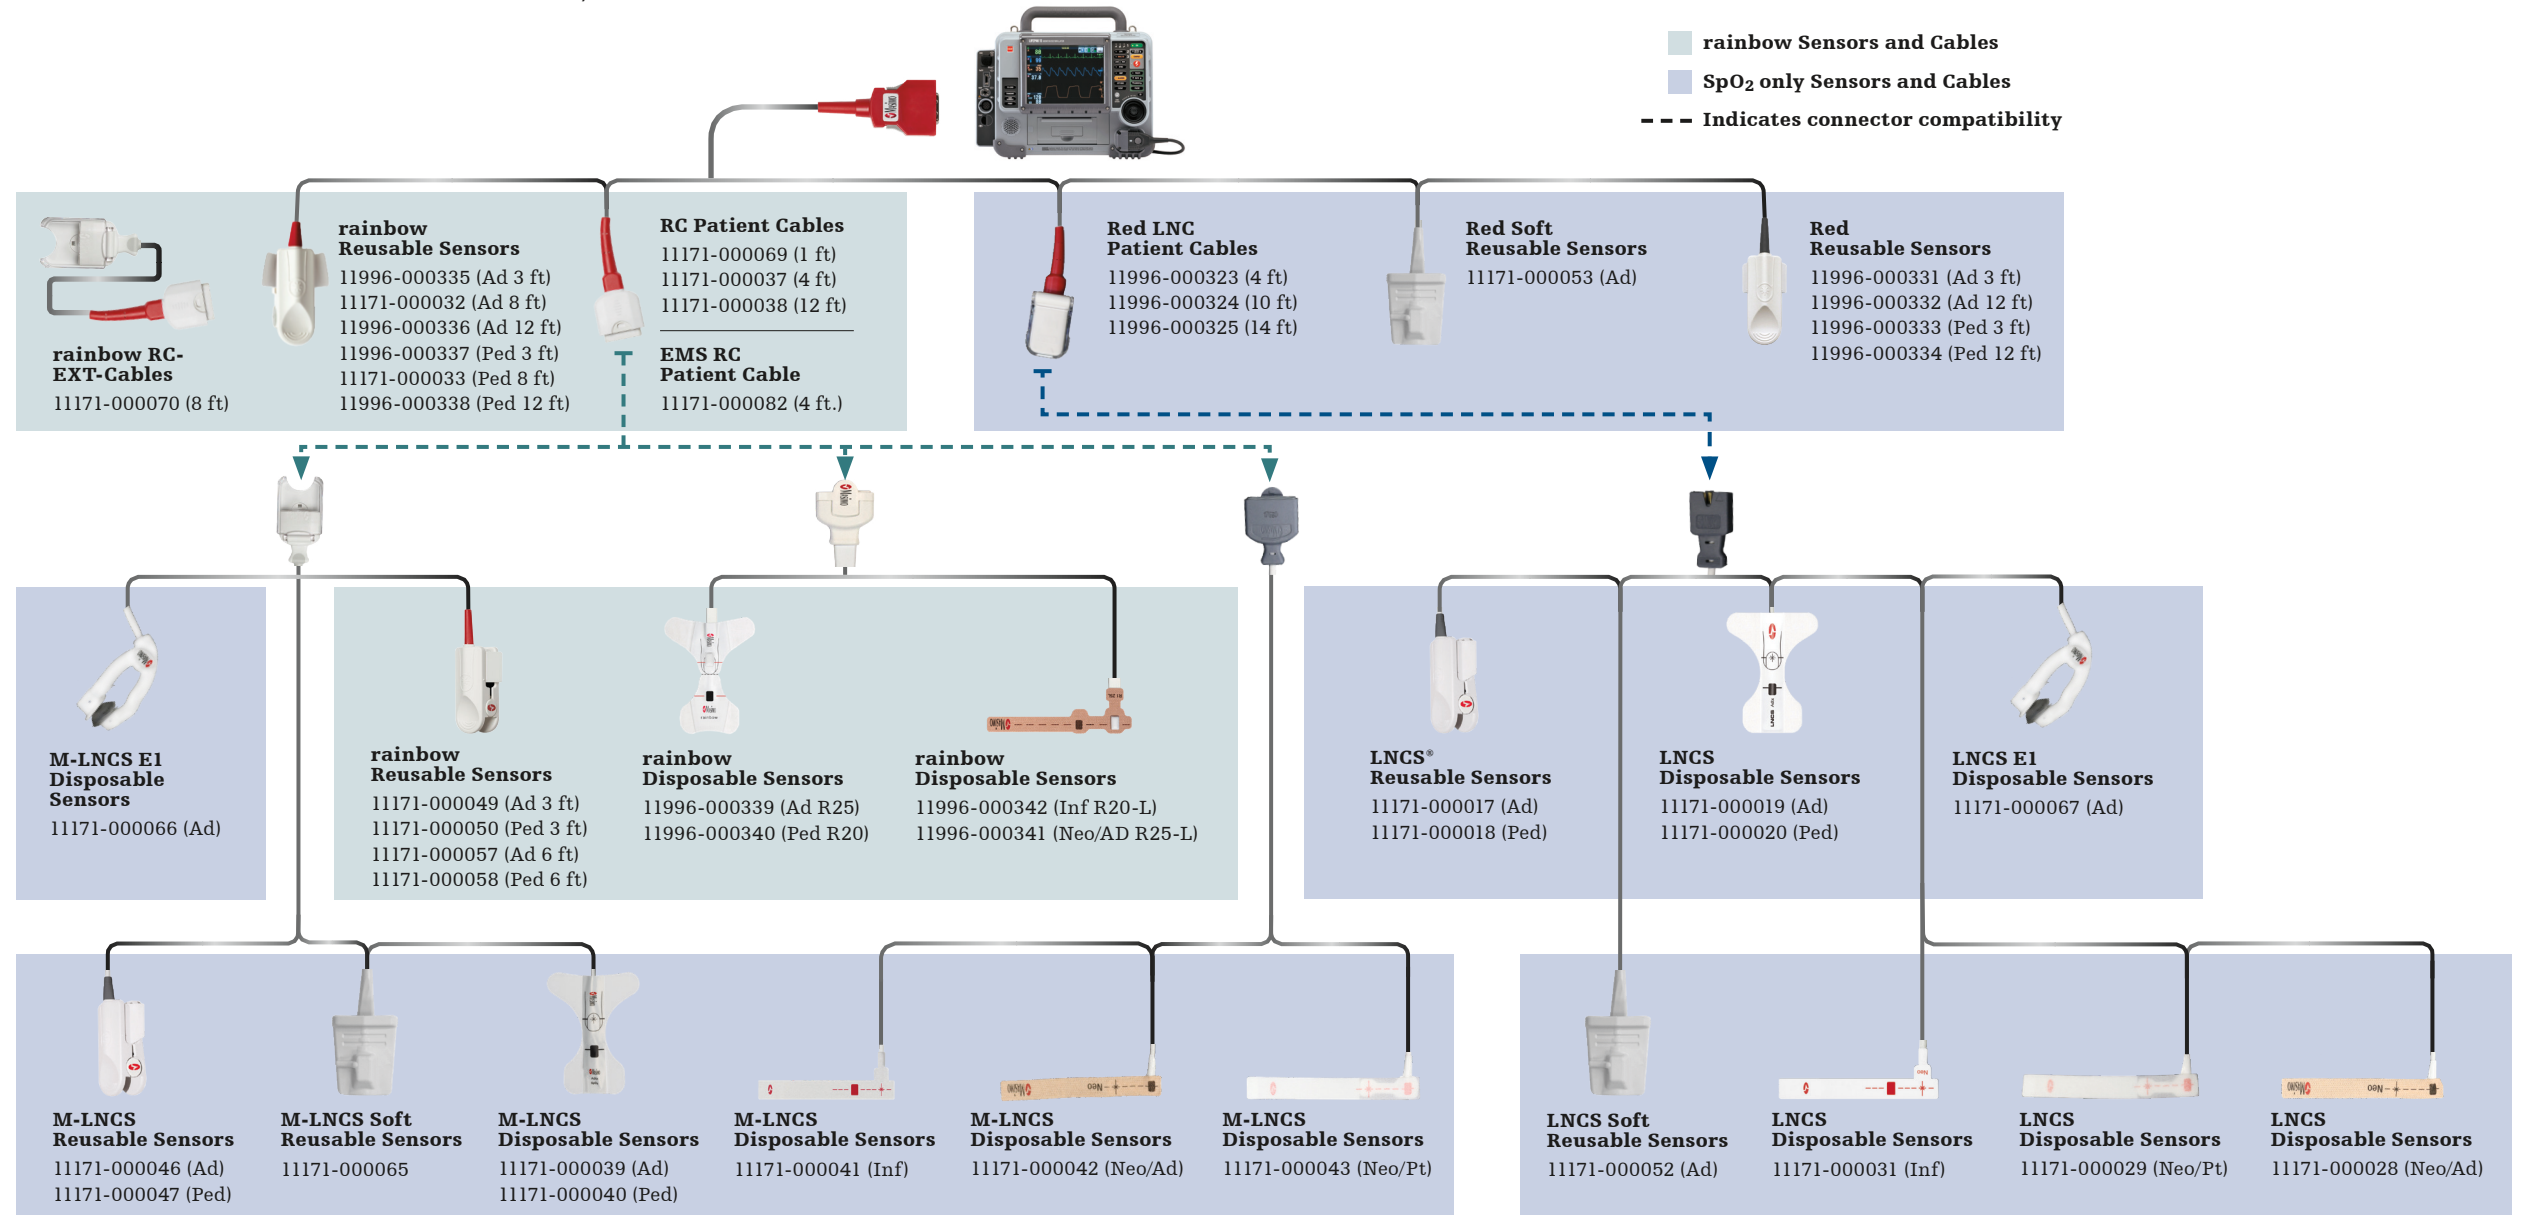

For further information, please contact Stryker at 800 442 1142 (U.S.), 800 668 8323 (Canada) or visit our website at strykeremergencycare.com

Emergency Care

Stryker or its affiliated entities own, use, or have applied for the following trademarks or service marks: LIFEPAK, Stryker, Masimo, the Radical logo, Rainbow and SET are registered trademarks of Masimo Corporation. All other trademarks are trademarks of their respective owners or holders.

The absence of a product, feature, or service name, or logo from this list does not constitute a waiver of Stryker’s trademark or other intellectual property rights concerning that name or logo.

Distributed in the US by:

Physio-Control, Inc.
11811 Willows Road NE
Redmond, WA, 98052 U.S.A.
Toll free 800 442 1142
strykeremergencycare.com

Distributed in Canada by:

Stryker Canada
2 Medicorum Place
Waterdown, Ontario
L8B 1W2
Canada
Toll free 800 668 8323