


1 Prepare for Liposana[®] implantation with sterile gloves, a sterile syringe (3 mL recommended), one sterile 18G or larger beveled needle, and one sterile 20G needle.



2 Remove Liposana[®] package from frozen storage. Inspect the package to ensure its integrity. **DO NOT USE** the product if the package integrity is compromised.


Note: Vial is aseptically packaged in two presterilized pouches.

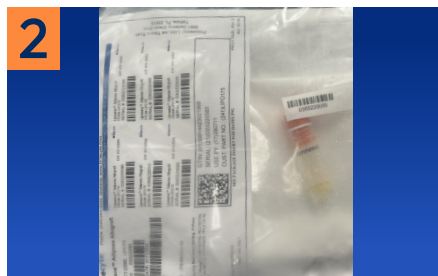

3 Remove outer pouch and place the inner pouch with the vial on a clean surface. Allow the product to thaw completely before use (approx. 30 minutes). **DO NOT RE-FREEZE** the product.



4 Retrieve the vial from the innermost pouch. If in an operating room, use aseptic technique to transfer the vial to a sterile field.

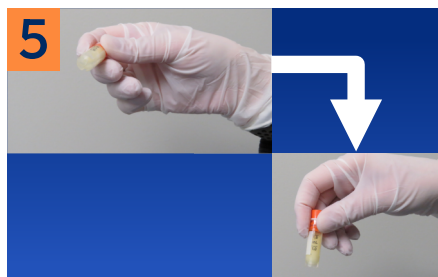


5 Shake the vial for 15-20 seconds and wrist “flick” the vial in the downward direction to ensure all product is on the bottom of the vial.



6 Immediately withdraw the product using a syringe with an 18G or larger beveled needle at a slow, steady pace.

Note: If the needle becomes clogged, expel clogged tissue. Repeat steps 5 and 6.

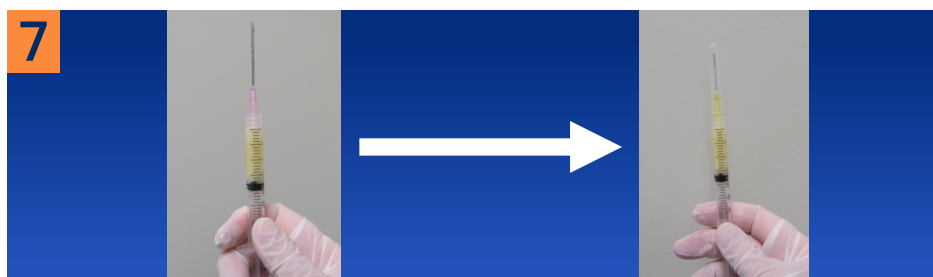

7 After the product is in the syringe, replace the 18G beveled needle with a new sterile 20G needle. Remove air bubbles from the syringe before implanting.

The product can remain in the syringe until the patient is ready for implantation.

Note: Using small bore needles may result in needle clogging during Liposana[®] implantation; product must be used the same day post-thaw.