

ⓘ When using this homepage, we recommend Chrome browser. Chrome can translate web

pages.

ABOUT US

PRODUCT

APPLICATIONS


FAQ

CONTACT

HIRANUMA APPLICATION DATA		Karl Fischer Titrator	Data No.	KF15	Nov.29, 2018
Water contents	Ketones – KF Coulometry, Direct-Injection Methyl ethyl ketone and Acetone				

1. Abstract

Water content of ketones could be determined by Karl Fischer coulometric titrator. In coulometric titration, iodine of Karl Fischer reagent is generated by electrolysis and generated iodine quantitatively reacts with water. Reaction formula is described below.



When the sample is liquid, generally sample is measured by direct injection into the titration cell. Anode solution containing methanol as solvent is generally used for various sample. However, in the measurement of ketones and aldehydes, since these react with methanol to produce water, the measurement result tends to be higher than the true value (formula (1)).



For above reason, Karl Fischer reagent without methanol should be used for water determination of ketones and aldehydes. There are commercially available reagents with a special composition for ketones and aldehydes. This chapter introduces an example for the water determination in methyl ethyl ketone and acetone. These samples are often used as paint solvents, raw materials of adhesives, and synthetic resins.

2. Apparatus and Reagents

(1) Apparatus

Titrator : HIRANUMA Karl Fischer Coulometric titrator AQ-series or MOICO-A19

Electrolytic cell : Standard Cell
Fritless Cell (No cathode solution required)

(2) Reagents

Anode solution : HYDRANAL Coulomat AK (for ketone, Honeywell)

Cathode solution : HYDRANAL Coulomat CG-K (for ketone, Honeywell)

3. Procedure

- (1) Fill 100 mL of anode solution and one ampoule of cathode solution into the electrolytic cell as shown in Fig.3.1. When fritless cell is used, cathode solution is not necessary.
- (2) Start blanking to attain stable background.
- (3) Wash the syringe with sample.
- (4) Draw the sample into syringe and then weigh the syringe.
- (5) Inject sample from rubber septum of electrolytic cell as shown in Fig.3.2.
- (6) Start titration. Measurement parameter is shown in Table 4.1.

ⓘ When using this homepage, we recommend Chrome browser. Chrome can translate web

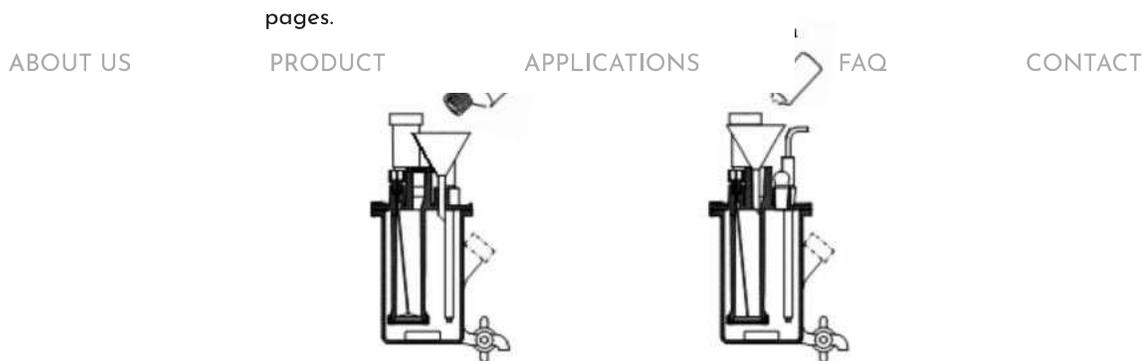


Fig.3.1. Preparation of the reagents. (Standard Cell)

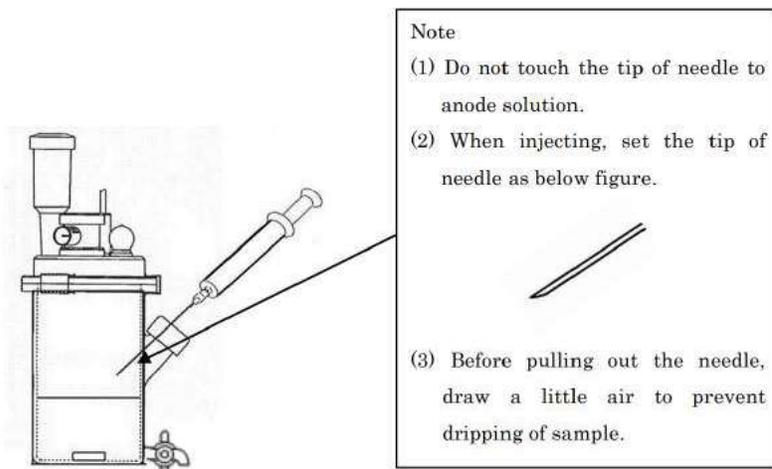


Fig.3.2. Injection of sample.

4. Parameters and results

Table 4.1. Parameters

Condition File	
Cal Mode	o:Sample weight(net) $X=(H_2O-BLANK)/SIZE$
Interval Time	30 sec
Current	SLOW
S-Timer	0 min
Blank Value	0 μ g
Unit Mode	AUTO
Auto Interval	0 g
Minimum Count	5 μ g
Back Ground	ON
Sample Size Input	Every Time
Cell Type	Standard/Fritless

 When using this homepage, we recommend Chrome browser. Chrome can translate websites.

ABOUT US	pages.		APPLICATIONS	titent)	FAQ	Statistics	Results
	PRODUCT						
Methyl ethyl ketone	Standard	0.4565	103.8	227.4	Avg.	223.9 ppm	
		0.4722	107.7	228.1	SD	6.7 ppm	
		0.4478	96.8	216.2	RSD	3.0 %	
	Fritless	0.4346	92.3	212.4	Avg.	209.3 ppm	
		0.4596	93.7	203.9	SD	4.7 ppm	
		0.2856	60.4	211.5	RSD	2.2 %	
Acetone	Standard	0.4515	102.6	227.2	Avg.	225.3 ppm	
		0.6059	136.0	224.5	SD	1.7 ppm	
		0.4945	110.8	224.1	RSD	0.7 %	
	Fritless	0.4535	100.8	222.3	Avg.	223.6 ppm	
		0.5513	124.1	225.1	SD	1.4 ppm	
		0.3330	74.4	223.4	RSD	0.6 %	

5. Note

- (1) When the side reaction cannot be suppressed even though you use reagent for ketons, phenomena such as unstable blanking or undetectable endpoint can be obtained. In that case, it may be improved by reducing the amount of sample or replacing titration solvent with new one.
- (2) Sample with high activity side reaction like cyclohexanone cannot be measured by coulometry – direct injection method. Since the boiling point of cyclohexanone is much higher than that of water and toluene, it can be measured by suppressing the influence of side reaction with coulometry – azeotropic distillation method (Refer to Application Data No. 16.)
- (3) The optimized electrolysis control for fritless cell of AQ series released after 2009 improves the measurement accuracy of fritless cell. It can be used with the evaporator as well. Suitable reagent for fritless cell is required. For example, Hydranal coulomat AG and AG-Oven are compatible with fritless cell.

Hydranal coulomat AK is a reagent designed to be used in standard type cell with diaphragm. When used in a fritless cell, it is said to have an error of a few % with respect to the result with standard cell. Results measured with fritless cell and coulomat AK are shown in the Table 4.2 as reference values

Keywords: Karl Fischer, Coulometric titration, Direct injection, Ketone, Fritless cell



 When using this homepage, we recommend Chrome browser. Chrome can translate web pages.

[JSE](#)

[PRIVACY POLICY](#)

[ABOUT US](#)

[PRODUCT](#)

[APPLICATIONS](#)

[FAQ](#)

[CONTACT](#)