

NC Controlled Substance License #:
NC-DHHS-1002881
DEA Controlled Substance License #:
RD0577986
ISO 17025 Certification:
PENDING
Proficiency Testing Enrolled:
Hemp PT Program U of Kentucky
Regulatory Services

ANALYTICAL
Delta 9 Analytical
Professional, Accurate, Responsive

Laboratory Location:
6308 Angus Drive, Ste B
Raleigh NC 27617
919-673-7153 / 919-450-1870
frank@delta9analytical.com
michael@delta9analytical.com

Remarketed by Legacy
Farms Cannabis Verified /
Inspected Production Partner

NC Processor Lic#: 14754
Received Date: 04092021
Reported Date: 04132021
Sample ID: 721

Sample:
Sample Type: Hemp Flower
Sample Matrix: Plant, Cured
Sample Size: 1.60g

Certificate of Analysis – Hemp




Scan to verify
CoFA at
www.delta9analytical.com

<0.05%
*TOTAL THC

ND
Δ9 THC

11.04%
*TOTAL
CBG

12.60%
*TOTAL
Cannabinoids

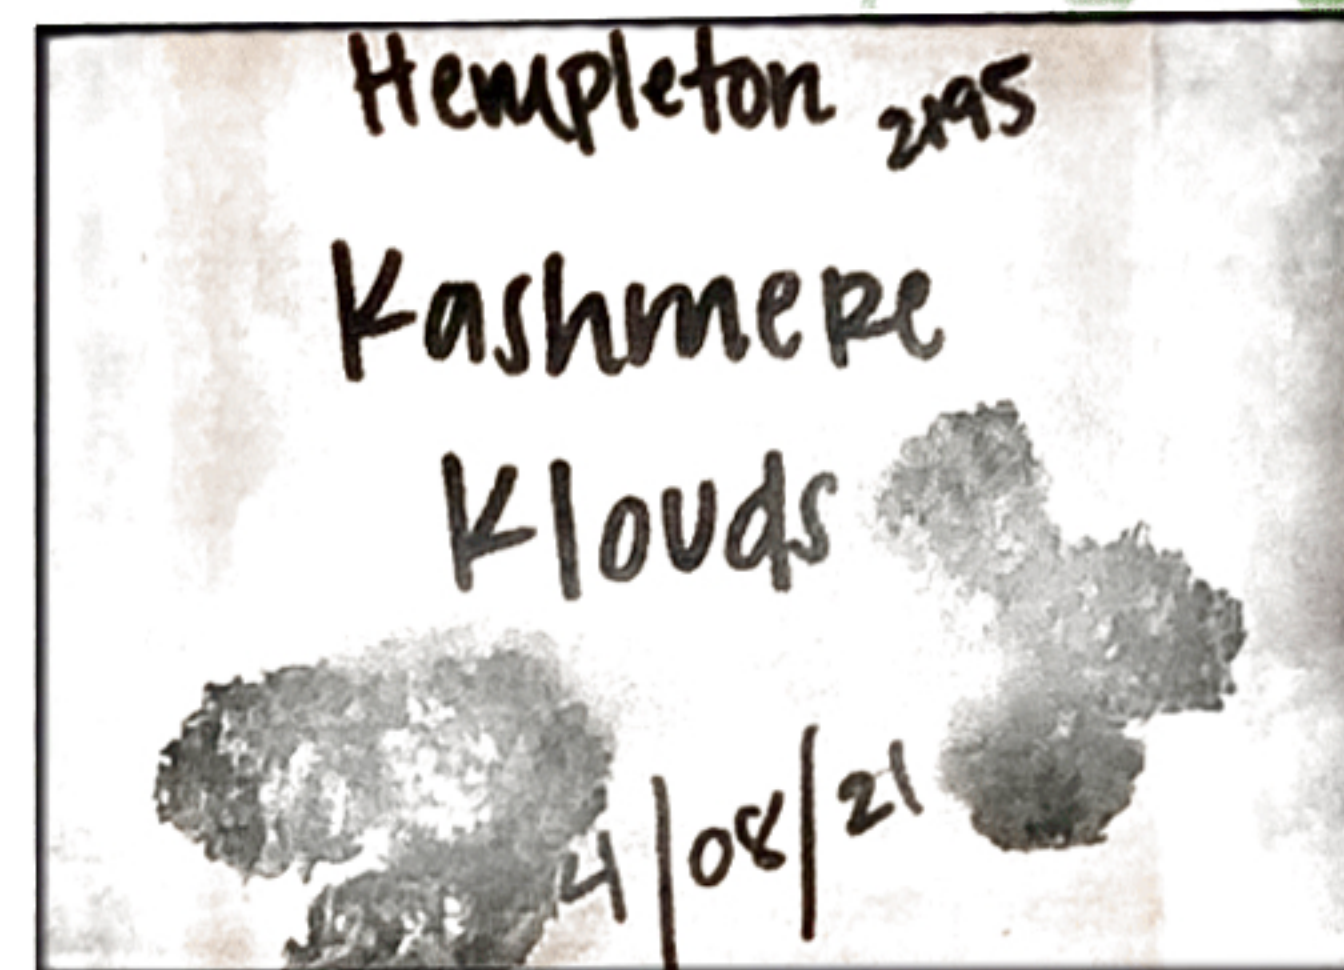

Batch Photo

Quick Summary


Moisture Test Results
2.27% (Loss on drying)

CANNABINOID PROFILE

(Tested by High-Performance Liquid Chromatography Mass Spectrometry)

<u>Cannabinoid</u>	<u>% Wt</u>	<u>Conc (mg/mL)</u>	<u>LOQ (%Wt)</u>
Cannabinol (CBN)	ND	ND	< 0.05
Δ8-THC	ND	ND	< 0.05
Cannabichromene (CBC)	0.0961	0.961	< 0.05
Cannabigerol (CBG)	0.6269	6.269	< 0.05
Cannabidiol (CBD)	ND	ND	< 0.05
Cannabigerolic Acid (CBGA)	11.875	118.75	< 0.05
Cannabidivarin (CBDV)	ND	ND	< 0.05
Cannabidolic Acid (CBDA)	ND	ND	< 0.05
Δ9-Tetrahydrocannabinolic Acid (THCA)	<0.05	<0.05	< 0.05
Tetrahydrocannabidvarin (THCV)	ND	ND	< 0.05
**Δ9-THC	ND	ND	< 0.05
*TOTAL CANNABINOIDS	12.598	125.98	< 0.05
*TOTAL THC	<0.05	<0.05	< 0.05
*TOTAL CBG	11.041	110.41	< 0.05

SAMPLE CERTIFICATION

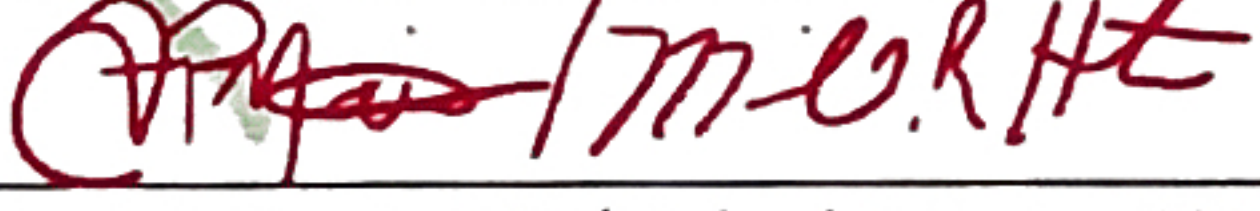
Frank P. Mauricio COO/Michael R. Horton CSO & Date 04132021

*Calculated as follows: Total CBD/G = CBD/GA% (0.877) + CBD/G%. Total THC = THCA % (0.877) + Δ9-THC %. *Total Cannabinoids is the absolute sum of all cannabinoids detected.

Testing results are based solely upon the sample submitted to Delta 9 Analytical, LLC. (D9A) In the condition it was received. D9A warrants that all analytical work is conducted professionally in accordance with all applicable standard practices using validated methods utilizing certified reference standards. **The uncertainty of measurement associated with the measurement result reported in this certificate is available from D9A upon request. This report may not be reproduced, except in full, without the written approval of D9A.