



Hocker Incorporated

13402 Weiman Road Houston, TX 77041
713-464-5829 Fax 713-464-3192

hi.cert@hockerinc.com

Performance Evaluation UV & White Light Meter

Customer PO #:	85480
Certification #:	21-0065
Evaluation Date:	Due Date:
01/14/2021	07/14/2021





F-LTMT-0		Operational When Received?		Yes	DLM-1000		Equipment Condition When Received?		
Company: P & B Testing, Inc.		In Tolerance when Received?		Yes					
Address: 6645 W.TIDWELL							New		
City: HOUSTON							X Good		
State: TX							Fair		
Zip: 77092		Phone: (713)290-8490					Poor		
Country: USA		Fax: (713)290-8627					Failed		
Contact: Buck Snider		File Loc.		P & B Testing, Inc._01142021_21-0065					
Equipment Used For This Eval.:		Serial #:		Cal. Date:	Due Date:	NIST#:			
DLM-1000 A Readout		142154 A		9/22/2020	3/22/2021	89803/153301			
DLM-1000 B UV SENSOR		142154 B		9/22/2020	3/22/2021	89803/00249/10540			
DLM-1000 C WL SENSOR		142154 C		9/22/2020	3/22/2021	89803/811,7481/Y25189/W10962			
% Tolerance Used:	5.0%	(+/-)	Meter Type:	Digital	3 pcs.	Equipment Mfg.:			
						Gould-Bass			
Equipment Owner:		Address:		City:		State:	Zip:		
P & B Testing, Inc.		6645 W.TIDWELL		HOUSTON		TX	77092		
DLM-1000 "B" Sensor				Temperature:	70°F	Humid.:	50%		
UV As Found	UV Meter As Received				UV As Left	UV Meter After Adjustment			
uW/sq.cm	uW/sq.cm	uW/sq.cm	% Diff.	Tolerance	uW/sq.cm	uW/sq.cm	uW/sq.cm	% Diff.	Tolerance
Ideal	Actual	Difference			Ideal	Actual	Difference		
0	0	0		In	0	0	0		In
950	990	40	4.2%	In	950	960	10	1.1%	In
2930	2980	50	1.7%	In	2930	2900	-30	-1.0%	In
4390	4570	180	4.1%	In	4390	4440	50	1.1%	In
Maximum Deviation		50	4.2%		Maximum Deviation		50	1.1%	
DLM-1000 "C" Sensor									
WL As Found	White Light Meter As Received				WL As Left	White Light Meter....No Adjustment or Repair Required			
Foot Candles	Foot Candles	Foot Candles	% Diff.	Tolerance	Foot Candles	Foot Candles	Foot Candles	% Diff.	Tolerance
Ideal	Actual	Difference			Ideal	Actual	Difference		
0.0	0.0	0.0		In	0.0	0.0	0.0		In
3.0	3.0	0.0	0.0%	In	3.0	3.0	0.0	0.0%	In
100.0	101.0	1.0	1.0%	In	100.0	101.0	1.0	1.0%	In
210.0	213.0	3.0	1.4%	In	210.0	213.0	3.0	1.4%	In
Maximum Deviation		3	1.4%		Maximum Deviation		3	1.4%	

Notes:

P & B Testing, Inc.

Certification #
Evaluation Date

21-0065
01/14/2021

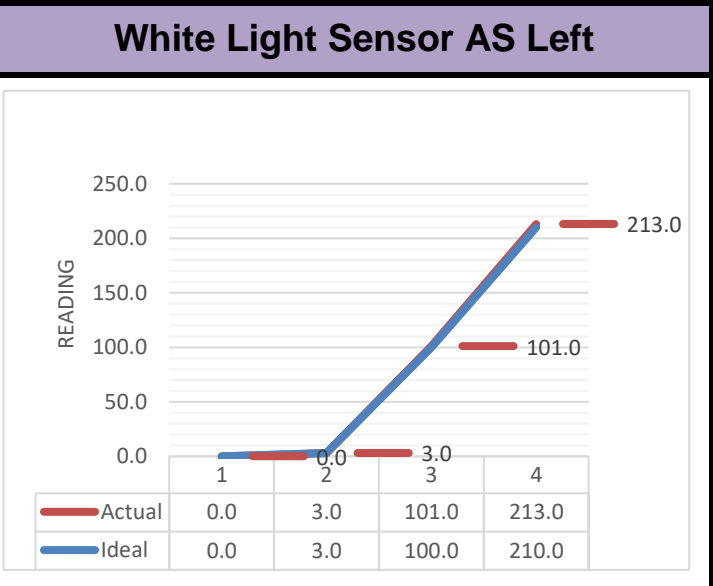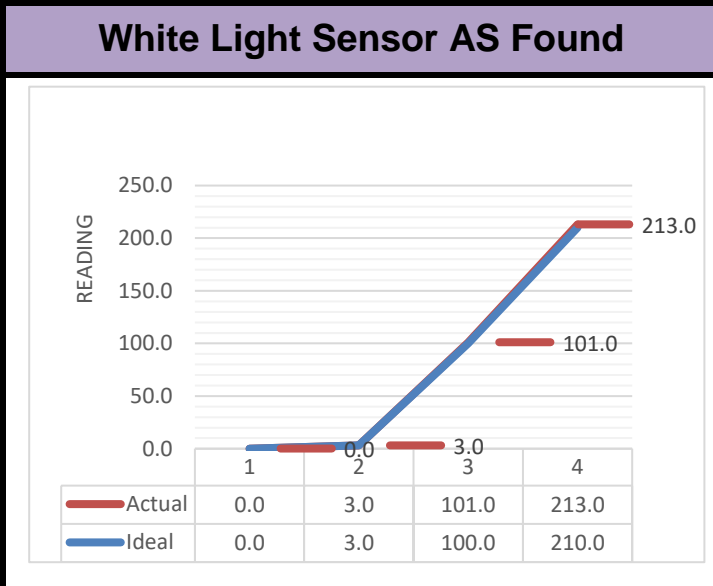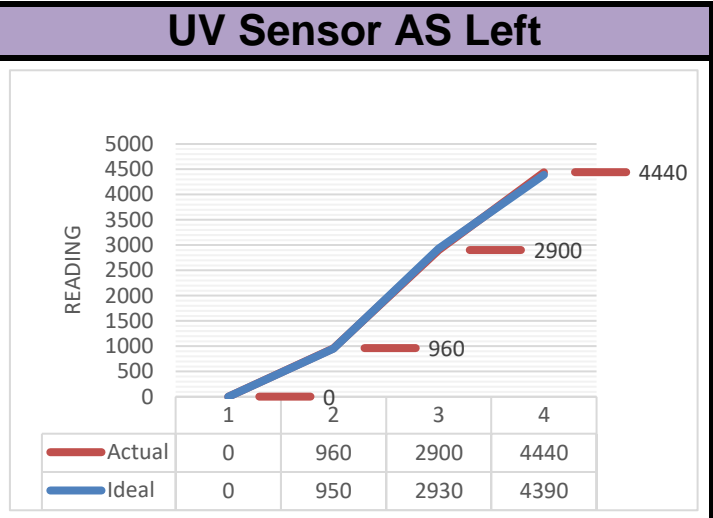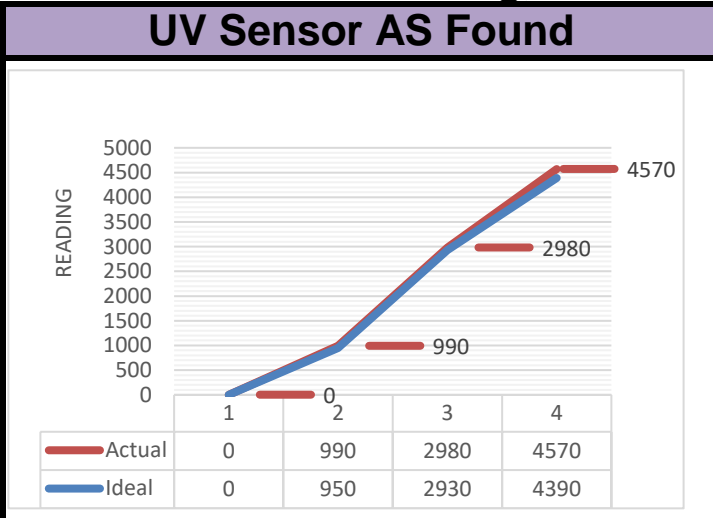

Notes:

This performance evaluation was done in accordance with ASTM-E-1444, ASTM E-709, and Hocker Incorporated procedure CP-LTMT- Rev 0. Test equipment and reference standards used to perform this evaluation are traceable to the National Institute of Standards and Technology. NIST numbers listed in this document and supporting documentation is on file.

In Conformance with 10CFR21, ANSI/NCSL 2540.3-2006 & ISO10012.

Technician Signature: Jacob Hocker

CP-LTMT- Rev 0 05/18/2018

Technician Performing Evaluation: Jacob Hocker

Date 01/14/2021

Approval Signature: Derrick Schumann

Approved By: Derrick Schumann

An ISO 9001:2015 Registered Company