

# OPERATING THEATRE

## Environmental Set-up Guide



## Contents

1. ***** Gynae / Obstetrics .....	6
2. Bartholin's Abscess .....	7
3. B.S.O – Bilateral Salingopaxy Oophorectomy .....	8
4. Cone Biopsy of the Cervix .....	9
5. D&C – Dilatation and Curettage .....	10
6. Ectopic Pregnancy - Laparoscopically .....	11
7. Hysteroscopy .....	12
8. Hysterectomy / Total Abdominal Hysterectomy / T.A.H .....	13
9. Hysterectomy / Vaginal / Laparoscopic .....	14
10. L.L.E.T.Z – Large Loop Excision of Transformation Zone .....	15
11. L.U.C.C.S – Lower Uterine Segment Caesarean Section .....	16
12. Pelvic Mass .....	17
13. P.P.H – Post Partum Haemorrhage .....	18
14. Salpingostomy .....	19
15. T.A.H – Total Abdominal Hysterectomy .....	20
16. Vaginal Hysterectomy .....	21
17. Trial By Forceps .....	22
18. Ventouse .....	23
19. Ventrosuspension .....	24
20. Vulvectomy .....	25
21. 3 <sup>rd</sup> Degree Tear .....	26
22. ***** Emergency .....	27
23. ***** General Surgery .....	28
24. Open Hernia Repairs / Herniorrhaphy .....	29
25. Esophagectomy .....	30
26. Open Appendicectomy / Gastrectomy / Laparotomy / Liver Resection / Right Hemicolectomy .....	31
27. Hemicolectomy Left / Anterior Resection / Ultra-Low .....	32
28. Hemicolectomy Right .....	33
29. Open Splenectomy / Lap Splenectomy .....	34
30. Closure Ostiomyespen .....	35
31. Lap Nissen Fundoplication .....	36
32. Hartman's Procedure .....	37
33. Whipples .....	38
34. Anal Fistula / Fissure / Haemorrhoidectomy / Perianal Abscess / Advancement Flaps / Prolapse .....	39
35. Thyroidectomy / Parathyroidectomy .....	40
36. Pilonidal Sinus V1 Lateral .....	41
37. Pilonidal Sinus V2 Prone .....	42
38. Laparoscopic Cholecystectomy .....	43
39. Hysteroscopy / D&C / Cystoscopy / Most General Gynae / Laparoscopic Ablation of Endometriosis / Lap Assisted .....	44
40. ***** Cardiac .....	45

41. ***** Neuro .....	46
42. Craniotomy.....	47
43. Burr Holes .....	48
44. Transsphenoidal Pituitary (set up as FESS) .....	49
45. Laminectomy / Microdiscectomy / Spinal Fusion.....	50
46. Craniotomy - With Stealth .....	51
47. INTER-CRANIAL ANEURYSM – With Stealth .....	52
48. Craniotomy / Shunt – With Axiom .....	53
49. Sub-Dural Haematoma / Burr Hole / EVD / ICP (Emergency) .....	54
50. Craniotomy- Intraoperative MRI With Skull Clamp.....	55
51. Trans-Sphenoidal Tumour Resection – Intraoperative MRI With Head Ring.....	56
52. Cervical Laminectomy – With Pillows “BOWS” With Xray .....	57
53. Cervical Laminectomy – With Montreal Mattress – With Xray .....	58
54. Cervical Laminectomy – Compress Roll – With Xray .....	59
55. Anterior Cervical Discectomy Fusion (ACDF) With Xray V1 .....	60
56. Anterior Cervical Discectomy Fusion (ACDF) With Xray V2.....	61
57. Anterior Cervical Discectomy Fusion (ACDF) With Xray V3.....	62
58. Anterior Cervical Discectomy Fusion (ACDF) With Xray V4.....	63
59. Anterior Cervical Discectomy Fusion (ACDF) With Xray V5.....	64
60. Laminectomy / Microdiscectomy – With Xray V1 .....	65
61. Laminectomy / Microdiscectomy – With Xray V2 .....	66
62. Spinal Fusion (Inc TLIF) With O-Arm.....	67
63. Spinal Fusion (XLIF) With Xray.....	68
64. Carpal Tunnel Repair (Right) .....	69
65. Carpal Tunnel Repair (Left).....	70
66. ***** Paediatrics .....	71
(Home).....	71
67. ***** Orthopaedics .....	72
68. P&P / Pin and Plate / Canulated Hip Screw.....	73
69. Achilles Tendon Repair.....	74
70. Carpel Tunnel Release .....	75
71. Cubital Tunnel Release .....	76
72. D.P.C / Direct Primary Closure.....	77
73. Dupuytren’s Contracture.....	78
74. Arthroscopy Knee.....	79
75. M.U.A / Manipulation under Anaesthetic / Ulna - Radius .....	80
76. O.I.F / Open Reduction Internal Fixation / Ankle .....	81
77. O.I.F / Open Reduction Internal Fixation / Clavicle.....	82
78. O.I.F / Open Reduction Internal Fixation / Distal Humorous.....	83
79. O.I.F / Open Reduction Internal Fixation / Proximal Humorous.....	84
80. O.I.F / Open Reduction Internal Fixation / Femur .....	85
81. O.I.F / Open Reduction Internal Fixation / Olecranon / Elbow .....	86
82. R.C.R / Rotator Cuff Repair .....	87
83. Tendo/ Repair / Nerve Repair / Upper Limb .....	88

84. Tibial Plateau .....	89
85. T.K.R / Total Knee Replacement .....	90
86. T.H.R / Total Hip Replacement .....	91
87. Vac Dressing Change .....	92
88. ***** Ophthalmic / Eyes .....	93
89. ***** Vascular .....	94
90. A.A.A / Abdominal Aortic Aneurysm .....	95
91. A.K.A / Above Knee Amputation / B.K/A / Below Knee Amputation .....	96
92. A.V / Arteriovenous / Fistula .....	97
93. Carotid Endarterectomy .....	98
94. E.V.A.R / Endovascular Aneurysm Repair .....	99
95. Femoral Embolectomy .....	100
96. Fasciotomy .....	101
97. F.P.B / Femoral Popliteal Bypass .....	102
98. Fistulotomy .....	103
99. Formation of RC (Radio Cephalic) AVF (Arteria Venous Fistula) .....	104
100. H.L.S / High Ligation & Strip / G.S.V / Greater Saphenous Vein .....	105
101. Ligation & Avulsion of Veins .....	106
102. ***** Plastics .....	107
103. ***** Maxillofacial .....	108
104. C.A.T / Combined Approach Tympanoplasty / M.R.M / Modified Radical Meatoplasty .....	109
105. Tracheostomy / Dental Extractions / Bilateral Neck Dissection / Lip Split / Resection of Lesion / Radical Forearm Flap Reconstruction .....	110
106. ***** E.N.T – Ear Nose and Throat .....	111
107. Tonsillectomy / Adenoidectomy / T.S / A.S .....	112
108. Modified Radical Mastoidectomy .....	113
109. Meatoplasty .....	114
110. Myringoplasty .....	115
111. Pre-Auricular .....	116
112. Tympanoplasty .....	117
113. Grommets .....	118
114. Exostosis .....	119
115. Microlaryngoscopy .....	120
116. Nasopharynx Biopsy .....	121
117. E.U.A Ear / Examination Under Microscope .....	122
118. Turbinectomy .....	123
119. Septoplasty .....	124
120. Papilloma .....	125
121. Tracheostomy .....	126
122. Tracheotomy .....	127
123. ***** Thoracic .....	128
124. Anterior Mediastinoscopy .....	129
125. Lobectomy / Excision of Lung Lobe .....	130
126. Lung Lavage .....	131

<b>127. Mediastinotomy</b>	132
<b>128. Pleurectomy</b>	133
<b>129. Peritoneal Shunt Insertion / Pleuro</b>	134
<b>130. Pneumonectomy</b>	135
<b>131. Thoracoscopy</b>	136
<b>132. Thoracotomy</b>	137
<b>133. ***** Urology</b>	138
<b>134. Circumcision</b>	139
<b>135. Cystectomy</b>	140
<b>136. Cystoscopy</b>	141
<b>137. Dorsal Slit</b>	142
<b>138. Excision Of Bladder Endometrioma (Laparoscopically)</b>	143
<b>139. Hydrocele</b>	144
<b>140. Ileal Conduit</b>	145
<b>141. Stent Insertion</b>	146
<b>142. Laparoscopic Deroofing of Renal Cyst</b>	147
<b>143. Lithotripsy</b>	148
<b>144. Lithopaxy / Litholapaxy / Cisto-Litholapaxy</b>	149
<b>145. Nephrectomy</b>	150
<b>146. Nephrostomy</b>	151
<b>147. Orchidectomy</b>	152
<b>148. Orchidopexy</b>	153
<b>149. Percutaneous Nephrolithotomy / P.C.N.L</b>	154
<b>150. Prostatectomy</b>	155
<b>151. Radical Cystectomy</b>	156
<b>152. Torsion of Testes</b>	157
<b>153. T.U.R.B.T / Trans Urethral Resection of Bladder Tumour</b>	158
<b>154. T.U.R.P / Trans Urethral Resection Prostatectomy</b>	159
<b>155. Ureterolithotomy</b>	160
<b>156. Vasectomy</b>	161
<b>157. ***** Colorectal</b>	162
<b>158. ***** Dental</b>	163
<b>159. ***** E.C.T / Electroconvulsive Therapy</b>	164
<b>160. ***** Revision Status</b>	165



# 1. \*\*\*\*\* Gynae / Obstetrics

[\(Home\)](#)



## 2. Bartholin's Abscess

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Overhead Lights / SCD's Machine / Bair Hugger machine / Diathermy machine / Suction Canaster Tree / Peri Table (Ask Surgeon) / Stool for Surgeon

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Out

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** A Bartholin's cyst is a fluid-filled lump near the vaginal opening

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

### 3. B.S.O – Bilateral Salingopaxy Oophorectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

#### In Theatre Requirements



#### In Room Equipment:

Pendant Stack and Monitors  
Overhead Lights  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree  
Ligature Machine  
3 Ltr Glycine

**Notes:** A bilateral salpingo-oophorectomy is a surgery to remove both fallopian tubes and both ovaries

#### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 4. Cone Biopsy of the Cervix

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** This procedure removes a cone-shaped piece of tissue containing the abnormal cells from the cervix

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 5. D&C – Dilatation and Curettage

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is a procedure to remove tissue from inside the uterus

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 6. Ectopic Pregnancy - Laparoscopically

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Salpingostomy and salpingectomy are two laparoscopic surgeries used to treat some ectopic pregnancies

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 7. Hysteroscopy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is a procedure used to examine the inside of the womb (uterus)

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 8. Hysterectomy / Total Abdominal Hysterectomy / T.A.H

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** A partial hysterectomy removes the uterus. A total hysterectomy removes the uterus and the cervix

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 9. Hysterectomy / Vaginal / Laparoscopic

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is a procedure to remove the uterus through an incision in the vagina

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 10. L.L.E.T.Z – Large Loop Excision of Transformation Zone

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is an operation done to remove abnormal cells from the cervix or the neck of the womb

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 11. L.U.C.C.S – Lower Uterine Segment Caesarean Section

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is the most commonly used type of Caesarean section.

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 12. Pelvic Mass

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is a growth that happens near or in the fallopian tubes, ovaries, uterus, and connecting tissues

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 13. P.P.H – Post Partum Haemorrhage

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is heavy bleeding after the birth

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 14. Salpingostomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is the surgical removal of a fallopian tube

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 15. T.A.H – Total Abdominal Hysterectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is the Surgical removal of the uterus along with the cervix through the abdomen

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 16. Vaginal Hysterectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is a procedure to remove the uterus through an incision in the vagina

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 17. Trial By Forceps

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Is an attempt to deliver a baby naturally before reverting to Caesarean Section

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 18. Ventouse

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is a method to assist delivery of a baby using a vacuum device

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 19. Ventrosuspension

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is the surgical fixation of a displaced uterus to the anterior abdominal wall

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 20. Vulvectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is a procedure where a surgeon removes all or part of the vulva

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 21. 3<sup>rd</sup> Degree Tear

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** is a tear that extends into the muscle that controls the anus (the anal sphincter)

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 22. \*\*\*\*\* Emergency

[\(Home\)](#)



## 23. \*\*\*\*\* General Surgery

[\(Home\)](#)





## 24. Open Hernia Repairs / Herniorrhaphy

Inguinal - Umbilical - Incisional - Hiatus - Epigastric - Femoral – Incarcerated

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Is the surgical repair of hernias

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Matt / Megadyne Matt or Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

...

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised

## 25. Esophagectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Harmonic Scalpel  
Suction Canaster Tree

**Notes:** is a surgical procedure to remove some or all of the swallowing tube between your mouth and stomach (esophagus) and then reconstruct it using part of another organ, usually the stomach

### Operating Table and patient positioning requirements



**Position:** Supine / **Arms out / tucked in?**

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 (or both arms tucked in) / Sheet on Table (Under Patient) / Heal Gels / Head Ring Gel / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 26. Open Appendicectomy / Gastrectomy / Laparotomy / Liver Resection / Right Hemicolectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Harmonic Scalpel  
Suction Canister Tree

Notes: ...

### Operating Table and patient positioning requirements



**Position:** Supine / **Arms out / tucked in?**

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 (or both arms tucked in) / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes: .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 27. Hemicolectomy Left / Anterior Resection / Ultra-Low

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree  
Harmonic Scalpel

**Notes:** is a surgery to remove the part of your large intestine called your colon

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 28. Hemicolectomy Right

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree  
Harmonic Scalpel

**Notes:** is a surgery to remove the part of your large intestine called your colon

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Megadyne Matt or Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised

## 29. Open Splenectomy / Lap Splenectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

(If Laparoscopic Pendant Stack Moved Into position)

SCD's Machine

Bair Hugger machine

Diathermy machine

2 x Suction Canaster Trees

**Notes:** is a surgical procedure to remove your spleen

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised

## 30. Closure Ostiomiespen

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

Notes: ....

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes: .....

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 31. Lap Nissen Fundoplication

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

##### Denyer Operating Table

Pendent Stack Moved Into position

SCD's Machine

Bair Hugger machine

Diathermy machine

Suction Canaster Tree

Harmonic Scalpel

**Notes:** In this procedure, the surgeon wraps the top of the stomach around the lower oesophagus

### Operating Table and patient positioning requirements



**Position:** Lithotomy / Reverse Trendelenburg 45 Degree / Arms Out

**Setup:** ½ Gel Matt / Diathermy Plate / Arm Boards x 2 & Coban or crape bandage to secure / Table Light End / Leg Stirrups / Trenguard / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

**Notes:** Denyer Operating Table Required.

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 32. Hartman's Procedure

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree  
Harmonic Scalpel  
Thunderbeat (on the left side)

**Notes:** is a type of colectomy that removes part of the colon and sometimes rectum (proctosigmoidectomy). The remaining rectum is sealed, creating what is known as Hartmann's pouch

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out (OR Lithotomy)

**Setup:** Gel Matt / Diathermy Plate / Arm Boards x 2 (or both arms strapped) / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

If Lithotomy – Light End / Stirrups / No Heal Gels

**Notes:** .....

#### Procedural Variations

Sometimes lithotomy (check with surgical team) – If Lithotomy Light end and Stirrups required

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 33. Whipples

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree  
Harmonic Scalpel  
Thunderbeat

**Notes:** is used to treat tumours and other disorders of the pancreas, intestine and bile duct

### Operating Table and patient positioning requirements



**Position:** Supine / Left Arm Tucked In

**Setup:** Gel Matt / Diathermy Plate / Arm Boards x 2 until anaesthetised, then left arm tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 34. Anal Fistula / Fissure / Haemorrhoidectomy / Perianal Abscess / Advancement Flaps / Prolapse

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

Notes: ...

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 35. Thyroidectomy / Parathyroidectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Is the surgical removal of the Thyroid and Parathyroid glands from the neck

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Tucked In

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Gel Head Ring / Sandbag / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 36. Pilonidal Sinus V1 Lateral

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is a small hole or tunnel in the skin at the top of the buttocks, where they divide (the cleft)

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

Can be Lateral or Prone (Consult Surgical Team)

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 37. Pilonidal Sinus V2 Prone

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is a small hole or tunnel in the skin at the top of the buttocks, where they divide (the cleft)

### Operating Table and patient positioning requirements



**Position:** Prone or Lateral (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards (until Anaesthetised) / 6 Pillows / Elastoplast or Slek to secure patient / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

Can be Prone or Lateral (Consult Surgical Team)

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 38. Laparoscopic Cholecystectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
 SCD's Machine  
 Bair Hugger machine  
 Diathermy machine  
 Suction Canaster Tree

**Notes:** is the inserting of a tiny video camera and special surgical tools through four small incisions to see inside the abdomen and remove the gallbladder

### Operating Table and patient positioning requirements



**Position:** Supine / 1 Arm Tucked In

**Setup:** Gel Matt / Diathermy Plate / Arm Boards x 2 until anaesthetised, then 1 arm tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 39. Hysteroscopy / D&C / Cystoscopy / Most General Gynae / Laparoscopic Ablation of Endometriosis / Lap Assisted

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

Notes: ....

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

#### Procedural Variations

....

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised



## 40. \*\*\*\*\* Cardiac

[\(Home\)](#)



# 41. \*\*\*\*\* Neuro

[\(Home\)](#)



## 42. Craniotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements




#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is the surgical removal of part of the bone from the skull to expose the brain

### Operating Table and patient positioning requirements

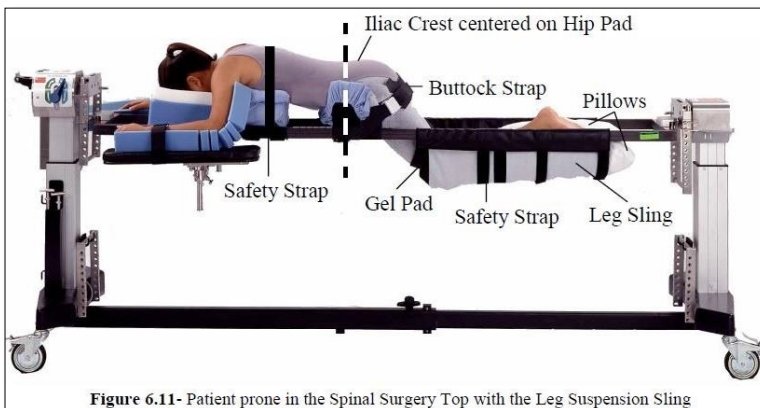

**Position:** ...

**Setup:** ...

**Notes:** .....

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 43. Burr Holes

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements




#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** are small holes that a neurosurgeon makes in the skull and are used to help relieve pressure on the brain when fluid, such as blood, builds up and starts to compress brain tissue

### Operating Table and patient positioning requirements

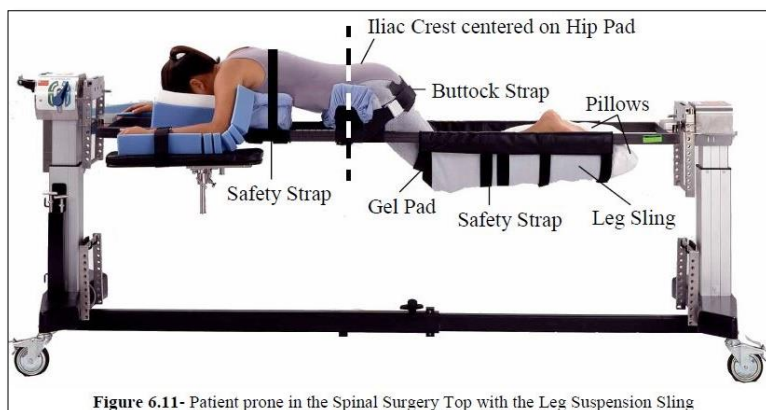

**Position:** ...

**Setup:** ...

**Notes:** .....

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 44. Transsphenoidal Pituitary (set up as FESS)

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements




#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** is a minimally invasive procedure where the pituitary tumour is removed by working through the nose

### Operating Table and patient positioning requirements

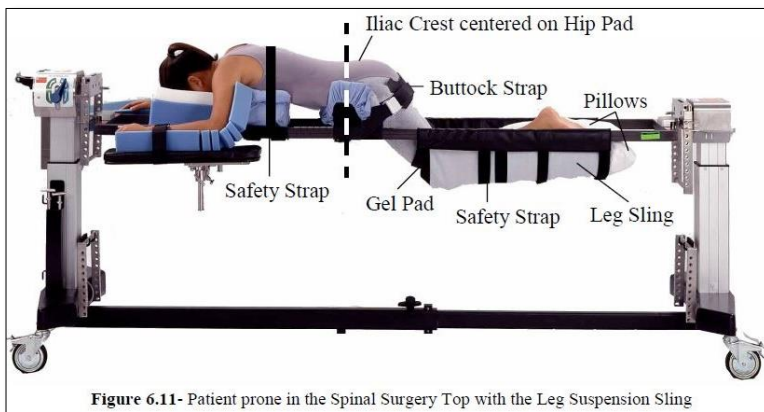

**Position:** ...

**Setup:** ...

**Notes:** .....

### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 45. Laminectomy / Microdiscectomy / Spinal Fusion

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements

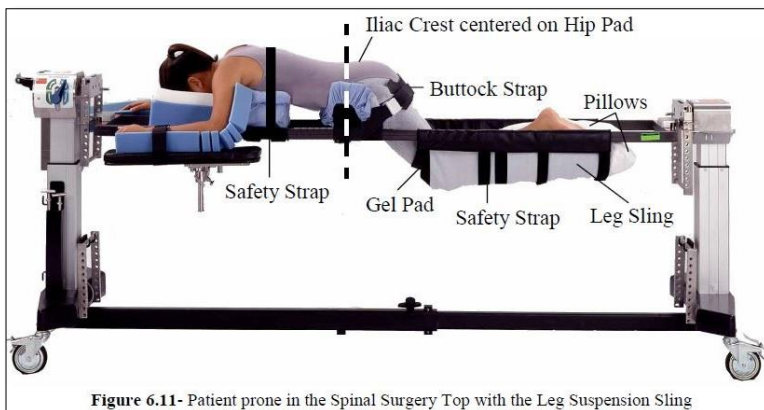


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

**Position:** ...

**Setup:** ...

**Notes:** .....

#### Procedural Variations


....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 46. Craniotomy - With Stealth

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

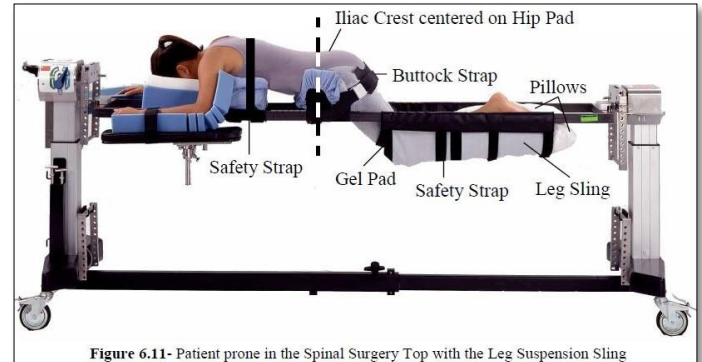


Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Mayfield/Doro Head Section w/ Skull Clamp	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do <b>NOT</b> over-tighten). Place skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile blue control plate and pointer (found in Stealth drawer) on the mayo stand with the head clamp and adjustable Medtronic arm. Attach foot pedal and position on floor at head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Only SDC required only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill remains attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. <b>Note:</b> If semi lateral Collar & Cuff will be required.



## 47. INTER-CRANIAL ANEURYSM – With Stealth

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

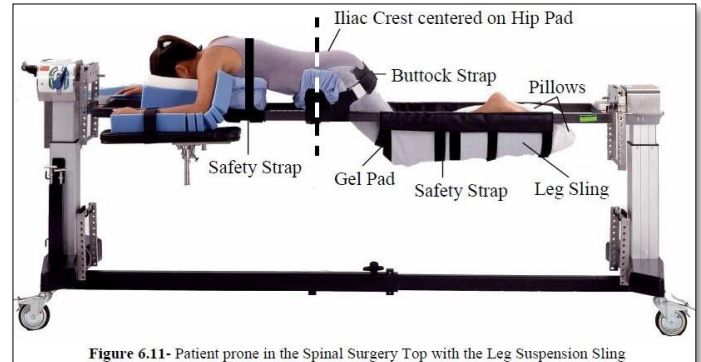


Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Doro Head Section	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do <b>NOT</b> over-tighten). Place Doro skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile blue control plate and pointer (found in Stealth drawer) on the mayo stand with the head clamp and adjustable Medtronic arm. Attach foot pedal and position on floor at head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
High Suction Unit	Fitted to anaesthetic ceiling boom. Place unit to patient's head, beside anaesthetic machine.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill remains attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Config of Tube to "Left and Right". Set User to "Infrared 800". Ensure eye piece fitted to correct side before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. <b>Note:</b> If semi lateral Collar & Cuff will be required.



## 48. Craniotomy / Shunt – With Axiom


**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

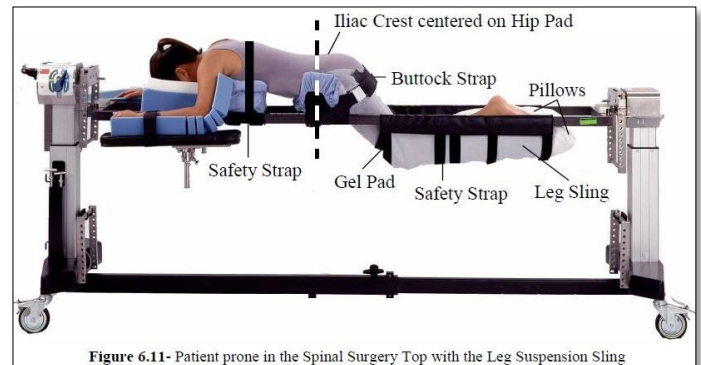

Equipment	Position and Settings
Eschmann Operating Table (Head Section Removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Mayfield/Doro Head Section w/ Horseshoe	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do <b>NOT</b> over-tighten).
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile corded tracer (found in Stealth drawer) on the mayo stand with adjustable Medtronic arm. <b>Note:</b> Use Medtronic arm with black frame attached, use tongue depressor or comb as a spacer when fitting to the Eschmann rail.
Medtronic Stealth Axiom	Hang Axiom on the foot end of the operating table, to the patient's left. Connect Axiom to Stealth system with corresponding coloured cables of which there are 3 as well as the power cord, ie: Green to green, blue to blue, etc. Connect foot pedal and position on floor to head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. SDC, camera and light box required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to be attached to IV pole behind suction unit with 1x 1L bag of room temperature sodium chloride hung above. Foot pedal to be placed at head end of operating table.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. <b>Note:</b> If semi lateral Collar & Cuff will be required.

## 49. Sub-Dural Haematoma / Burr Hole / EVD / ICP (Emergency)

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

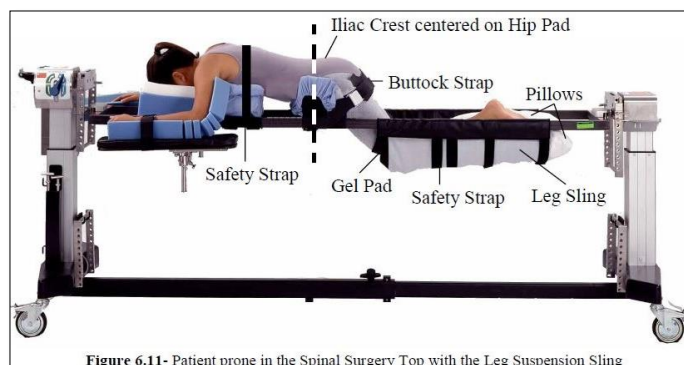

Equipment	Position and Settings
Eschmann Operating Table (Head Section Removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Mayfield/Doro Head Section w/ Horseshoe	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do <b>NOT</b> over-tighten).
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Only SDC required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. <u>Note:</u> If semi lateral Collar & Cuff will be required.

## 50. Craniotomy- Intraoperative MRI With Skull Clamp

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

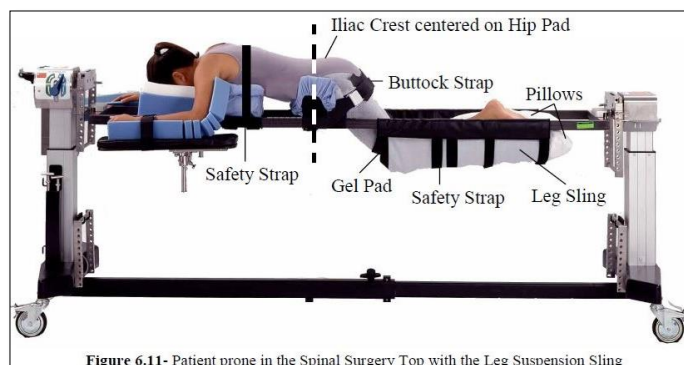


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Equipment	Position and Settings
Maquet Magnus w/ Transfer Bed and Trolley	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted.
Carbon Fibre Headset w/ Carbon Fibre Clamp (MRI Compatible Tray)	Fit square plate to head end of table with four lug screws. Use black handled 'star' screwdriver to loosen all joints. Place carbon fibre head clamp (with un-threaded centre hole) on Mayo stand with MRI safe pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Settings for Bi/Monopolar, from left to right, are as follows: 15/0/25. <b>Note:</b> Do NOT use Megadyne gel mattress for MRI transfers).
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile blue control plate, and tracer (found in Stealth drawer) on the mayo stand with the head clamp and adjustable <u>MRI compatible</u> Medtronic arm. Attach foot pedal and position on floor at head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Only SDC required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	1x Pillow, 2x MRI J boards, 2x Heel gels, Half-length gel mat, 2x Arm gels, Shoulder roll (size may vary), SCD machine, Side support w/ Leg strap required if tilting operating table, 2x MRI clearance spacers, 1x Extra Maquet knuckle and ENT arm rest found OT14 (only if ENT surgeon present), bear hugger, foam for pressure areas.



## 51. Trans-Sphenoidal Tumour Resection – Intraoperative MRI With Head Ring

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

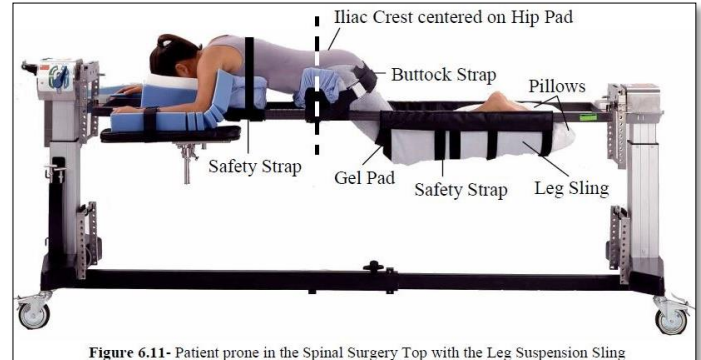



Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Equipment	Position and Settings
Maquet Magnus w/ Transfer Bed and Trolley	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Head ring placed under patient's head. <b>Note:</b> If table slide not in correct orientation, table remote will alarm when use attempted.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Settings for Bi/Monopolar, from left to right, are as follows: 15/0/25. <b>Note:</b> Do NOT use Megadyne gel mattress for MRI transfers).
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile corded tracer (found in Stealth drawer) on the mayo stand with adjustable MRI compatible Medtronic arm. <b>Note:</b> If using ENT user settings scrub team to provide unsterile metal tracer.
Medtronic Stealth Axiom	Hang Axiom on the foot end of the operating table, to the patient's left. Connect Axiom to Stealth system with corresponding coloured cables of which there are 3 as well as the power cord, ie: Green to green, blue to blue, etc. Connect foot pedal and position on floor to head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. SDC, camera and light box required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to be attached to IV pole behind suction unit with 1x 1L bag of room temperature sodium chloride hung above. Foot pedal to be placed at head end of operating table.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	1x Pillow, 2x MRI J boards, 2x Heel gels, Half-length gel mat, 2x Arm gels, Shoulder roll (size may vary), SCD machine, Side support w/ Leg strap required if tilting operating table, 2x MRI clearance spacers, 1x Extra Maquet knuckle and ENT elbow rest found OT14 (required only if ENT surgeon present), bear hugger, foam for pressure areas.



## 52. Cervical Laminectomy – With Pillows “BOWS” With Xray


**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

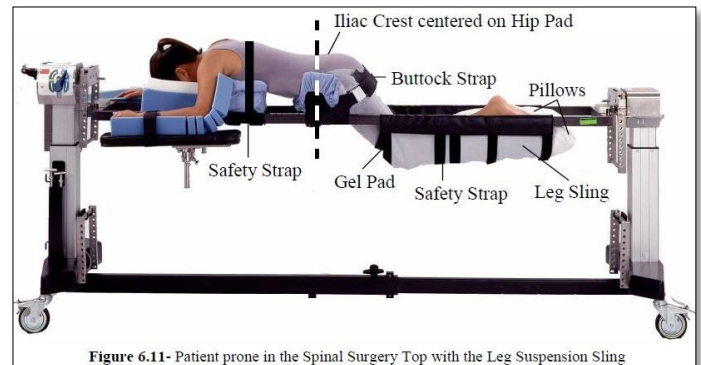

Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Arm boards removed. Sheet draped laterally across table, on top of pillows, for arm tuck. Brakes applied.
Mayfield/Doro Head Section	Fit to head end of table. Horseshoe not required. Ensure all sections secure together firmly (do <b>NOT</b> over-tighten). Place skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to “Face to Face”. Set User to “Neurosurgery User”. Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	5x Pillows (four taped together in pairs, one at the feet), 3x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas

## 53. Cervical Laminectomy – With Montreal Mattress – With Xray

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

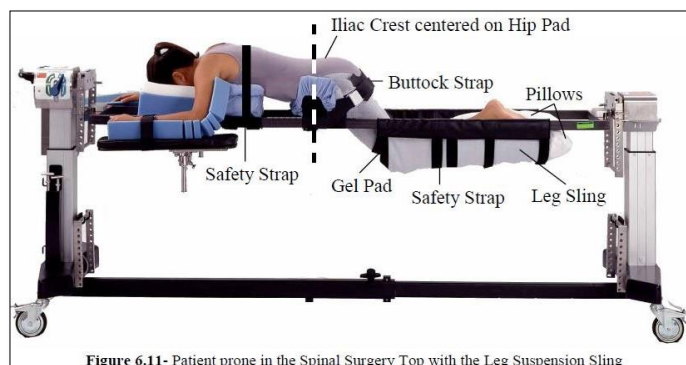

Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Arm boards removed. Sheet draped laterally across table, on top of Montreal Mattress, for arm tuck. Brakes applied.
Montreal Mattress	Placed directly onto Eschmann pads, to head end of table.
Mayfield/Doro Head Section	Fit to head end of table. Horseshoe not required. Ensure all sections secure together firmly (do <b>NOT</b> over-tighten). Place skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x Pillows, 1x sheet, 3x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas.

## 54. Cervical Laminectomy – Compress Roll – With Xray

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

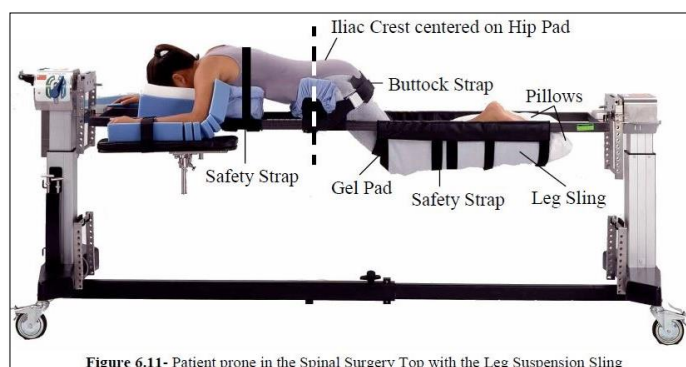


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Equipment	Position and Settings
Jackson Operating Table w/ Flat Top	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pin top "H" bar to both head end, and foot end of Jackson table. <b>Note:</b> Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Spinal Frame	Head rest and sling removed. Pre-fit frame with chest pad, Regular Patient hip pads, 2x foot plates and all Mizuno-Osi pad covers. Have 2 Jackson pins ready to fit to top "H" frame when. 6 (six) straps will be required to secure patient for the roll, these will be found with Doro Frame inside Blue "Spinal Kit" in the set-up room.
Jackson Compatible Doro Frame w/ Skull Clamp	Doro frame will secure to central "H" bar at head-end of Jackson operating table. Patient will be pinned and secured before the roll occurs.
Jackson Pad Pack	1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Jackson Table w/ Flat Top	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pin top "H" frame to head end of Jackson table. 1x bed sheet draped across for arm tuck.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	4x Pillows, 1x gel mat, 2x sheets, 3x roll of wide Elastoplast, 6x straps, SCD, bear hugger, foam for pressure areas.




## 55. Anterior Cervical Discectomy Fusion (ACDF) With Xray V1

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Li Yang

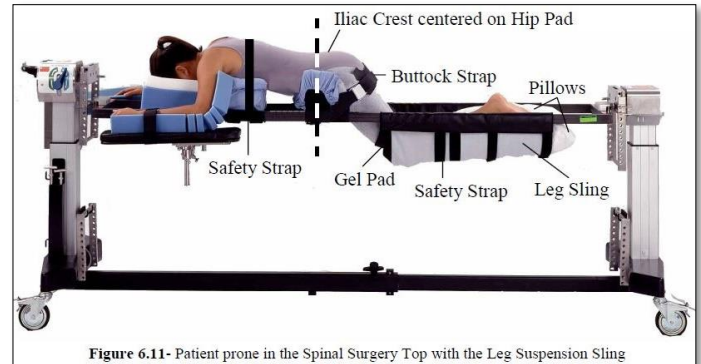

Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Arm boards removed. Sheet draped laterally across table for arm tuck. Desired head-ring placed, on absorbent pad, at head end of table. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll (size may vary), 2x arm gel, 1x sheet (arm tuck), 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas.




## 56. Anterior Cervical Discectomy Fusion (ACDF) With Xray V2

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Li Yang

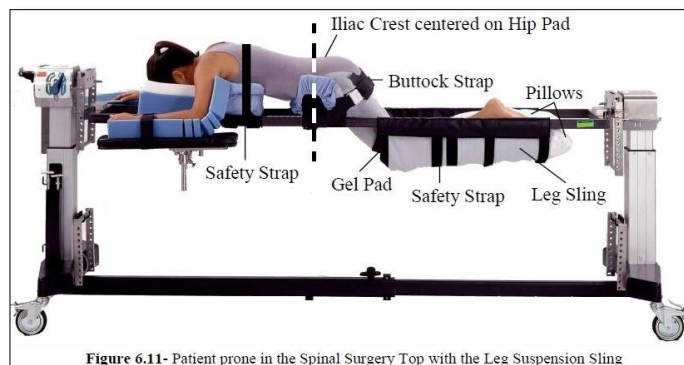


Equipment	Position and Settings
Jackson Table w/ Flat Top	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pin top "H" bar to head end of Jackson table. 1x bed sheet draped across for arm tuck. <b>Note:</b> Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll, 2x arm gel, 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas

## 57. Anterior Cervical Discectomy Fusion (ACDF) With Xray V3

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Jonathan, Dr. Stephenson & Dr. Withers

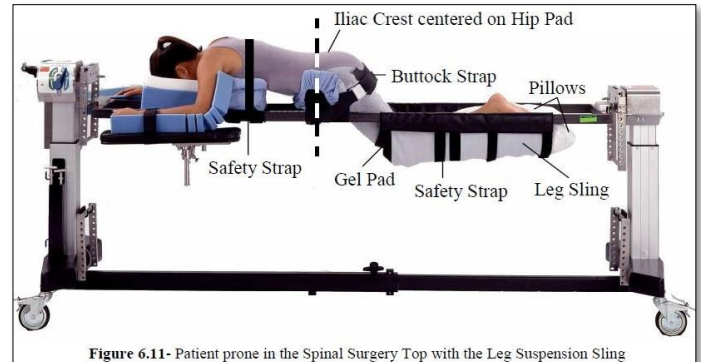


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Arm boards removed. Sheet draped laterally across table for arm tuck. Desired head-ring placed, on absorbent pad, at head end of table. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll (size may vary), 2x arm gel, 1x sheet (arm tuck), 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas

## 58. Anterior Cervical Discectomy Fusion (ACDF) With Xray V4

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Wayne Ng

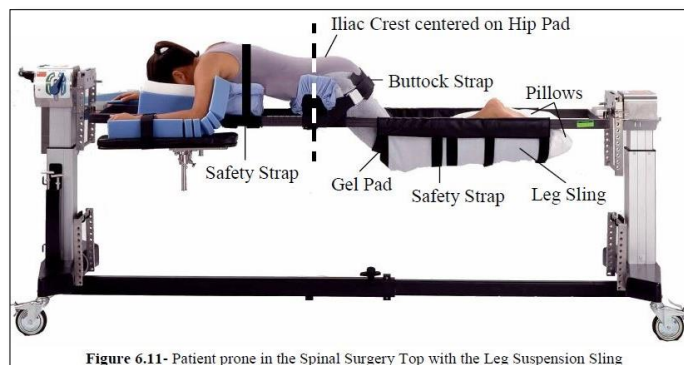

Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Arm boards removed. Sheet draped laterally across table for arm tuck. Gel head-ring placed at head end on top of absorbent pad. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll, 2x arm gel, 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas.




## 59. Anterior Cervical Discectomy Fusion (ACDF) With Xray V5

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Withers, Dr. Stephenson, Dr. Li Yang & Dr. Poulgrain

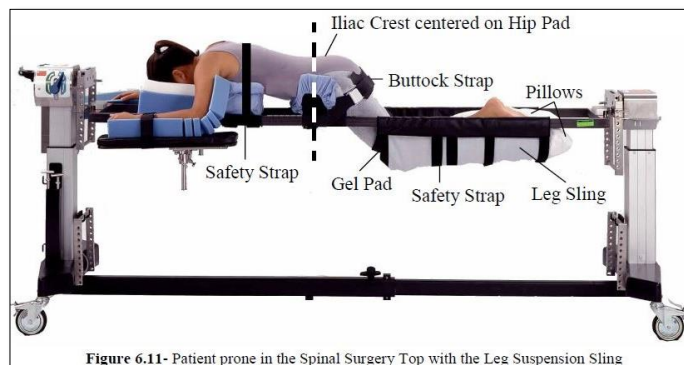

Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). <b>Note:</b> Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, chest plate, 2x regular patient pads, sling fitted with gel mattress and 3 pillows. Black Jackson knuckle to be fitted to frame for surgical retractor, confirm position with surgical registrar.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam, 1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 3x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger.




## 60. Laminectomy / Microdiscectomy – With Xray V1

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Jonathan

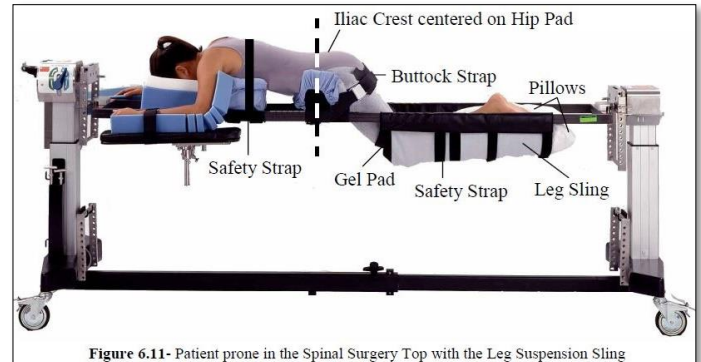


Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). <b>Note:</b> Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, chest plate, 2x thigh pads, sling fitted with gel mattress and 3 pillows. Black Jackson knuckle to be fitted to frame for surgical retractor, confirm position with surgical registrar.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam, 1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 3x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger

## 61. Laminectomy / Microdiscectomy – With Xray V2

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Wayne Ng

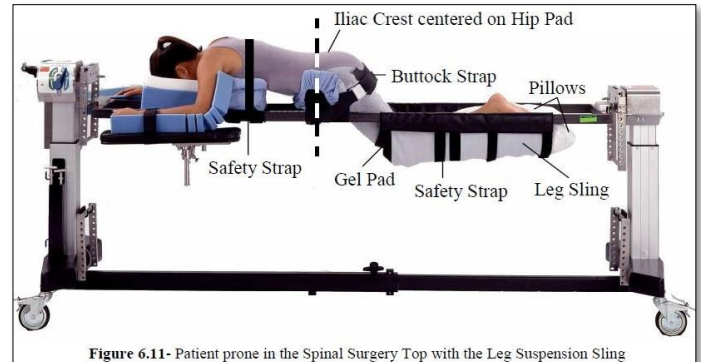


Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Head-end of spinal frame pinned at 5 <sup>th</sup> hole from the bottom of "H" bar, foot-end of spinal frame pinned at lowest hole. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). <b>Note:</b> Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, Wilson Frame, 2x foot plates with gel mattress and 2 pillows. Black Jackson knuckle to be fitted to frame for surgical retractor, confirm position with surgical registrar.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 3x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger.

## 62. Spinal Fusion (Inc TLIF) With O-Arm

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Stephenson, Dr. Wayne Ng & Dr. Li Yang

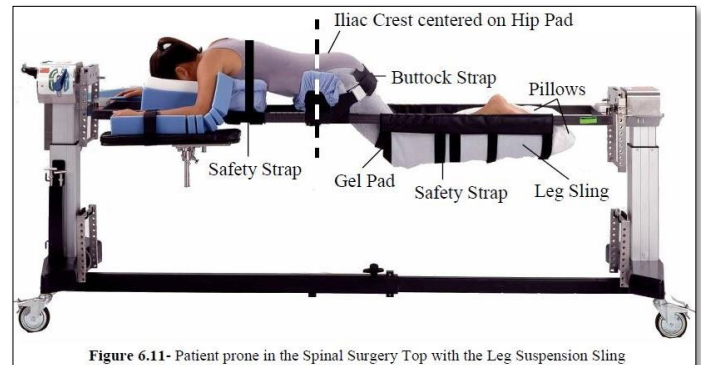

Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). <b>Note:</b> Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, chest plate, 4x regular patient pads, 2x foot plate with gel mattress and 2 pillows.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam, 1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, beside Stealth. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic Stealth	Positioned to left of theatre stack. VGA cable to connect to ANA socket on theatre stack with feed linked to Monitor 1.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 2x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger



## 63. Spinal Fusion (XLIF) With Xray

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Stephenson, Dr. Wayne Ng & Dr. Li Yang

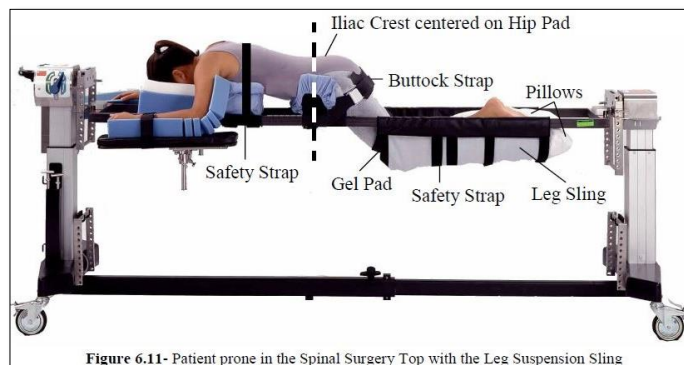


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	2x Pillows, 1x shoulder roll, 2x lateral supports, 1x arm gutter, 4x Elastoplast (wide), SCD, bear hugger, foam for pressure areas

## 64. Carpal Tunnel Repair (Right)

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** Dr. Stephenson, Dr. Wayne Ng & Dr. Li Yang

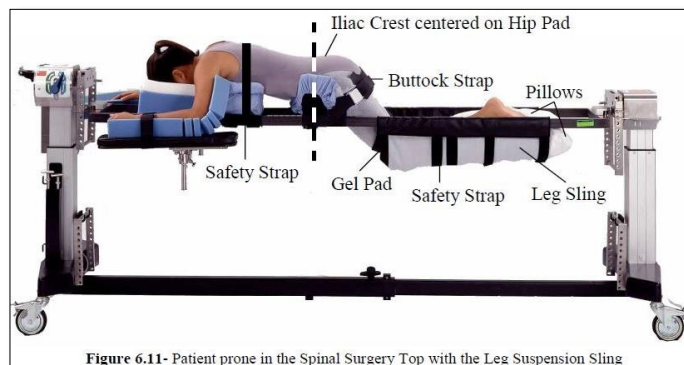


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Arm Table	To be fitted to patient's right once positioned on the bed.
Tourniquet	<b>Note:</b> Only Dr. Poulgrain will use tourniquet, and only if procedure performed under general anaesthesia.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor under arm table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Extras Required	1x Pillows, 1x shoulder roll, SCD, bear hugger, foam for pressure areas

## 65. Carpal Tunnel Repair (Left)

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



**Consultants:** All

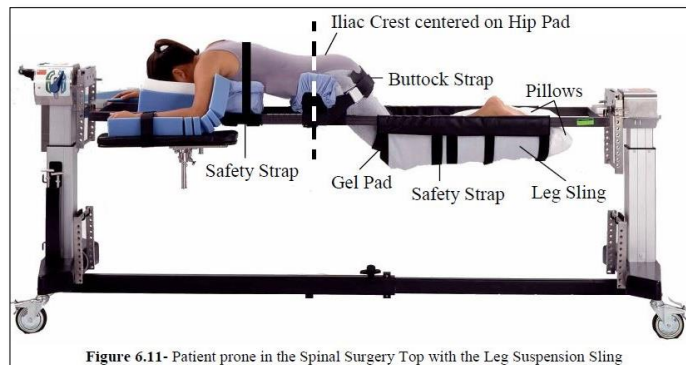

Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table laterally, from left-to-right, under ceiling light podium, with foot end towards theatre window. Arm boards removed. Brakes applied.
Arm Table	To be fitted to patient's left once positioned on the bed.
Tourniquet	<b>Note:</b> Only Dr. Poulgrain will use tourniquet, and only if procedure performed under general anaesthesia.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor under arm table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, beside Stealth. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Extras Required	1x Pillows, 2x J-boards, 1x shoulder roll, SCD, bear hugger, foam for pressure areas



## 66. \*\*\*\*\* Paediatrics

[\(Home\)](#)



## 67. \*\*\*\*\* Orthopaedics

[\(Home\)](#)



## 68. P&P / Pin and Plate / Canulated Hip Screw

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Tucked In

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 69. Archilles Tendon Repair

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Tucked In

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 70. Carpel Tunnel Release

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 71. Cubital Tunnel Release

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 72. D.P.C / Direct Primary Closure

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Tale / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 73. Dupuytren's Contracture

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Tucked In

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised

## 74. Arthroscopy Knee

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Bone Foam / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 75. M.U.A / Manipulation under Anaesthetic / Ulna - Radius

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 76. O.I.F / Open Reduction Internal Fixation / Ankle

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 77. O.I.F / Open Reduction Internal Fixation / Clavicle

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Table – Beach Chair  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Beach Chair

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 78. O.I.F / Open Reduction Internal Fixation / Distal Humorous

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 79. O.I.F / Open Reduction Internal Fixation / Proximal Humeral

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 80. O.I.F / Open Reduction Internal Fixation / Femur

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised

## 81. O.I.F / Open Reduction Internal Fixation / Olecranon / Elbow

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 82. R.C.R / Rotator Cuff Repair

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Table Beach Chair  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Beach Chair

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 83. Tendo/ Repair / Nerve Repair / Upper Limb

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 84. Tibial Plateau

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 85. T.K.R / Total Knee Replacement

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 86. T.H.R / Total Hip Replacement

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



#### Position: Lateral

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 87. Vac Dressing Change

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

**In theatre assistance requirements:**

EG: Reposition Patient once anaesthetised

## 88. \*\*\*\*\* Ophthalmic / Eyes

[\(Home\)](#)



## 89. \*\*\*\*\* Vascular

[\(Home\)](#)



## 90. A.A.A / Abdominal Aortic Aneurysm

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree  
Light Source  
Cell Saver

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 91. A.K.A / Above Knee Amputation / B.K/A / Below Knee Amputation

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 92. A.V / Arteriovenous / Fistula

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out / Arm Table

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 93. Carotid Endarterectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Tucked In

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Gel Head Ring / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 94. E.V.A.R / Endovascular Aneurysm Repair

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 95. Femoral Embolectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine / Arms Out

**Setup:** Gel Mat / Diathermy Plate / Arm Boards x 2  
/ Sheet on Table (Under Patient) / Heal Gels /  
Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 96. Fasciotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 97. F.P.B / Femoral Popliteal Bypass

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 98. Fistulotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 99. Formation of RC (Radio Cephalic) AVF (Arteria Venous Fistula)

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 100. H.L.S / High Ligation & Strip / G.S.V / Greater Saphenous Vein

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 101. Ligation & Avulsion of Veins

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 102. \*\*\*\*\* Plastics

[\(Home\)](#)





# 103. \*\*\*\*\* Maxillofacial

[\(Home\)](#)



## 104. C.A.T / Combined Approach Tympanoplasty / M.R.M / Modified Radical Meatoplasty

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 105. Tracheostomy / Dental Extractions / Bilateral Neck Dissection / Lip Split / Resection of Lesion / Radical Forearm Flap Reconstruction

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

# 106. \*\*\*\*\* E.N.T – Ear Nose and Throat

[\(Home\)](#)





## 107. Tonsillectomy / Adenoidectomy / T.S / A.S

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 108. Modified Radical Mastoidectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 109. Meatoplasty

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 110. Myringoplasty

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 111. Pre-Auricular

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 112. Tympanoplasty

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 113. Grommets

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 114. Exostosis

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 115. Microlaryngoscopy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 116. Nasopharynx Biopsy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 117. E.U.A Ear / Examination Under Microscope

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 118. Turbinectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 119. Septoplasty

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 120. Papilloma

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 121. Tracheostomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 122. Tracheotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** .....

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 123. \*\*\*\*\* Thoracic

[\(Home\)](#)



## 124. Anterior Mediastinoscopy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 125. Lobectomy / Excision of Lung Lobe

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 126. Lung Lavage

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 127. Mediastinotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 128. Pleurectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 129. Peritoneal Shunt Insertion / Pleuro

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 130. Pneumonectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 131. Thoracoscopy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 132. Thoracotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

# 133. \*\*\*\*\* Urology

[\(Home\)](#)



## 134. Circumcision

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 135. Cystectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 136. Cystoscopy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Treguard (consult surgical team)

**Notes:** May Require Treguard (Consult surgical team)

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 137. Dorsal Slit

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 138. Excision Of Bladder Endometrioma (Laparoscopically)

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** May Require Trenguard (Consult surgical team)

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 139. Hydrocele

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 140. Ileal Conduit

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 141. Stent Insertion

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** May Require Trenguard (Consult surgical team)

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 142. Laparoscopic Deroofing of Renal Cyst

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

### Procedural Variations

.....

### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 143. Lithotripsy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** May Require Trenguard (Consult surgical team)

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 144. Lithopaxy / Litholapaxy / Cisto-Litholapaxy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** May Require Trenguard (Consult surgical team)

### Procedural Variations

....

### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 145. Nephrectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 146. Nephrostomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 147. Orchidectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 148. Orchidopexy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 149. Percutaneous Nephrolithotomy / P.C.N.L

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** May Require Trenguard (Consult surgical team)

#### Procedural Variations

Starting in Lithotomy – Then Going Prone

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 150. Prostatectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 151. Radical Cystectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Treguard (consult surgical team)

**Notes:** May Require Treguard (Consult surgical team)

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 152. Torsion of Testes

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 153. T.U.R.B.T / Trans Urethral Resection of Bladder Tumour

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Treguard (consult surgical team)

**Notes:** May Require Treguard (Consult surgical team)

#### Procedural Variations

....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 154. T.U.R.P / Trans Urethral Resection Prostatectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



### In Room Equipment:

Pendent Stack Moved Into position  
SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lithotomy/ Arms Tucked In

**Setup:** ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

**Notes:** May Require Trenguard (Consult surgical team)

### Procedural Variations

....

### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised



## 155. Ureterolithotomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canaster Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Lateral or Prone (ask surgeon)

**Setup - Lateral:** Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

## 156. Vasectomy

**(Home) Important:** Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

### In Theatre Requirements



#### In Room Equipment:

SCD's Machine  
Bair Hugger machine  
Diathermy machine  
Suction Canister Tree

**Notes:** Position Pendant Lights:

### Operating Table and patient positioning requirements



**Position:** Supine

**Setup:** ...

**Notes:** .....

#### Procedural Variations

.....

#### In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

# 157. \*\*\*\*\* Colorectal

[\(Home\)](#)



## 158. \*\*\*\*\* Dental

[\(Home\)](#)





# 159. \*\*\*\*\* E.C.T / Electroconvulsive Therapy

[\(Home\)](#)



# 160. \*\*\*\*\* Revision Status

[\(Home\)](#)

## Version History

Version	Date	Updated By	Reason For Update
1.0	16/02/2023	288729 - Mr Anton Vick	Creation