

Endoscopy


Environmental Set-up Guide



Contents

1. Endoscopy Theatre 1 - Gastroscopy	3
2. Endoscopy Theatre 1 - Colonoscopy	3
3. Endoscopy Theatre 1 – Bronc / EBUS	4
4. Endoscopy Theatre 1 – Bronchoscopy	4
5. Endoscopy Theatre 1 – Radial EBUS	5
6. Endoscopy Theatre 2 – Colonoscopy	5
7. Endoscopy Theatre 2 – Gastroscopy	6
8. Endoscopy Theatre 2 – Enteroscopy	6
9. Endoscopy Theatre 3 – Colonoscopy	7
10. Endoscopy Theatre 3 – Gastroscopy	7
11. Endoscopy Theatre 3 – EUS	8
12. Endoscopy Theatre 4 – Colonoscopy	8
13. Endoscopy Theatre 4 – Gastroscopy	9
14. Endoscopy Theatre 4 – EUS / FNA	9
15. Endoscopy Theatre 4 – Enteroscopy	10
16. Endoscopy Theatre 4 – ERCP	10


1. Endoscopy Theatre 1 - Gastroscopy

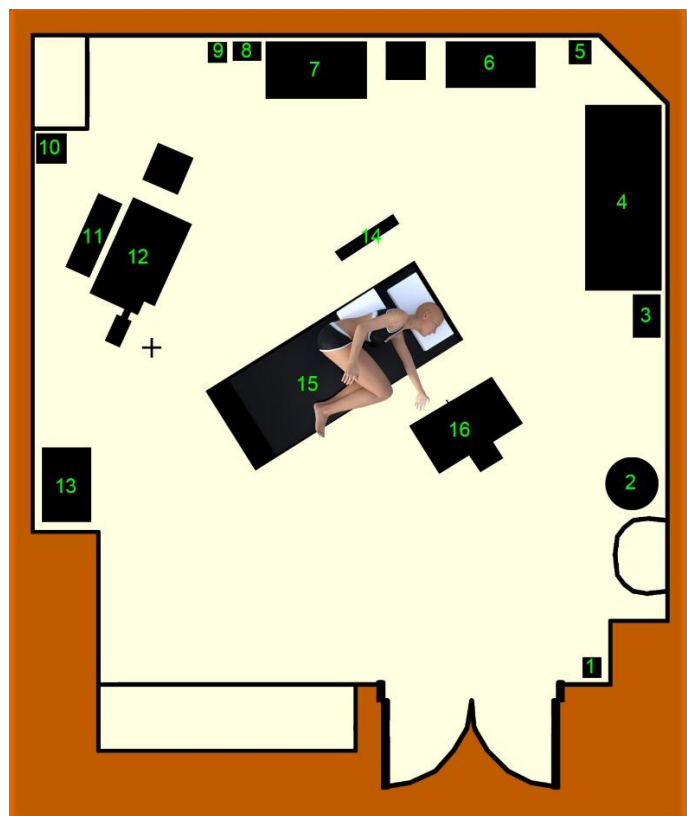

ENDOSCOPY Theatre 1

GASTROSCOPY

- 1 - Small Waste Bin
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - Large Sharps Container
- 6 - S/Steel Trolley
- 7 - Anasthetics Cart
- 8 - Standard Sharps Container
- 9 - Small Waste Bin
- 10 - Drug Safe
- 11 - Utilities Pendant
- 12 - Anasthetics Machine
- 13 - Anaesthetics Airway Trolley
- 14 - Pendant Monitor
- 15 - Patient Trolley / Bed
- 16 - Camera Pendant

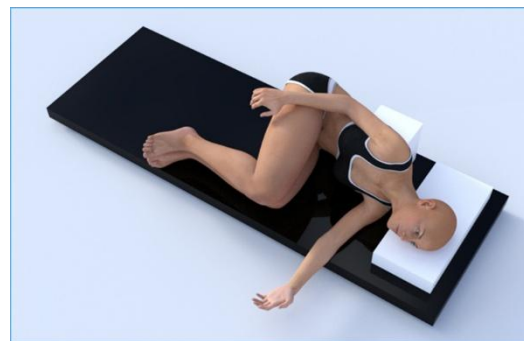

Requirements


Head - Pillow (Standard)

Head - Absorbant Pad

Back - Pillow Standard

Underbody - Slide Sheet (conditional)

2. Endoscopy Theatre 1 - Colonoscopy

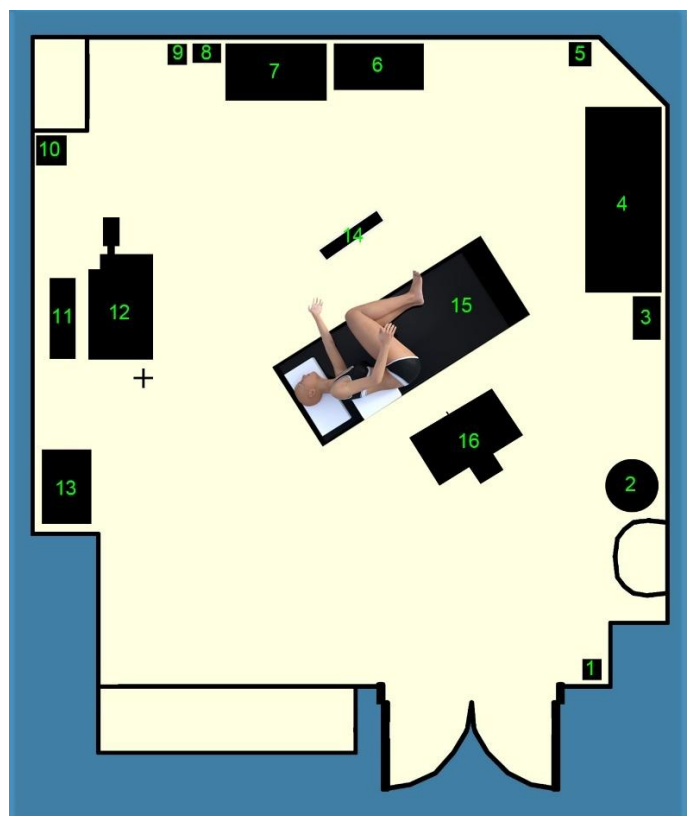

ENDOSCOPY Theatre 1

COLONOSCOPY

- 1 - Small Waste Bin
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - Large Sharps Container
- 6 - S/Steel Trolley
- 7 - Anasthetics Cart
- 8 - Standard Sharps Container
- 9 - Small Waste Bin
- 10 - Drug Safe
- 11 - Utilities Pendant
- 12 - Anasthetics Machine
- 13 - Anaesthetics Airway Trolley
- 14 - Pendant Monitor
- 15 - Patient Trolley / Bed
- 16 - Camera Pendant



Requirements


Head - Pillow (Standard)

Waist - Safety Belt

Buttocks - Absorbant Pad

Underbody - Slide Sheet

3. Endoscopy Theatre 1 – Bronc / EBUS

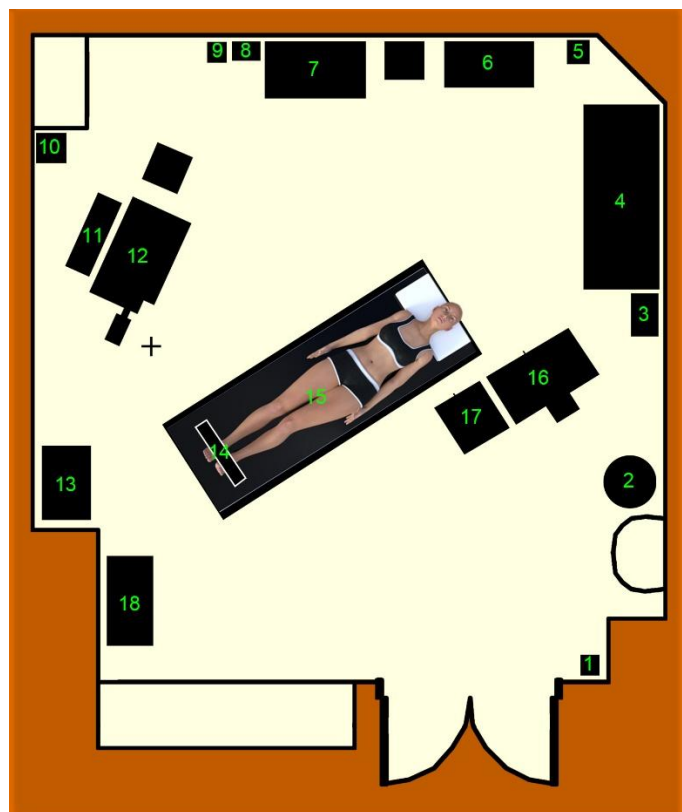


ENDOSCOPY Theatre 1

BRONC / EBUS

Bronchoscopy / Endoscopic
Bronchial Ultrasound


- 1 - Small Waste Bin
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - Large Sharps Container
- 6 - S/Steel Trolley
- 7 - Anesthetics Cart
- 8 - Standard Sharps Container
- 9 - Small Waste Bin
- 10 - Drug Safe
- 11 - Utilities Pendant
- 12 - Anesthetics Machine
- 13 - Anaesthetics Airway Trolley
- 14 - Pendant Monitor
- 15 - Patient Trolley / Bed
- 16 - Camera Pendant
- 17 - EUS / Ultrasound
- 18 - Microscope Trolley

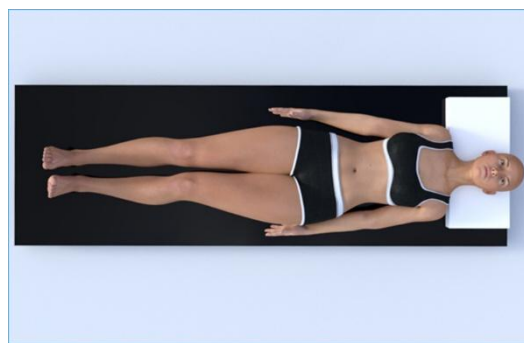

Requirements

Head - Pillow (Standard)

4. Endoscopy Theatre 1 – Bronchoscopy

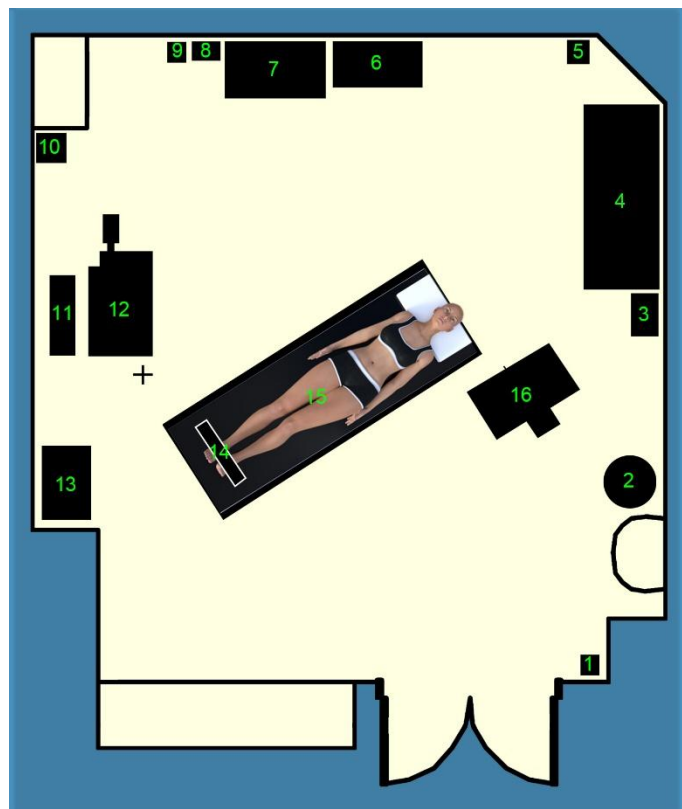


ENDOSCOPY Theatre 1

BRONC

Bronchoscopy


- 1 - Small Waste Bin
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - Large Sharps Container
- 6 - S/Steel Trolley
- 7 - Anesthetics Cart
- 8 - Standard Sharps Container
- 9 - Small Waste Bin
- 10 - Drug Safe
- 11 - Utilities Pendant
- 12 - Anesthetics Machine
- 13 - Anaesthetics Airway Trolley
- 14 - Pendant Monitor
- 15 - Patient Trolley / Bed
- 16 - Camera Pendant

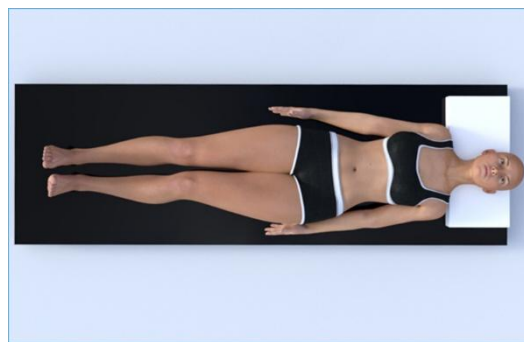

Requirements

Head - Pillow (Standard)

5. Endoscopy Theatre 1 – Radial EBUS

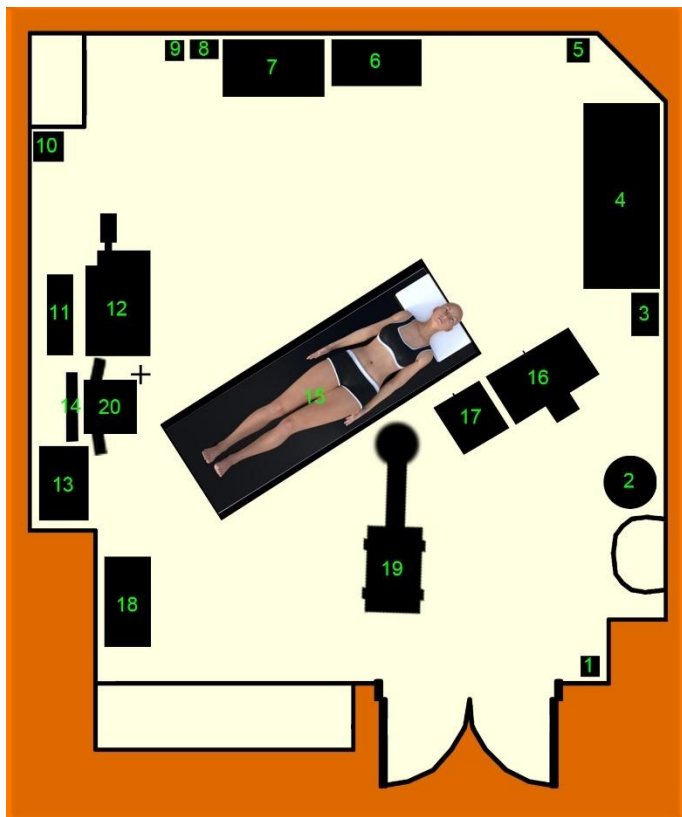


ENDOSCOPY Theatre 1

Radial EBUS

Bronchoscopy / Endoscopic
Bronchial Ultrasound using
X-Ray


- 1 - Small Waste Bin
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - Large Sharps Container
- 6 - S/Steel Trolley
- 7 - Anaesthetics Cart
- 8 - Standard Sharps Container
- 9 - Small Waste Bin
- 10 - Drug Safe
- 11 - Utilities Pendant
- 12 - Anaesthetics Machine
- 13 - Anaesthetics Airway Trolley
- 14 - Pendant Monitor
- 15 - Patient Trolley / Bed
- 16 - Camera PendantE
- 17 - US / Ultrasound
- 18 - Microscope Trolley
- 19 - II C Arm
- 20 - II Monitor

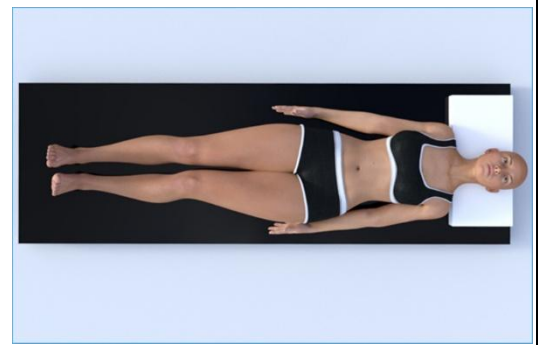

Requirements

Head - Pillow (Standard)


6. Endoscopy Theatre 2 – Colonoscopy

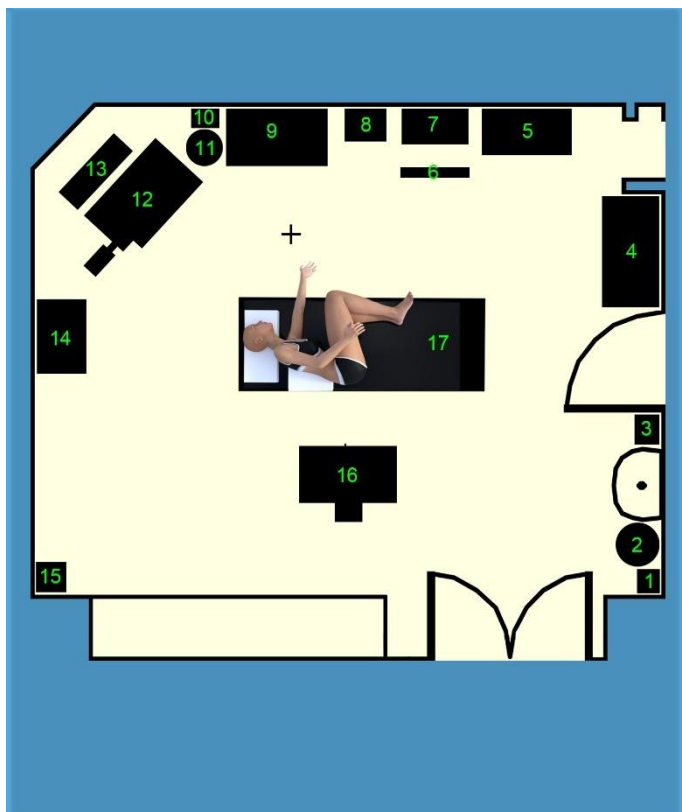

ENDOSCOPY Theatre 2

COLONOSCOPY


- 1 - Standard Sharps Container
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - S/Steel Trolley
- 6 - Pendant Monitor
- 7 - COW
- 8 - Diathermy Machine
- 9 - Anaesthetics Cart
- 10 - Large Sharps Container
- 11 - Large Waste Bin
- 12 - Anaesthetics Machine
- 13 - Utilities Pendant
- 14 - Anaesthetics Airway Trolley
- 15 - Drug Safe
- 16 - Olympus Camera Pendant
- 17 - Patient Trolley / Bed

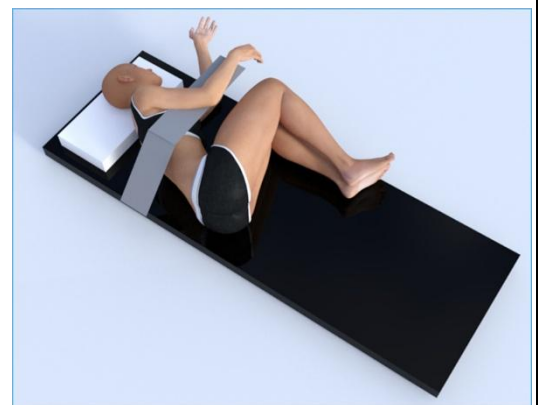

Requirements

Head - Pillow (Standard)
Waist - Safety Belt
Buttocks - Absorbant Pad
Underbody - Slide Sheet

7. Endoscopy Theatre 2 – Gastroscopy

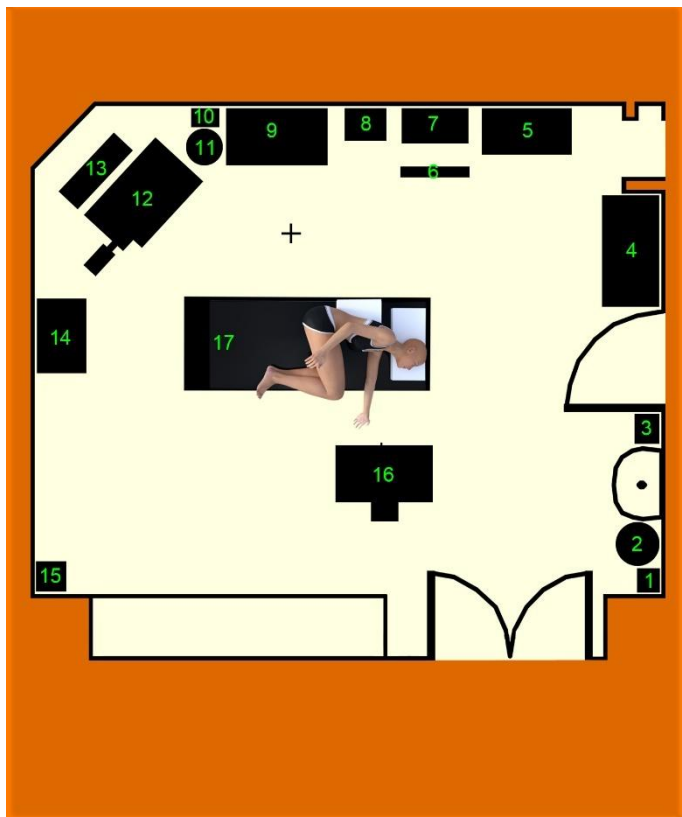

ENDOSCOPY Theatre 2

GASTROSCOPY


- 1 - Standard Sharps Container
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - S/Steel Trolley
- 6 - Pendant Monitor
- 7 - COW
- 8 - Diathermy Machine
- 9 - Anasthetics Cart
- 10 - Large Sharps Container
- 11 - Large Waste Bin
- 12 - Anasthetics Machine
- 13 - Utilities Pendant
- 14 - Anaesthetics Airway Trolley
- 15 - Drug Safe
- 16 - Camera Pendant
- 17 - Patient Trolley / Bed



Requirements

Head - Pillow (Standard)
 Head - Absorbant Pad
 Back - Pillow Standard
 Underbody - Slide Sheet (conditional)


8. Endoscopy Theatre 2 – Enteroscopy

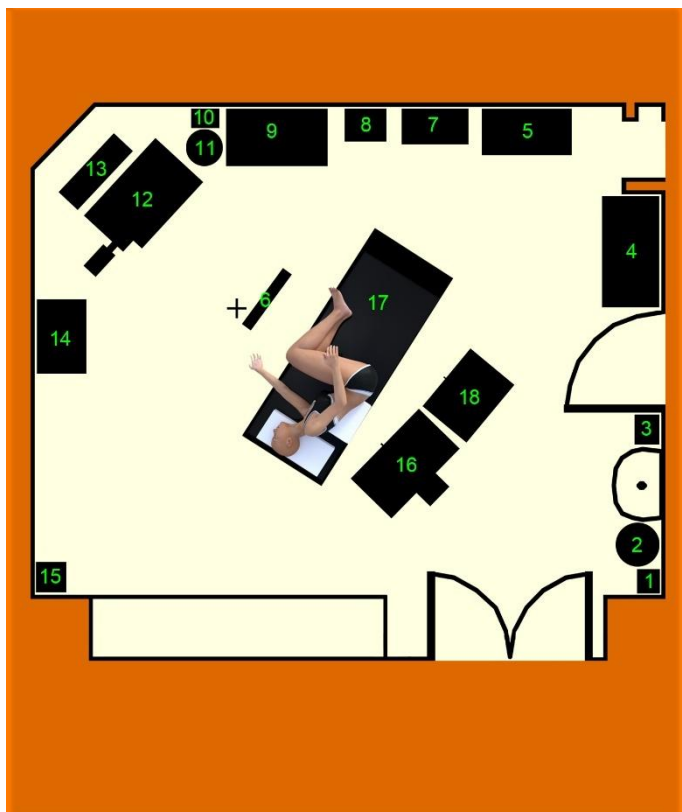

ENDOSCOPY Theatre 2

ENTEROSCOPY


- 1 - Standard Sharps Container
- 2 - Large Waste Bin
- 3 - Biological Waste Bin
- 4 - Camera Accessory Cupboard
- 5 - S/Steel Trolley
- 6 - Pendant Monitor
- 7 - COW
- 8 - Diathermy Machine
- 9 - Anasthetics Cart
- 10 - Large Sharps Container
- 11 - Large Waste Bin
- 12 - Anasthetics Machine
- 13 - Utilities Pendant
- 14 - Anaesthetics Airway Trolley
- 15 - Drug Safe
- 16 - Olympus Camera Pendant
- 17 - Patient Trolley / Bed
- 18 - Enteroscope Machine

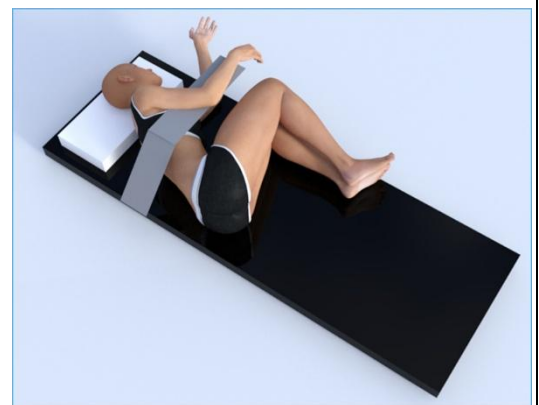

Requirements

Head - Pillow (Standard)
 Waist - Safety Belt
 Buttocks - Absorbant Pad
 Underbody - Slide Sheet


9. Endoscopy Theatre 3 – Colonoscopy

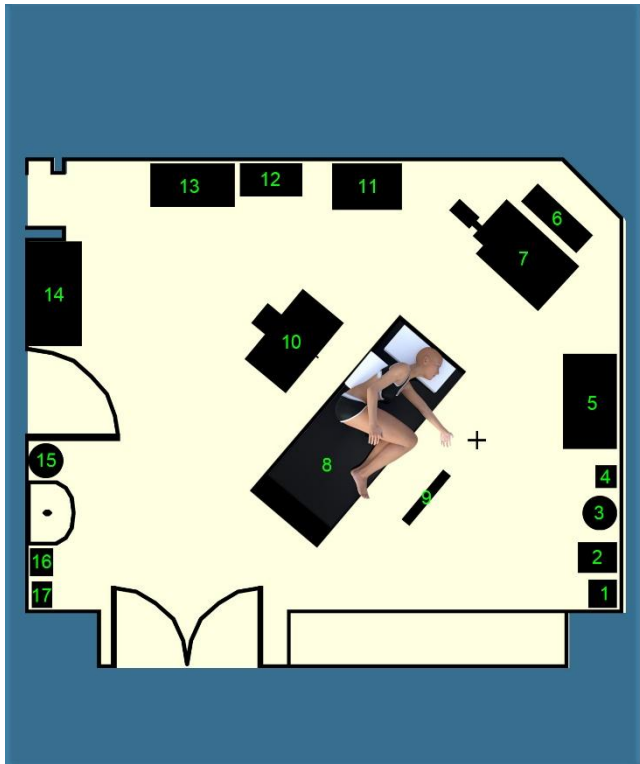

ENDOSCOPY Theatre 3

COLONOSCOPY


- 1 - Drug Safe
- 2 - Diathermy Machine
- 3 - Large Waste Bin
- 4 - Standard Sharps Container
- 5 - Anesthetics Cart
- 6 - Utilities Pendant
- 7 - Anesthetics Machine
- 8 - Patient Trolley / Bed
- 9 - Pendant Monitor
- 10 - Olympus Camera Pendant
- 11 - Anaesthetics Airway Trolley
- 12 - COW
- 13 - S/Steel Trolley
- 14 - Camera Accessory Cupboard
- 15 - Large Waste Bin
- 16 - Biological Waste Bin
- 17 - Large Sharps Container

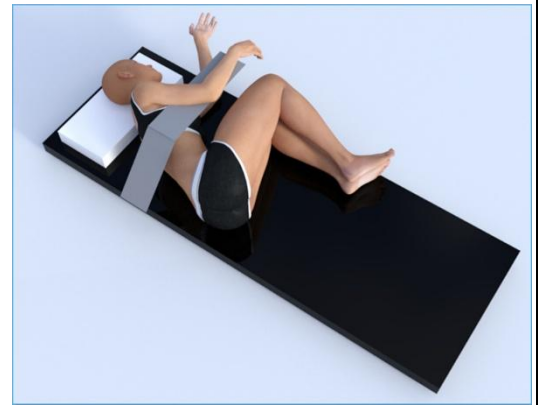

Requirements

Head - Pillow (Standard)
Waist - Safety Belt
Buttocks - Absorbant Pad
Underbody - Slide Sheet


10. Endoscopy Theatre 3 – Gastroscopy

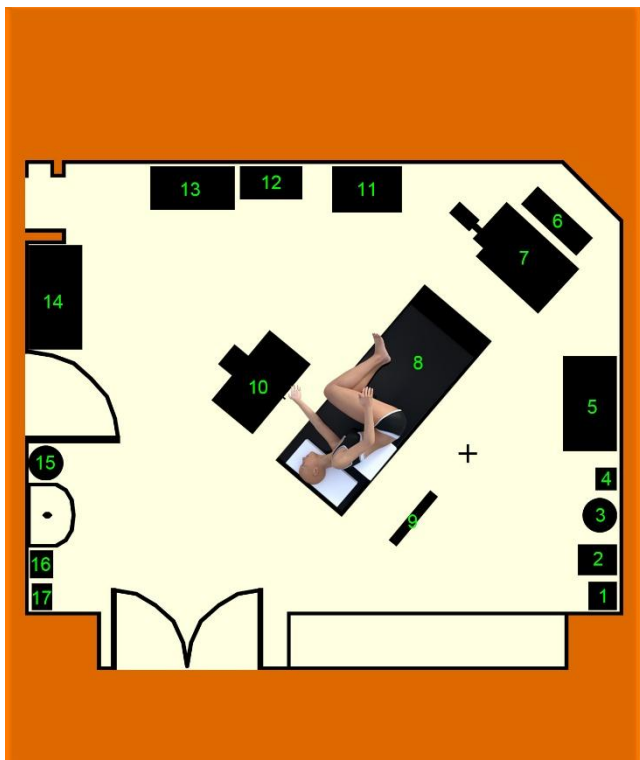

ENDOSCOPY Theatre 3

GASTROSCOPY


- 1 - Drug Safe
- 2 - Diathermy Machine
- 3 - Large Waste Bin
- 4 - Standard Sharps Container
- 5 - Anesthetics Cart
- 6 - Utilities Pendant
- 7 - Anesthetics Machine
- 8 - Patient Trolley / Bed
- 9 - Pendant Monitor
- 10 - Olympus Camera Pendant
- 11 - Anaesthetics Airway Trolley
- 12 - COW
- 13 - S/Steel Trolley
- 14 - Camera Accessory Cupboard
- 15 - Large Waste Bin
- 16 - Biological Waste Bin
- 17 - Large Sharps Container

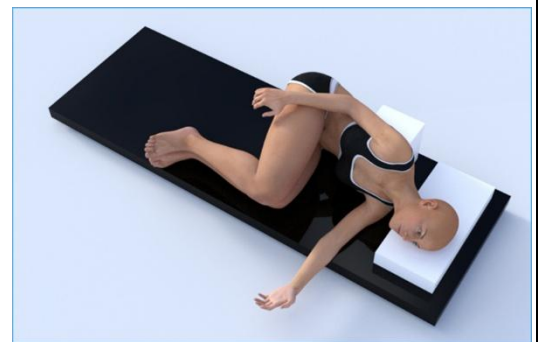

Requirements

Head - Pillow (Standard)
Head - Absorbant Pad
Back - Pillow Standard
Underbody - Slide Sheet (conditional)

11. Endoscopy Theatre 3 – EUS

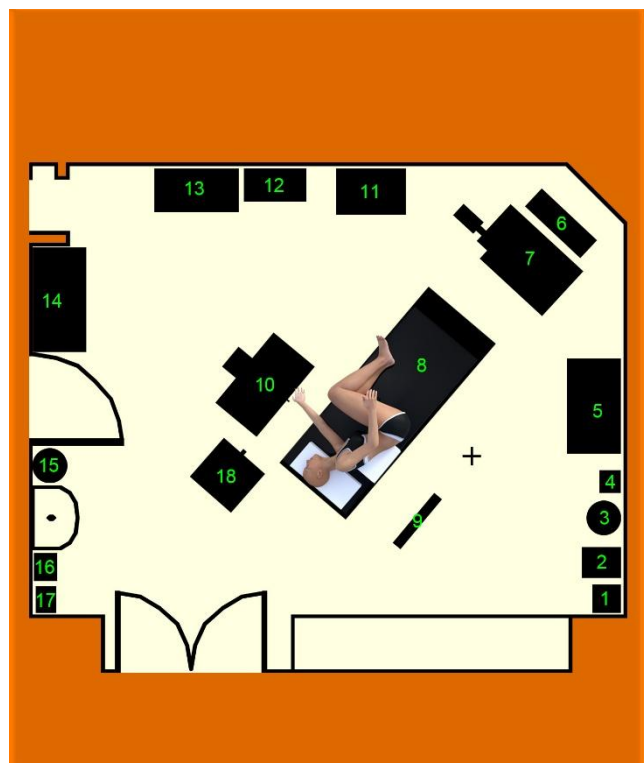


ENDOSCOPY Theatre 3

GASTROSCOPY - EUS

Endoscopic Ultrasound

- 1 - Drug Safe
- 2 - Diathermy Machine
- 3 - Large Waste Bin
- 4 - Standard Sharps Container
- 5 - Anasthetics Cart
- 6 - Utilities Pendant
- 7 - Anasthetics Machine
- 8 - Patient Trolley / Bed
- 9 - Pendant Monitor
- 10 - Olympus Camera Pendant
- 11 - Anaesthetics Airway Trolley
- 12 - COW
- 13 - S/Steel Trolley
- 14 - Camera Accessory Cupboard
- 15 - Large Waste Bin
- 16 - Biological Waste Bin
- 17 - Large Sharps Container
- 18 - EUS

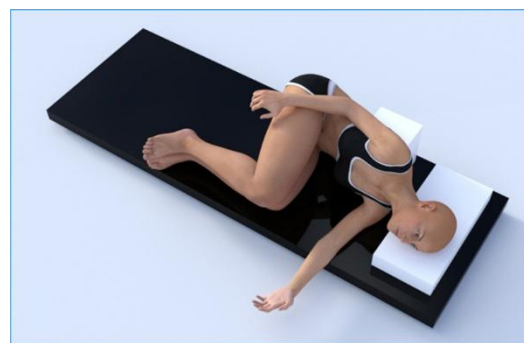

Requirements


Head - Pillow (Standard)

Head - Absorbant Pad

Back - Pillow Standard

Underbody - Slide Sheet (conditional)


12. Endoscopy Theatre 4 – Colonoscopy

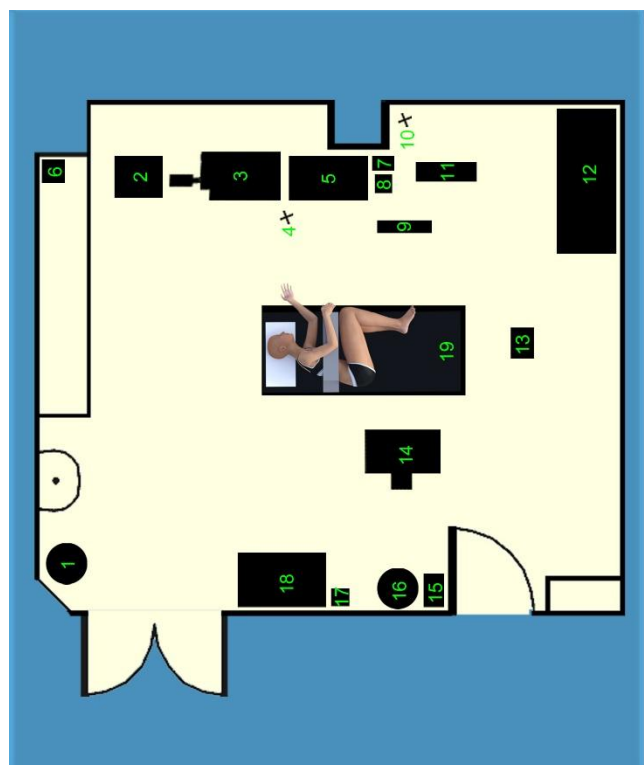

ENDOSCOPY Theatre 4

COLONOSCOPY

- 1 - Large Waste Bin
- 2 - Anaesthetics Airway Trolley
- 3 - Anasthetics Machine
- 4 - Syringe Driver & Fluids Pole
- 5 - Anaesthetics Cart
- 6 - Drug Safe
- 7 - Standard Sharps Container
- 8 - Small Waste Bin
- 9 - Pendant Monitor
- 10 - Fluids Pole
- 11 - Utilities Pendant
- 12 - Camera Accessory Cupboard
- 13 - Diathermy Machine
- 14 - Camera Pendant
- 15 - Biological Waste Bin
- 16 - Large Waste Bin
- 17 - Large Sharps Container
- 18 - Nurses Cupboard
- 19 - Patient Trolley / Bed

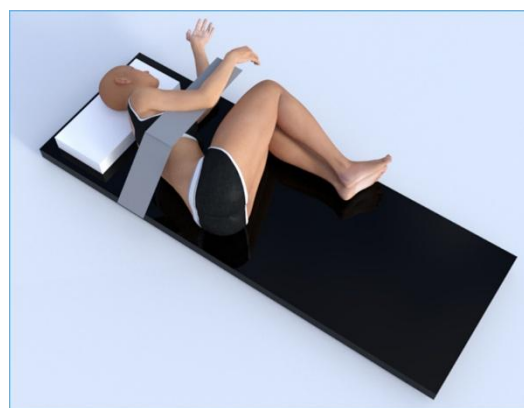

Requirements


Head - Pillow (Standard)

Waist - Safety Belt

Buttocks - Absorbant Pad

Underbody - Slide Sheet


13. Endoscopy Theatre 4 – Gastroscopy

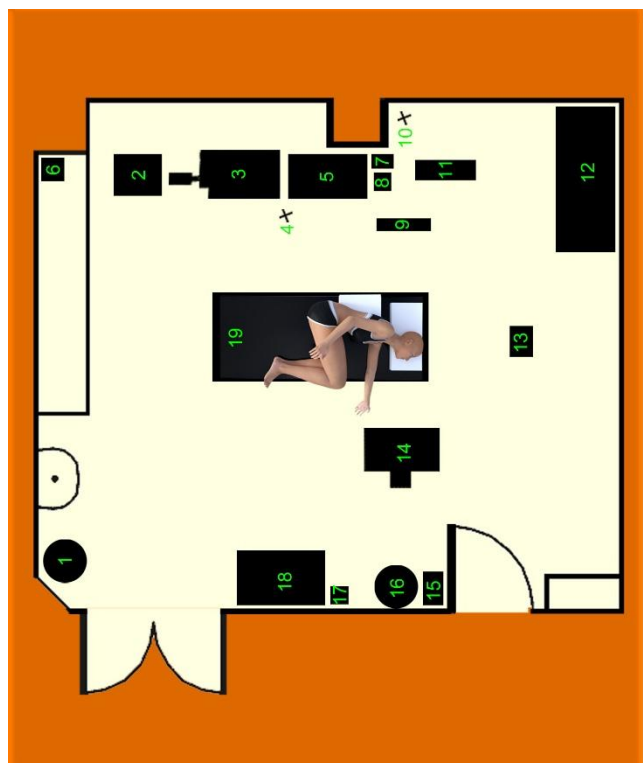

ENDOSCOPY Theatre 4

GASTROSCOPY

- 1 - Large Waste Bin
- 2 - Anaesthetics Airway Trolley
- 3 - Anaesthetics Machine
- 4 - Syringe Driver & Fluids Pole
- 5 - Anaesthetics Cart
- 6 - Drug Safe
- 7 - Standard Sharps Container
- 8 - Small Waste Bin
- 9 - Pendant Monitor
- 10 - Fluids Pole
- 11 - Utilities Pendant
- 12 - Camera Accessory Cupboard
- 13 - Diathermy Machine
- 14 - Camera Pendant
- 15 - Biological Waste Bin
- 16 - Large Waste Bin
- 17 - Large Sharps Container
- 18 - Nurses Cupboard
- 19 - Patient Trolley / Bed

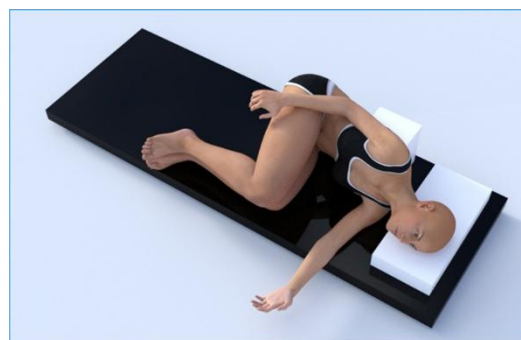

Requirements


Head - Pillow (Standard)

Head - Absorbant Pad

Back - Pillow Standard

Underbody - Slide Sheet (conditional)

14. Endoscopy Theatre 4 – EUS / FNA

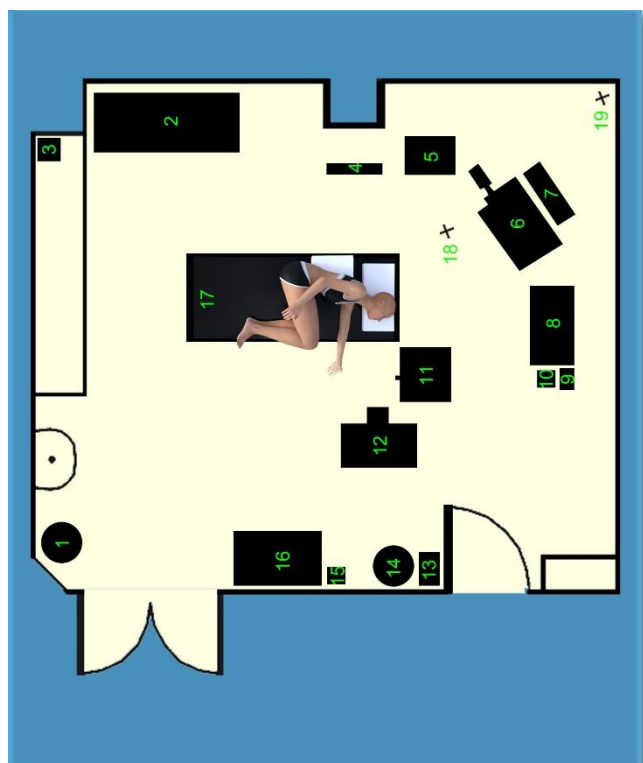


ENDOSCOPY Theatre 4

EUS & FNA

Endoscopic Ultrasound & Fine Needle Aspiration

- 1 - Large Waste Bin
- 2 - Camera Accessory Cupboard
- 3 - Drug Safe
- 4 - Pendant Monitor
- 5 - Anaesthetics Airway Trolley
- 6 - Anaesthetics Machine
- 7 - Utilities Pendant
- 8 - Anaesthetics Cart
- 9 - Standard Sharps Container
- 10 - Small Waste Bin
- 11 - EUS (Ultrasound)
- 12 - Camera Pendant
- 13 - Biological Waste Bin
- 14 - Large Waste Bin
- 15 - Large Sharps Container
- 16 - Nurses Cupboard
- 17 - Patient Trolley / Bed
- 18 - Syringe Driver & Fluids Pole
- 19 - Fluids Pole

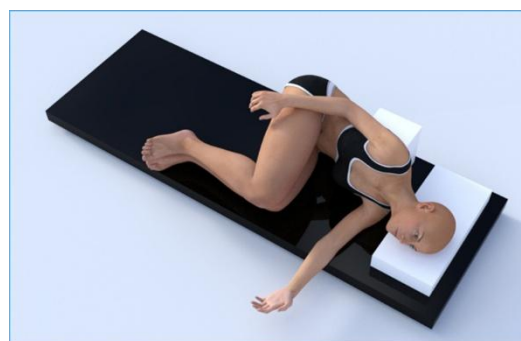

Requirements


Head - Pillow (Standard)

Head - Absorbant Pad

Back - Pillow Standard

Underbody - Slide Sheet (conditional)


15. Endoscopy Theatre 4 – Enteroscopy

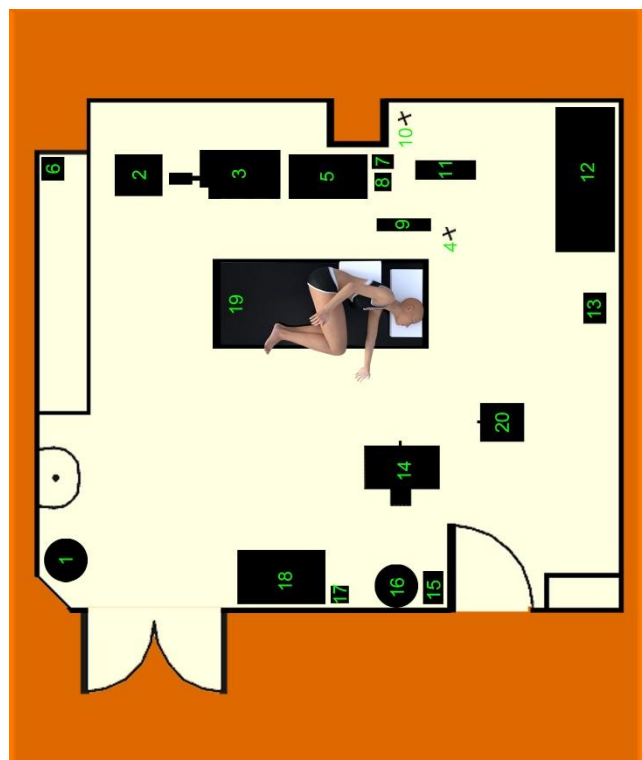

ENDOSCOPY Theatre 4

ENTEROSCOPY


- 1 - Large Waste Bin
- 2 - Anaesthetics Airway Trolley
- 3 - Anaesthetics Machine
- 4 - Syringe Driver & Fluids Pole
- 5 - Anaesthetics Cart
- 6 - Drug Safe
- 7 - Standard Sharps Container
- 8 - Small Waste Bin
- 9 - Pendant Monitor
- 10 - Fluids Pole
- 11 - Utilities Pendant
- 12 - Camera Accessory Cupboard
- 13 - Diathermy Machine
- 14 - Camera Pendant
- 15 - Biological Waste Bin
- 16 - Large Waste Bin
- 17 - Large Sharps Container
- 18 - Nurses Cupboard
- 19 - Patient Trolley / Bed
- 20 - Enteroscope

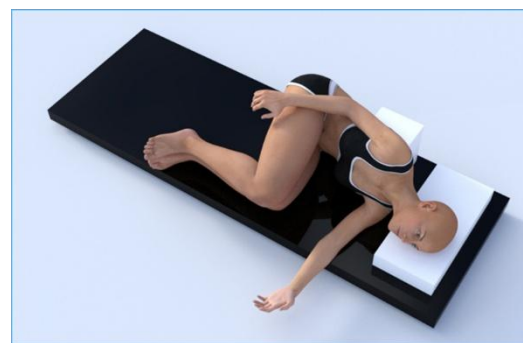

Requirements

Head - Pillow (Standard)
 Head - Absorbant Pad
 Back - Pillow Standard
 Underbody - Slide Sheet (conditional)

16. Endoscopy Theatre 4 – ERCP

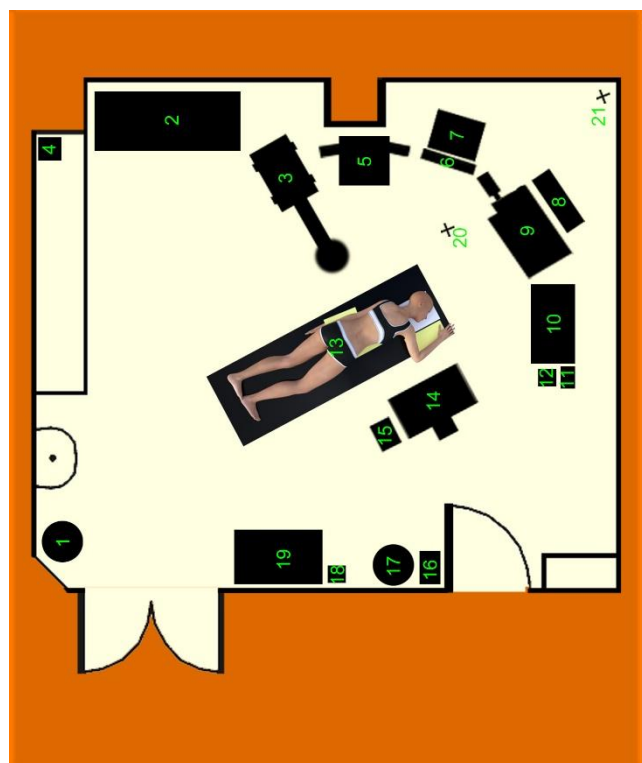

ENDOSCOPY Theatre 4

ERCP

Endoscopic Retrograde Cholangiopancreatography

- 1 - Large Waste Bin
- 2 - Camera Accessory Cupboard
- 3 - II C-Arm
- 4 - Drug Safe
- 5 - II Processor
- 6 - Pendant Monitor
- 7 - Anaesthetics Airway Trolley
- 8 - Utilities Pendant
- 9 - Anaesthetics Machine
- 10 - Anaesthetics Cart
- 11 - Standard Sharps Container
- 12 - Small Waste Bin
- 13 - Patient Trolley / Bed
- 14 - Camera Pendant
- 15 - Diathermy Machine
- 16 - Biological Waste Bin
- 17 - Large Waste Bin
- 18 - Large Sharps Container
- 19 - Nurses Cupboard
- 20 - Syringe Driver & Fluids Pole
- 21 - Fluids Pole



Requirements

Underbody - Slide Sheet
 Head - Pillow (Small / Slimline)
 Head - Absorbant Pad
 Arm Front - Gell Pad
 Arm - Rear - Gell Pad
 Stomach - Gell Roll