



**CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS
MAINTAINED IN THE REGULAR COURSE OF BUSINESS**

I, Steven J. Carluccio, Highway Safety Equipment Technical Supervisor, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NATL PATENT ANALYTICAL SYSTEM, DATAMASTER DMT breath test instrument, serial number 113808, performed on July 20, 2022 by Office of Public Safety employee George Coffin, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Steven J. Carluccio".

Digitally signed under ESRA
by Steven J. Carluccio
on 07/28/2022 02:35 PM

Steven J. Carluccio
Highway Safety Equipment Technical Supervisor
Office of Public Safety

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: North Syracuse Village Police Department

Manufacturer: NATL PATENT ANALYTICAL SYSTEM

Model: DATAMASTER DMT

Serial Number: 113808

Date: July 20, 2022

Reference Solution Lot Number : 22120

Reference Solution Standard : 0.10% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.097 %	34.00 degrees centigrade
2	0.099 %	34.01 degrees centigrade
3	0.097 %	34.00 degrees centigrade
4	0.098 %	34.01 degrees centigrade

Reference Solution Lot Number : 21310

Reference Solution Standard : 0.08% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.077 %	34.00 degrees centigrade
2	0.077 %	34.01 degrees centigrade
3	0.077 %	34.01 degrees centigrade
4	0.076 %	34.01 degrees centigrade

Reference Solution Lot Number : 22060

Reference Solution Standard : 0.18% at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.179 %	34.00 degrees centigrade
2	0.181 %	34.01 degrees centigrade
3	0.181 %	34.00 degrees centigrade
4	0.181 %	34.00 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NATL PATENT ANALYTICAL SYSTEM breath test instrument model DATAMASTER DMT, serial number 113808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.


I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.

Performed by:



Digitally signed under ESRA
by George Coffin
on 07/20/2022 02:08 PM

Reviewed by:

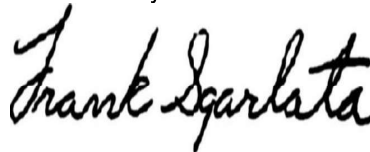

Digitally signed under ESRA
by Frank Sgarlata
on 07/20/2022 02:50 PM

George Coffin
Highway Safety Equipment Technician
Breath Analysis Operator Permit #48534

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: North Syracuse Village Police Department
Manufacturer: NATL PATENT ANALYTICAL SYSTEM
Model: DATAMASTER DMT
Serial Number: 113808
Date: July 20, 2022

- 1. General appearance and condition of this device -----: OK

- 2. Check controls and indicators -----: OK

- 3. Check breath flow system -----: OK

- 4. Check printer operation -----: OK

- 5. System cycles through all modes -----: OK



6. Record any repairs made to this instrument and list services provided : INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION.

Performed by:

Digitally signed under ESRA
by George Coffin
on 07/20/2022 02:08 PM

Reviewed by:

Digitally signed under ESRA
by Frank Sgarlata
on 07/20/2022 02:50 PM

George Coffin
Highway Safety Equipment Technician
Breath Analysis Operator Permit #48534

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

NORTH SYRACUSE
 VILLAGE POLICE DEPT
 DATAMASTER dmt: 113808





Date: 07/20/2022

OPERATOR NAME:
 GEORGE R COFFIN
 Permit #: 48534
 Operator Agency/Dept: N. SYRACUSE VILL. PD
 Reference Standard #: 21310

Nominal = 0.080 g/210L

BLANK TEST	0.000	11:30
INTERNAL STANDARD	VERIFIED	11:30
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.077	11:30
BLANK TEST	0.000	11:31
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.077	11:32
BLANK TEST	0.000	11:32
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.077	11:33
BLANK TEST	0.000	11:34
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.076	11:34
BLANK TEST	0.000	11:35

Average = 0.0768
 Std Dev = 0.0005

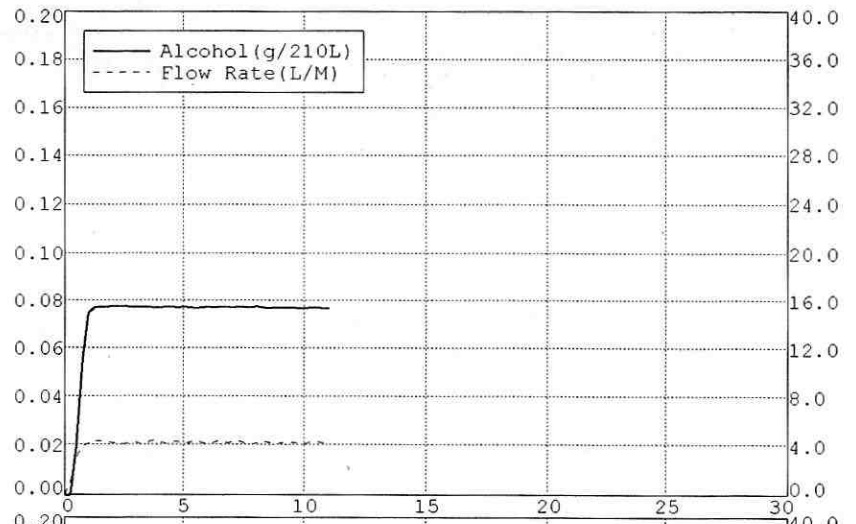

TECHNICIAN TEST

NORTH SYRACUSE
 VILLAGE POLICE DEPT
 DATAMASTER dmt: 113808





Date: 07/20/2022

OPERATOR NAME:
 GEORGE R COFFIN
 Permit #: 48534
 Operator Agency/Dept: N. SYRACUSE VILL. PD
 Reference Standard #: 22120

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:41
INTERNAL STANDARD	VERIFIED	11:41
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.097	11:42
BLANK TEST	0.000	11:42
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.099	11:43
BLANK TEST	0.000	11:44
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.097	11:44
BLANK TEST	0.000	11:45
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.098	11:45
BLANK TEST	0.000	11:46

Average = 0.0978
 Std Dev = 0.0010



TECHNICIAN TEST

NORTH SYRACUSE
 VILLAGE POLICE DEPT
 DATAMASTER dmt: 113808





Date: 07/20/2022

OPERATOR NAME:
 GEORGE R COFFIN
 Permit #: 48534
 Operator Agency/Dept: N. SYRACUSE VILL. PD
 Reference Standard #: 22060

Nominal = 0.180 g/210L

BLANK TEST	0.000	11:49
INTERNAL STANDARD	VERIFIED	11:49
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.179	11:49
BLANK TEST	0.000	11:50
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.181	11:51
BLANK TEST	0.000	11:52
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.181	11:52
BLANK TEST	0.000	11:53
REFERENCE STANDARD TEMP	34.00c	
REFERENCE STANDARD	0.181	11:53
BLANK TEST	0.000	11:54

Average = 0.1805
 Std Dev = 0.0010



SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
80 South Swan Street
Albany, NY 12210
Ph: 518-485-7636 / 518-402-0689
Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. **PLEASE SIGN AND DATE FORM.**

SECTION I - AGENCY INFORMATION

Name of Agency North Syracuse Police Department		Today's Date 07/20/2022
Address 600 South Bay Road		City, State, ZIP North Syracuse, NY 13212
Contact Person Sergeant Jeffrey D. Tripp		Contact Telephone 315-418-7938/ 315-458-5670
Contact Email jtripp@northsyracuse.ny.gov		Best Way to Reach You During Appointment Period 315-418-7938 (work cell)

SECTION II - INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle) NPAS DMT GUTH Applied Concepts(Stalker) Decatur(Genesis) Kustom(Eagle/Falcon) MPH Alco-Sensor Other:		
Model Number Datamaster DMT		Instrument Serial Number 113808
Antenna Serial Number (if applicable) Antenna 1 -- / Antenna 2 --		Type of maintenance (check appropriate) <input checked="" type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction Calibration Check		
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)		
DMT/SIM: 113808		Radar:
<input checked="" type="checkbox"/> DMT	SIM <input checked="" type="checkbox"/> Tubes	Control Unit Antenna(s) Antenna Cable(s)
<input checked="" type="checkbox"/> Keyboard	Other: POWER CORD, CABLES TO SIM, PEN	Power Cord Forks Other:
<i>I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.</i>		
Signature 		Date 07/20/2022

DCJS USE ONLY

<p><i>Inspected instrument, checked setup messages, print & remote operation. Performed calibration / adjustment procedure, run subject, technician + diagnostic tests, verified calibration.</i></p>
