



Division of Criminal Justice Services

CERTIFICATION PURSUANT TO CPLR 4518 OF RECORDS MAINTAINED IN THE REGULAR COURSE OF BUSINESS

I, Joshua Vinehout, Supervisor of Public Safety Programs, Office of Public Safety, New York State Division of Criminal Justice Services, 80 South Swan Street, Albany, New York 12210, having been duly designated and authorized by the Commissioner of the Division of Criminal Justice Services, do hereby certify and authenticate, as provided by subdivision c of Rule 4518 of the Civil Practice Law and Rules, that the document annexed hereto is an exact copy of an electronic record of the Office of Public Safety which is in my possession, custody and control. This record, once created, is stored in an electronic format that cannot thereafter be altered or modified.

I further certify that the original electronic record of inspection/maintenance/calibration of NAT'L PATENT ANALYTICAL SYS, DATAMASTER DMT breath test instrument, serial number 113808, performed on July 29, 2021 by Office of Public Safety employee Martin Schilling, of which the annexed is an exact copy, was made in the regular course of business of the New York State Division of Criminal Justice Services, Office of Public Safety, that such record was made at the time such inspection/ maintenance/calibration was performed or within a reasonable time thereafter, and further that it is the regular course of the Office of Public Safety's business to make such records at the time such inspection/maintenance /calibration is performed, or within a reasonable time thereafter, and to provide such instrument's records to the agency that requested them.

A handwritten signature in black ink that reads "Joshua Vinehout".

Digitally signed under
ESRA by Joshua Vinehout
on 8/3/2021 1:21 PM

Joshua Vinehout
Supervisor of Public Safety Programs
Office of Public Safety

An Equal Opportunity/Affirmative Action Agency

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: North Syracuse Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS Model: DATAMASTER DMT
Date: July 29, 2021 Serial Number: 113808

Reference Solution Lot Number: 20361
Reference Solution Standard: 0.10 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.102 %	34.01 degrees centigrade
2	0.102 %	34.01 degrees centigrade
3	0.102 %	34.01 degrees centigrade
4	0.103 %	34.01 degrees centigrade

Reference Solution Lot Number: 20470
Reference Solution Standard: 0.08 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.083 %	34.01 degrees centigrade
2	0.082 %	34.01 degrees centigrade
3	0.082 %	34.01 degrees centigrade
4	0.082 %	34.01 degrees centigrade

Reference Solution Lot Number: 21130
Reference Solution Standard: 0.180 % at 34.0 degrees centigrade

Test No	Test Result	Simulator Temperature
1	0.183 %	34.01 degrees centigrade
2	0.183 %	34.01 degrees centigrade
3	0.183 %	34.01 degrees centigrade
4	0.183 %	34.01 degrees centigrade

I hereby certify that I have performed any necessary maintenance procedures and calibrated NAT'L PATENT ANALYTICAL SYS breath test instrument model DATAMASTER DMT, serial number 113808, and have determined that it is accurate and reliable for the determination of ethyl alcohol in the blood by analysis of the breath. The instrument's test results are recorded above and this instrument satisfies all limits and standards established by the New York State Commissioner of Health as enumerated in Part 59, Subchapter D of Chapter II, TITLE 10 (Health) of the Official Compilation of Codes, Rules and Regulations of the State of New York, (10 NYCRR Part 59) as amended.

I further certify that I made the entries in these records of inspection/maintenance/calibration at the time that such inspection/maintenance/calibration of the above identified breath test instrument was performed, or within a reasonable time thereafter.


Performed by:



Digitally signed under
ESRA by Martin Schilling
on 7/29/2021 1:02 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45926

Reviewed by:



Digitally signed under
ESRA by Frank Sgarlata
on 8/2/2021 1:34 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

**BREATH TEST INSTRUMENT
RECORD OF INSPECTION / MAINTENANCE / CALIBRATION**

Name of Submitting Agency: North Syracuse Village Police Department
Manufacturer: NAT'L PATENT ANALYTICAL SYS
Model: DATAMASTER DMT
Serial Number: 113808
Date: July 29, 2021

1. General Appearance and condition of this device -----: OK

2. Check controls and indicators -----: OK

3. Check breath flow system -----: OK

4. Check printer operation -----: OK

5. System cycles through all modes -----: OK

6. Record any repairs made to this instrument and list services provided: INSPECTED INSTRUMENT, CHECKED SETUP VOLTAGES PRINT AND REMOTE OPERATION. PERFORMED CALIBRATION/ADJUSTMENT PROCEDURE, RAN SUBJECT, TECHNICIAN AND DIAGNOSTIC TESTS, VERIFIED CALIBRATION



Performed by:

Digitally signed under
ESRA by Martin Schilling
on 7/29/2021 1:02 PM

Martin Schilling
Highway Safety Equipment Technician
Breath Analysis Operator Permit # 45926

Reviewed by:

Digitally signed under
ESRA by Frank Sgarlata
on 8/2/2021 1:34 PM

Frank Sgarlata
Breath Analysis Technical Supervisor

TECHNICIAN TEST

NORTH SYRACUSE
 VILLAGE POLICE DEPT
 DATAMASTER dmt: 113808





Date: 07/29/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: N. SYRACUSE VILL. PD
 Reference Standard #: 20361

Nominal = 0.100 g/210L

BLANK TEST	0.000	11:55
INTERNAL STANDARD	VERIFIED	11:55
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.102	11:55
BLANK TEST	0.000	11:56
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.102	11:56
BLANK TEST	0.000	11:57
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.102	11:58
BLANK TEST	0.000	11:58
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.103	11:59
BLANK TEST	0.000	12:00

Average = 0.1022
 Std Dev = 0.0005



TECHNICIAN TEST

NORTH SYRACUSE
 VILLAGE POLICE DEPT
 DATAMASTER dmt: 113808





Date: 07/29/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: N. SYRACUSE VILL. PD
 Reference Standard #: 20470

Nominal = 0.080 g/210L

BLANK TEST	0.000	12:03
INTERNAL STANDARD	VERIFIED	12:03
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.083	12:03
BLANK TEST	0.000	12:04
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.082	12:04
BLANK TEST	0.000	12:05
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.082	12:05
BLANK TEST	0.000	12:06
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.082	12:07
BLANK TEST	0.000	12:08

Average = 0.0822
 Std Dev = 0.0005

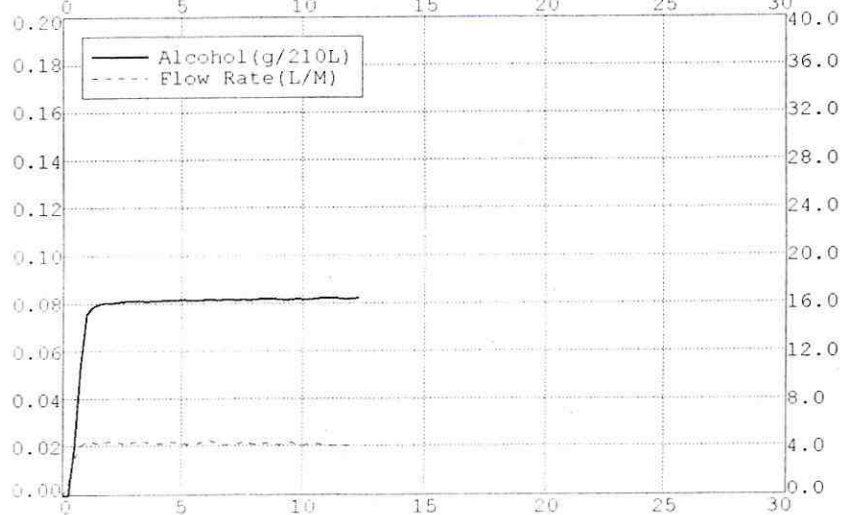

TECHNICIAN TEST

NORTH SYRACUSE
 VILLAGE POLICE DEPT
 DATAMASTER dmt: 113808


Date: 07/29/2021

OPERATOR NAME:
 MARTIN J SCHILLING
 Permit #: 45926
 Operator Agency/Dept: N. SYRACUSE VILL. PD
 Reference Standard #: 21130

Nominal = 0.180 g/210L

BLANK TEST	0.000	12:12
INTERNAL STANDARD	VERIFIED	12:12
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	12:13
BLANK TEST	0.000	12:14
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	12:14
BLANK TEST	0.000	12:15
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	12:16
BLANK TEST	0.000	12:16
REFERENCE STANDARD TEMP	34.01c	
REFERENCE STANDARD	0.183	12:17
BLANK TEST	0.000	12:18

Average = 0.1830
 Std Dev = 0.0000




SERVICE AUTHORIZATION FORM
Highway Safety Technology Unit
 80 South Swan Street
 Albany, NY 12210
 Ph: 518-485-7636 / 518-402-0689
 Fax: 518-457-6869

THIS FORM IS USED TO AUTHORIZE THE DIVISION OF CRIMINAL JUSTICE SERVICES TO PERFORM SERVICE ON THE INSTRUMENT IDENTIFIED. THIS AUTHORIZATION MUST ACCOMPANY EACH PIECE OF EQUIPMENT WHEN IT IS PRESENTED TO THE EQUIPMENT REPAIR CENTER FOR SERVICE. PLEASE SIGN AND DATE FORM.

SECTION I – AGENCY INFORMATION

Name of Agency North Syracuse PD		Today's Date 7/29/21	
Address 600 South Bay Rd.		City, State, ZIP	
Contact Person		Contact Telephone	
Contact Email		Best Way to Reach You During Appointment Period	

SECTION II – INSTRUMENT INFORMATION

Instrument Manufacturer (Please Circle)			
NPAS DMT	GUTH	Applied Concepts(Stalker)	Decatur(Genesis)
Kustom(Eagle/Falcon)		MPH	Alco-Sensor
Other:			
Model Number Datamaster DMT		Instrument Serial Number 113808	
Antenna Serial Number (if applicable)			Type of maintenance (check appropriate)
Antenna 1 --	/ Antenna 2 --		<input type="checkbox"/> Calibration Check <input type="checkbox"/> Repair
Brief Description of Malfunction			
List all parts, cables and/or accessories being submitted. Tuning forks must accompany all radar units (if applicable). (Please Circle)			
DMT/SIM:		Radar:	
DMT	SIM	Tubes	Control Unit Antenna(s) Antenna Cable(s)
Keyboard	Other:		Power Cord Forks Other:.
<small>I acknowledge I am signing this Service Authorization Form as an act and deed of said agency, organization, or municipality, and that I am duly authorized to sign same for the uses and purposes mentioned herein. PLEASE SIGN AND DATE.</small>			
Signature 		Date 07-29-2021	

DCJS USE ONLY

Suspected instrument. Checked power voltages print and remote operation. Performed calibration/adjustment procedure. Per subject, tubes and diagnostic tests. Verified calibration.