


Airway at narrowest point measures 8mms = 50.24 sq mms

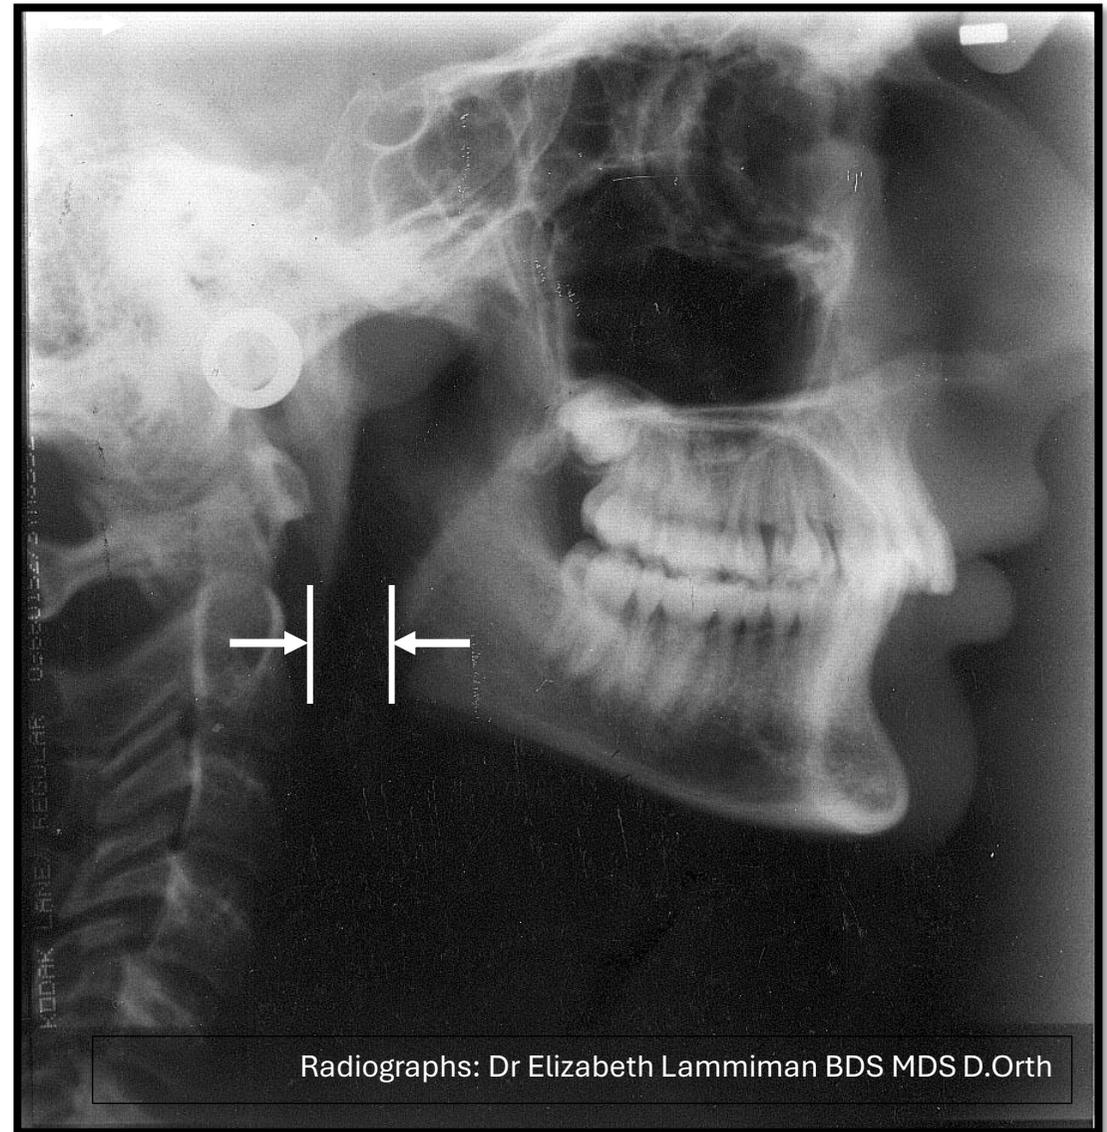

Airway at narrowest point measures 14mms = 154 sq mms

Angles Class II division 1 malocclusion, treated non-extraction with Clark Twin Block functional appliances.

Note 1: Area of airway at narrowest point increased three-fold.

Note 2: Reduced lordosis and increased length of cervical spine.