



Before testing, scan the QR code to watch the "how to use" video.

BEFORE STARTING

Wash your hands with soap and water for at least 20 seconds before and after test. If soap and water are not available, use hand sanitizer with at least 60% alcohol.




1. PREPARE FOR THE TEST

- 1A. Check the expiration date on the box.**
Do not use if the kit has been damaged or has expired.
- 1B. Ensure kit is at room temperature for at least 30 minutes prior to use.**
Open the box carefully as it will be used in a later step (1D).
Do not open individual components until instructed.
Note: A timing device (clock, timer, phone etc.) is required, but not provided.

1C. Remove the cover of the tube with extraction buffer.


- 1D. Put the tube in the tube holder in the box.**
Note: Being careful not to spill the tube contents.



2. NASAL SWAB SPECIMEN COLLECTION

- 2A. Open swab protective pouch.**
Remove the sterile swab from the pouch.


! Keep fingers away from the swab end.
Touch the stick end only.



2B. Swabbing both nostrils.

Insert the soft end of the swab into your nostril until you feel resistance (Approx. 2cm up your nose).

Slowly twist the swab, rubbing it along the insides of your nostril, 5-10 times against the nasal wall.
Gently remove Swab from nostril.




- 2C. Using the same swab, repeat step 2B, in your other nostril.**
Withdraw the swab.

Note:

- This may feel uncomfortable. Do not insert the swab any deeper if you feel strong resistance or pain.
- When the nasal mucosa is damaged or bleeding, nasal swab collection is not recommended.
- If you are swabbing others, please wear a face mask. With children, you may not need to insert the swab as far into the nostril.
- For very young children, you may need another person to steady the child's head while swabbing.


2D. Insert the swab into the extraction tube.

Ensure it is touching the bottom and stir the swab to mix well. Press the swab head against the tube and rotate the swab for 10-15 seconds.



2E. Hold the tube firmly with one hand.

Remove the swab while squeezing the swab head against the inside of the extraction tube.
Place the swab in a plastic bag.

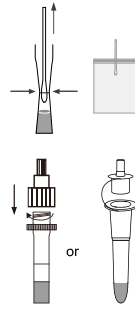

2F. Close the cap of the extraction tube

Return the tube to the Kit Box tube holder before proceeding to the next step.


3. PERFORM THE TEST

3A. Remove the test cassette from the sealed foil pouch and use it within one (1) hour.

Note: Best results will be obtained if the test is performed immediately after opening the foil pouch.
Place the test cassette on a flat and level surface.

! Do not move the test cassette during test developing.

3B. Invert the specimen extraction tube and add 3 drops of extracted specimen to each sample well (S) of the test cassette.



Start the timer. Secure tube cap back on extraction tube and wait 10 minutes.

! Do not touch the test device during this period.

3C. Read the result at 10 minutes.


Keep test device flat on table.
Do not read the result earlier than 10 minutes or after 20 minutes.



4. READING THE RESULTS


Please share your test result with your healthcare provider.

POSITIVE SARS-CoV-2 RSV




POSITIVE SARS-CoV-2/RSV:* Two colored lines appear in the COVID-19/RSV window.

One colored line should be in the control region (C) and another colored line should be in the Test region (T).




POSITIVE Influenza A:* Two colored lines appear in the FLU A+B window.

One colored line should be in the control region (C) and another colored line should be in the Influenza A region (A).



POSITIVE Influenza B:* Two colored lines appear in the FLU A+B window.

One colored line should be in the control region (C) and another colored line should be in the Influenza B region (B).




POSITIVE Influenza A and Influenza B:* Three colored lines appear in the FLU A+B window.

One colored line should be in the control region (C) and two colored line should be in the Influenza A region (A) and Influenza B region (B) respectively.

***NOTE:** The intensity of the colored line in the test line region (T/B/A) varies based on the amount of SARS-CoV-2, Influenza A/Influenza B and/or RSV antigen present in the specimen. So any shade of color in the test region (T/B/A) should be considered positive.
A positive result means it is very likely you have COVID-19, Influenza A/Influenza B and/or RSV, but the positive specimens should be confirmed to reflect this. Immediately go into self-isolation in accordance with the local guidelines, immediately contact your general practitioner/doctor or the local health department and obtain guidance on confirmation testing if necessary in accordance with the instructions of your local authorities. Seek medical assistance if you feel unwell.

NEGATIVE



NEGATIVE: One colored line appears in the control region (C). No colored line appears in the test line region (T/B/A).

You are unlikely to have COVID-19, Influenza A/Influenza B and/or RSV. However, it is possible for this test to give a negative result that is incorrect (a false negative) in some people with COVID-19, Influenza A/Influenza B and/or RSV. This means you could possibly still have COVID-19, Influenza A/Influenza B and/or RSV even though the test is negative.
In addition, you can repeat the test with a new test kit. In case of suspicion, repeat the test after 1-2 days, as the coronavirus/Influenza virus/Respiratory syncytial virus cannot be precisely detected in all phases of an infection.
Even with a negative test result, distance and hygiene rules must be observed. Migration/traveling, attending events and etc. should be done following your local COVID/Influenza/RSV guidelines/requirements.

INVALID




INVALID: Control line fails to appear.

Insufficient specimen volume or incorrect procedural techniques are the most likely reasons for control line failure. Review the procedure and repeat the test with a new test or contact with a COVID-19 and/or Influenza test center. If an invalid result continues after repeating, advice to contact the sponsor.

5. DISPOSE THE TEST KIT

After the test is complete, place all the components in a plastic bag and tightly sealed, then dispose in household waste or rubbish bin.

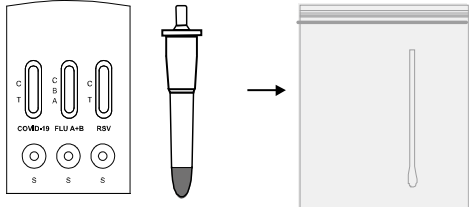

[INDEX OF SYMBOLS]

	Consult instructions for use or consult electronic instructions for use		Contains sufficient for <n> tests		Temperature limit
	In vitro diagnostic medical device		Batch code		Catalogue number
	Manufacturer		Use-by date		Do not re-use
	Do not use if package is damaged and consult instructions for use		Caution		

Hangzhou AllTest Biotech Co., Ltd.
#550, Yinhai Street
Hangzhou Economic & Technological Development Area
Hangzhou, 310018 P.R. China
Web: www.alltests.com.cn Email: info@alltests.com.cn

Australian Sponsor:
ACESO DIAGNOSTICS PTY LTD
Level 25, 100 Mount Street,
North Sydney, NSW, 2060.

For Customer Support Helpline: Call (02) 9959 2243 9am-7pm (AEST), 7 days per week for information on the correct use of this test and for interpretation of the test results.