

adapt[®] 500 easiSpec


Seating Assessment / Specification Form

User Weight






User Height

Min: 1560mm
Max: 2210mm

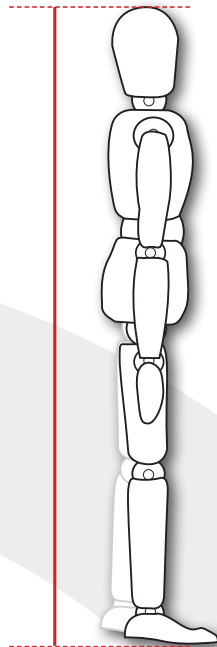

Chair Action

Asynchronous Pelvic-Tilt

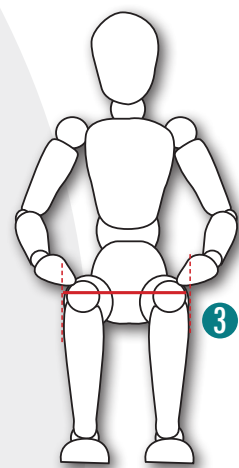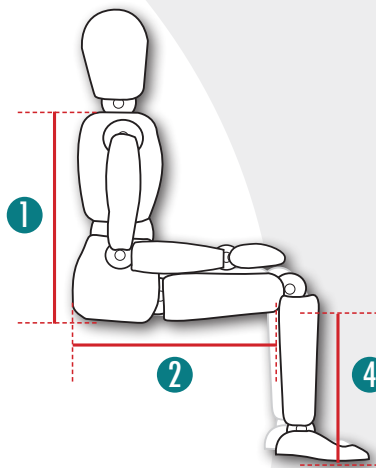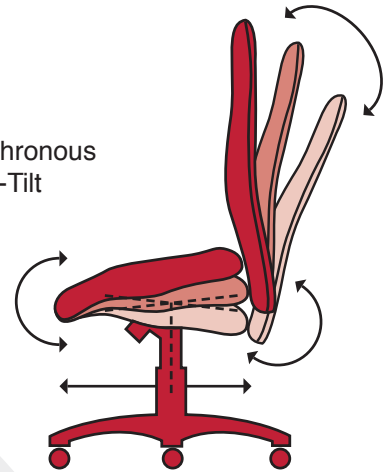

- 1 Seat to Shoulder (Back Height)
- 2 Back of Buttock to Back of Knee (Seat Depth)
- 3 Hip Width at widest point (Seat width)
- 4 Floor to Underside of Knee (Seat Height)

Min	Max
420mm	640mm
410mm	610mm
410mm	610mm
430mm	620mm*

*Higher gas columns available for use in specific environments

Client

Company

Assessor


Date

Seating Assessment / Specification Form

BACK REST



Please tick box option and state the required dimensions if different from those shown

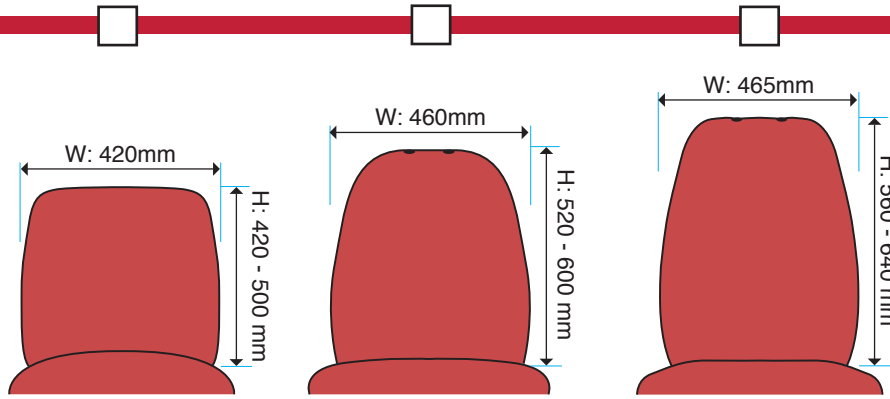

The Back rest sizes on the adapt[®]500 range are fixed and cannot be altered

If you require a specific sized Back Rest (particularly if using a neck support) please refer to the adapt[®]600 range which can be customised to suit virtually any requirement

CHAIR CODE

Width Reduction
Height Reduction

511/512

Not Available
Not Available

521/522

Not Available
Not Available

531/532


Not Available
Not Available

- If using a neck support, subtract 80mm from the Nape of Neck measurement in order to calculate correct back height

SEAT



Please tick box option and state the required dimensions if different from those shown

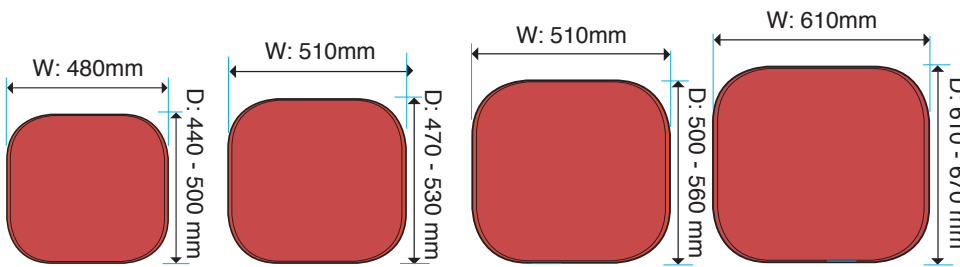

CHAIR CODE

Width Reduction
Depth Reduction

511/521/531

REDW: to.....mm
REDD: to.....mm

512/522/532

REDW: to.....mm
REDD: to.....mm

XL

REDW: to.....mm
REDD: to.....mm

XXL (Max)


REDW: to mm
REDD: to mm

- Use Back of Buttock to Back of Knee measurement and SUBTRACT 30mm to calculate optimum seat depth
- Use Hip to Hip measurement and ADD 50mm to calculate the optimum seat width
- **MINIMUM SEAT WIDTH IS 410mm AND MINIMUM SEAT DEPTH IS 410mm (with seat slide)**

SEAT HEIGHT



Please tick required option (approx heights)

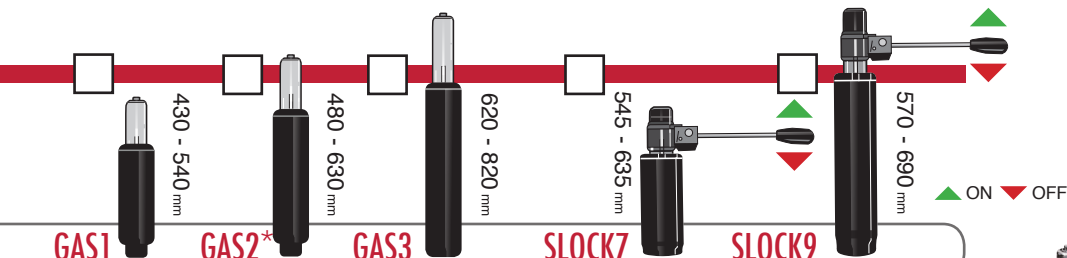

GAS CODE

GAS1

GAS2*

GAS3

SLOCK7

SLOCK9


STANDARD GAS COLUMN

SWIVEL LOCK

BASE




Please tick required option

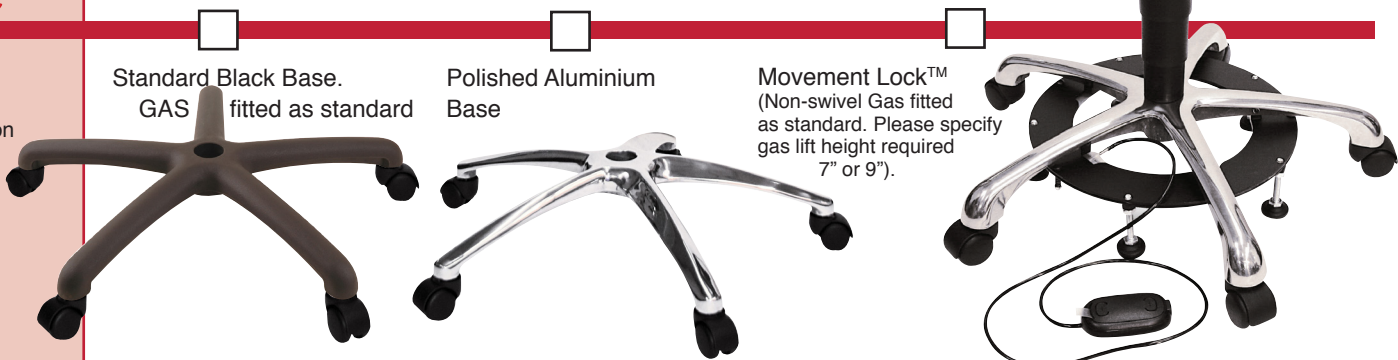

ARM OPTIONS

Level One Adaptations

Please tick required option

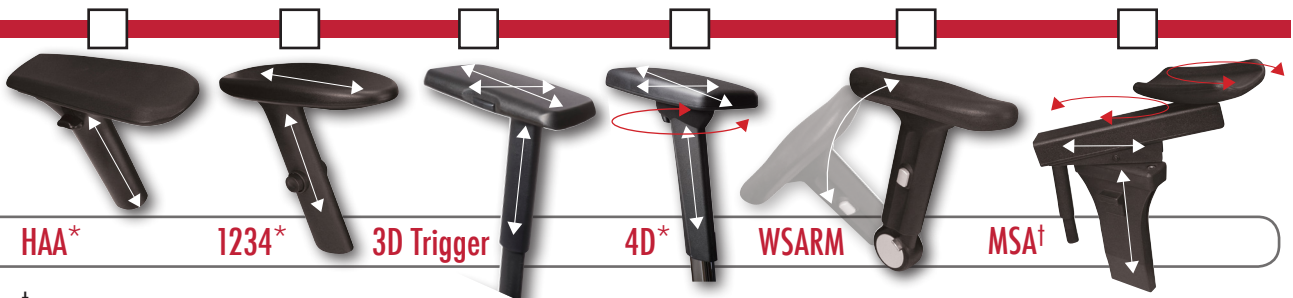

ARM CODE HAA* 1234* 3D Trigger 4D* WSARM MSA†

ARM PAD ENHANCEMENTS

Please tick required option



PAD CODE UPARM GEL PADS

*ADARM +50mm *ADARM -50mm


ADARM bracket will add or subtract 50mm from arm height (measured from seat surface to top of arm pad). Applies only to arm options marked with asterisk.

Compatible with HAA & 1234
 • Standard seat surface to underside of arm Arm Height is 150 - 240mm. If not suitable use **ADARM** option



HEAD SUPPORT

Please tick required option

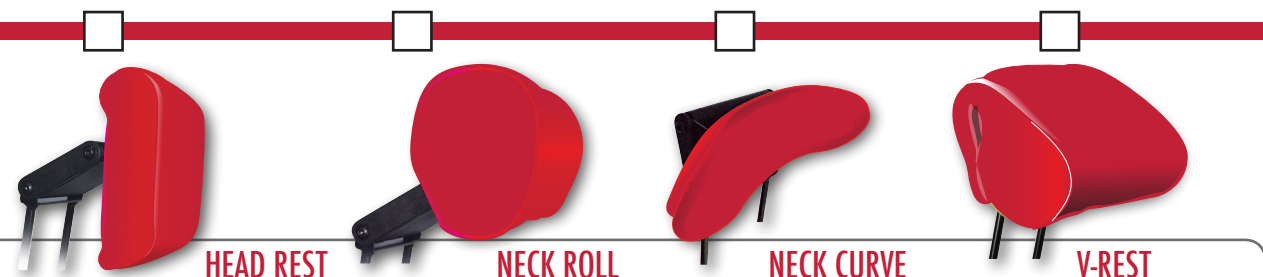


HEAD CODE HEAD REST NECK ROLL NECK CURVE V-REST

SEAT ENHANCEMENT


Level Two Adaptations

Please tick required option

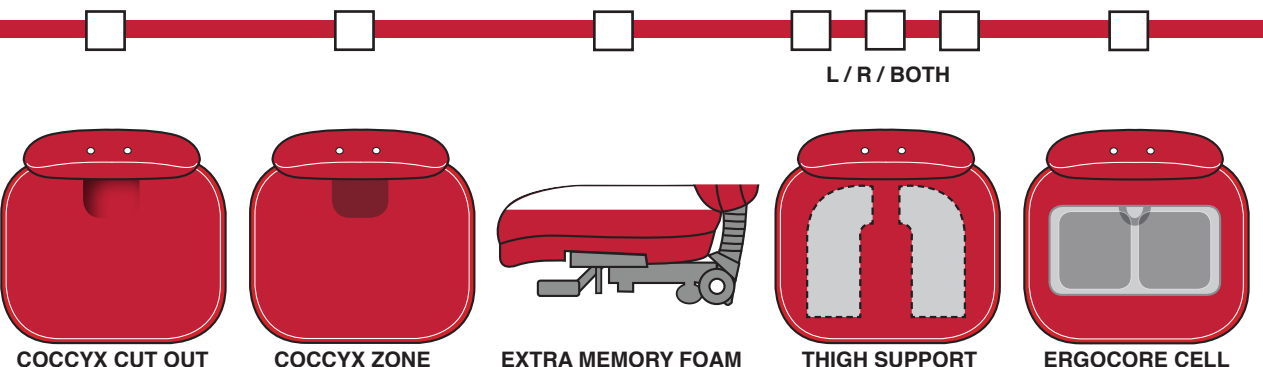

ENHANCE CODE /CC /CZ /MFS /TS /ECORE

Please tick required option

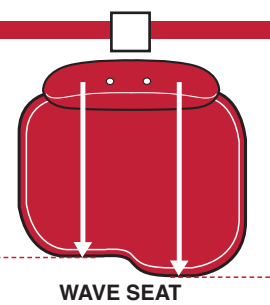

ENHANCE CODE WAVE

Please specify required SEAT DEPTH
 ie. Back Buttock to Back of Knee L&R -30mm
R (when sitting)mm (allow for 30mm clearance behind knee)
L (when sitting)mm (allow for 30mm clearance behind knee)

**(OPTIONAL)
BACK
ENHANCEMENTS**

Seating Assessment/Specification

Please tick required option

THORACIC CELL
Thoracic cell with bulb pump




ENHANCE CODE /THOR

STANDARD LUMBAR
Standard Lumbar Cell with bulb pump



RIGHT when seated LEFT when seated

/VSR /VSL VERTICAL CELL
Vertical cell with bulb pump

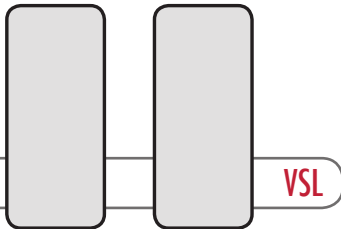

ENHANCE CODE

VSR

VSL


SACRAL CELL
Sacral Cell with bulb pump



ENHANCE CODE


SACRAL CELL

/3LUM REACTIVE LUMBAR CELL
Reactive Triple Lumbar Cell with bulb pump (combined, variable support over 3 cells)
where specified this will replace standard lumbar cell



ENHANCE CODE

/THOR

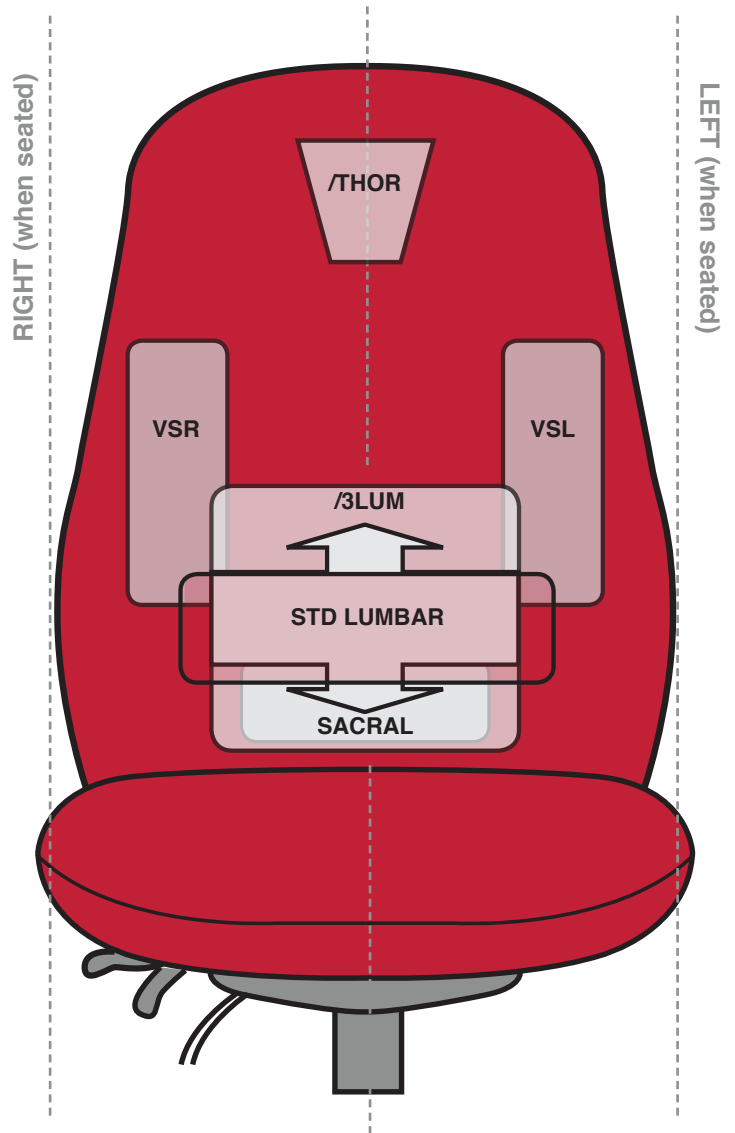

The adapt[®]500 uses fixed positions for air cells relative to the size of each back. If you require specific positioning for air cells please use adapt[®]600

SOFT WHEEL CASTORS

CODE SWC

BRAKE UNLOADED CASTORS

CODE BUC

BRAKE LOADED CASTORS

CODE BLC