2003 Siemens Symphony Maestro

Symphony
Maestro Class

Coils

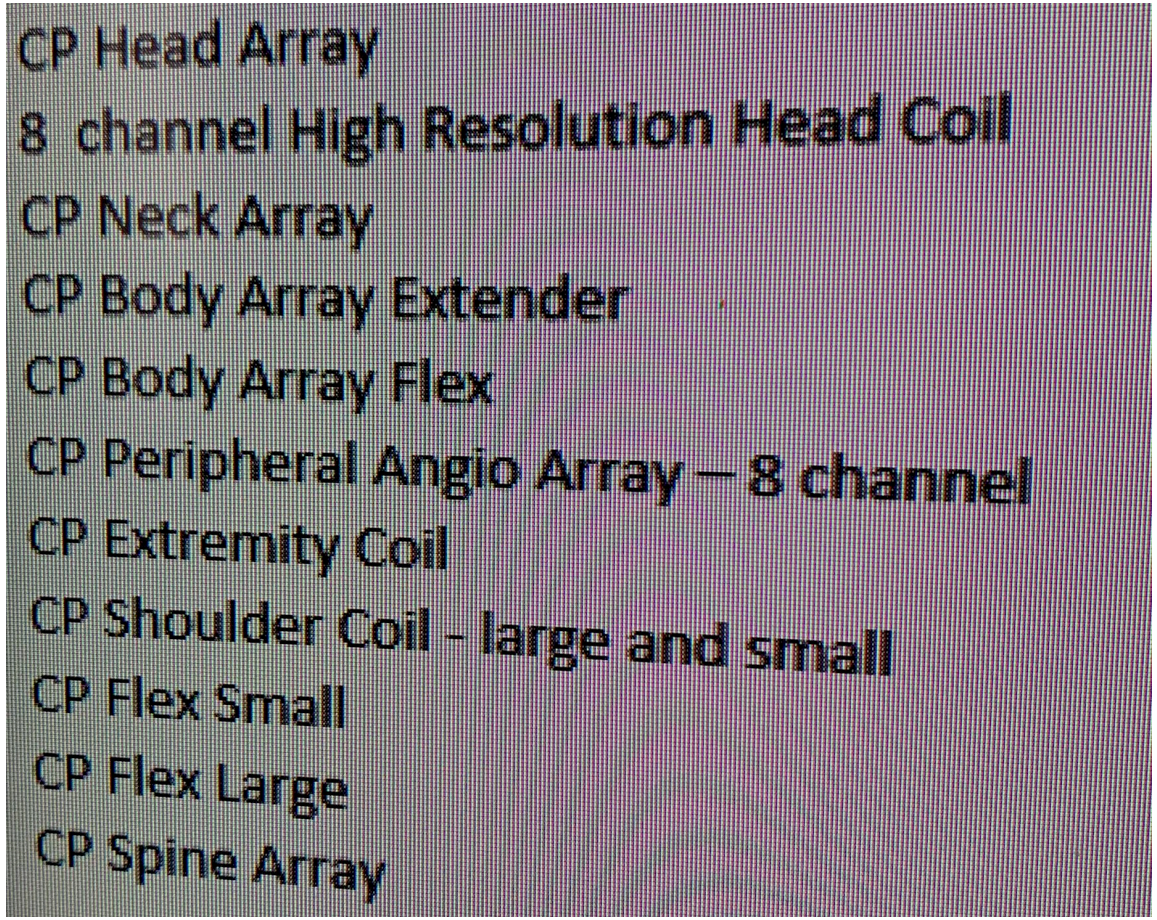
CP Head Array
8 channel High Resolution Head Coil
CP Neck Array
CP Body Array Extender
CP Body Array Flex
CP Peripheral Angio Array – 8 channel
CP Extremity Coil
CP Shoulder Coil - large and small
CP Flex Small
CP Flex Large
CP Spine Array

Symphony

Copyright (c) SIEMENS AG 2006. All rights reserved.

Series Number:

Software: NUMARIS/4

Version: syngo MR A30 DHHS

Siemens Software Packages:

COEM VD20I
syngo VE31G
N4_VA30A_LATEST_20070315
Revision B
N4_VA30A_LATEST_20070315_P4

This product is licensed to:

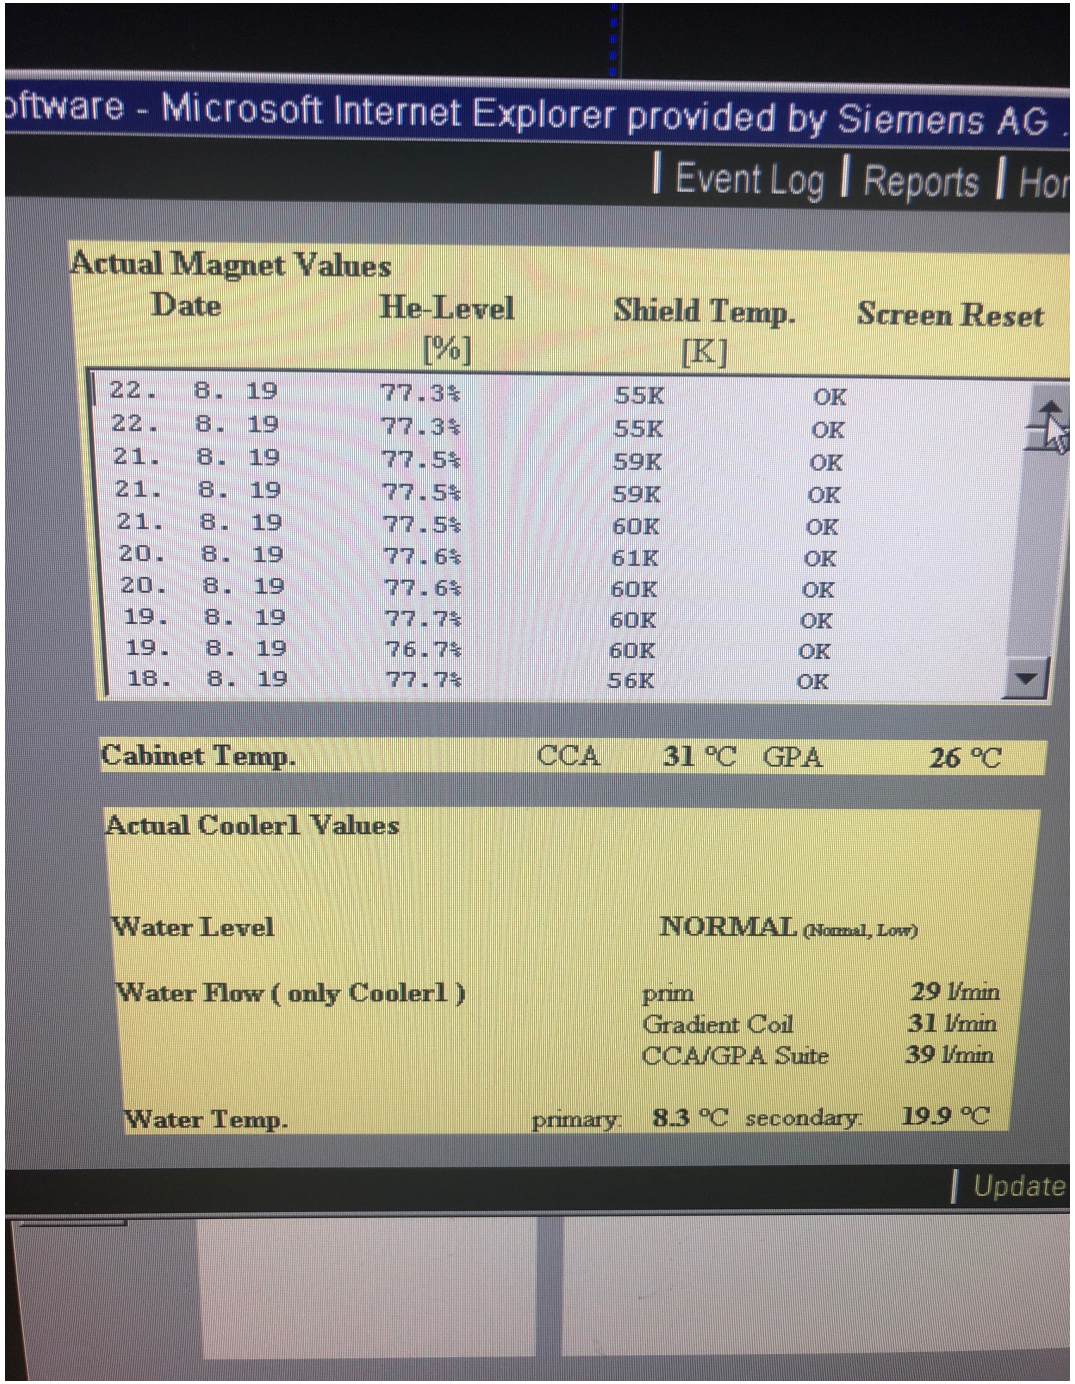
oftware - Microsoft Internet Explorer provided by Siemens AG
Event Log
Reports
Hor
Actual Magnet Values
Date
He-Level [%]
Shield Temp. [K]
Screen Reset
22. 8. 19 77.3% 55K OK
22. 8. 19 77.3% 55K OK
21. 8. 19 77.5% 59K OK
21. 8. 19 77.5% 59K OK
21. 8. 19 77.5% 60K OK
20. 8. 19 77.6% 61K OK
20. 8. 19 77.6% 60K OK
19. 8. 19 77.7% 60K OK
19. 8. 19 76.7% 60K OK
18. 8. 19 77.7% 56K OK
Cabinet Temp. CCA 31 °C GPA 26 °C
Actual Cooler1 Values
Water Level NORMAL (Normal, Low)
Water Flow (only Cooler1) prim 29 l/min
Gradient Coil 31 l/min
CCA/GPA Suite 39 l/min
Water Temp. primary: 8.3 °C secondary: 19.9 °C
Update