


Mobile Veterinary GE Signa 9x

- DOM: 2001
- Software level: 9.1
- Coils: 4 Ch. Torso, 4 ch. CTL, array head coil, flex coil, and birdcage knee coil
- Current DOT tags (not verified)







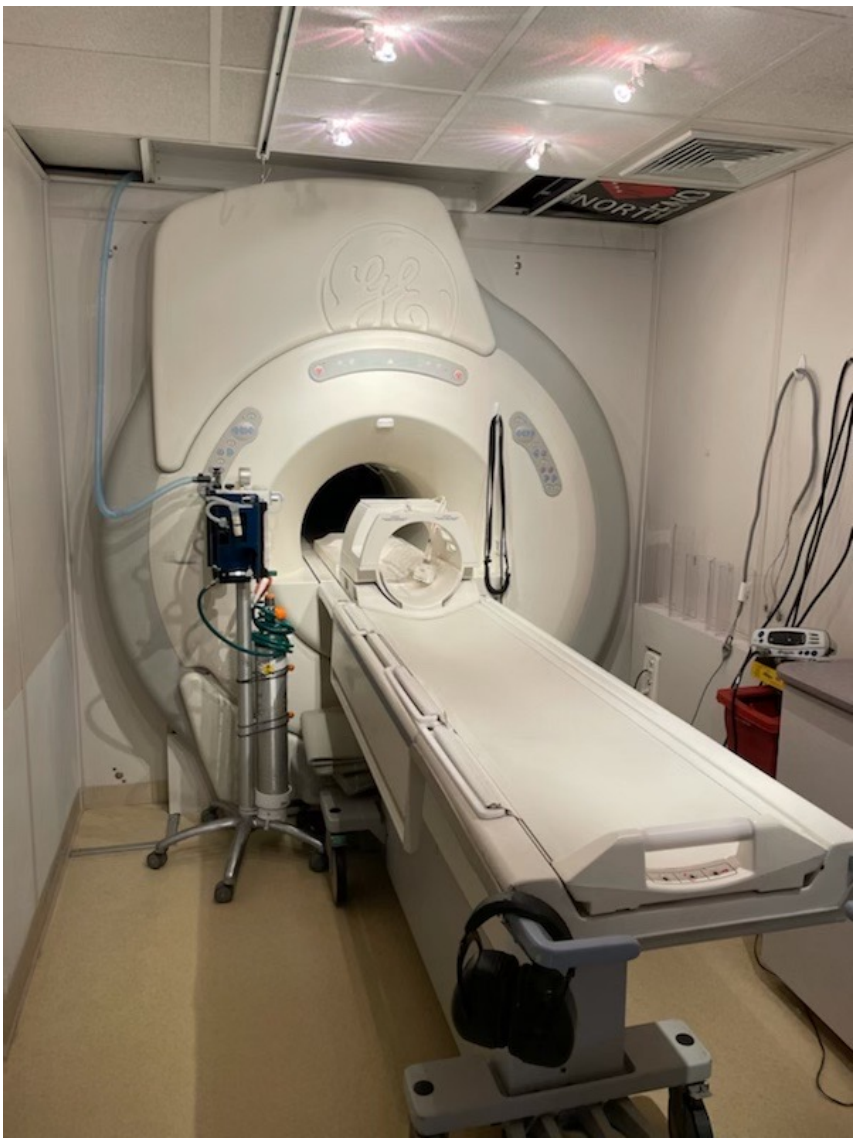

Hospital Information	
Hospital Name :	
System Id :	
Time Zone :	America/Indianapolis EST5 none
Computer type :	OCTANE
Suite Id :	FSH
Language :	English
Magnet Serial Number :	R1295
Operator Workspace IP :	192.168.5.41
Gradient Amplifier :	8915
Field Strength :	15000
System Health Information	
The system health check is not available under non-proprietary mode	







