

Tools & Equipment

TIGO-02

Cannulated Quick Connect Handle




TIGO-18

Button Outer Insertor



TIGO-17

Button Inner Insertor

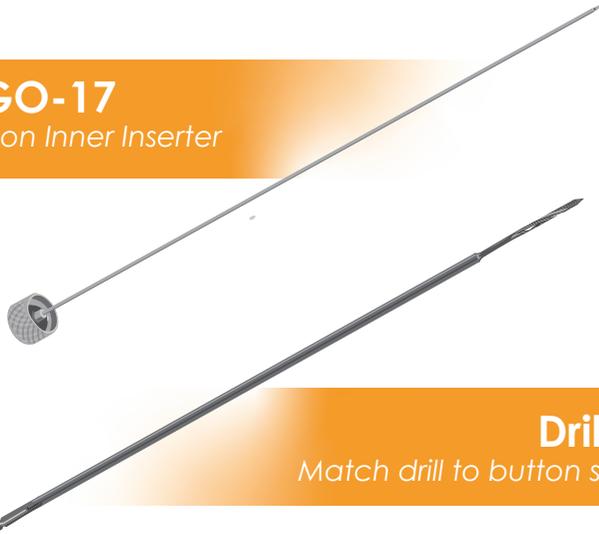

Drill

Match drill to button size

Boomerang Button

Available in various sizes



MIX.
MATCH.
MAXIMIZE.™

GREENREPAIR®



TIGON MEDICAL

Surgical Technique Boomerang Button

Use: Fixation of soft tissue to bone or bone to bone
Technique: Unicortical Onlay

Biceps Tenodesis



(410) 544-2833

office@tigonmedical.com


303 Najoles Rd, Ste. 104
Millersville, MD 21108

www.tigonmedical.com

MST5, REV C

TIGON MEDICAL

1

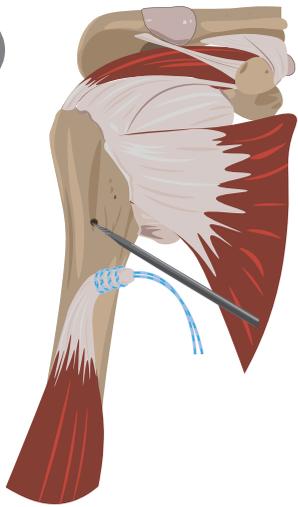

Drill through the first cortex using the appropriately sized drill bit for the desired button.


2

Connect the Outer Inserter (TIGO-18) to the Cannulated Quick Connect Handle (TIGO-02).




3

Insert the Inner Inserter (TIGO-17) through the Cannulated Quick Connect Handle and Outer Inserter. Align laser line on Outer Inserter with laser line on the button (or button caddy). Turn the Inner Inserter knob clockwise to secure the button.

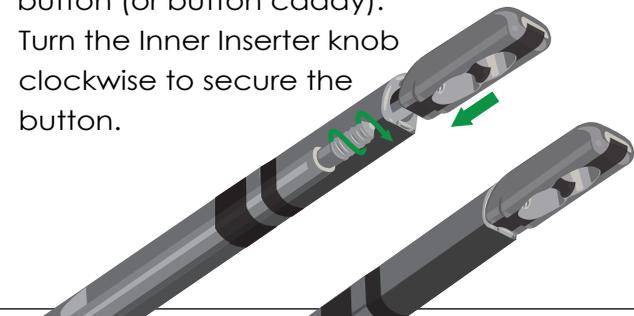


4

Pass one limb of suture through the laser-lined face of the button. First through the proximal eyelet of the button, then out the distal eyelet. Pass the remaining limb of suture in reverse order.

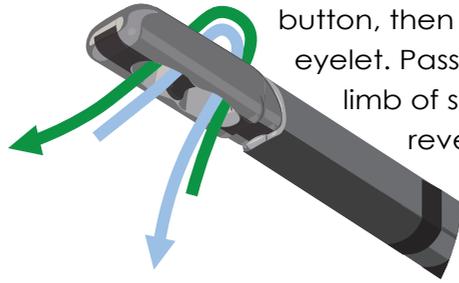


5

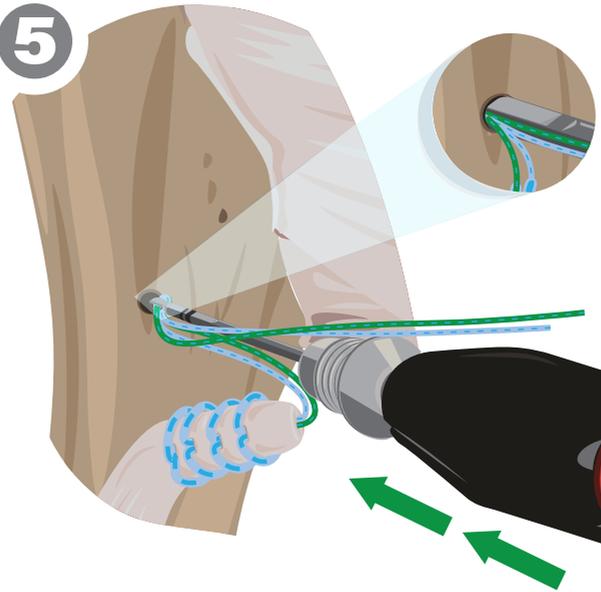

Insert the button inserter into the bone up to the second (wider) circumferential laser line.

6

Remove the Inner Inserter by rotating it counterclockwise until it releases from the button, then slide it out of the Cannulated Quick Connect Handle.

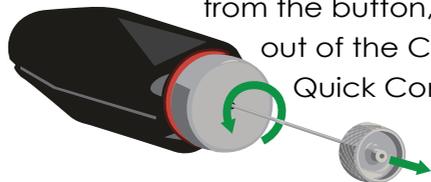

7

Firmly grasp and pull the suture tail that was passed first through the proximal eyelet and then the distal eyelet.

While pulling tension on the suture limbs, slowly retreat the button inserter to the distal (narrower) laser line.

Plunge inserter again to the proximal (wider) laser line, rotating the button fully.

8

Remove inserter and release suture. You may now shuttle tendon down to the bone. Tie suture.

