

International Scientific Instruments

(Importers and Distributors of Electronic Equipment)

31 Elgar Grove

Portsea, Vic. 3944, Australia

Telephone: (03) 5984 1050 International: 61 3 5984 1050

M8 x 125

90.0°

6.8

M8 x 1.25

THREAD

E-mail: sales@interscientific.com.au
Web: www.interscientific.com.au


45.0°

IJ.

VIBRATION CONDITION MONITORING SYSTEM SCREW IN M8 X 10-32 UNF ACCELEROMETER MOUNTING STUD

PART NO.: F/1032 M8 REV B **\$25 plus GST**

MATERIAL: Grade 431 Magnetic Stainless Steel

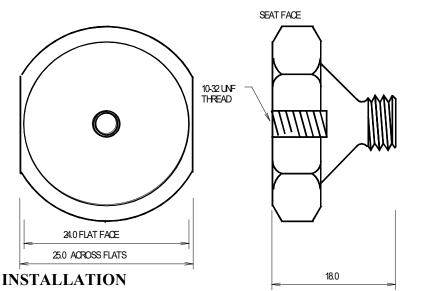

- 1. Drill a 6.8 mm (17/64") diameter hole x 9 mm deep (ie 11.5 mm max hole depth to drill point) at the selected monitoring location. (NB. The stud location should allow sufficient clearance for use of either a 26 or a 42 mm diameter accelerometer.)
- 2. Machine a chamfered mounting seat using a 90° countersinking tool to provide no more than 1-1.5 mm wide seat face.
- Tap hole with an M8 x 1.25 mm pitch thread to provide 8 mm of full thread.
 NB. Use a plug tap and ensure that the hole and thread are thoroughly cleaned out.
- 4. Install the stud to seat evenly on the countersink and lightly torque to 10-15 Nm. It is important that the stud does not bottom in the hole or mate with the machine surface except by the seat face. (These conditions can produce excessive / reduced transmitted vibration levels.)

NB. Use a thread locking compound (eg Loctite) on machines having high vibration.