



Venner
WireSafe™



References:

1. Horberry T. et al. 2014, International Journal of Risk & Safety in Medicine, **26**: 23-37
2. NHS. 2016, <https://www.england.nhs.uk/patientsafety/never-events/>
3. Green J. Butterworth J. 2013, Anesthesia & Analgesia, **117(1)**: 1-2
4. Schummer W. et al. 2002, BJA, **88(1)**: 144-146
5. Vannucci A. et al. 2013, Anesthesia & Analgesia, **117(1)**: 102-108
6. Peh W.M. et al. 2016, BMJ, Feb **12**:5(1)
7. Livesay A. et al. 2016, EJA, **33**(e-supplement 54): 462
8. Heberer M. 1984, Infusionsther Klin Ernahr, **11(5)**: 254-61
9. Mariyaselvam M.Z.A. 2017, Anesthesiology, **10**;127(4): 658-665



Scan for more information



Qualitech Healthcare Limited,
16 Cordwallis Park, Clivemont Rd,
Maidenhead, Berkshire, SL6 7BU

Tel no. +44 (0) 1628 854042

email: info@qualitechhealthcare.co.uk

www.qualitechhealthcare.co.uk

Copyright© 2017 Venner Medical Technologies SA. All rights reserved.
Venner and WireSafe are trademarks of the Venner Group of Companies.

PREVENTING THE “NEVER EVENT”
OF RETAINED GUIDEWIRES

VENNER WIRESAFE™ FACILITATING PREVENTION OF GUIDEWIRE RETENTION

Central Venous Catheterisation (CVC) is a common hospital procedure.¹ After swabs, retained guidewires are the commonest retained object Never Event in the NHS.²

Human error is a major factor for guidewire retention^{1,3} and can be caused by many factors:

- Inattention^{4,5}
- Inexperienced operators^{1,4,6}
- Inadequate supervision of trainees^{1,4,5,6}
- Overtired staff^{1,4}
- Multiple guidewires in the surgical field⁵
- Lack of reminders⁶

CONSEQUENCES OF GUIDEWIRE RETENTION

- Arrhythmias⁴
- Vascular damage⁴
- Thrombosis^{4,6}
- Tamponade⁶
- Infectious complications^{5,6}
- Increased cost of care⁵
- Increased mortality⁸

Complications of guidewire retention occur in:

333

OUT OF
EVERY MILLION
PROCEDURES⁵

ONE
IN
3000

CASES⁵

1
IN
5

REPORTED
MORTALITY⁴

"Never Events
are serious
incidents that
are wholly
preventable"
(NHS 2016)

No.2

RETAINED
FOREIGN OBJECT
AFTER SWABS²

VENNER WIRESAFE™ YOUR SOLUTION TO GUIDEWIRE RETENTION


Venner WireSafe™ is an innovative procedural pack designed with an engineered solution to:

- Prevent guidewire retention⁷
- Facilitate a safe completion of the procedure⁷
- Allow safe disposal of sharps and wires⁷

TO PREVENT THE RETENTION OF GUIDEWIRES
USE THE SIMPLE GUIDEWIRE UNLOCKING
CHANNEL TO ACCESS THE CONTENTS WITHIN
VENNER WIRESAFE™

100%

SUCCESS RATE
PREVENTING GUIDEWIRE
RETENTION (p=0.0001)^{7,9}

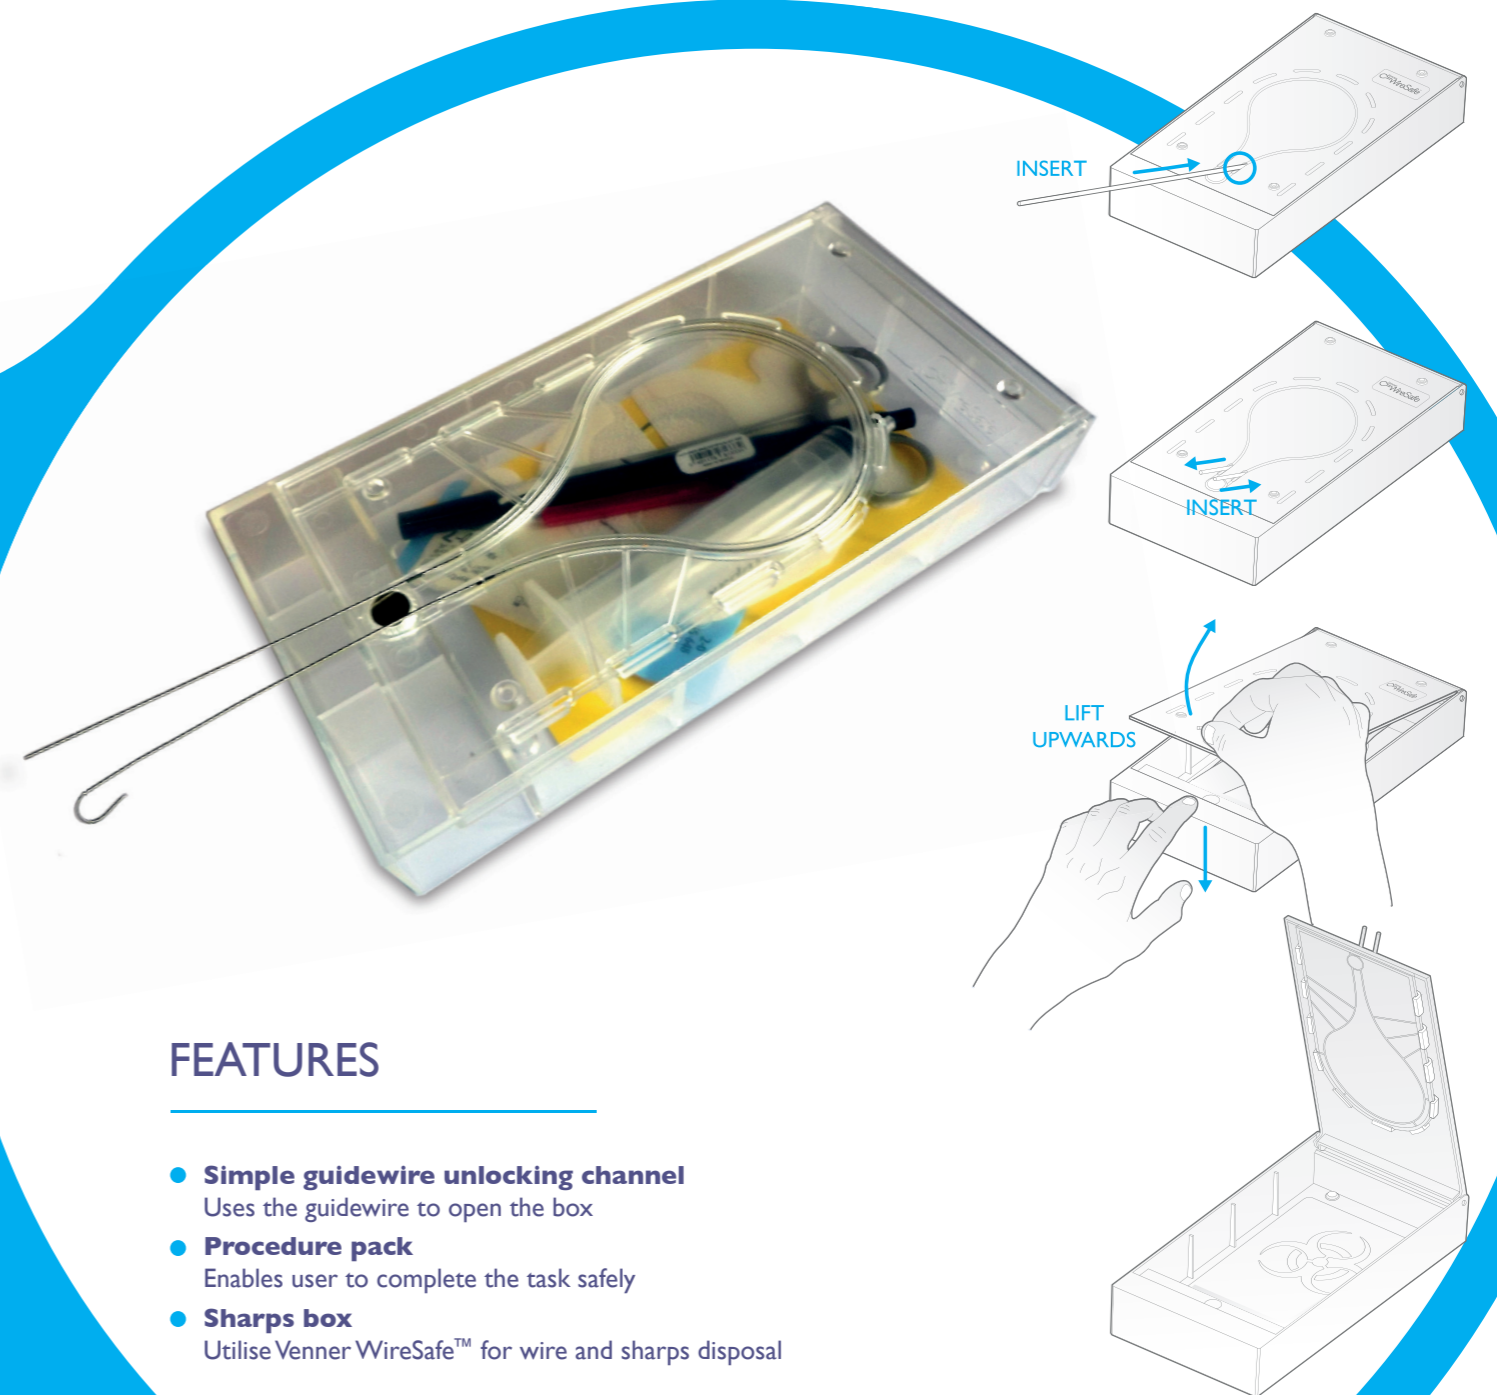

FEATURES

- **Simple guidewire unlocking channel**
Uses the guidewire to open the box
- **Procedure pack**
Enables user to complete the task safely
- **Sharps box**
Utilise Venner WireSafe™ for wire and sharps disposal