Flowflex® COVID-19 Antigen Home Test

Quick Reference Instructions

1 Wash

2 Prepare

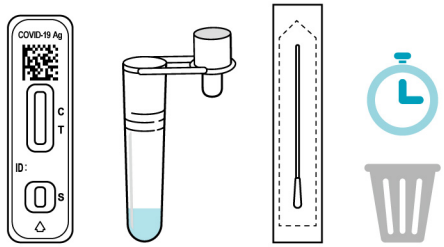

3 Peel and Place

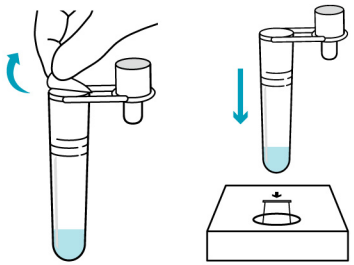

4 Open



5 Collect Sample

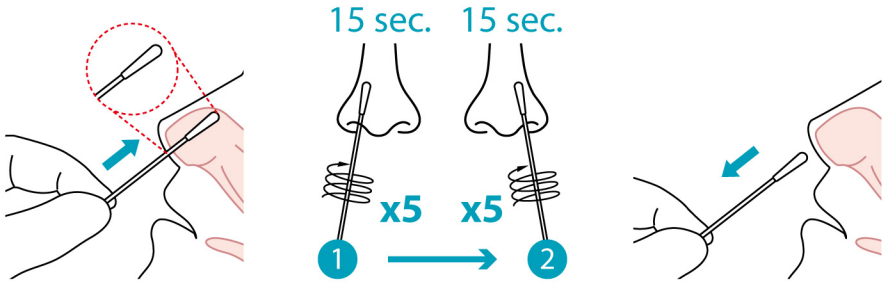

Insert | Swab | Remove

6 Prepare Sample

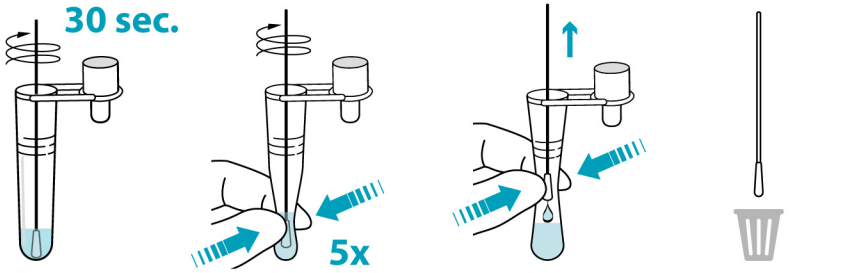

Swirl | Squeeze | Remove | Dispose

7 Process Sample

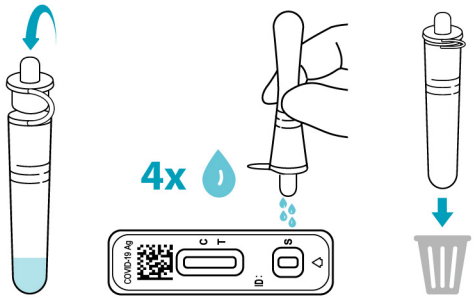

Cap | Dispense | Dispose

8 Wait

15 MIN

9 Read Result

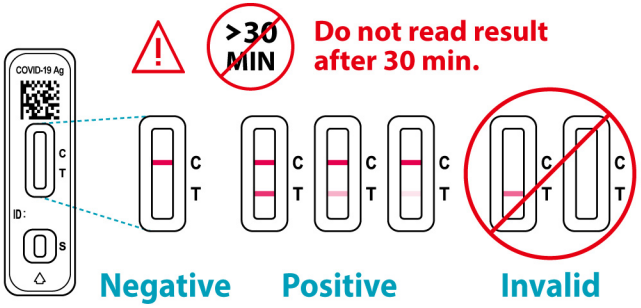

10 Dispose

Repeat test using a new cassette

ACON®

***ACON* Laboratories, Inc.**
San Diego, CA 92121, USA
Customer Support 1-800-838-9502
flowflexcovid.com

Number: 1151321502 Effective date: 2022-10-14