

Peak Details



2 (Agilent1260_HPLC-2025-11-06 09-57-00-08-00.dlx)


DAD1A,Sig=250,4 Ref=off



Chromatograms



Display mode by Signal name

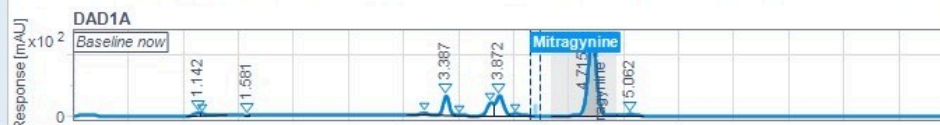

Injection Results



Peaks		Summary									
#	Name	Signal description	RT (min)	Area (mAU-s)	Area%	Height (mAU)	Height%	Amount	Concentration	Start time (min)	End time (min)
1		DAD1A,Sig=250,4 Ref=off	1.142	41.859	1.787	10.220	2.12			1.038	1.169
2		DAD1A,Sig=250,4 Ref=off	1.178	20.741	0.885	8.528	1.77			1.169	1.405
3		DAD1A,Sig=250,4 Ref=off	1.581	2.723	0.116	2.095	0.43			1.566	1.603
4		DAD1A,Sig=250,4 Ref=off	3.195	51.820	2.212	9.878	2.05			3.043	3.280
5		DAD1A,Sig=250,4 Ref=off	3.387	250.489	10.694	65.610	13.61			3.280	3.468
6		DAD1A,Sig=250,4 Ref=off	3.512	17.183	0.734	4.245	0.88			3.468	3.666
7		DAD1A,Sig=250,4 Ref=off	3.793	181.278	7.739	45.413	9.42			3.667	3.825
8		DAD1A,Sig=250,4 Ref=off	3.872	311.092	13.281	66.926	13.89			3.825	3.969
9		DAD1A,Sig=250,4 Ref=off	4.017	36.794	1.571	7.065	1.47			3.969	4.200
10	Mitragynine	DAD1A,Sig=250,4 Ref=off	4.715	1396.607	59.623	256.569	53.23	1785.464	89273.213	4.351	4.941
11		DAD1A,Sig=250,4 Ref=off	5.062	31.821	1.358	5.428	1.13			4.941	5.191