

Pulsed ElectroMagnetic Field Therapy



850 Series
User Manual

850 SERIES

850-Pro



Desktop:

Voltage input:
120 to 230 VAC
50 to 60Hz

Current input:
1.6 Amp maximum

Dimensions:
39cm x 29cm x 14cm
15.5" x 11.5" x 5.5"

Weight:
6.5 kg
14.3 lbs

Shipping weight:
10 kg
22.05 lbs

850-N920



Portable:

Voltage input:
120 to 230 VAC
50 to 60Hz

Current input:
1.6 Amp maximum

Dimensions:
42cm x 34cm x 17cm
16.5" x 13.4" x 6.7"

Weight:
6.5 kg
14.3 lbs

Shipping weight:
10 kg
22.05 lbs

850-S2500



Roll Away:

Voltage input:
120 to 230 VAC
50 to 60Hz

Current input:
1.6 Amp maximum

Dimensions:
58cm x 37cm x 22cm
22.8" x 14.6" x 8.7"

Weight:
12 kg
26.45 lbs

Shipping weight:
16 kg
35.27 lbs

850-S2500AT



All Terrain:

Voltage input:
120 to 230 VAC
50 to 60Hz

Current input:
1.6 Amp maximum

Dimensions:
67cm x 44cm x 30cm
26.4" x 17.3" x 11.8"

Weight:
15 kg
33.07 lbs

Shipping weight:
19 kg
41.89 lbs

AVAILABLE TREATMENT COILS



SMALL MAT

12" x 22" / 22cm x 56cm

Pigtail length:

- 6 ft./ 1m83



LARGE MAT

18" x 23" / 46cm x 58cm

Pigtail lengths:

- 6 ft./ 1m83

- 12 ft./ 3m66 Equine



TRIFOLD MAT

24" x 72"

61cm x 1m83



PADDLE

7" / 18cm

Pigtail lengths:

- 6 ft./ 1m83

- 12 ft./ 3m66 Equine



DOUBLE LOOP

Options:

Loop diameter Pigtail lengths:
- 9"/ 23cm standard - 6 ft./ 1m83
- 7"/ 18cm custom - 12 ft./ 3m66
- 24"/ 61cm Equine Equine
- 18"/ 46cm custom



SINGLE LOOP

Options:

Loop diameter: Pigtail length:
- 14"/ 35.5cm- - 6 ft./ 1m83
- 24"/ 61cm



STRAIGHT

Options:

Wrapping length:
- 20 ft./ 6m10
- 30 ft./ 9m15 Equine

WHAT'S INCLUDED IN THE BOX

- 850 series Control unit
- Medical grade MAINS power cord
- Surge protector
- User Manual
- Warranty Registration Card
- Selected Treatment Coils

INDICATIONS FOR USE

The 850 series, comprised of the 850-Pro, the 850-N920, the 850-S2500 and the 850-S2500AT, is to be used as an adjunct therapy for the:

- Relaxation of muscle spasms
- Prevention or retardation of disuse muscle atrophy
- Increasing local blood circulation
- Immediate post-surgical stimulation of calf muscles to prevent venous thrombosis
- Muscle re-education, and
- Maintaining or increasing range of motion.

DESCRIPTION

The 850 series are non-contact, non-invasive pulsed electro-magnetic field (“PEMF”) generators used to provide a pulsed magnetic stimulation of nerves and muscles. The 850 series have two independent PEMF generators in a sealed unit that can be used independently or synchronised to double the power output. There is no user access and no user serviceable parts. The 850 series are stationary (not worn or carried). The PEMF generators use standard household electrical current. There are three user-operated controls located on the PEMF generators: a standard power rocker switch, a push button membrane switch with a choice of treatment duration (either 5 or 10 minutes) and an intensity selector to either increase the pulse intensity (signified by the up arrow) or decrease the pulse intensity (signified by the down arrow).

Your shipment comes with the PEMF generator you ordered (either the 850-Pro, the 850-N920, the 850-S2500 or 850-S2500AT) and the treatment coils you selected.

FREQUENCY OF USE

The pulsed magnetic stimulation cycle lasts 5 min. or 10 min.

On the first use, the recommended treatment is one 5 min. cycle per area treated. Thereafter, the pulsed magnetic stimulation can be increased to one 10 min. treatment cycle per area treated per day.

Additional pulsed magnetic stimulation of the same area on the same day is not hazardous but does not offer additional therapeutic benefits.

CONTRAINDICATIONS

DO NOT USE pulsed magnetic stimulation:

- If you are or may be pregnant,
- If you are receiving chemotherapy.
- If you have cancer, cancerous lesions, or malignant tumors.
- If you have had surgery in the past 24 hours.
- If you have hemorrhagic tendencies, Purpura, or Hemophilia,
- If you have major metabolic diseases uncontrolled by medication (HIV, ulcers, seizures...),
- With cardiac demand pacemakers, defibrillators, or any other implanted electronic devices,
- Within 25cm of metallic implants (stents, pins, rods, or screws),
- Soon after taking any medication as their effects may be intensified.
- Consult your health care provider to discuss using the PEMF generator if you think you are at risk for any of these contraindications.

WARNINGS

- Pulsed magnetic stimulation should not be applied over the carotid sinus nerves, particularly in patients with a known sensitivity to the carotid sinus reflex.
- Strong pulsed magnetic stimulation should not be applied over the heart as it may cause cardiac arrhythmias.
- Strong pulsed magnetic stimulation should not be applied over the neck or mouth. Severe spasms of the laryngeal and pharyngeal muscles may occur, and the contractions may be strong enough to close the airway or cause difficulty in breathing.
- Strong pulsed magnetic stimulation should not be applied trans cerebrally.
- Strong pulsed magnetic stimulation should not be applied over swollen, infected, or inflamed areas or skin eruptions, e.g.: phlebitis, thrombophlebitis, varicose veins, etc.

PRECAUTIONS

- Safety of PEMF generators for use during pregnancy has not been established.
- Caution should be used for patients with suspected or diagnosed heart problems.
- Caution should be used for patients with suspected or diagnosed epilepsy.
- Caution should be used in the presence of the following:
 - When there is a tendency to hemorrhage following acute trauma or fracture,
 - Following recent surgical procedures as muscle contraction may disrupt the healing process,
 - Over the menstruating or pregnant uterus, and
 - Over areas of the skin which lack normal sensation.
- Do not place the treatment coil over a suture line within 3 days after surgery.
- Treatment coil placement and pulsed magnetic stimulation settings should be based on the guidance of the prescribing practitioner.
- Users with low blood pressure may feel temporarily dizzy when first standing up after pulsed magnetic stimulation.
- Pulsed electro-magnetic field generators should be used only with the treatment coils recommended for use by the manufacturer.
- Users taking pain, anxiety, depression, or any other medication should be carefully monitored when using the PEMF generator as medication effectiveness may be intensified.
- Detoxication may occur, drink plenty of water after pulsed magnetic stimulation.
- Overuse may cause muscle soreness.
- In the event of any adverse effects, stop using the PEMF generator and consult a physician.

GENERAL SAFETY

- ALWAYS use the enclosed surge protector that has an output light indicator with the PEMF generator. The output light indicator must be on to safely use the PEMF generator. If the output light indicator is out, replace the surge protector with another that also has an output light indicator and low clamping voltage, 1000+ Joules rating and a 15 Amp breaker.
- Dangerous voltage is present inside the PEMF generator, DO NOT tamper with or try to open the PEMF generator.
- DO NOT USE the PEMF generator near credit cards, security access cards, car keys, hearing aids, watches, cell phones, iPods, laptops, remote controls, or any other electronic media. The pulsed electro magnetic fields may disrupt their functioning and/or demagnetize them.
- DO NOT USE while operating any machinery or during any activity in which involuntary muscle contractions may put the user at undue risk of injury.
- DO NOT USE in wet environments. Do not immerse any part of or pour any liquids on the PEMF generator. Keep away from sources of heat and moisture.
- Pulsed electro-magnetic field generators, cables and packing materials should be kept out of the reach of children. Children may be at risk of strangulation with the power cord and the treatment coil pigtails.or risk of asphyxiation with the packing materials.
- Metal objects, jewelry and metal chains will heat with prolonged exposure to pulsed electromagnetic fields. Use the PEMF generator for one 5-minute treatment cycle followed by a five-minute pause within 25cm of any implanted metal objects before treating again.

USER CONTROLS AND SYMBOLS

MAINS socket to plug the medical grade power cord into.




The MAINS power rocker switch turns the PEMF generator on "I" and off "O".



Press the 5 or 10 min. pushbutton to begin a 5 or 10 min. pulsed magnetic stimulation cycle. Five or 10 blue lights will illuminate when the corresponding treatment is active and incrementally turn off as time elapses.

Press "Synchronize" to select the synchronized operation of the two PEMF generators; the corresponding blue light will illuminate. When not selected, the two PEMF generators will operate independently.

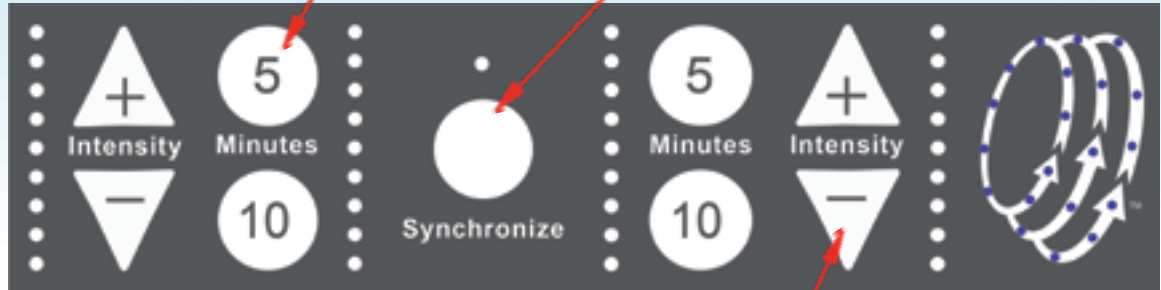

Two coil connector sockets allow one or two treatment coils to be safely and securely locked into place.



Intensity pushbuttons with up (+) and down (-) arrows; press ▲ to increase or ▼ to decrease the intensity to one of the nine preset intensity levels. One to nine blue lights will illuminate.

DEFINITION OF SYMBOLS, LABELS AND MARKINGS



Read the entire User Manual BEFORE using the device



Medical Device



Type B Applied Parts



Type II Equipment



Non-ionizing Radiation



MAINS Power ON



MAINS Power OFF



Catalogue or Reference Number



Serial Number



Manufacturer's Identification
with Date of Manufacture

DIRECTIONS FOR USE

Pulsed Magnetic Stimulation Cycle

A pulsed magnetic stimulation cycle lasts 5 min. or 10 min. Press the desired pushbutton to begin the pulsed magnetic stimulation. Each treatment cycle may be set at one of five intensity levels by pressing the up and down arrows.

Getting Started

Plug the enclosed surge protector into the MAINS.

Plug the supplied power cord into the MAINS socket on the back of the PEMF generator and into the surge protector on the other end.

Always lock a treatment coil connector into the connector socket on the front of the PEMF generator before turning the MAINS power switch on "I". The PEMF generator will not start if the treatment coil is not properly connected.

Inserting/Changing a Treatment Coil

To connect a treatment coil, align the arrow on the coil connector with the arrow on the coil connector socket of the PEMF generator. Push the connector into the socket until you hear a "click". The treatment coil is now locked into place.

To remove the treatment coil, turn the end of the coil connector to the left (counterclockwise) to disengage and pull it out.

DO NOT plug or unplug the treatment coil during an active treatment cycle.

Beginning Pulsed Magnetic Stimulation

Place a treatment coil on or around the desired treatment area. The closer the coil is to the treatment area, the more effective the pulsed magnetic stimulation will be. Users can remain fully clothed and no direct contact between the coil and the skin is necessary for the pulsed magnetic stimulation to be effective.

Press the 5 min. or 10 min. pushbutton to begin the desired pulsed magnetic stimulation. Set the desired intensity level from one to five using the up and down arrows. A corresponding number of blue lights will illuminate. The blue lights will turn off and the PEMF generator will emit a single long beep when the cycle ends.

Push the up or down arrow to select the desired intensity. One to nine blue lights will illuminate accordingly.

Press a 5 min. or 10 min. pushbutton again to begin another treatment cycle.

Pausing/Resetting/Ending the Treatment Cycle

During the treatment cycle, briefly press the active pushbutton to pause the pulsed magnetic stimulation. The corresponding blue light flashes continuously while in "pause mode". To resume the cycle, briefly press the same pushbutton again.

To end the pulsed magnetic stimulation prior to completion, press and hold the active pushbutton until you hear a single long beep and the blue lights turn off.

FOOT



ANKLE



ANKLE



KNEE



KNEE



KNEE



KNEE



ELBOW



ELBOW



HAND & WRIST



NECK



NECK



SHOULDER



SHOULDER



CHEST & SHOULDER



ABDOMEN



CHEST



UPPER BACK



MID BACK



MID TO LOW BACK




MID TO LOW BACK



LOW BACK



HIPS

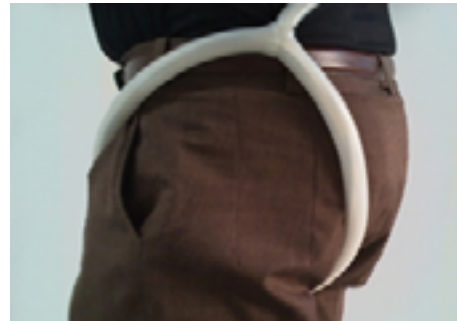

HIPS



TROUBLESHOOTING

If the device fails to function after following the instructions detailed in the “Directions for Use” on page 4, use the following troubleshooting steps:

If there are beeping sounds:

Proceed to identify the beep sequence the device emits:

- ***Single two second beep*** = End of session

Solution: Press a start pushbutton to begin a new treatment.

- ***Three short beeps & one long beep*** = The coil is not connected properly or was disconnected while the device was in use

Solution: Connect the coil properly following the instructions on page 4 and press a start pushbutton to begin a treatment.

- ***Two short beeps three times followed by one long beep*** = Device overheating

Solution: Allow the device to cool down for 10 minutes by leaving the power on while no treatment is activated. The cooling fan will cool the device. Press a start pushbutton to begin a treatment after the 10 minutes have elapsed.

If the lights do not illuminate and there are no beeping sounds:

- Make sure the MAINS power cord is properly connected at the control unit and a MAINS outlet.
- Make sure the MAINS outlet is functional. Try plugging another electrical appliance into the outlet to determine if it works. If the outlet works, test the device with another MAINS power cord.

If the device still fails to start or function properly, contact the manufacturer, listed on page 8 to get a Return Merchandise Authorization (RMA) number. Disconnect the coil and the power cord. Package the device securely and return it to the manufacturer for servicing with the RMA number and your contact information.

MAINTENANCE

Service

The PEMF generator has no user serviceable parts and must be returned to the manufacturer for servicing.

Treatment coils, mats and MAINS power cords are available from the manufacturer.

Dangerous Voltage inside; DO NOT remove the cover or tamper with the PEMF generator.

REMOVING THE COVER OR TAMPERING WITH THE PEMF GENERATOR VOIDS THE WARRANTY.

Contact the distributor for assistance in setting up, using or maintaining the PEMF generator.

Disposal

This PEMF generator is an electronic device. Electronics should never be disposed of with regular trash.

Take non-working electronics to an electronics recycling center.

Cleaning

The PEMF generator is a sealed unit and lint, dust, dirt, etc. have no effects on it.

There is no mandatory or scheduled cleaning, maintenance or sterilizing necessary.

If you choose to clean the PEMF generator:

- Disconnect the PEMF generator from the MAINS before cleaning,
- DO NOT immerse any part or pour any liquids on the PEMF generator.

STORAGE & TRANSPORTATION


Keep the PEMF generator dry and store it in a dry place. Storage in a damp place may cause corrosion.

Store and transport at temperatures between 5° to 50°C at a relative humidity of up to 93% non-condensing.

Remove the MAINS power cord and the detachable treatment coils from the PEMF generator and pack all parts of the PEMF generator securely before transporting.

ELECTROMAGNETIC IMMUNITY EMI

Immunity Test	IEC 61001 Test Level	Compliance Level	Electromagnetic Environment - Guidance
Electrostatic discharge (ESD) IEC 61000-4-2	±6 kV contact ±8 kV air	±6 kV contact ±8 kV air	Floors should be wood, concrete, or ceramic tile. If floors are covered with synthetic material, the relative humidity should be at least 30%.
Electrical fast transient/burst IEC 61000-4-4	±2kV for power supply lines ±1 kV for input/output lines	±2kV for power supply lines N/A - No Input/Output lines	Mains power quality should be that of a typical commercial or hospital environment.
Surge IEC 61000-4-5	±1 kV differential mode ±2 kV common mode	±1 kV differential mode ±2 kV common mode	Mains power quality should be that of a typical commercial or hospital environment.
Voltage dips, short interruptions and voltage variations on power supply input lines IEC 61000-4-11	<5% U _n (>65% dip in U _n) for 0.5 cycle 40% U _n (60% dip in U _n) for 5 cycles 70% U _n (30% dip in U _n) for 25 cycles <5% U _n (>65% dip in U _n) for 5 sec	<5% U _n (>65% dip in U _n) for 0.5 cycle 40% U _n (60% dip in U _n) for 5 cycles 70% U _n (30% dip in U _n) for 25 cycles <5% U _n (>65% dip in U _n) for 5 sec	Mains power quality should be that of a typical commercial or hospital environment. If the user of the PEMF Family Group requires continued operation during power mains interruptions, it is recommended that the device be powered from an uninterruptible power supply or a battery.
Power frequency (50/60Hz) magnetic field IEC 61000-4-8	3 A/m	3 A/m	Power frequency magnetic fields should be at levels characteristic of a typical location in a typical commercial or hospital environment.

Immunity Test	IEC 61001 Test Level	Compliance Level	Electromagnetic Environment - Guidance
			Portable and mobile RF communications equipment should be used no closer to any part of the PEMF Family Group, including cables, than the recommended separation distance calculated from the equation applicable to the frequency of the transmitter.
			Recommended separation distance:
Conducted RF IEC 61000-4-6	3 Vrms 150 kHz to 80 MHz	3 Vrms	$d = \frac{[3.5] \sqrt{P}}{V_1}$
Radiated RF IEC 61000-4-3	3 V/m 80 MHz to 2.5 GHz	3 V/m	$d = \frac{[3.5] \sqrt{P}}{E_1}$ 80 MHz to 800 MHz $d = \frac{[7] \sqrt{P}}{E_1}$ 800 MHz to 2.5 GHz
			where P is the maximum output power rating of the transmitter in watts (W) according to the transmitter manufacturer and d is the recommended separation distance in meters (m). Field strengths from fixed RF transmitters, as determined by an electromagnetic site survey, should be less than the compliance level in each frequency range ² . Interference may occur in the vicinity of equipment marked with the following symbol: 

ELECTROMAGNETIC EMISSIONS EMC

Emission Tests		Compliance	Electromagnetic Environment - Guidance
RF emissions CISPR 11	Group 1		The PEMF Family Group uses RF energy only for its internal function. Therefore, its RF emissions are very low and are not likely to cause any interference in nearby electronic equipment.
RF emissions CISPR 11	Class A		The PEMF Family Group is suitable for use in all establishments, other than domestic, and those directly connected to the public low-voltage power supply network that supplies buildings used for domestic purposes.
Harmonic emissions IEC 61000-3-2	Class A		
Voltage fluctuations/Flicker Emissions IEC 61000-3-3	Complies		

SEPARATION DISTANCES FROM PORTABLE AND MOBILE RF EQUIPMENT

Rated Maximum Output Power of Transmitter W	Separation Distance According to Frequency of Transmitter m		
	150 kHz to 80 MHz	80 MHz to 800 MHz	800 MHz to 2.5 GHz
	$d = \frac{[3.5]\sqrt{P}}{V_i}$	$d = \frac{[3.5]\sqrt{P}}{E_i}$	$d = \frac{[2]\sqrt{P}}{E_i}$
0.01	0.12	0.12	0.23
0.1	0.38	0.38	0.73
1	1.2	1.2	2.3
10	3.8	3.8	7.3
100	12	12	23

WARRANTY

The Warranty Registration Card must be filled out and returned to the manufacturer within 30 days of the date of purchase to activate the warranty.

The manufacturer warrants this PEMF generator to operate properly for a period of three years from the date of the original purchase invoice. In the event of a malfunction during the warranty period, the manufacturer will, at its discretion, replace or repair the PEMF generator to its original operating condition.

Freight and insurance to and from the manufacturer's repair facility are not included. Freight and Insurance are the responsibility of the registered owner.

A Return Material Authorization (RMA) number must be obtained from the manufacturer prior to returning any PEMF generator or accessory for service. The PEMF generator must be delivered with prepaid freight, the RMA provided, the registered owner's name and address, and a brief description of the difficulties encountered. The PEMF generator is to be shipped to the address designated by the manufacturer.

Such service, repair, or adjustment of the PEMF generator is guaranteed to the original purchaser provided the PEMF generator has not been tampered with, does not have any physically broken parts and the PEMF generator was not opened, altered, or damaged as a result of misuse, accident, water, grit, impact, or lack of proper care.



QARAD
Cipalstraat 3
B-2440 Geel
Belgium

CONTACT INFORMATION:

PEMF Systems, Inc.
+1 (702) 448-2660
support@pemfsystems.com
www.pemfsystems.com



PEMF Systems, Inc.
422 Kirkstone Way
Las Vegas, NV 89123