

OPERATING THEATRE

Environmental Set-up Guide



Structurally Complete

Contents

1. ***** Cardiac	6
2. ?????/	7
3. ?????/	8
4. ***** Colorectal	9
5. ?????/	10
6. ?????/	11
7. ***** Dental	12
8. ??????	13
9. ??????	14
10. ***** ECT	15
11. ??????	16
12. ??????	17
13. ***** Emergency	18
14. ??????	19
15. ??????	20
16. ***** ENT	21
17. Tonsillectomy / Adenoidectomy / T.S / A.S.....	22
18. Modified Radical Mastoidectomy	23
19. Meatoplasty	24
20. Myringoplasty	25
21. Pre-Auricular	26
22. Tympanoplasty	27
23. Grommets	28
24. Exostosis	29
25. Microlaryngoscopy	30
26. Nasopharynx Biopsy	31
27. E.U.A Ear / Examination Under Microscope	32
28. Turbinectomy	33
29. Septoplasty	34
30. Papilloma	35
31. Tracheostomy	36
32. Tracheotomy	37
33. ***** Eyes or Ophthalmic	38
34. ??????	39
35. ??????	40
36. ***** General	41
37. Open Hernia Repairs / Herniorrhaphy	42
38. Esophagectomy	43
39. Open Appendicectomy / Gastrectomy / Laparotomy / Liver Resection / Right Hemicolectomy	44
40. Hemicolectomy Left / Anterior Resection / Ultra-Low	45
41. Hemicolectomy Right	46
42. Open Splenectomy / Lap Splenectomy	47
43. Closure Ostiomiespen	48

44. Lap Nissen Fundoplication	49
45. Hartman's Procedure	50
46. Whipples	51
47. Anal Fistula / Fissure / Haemorrhoidectomy / Perianal Abscess / Advancement Flaps / Prolapse	52
48. Thyroidectomy / Parathyroidectomy	53
49. Pilonidal Sinus V1 Lateral	54
50. Pilonidal Sinus V2 Prone.....	55
51. Laparoscopic Cholecystectomy	56
52. Hysteroscopy / D&C / Cystoscopy / Most General Gynae / Laparoscopic Ablation of Endometriosis / Lap Assisted	57
53. ***** Gynae	58
54. Bartholin's Abscess	59
55. B.S.O – Bilateral Salingopaxy Oophorectomy	60
56. Cone Biopsy of the Cervix	61
57. D&C – Dilatation and Curettage	62
58. Ectopic Pregnancy - Laparoscopically	63
59. Hysteroscopy	64
60. Hysterectomy / Total Abdominal Hysterectomy / T.A.H	65
61. Hysterectomy / Vaginal / Laparoscopic	66
62. L.L.E.T.Z – Large Loop Excision of Transformation Zone	67
63. L.U.C.C.S – Lower Uterine Segment Caesarean Section	68
64. Pelvic Mass	69
65. P.P.H – Post Partum Haemorrhage	70
66. Salpingostomy	71
67. T.A.H – Total Abdominal Hysterectomy	72
68. Vaginal Hysterectomy	73
69. Trial By Forceps	74
70. Ventouse	75
71. Ventrosuspension	76
72. Vulvectomy	77
73. 3 rd Degree Tear.....	78
74. ***** Maxillo Facial	79
75. C.A.T / Combined Approach Tympanoplasty / M.R.M / Modified Radical Meatoplasty	80
76. Tracheostomy / Dental Extractions / Bilateral Neck Dissection / Lip Split / Resection of Lesion / Radical Forearm Flap Reconstruction	81
77. ***** Neuro	82
78. Craniotomy - With Stealth	83
79. INTER-CRANIAL ANEURYSM – With Stealth	84
80. Craniotomy / Shunt – With Axiom	85
81. Sub-Dural Haematoma / Burr Hole / EVD / ICP (Emergency)	86
82. Craniotomy- Intraoperative MRI With Skull Clamp.....	87
83. Trans-Sphenoidal Tumour Resection – Intraoperative MRI With Head Ring.....	88
84. Cervical Laminectomy – With Pillows “BOWS” With Xray	89
85. Cervical Laminectomy – With Montreal Mattress – With Xray.....	90

86. Cervical Laminectomy – Compress Roll – With Xray	91
87. Anterior Cervical Discectomy Fusion (ACDF) With Xray V1	92
88. Anterior Cervical Discectomy Fusion (ACDF) With Xray V2	93
89. Anterior Cervical Discectomy Fusion (ACDF) With Xray V3	94
90. Anterior Cervical Discectomy Fusion (ACDF) With Xray V4	95
91. Anterior Cervical Discectomy Fusion (ACDF) With Xray V5	96
92. Laminectomy / Microdiscectomy – With Xray V1	97
93. Laminectomy / Microdiscectomy – With Xray V2	98
94. Spinal Fusion (Inc TLIF) With O-Arm	99
95. Spinal Fusion (XLIF) With Xray	100
96. Carpal Tunnel Repair (Right)	101
97. Carpal Tunnel Repair (Left)	102
98. ***** Orthopaedics	103
99. P&P / Pin and Plate / Canulated Hip Screw	104
100. Archilles Tendon Repair	105
101. Carpel Tunnel Release	106
102. Cubital Tunnel Release	107
103. D.P.C / Direct Primary Closure	108
104. Dupuytren's Contracture	109
105. Arthroscopy Knee	110
106. M.U.A / Manipulation under Anaesthetic / Ulna - Radius	111
107. O.I.F / Open Reduction Internal Fixation / Ankle	112
108. O.I.F / Open Reduction Internal Fixation / Clavicle	113
109. O.I.F / Open Reduction Internal Fixation / Distal Humorous	114
110. O.I.F / Open Reduction Internal Fixation / Proximal Humorous	115
111. O.I.F / Open Reduction Internal Fixation / Femur	116
112. O.I.F / Open Reduction Internal Fixation / Olecranon / Elbow	117
113. R.C.R / Rotator Cuff Repair	118
114. Tendo/ Repair / Nerve Repair / Upper Limb	119
115. Tibial Plateau	120
116. T.K.R / Total Knee Replacement	121
117. T.H.R / Total Hip Replacement	122
118. Vac Dressing Change	123
119. ***** Paediatrics	124
120. ??????	125
121. ??????	126
122. ***** Thoracic	127
123. Anterior Mediastinoscopy	128
124. Lobectomy / Excision of Lung Lobe	129
125. Lung Lavage	130
126. Mediastinotomy	131
127. Pleurectomy	132
128. Peritoneal Shunt Insertion / Pleuro	133
129. Pneumonectomy	134

130. Thoracoscopy	135
131. Thoracotomy	136
132. ***** Urology	137
133. Circumcision	138
134. Cystectomy	139
135. Cystoscopy	140
136. Dorsal Slit.....	141
137. Excision Of Bladder Endometrioma (Laparoscopically)	142
138. Hydrocele	143
139. Ileal Conduit	144
140. Stent Insertion	145
141. Laparoscopic Deroofing of Renal Cyst	146
142. Lithotripsy	147
143. Lithopaxy / Litholapaxy / Cisto-Litholapaxy	148
144. Nephrectomy	149
145. Nephrostomy	150
146. Orchidectomy	151
147. Orchidopexy	152
148. Percutaneous Nephrolithotomy / P.C.N.L	153
149. Prostatectomy	154
150. Radical Cystectomy	155
151. Torsion of Testes	156
152. T.U.R.B.T / Trans Urethral Resection of Bladder Tumour	157
153. T.U.R.P / Trans Urethral Resection Prostatectomy	158
154. Ureterolithotomy	159
155. Vasectomy	160
156. ***** Vascular	161
157. A.A.A / Abdominal Aortic Aneurysm	162
158. A.K.A / Above Knee Amputation / B.K/A / Below Knee Amputation	163
159. A.V / Arteriovenous / Fistula	164
160. Carotid Endarterectomy	165
161. E.V.A.R / Endovascular Aneurysm Repair	166
162. Femoral Embolectomy	167
163. Fasciotomy	168
164. F.P.B / Femoral Popliteal Bypass	169
165. Fistulotomy	170
166. Formation of RC (Radio Cephalic) AVF (Arteria Venous Fistula)	171
167. H.L.S / High Ligation & Strip / G.S.V / Greater Saphenous Vein	172
168. Ligation & Avulsion of Veins	173

1. ***** Cardiac

[\(Home\)](#)



2. ?????/

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Notes: is the surgical removal of part of the bone from the skull to expose the brain

Operating Table and patient positioning requirements

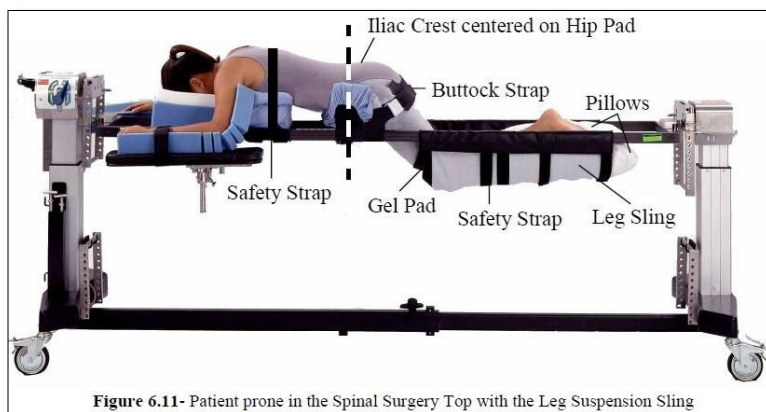


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Position: ...

Setup: ...

Notes:

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

3. ?????/

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements




In Room Equipment:

?????

Notes: is the surgical removal of part of the bone from the skull to expose the brain

Operating Table and patient positioning requirements

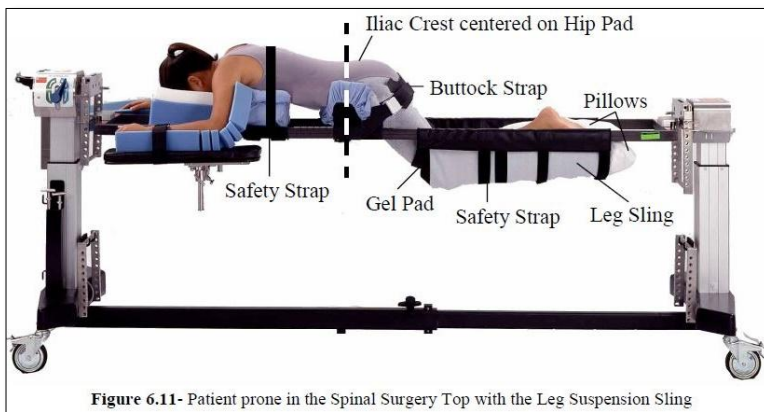

Position: ...

Setup: ...

Notes:

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

4. ***** Colorectal

[\(Home\)](#)



5. ?????/

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Notes: is the surgical removal of part of the bone from the skull to expose the brain

Operating Table and patient positioning requirements

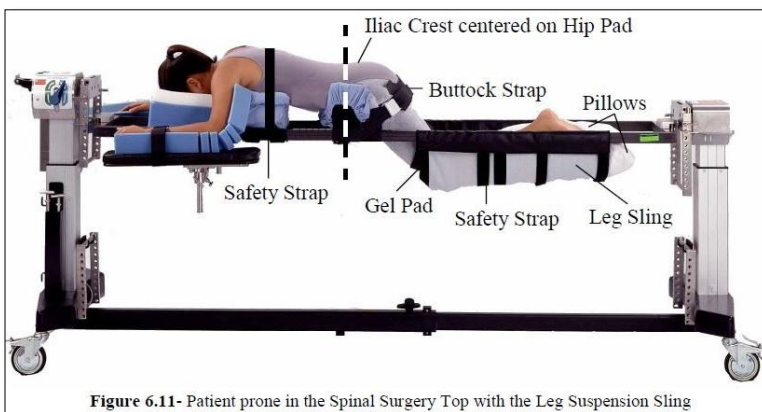


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Position: ...

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

6. ?????/

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Notes: is the surgical removal of part of the bone from the skull to expose the brain

Operating Table and patient positioning requirements

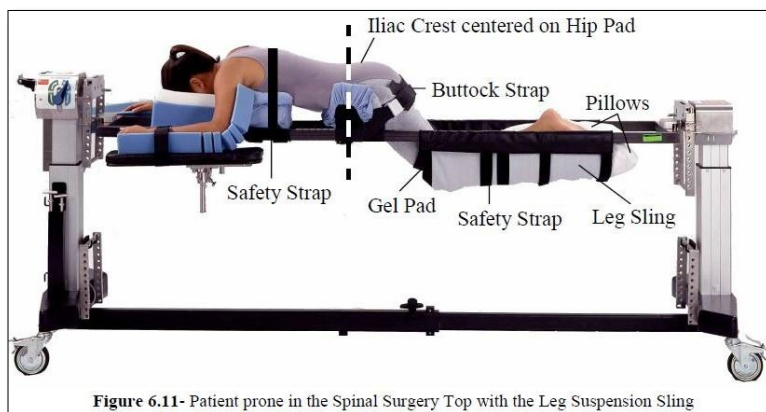


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Position: ...

Setup: ...

Notes:

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

7. ***** Dental

[\(Home\)](#)



8. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ????? is a

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

9. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ????? is a

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

10. ***** ECT

[\(Home\)](#)



11. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ???? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

12. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ???? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

13. ***** Emergency

[\(Home\)](#)



14. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ???? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

15. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ???? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

16. ***** ENT

[\(Home\)](#)



17. Tonsillectomy / Adenoidectomy / T.S / A.S

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

18. Modified Radical Mastoidectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

19. Meatoplasty

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

20. Myringoplasty

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

21. Pre-Auricular

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

22. Tympanoplasty

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

23. Grommets

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

24. Exostosis

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

25. Microlaryngoscopy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

26. Nasopharynx Biopsy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

27. E.U.A Ear / Examination Under Microscope

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

28. Turbinectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

29. Septoplasty

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

30. Papilloma

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

31. Tracheostomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

32. Tracheotomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

33. ***** Eyes or Ophthalmic

[\(Home\)](#)



34. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ????? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

35. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

Notes: A ????? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

36. ***** General

[\(Home\)](#)



37. Open Hernia Repairs / Herniorrhaphy

Inguinal - Umbilical - Incisional - Hiatus - Epigastric - Femoral – Incarcerated

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Is the surgical repair of hernias

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Matt / Megadyne Matt or Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

...

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

38. Esophagectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Harmonic Scalpel
Suction Canaster Tree

Notes: is a surgical procedure to remove some or all of the swallowing tube between your mouth and stomach (esophagus) and then reconstruct it using part of another organ, usually the stomach

Operating Table and patient positioning requirements



Position: Supine / **Arms out / tucked in?**

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 (or both arms tucked in) / Sheet on Table (Under Patient) / Heal Gels / Head Ring Gel / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

39. Open Appendicectomy / Gastrectomy / Laparotomy / Liver Resection / Right Hemicolectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Harmonic Scalpel
Suction Canaster Tree

Notes: ...

Operating Table and patient positioning requirements



Position: Supine / **Arms out / tucked in?**

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 (or both arms tucked in) / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

40. Hemicolectomy Left / Anterior Resection / Ultra-Low

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree
Harmonic Scalpel

Notes: is a surgery to remove the part of your large intestine called your colon

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

41. Hemicolectomy Right

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree
Harmonic Scalpel

Notes: is a surgery to remove the part of your large intestine called your colon

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Megadyne Matt or Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

42. Open Splenectomy / Lap Splenectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

(If Laparoscopic Pendant Stack Moved Into position)

SCD's Machine

Bair Hugger machine

Diathermy machine

2 x Suction Canaster Trees

Notes: is a surgical procedure to remove your spleen

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

43. Closure Ostiomyelitis

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

44. Lap Nissen Fundoplication

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Denyer Operating Table

Pendent Stack Moved Into position

SCD's Machine

Bair Hugger machine

Diathermy machine

Suction Canaster Tree

Harmonic Scalpel

Notes: In this procedure, the surgeon wraps the top of the stomach around the lower oesophagus

Operating Table and patient positioning requirements



Position: Lithotomy / Reverse Trendelenburg 45 Degree / Arms Out

Setup: ½ Gel Matt / Diathermy Plate / Arm Boards x 2 & Coban or crape bandage to secure / Table Light End / Leg Stirrups / Trenguard / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

Notes: Denyer Operating Table Required.

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

45. Hartman's Procedure

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree
Harmonic Scalpel
Thunderbeat (on the left side)

Notes: is a type of colectomy that removes part of the colon and sometimes rectum (proctosigmoidectomy). The remaining rectum is sealed, creating what is known as Hartmann's pouch

Operating Table and patient positioning requirements



Position: Supine / Arms Out (OR Lithotomy)

Setup: Gel Matt / Diathermy Plate / Arm Boards x 2 (or both arms strapped) / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

If Lithotomy – Light End / Stirrups / No Heal Gels

Notes:

Procedural Variations

Sometimes lithotomy (check with surgical team) – If Lithotomy Light end and Stirrups required

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

46. Whipples

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree
Harmonic Scalpel
Thunderbeat

Notes: is used to treat tumours and other disorders of the pancreas, intestine and bile duct

Operating Table and patient positioning requirements



Position: Supine / Left Arm Tucked In

Setup: Gel Matt / Diathermy Plate / Arm Boards x 2 until anaesthetised, then left arm tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

47. Anal Fistula / Fissure / Haemorrhoidectomy / Perianal Abscess / Advancement Flaps / Prolapse

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: ...

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

48. Thyroidectomy / Parathyroidectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Is the surgical removal of the Thyroid and Parathyroid glands from the neck

Operating Table and patient positioning requirements



Position: Supine / Arms Tucked In

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Gel Head Ring / Sandbag / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

49. Pilonidal Sinus V1 Lateral

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is a small hole or tunnel in the skin at the top of the buttocks, where they divide (the cleft)

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

Can be Lateral or Prone (Consult Surgical Team)

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

50. Pilonidal Sinus V2 Prone

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is a small hole or tunnel in the skin at the top of the buttocks, where they divide (the cleft)

Operating Table and patient positioning requirements



Position: Prone or Lateral (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards (until Anaesthetised) / 6 Pillows / Elastoplast or Slek to secure patient / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

Can be Prone or Lateral (Consult Surgical Team)

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

51. Laparoscopic Cholecystectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position

SCD's Machine

Bair Hugger machine

Diathermy machine

Suction Canaster Tree

Notes: is the inserting of a tiny video camera and special surgical tools through four small incisions to see inside the abdomen and remove the gallbladder

Operating Table and patient positioning requirements



Position: Supine / 1 Arm Tucked In

Setup: Gel Matt / Diathermy Plate / Arm Boards x 2 until anaesthetised, then 1 arm tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

52. Hysteroscopy / D&C / Cystoscopy / Most General Gynae / Laparoscopic Ablation of Endometriosis / Lap Assisted

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

53. ***** Gynae

[\(Home\)](#)



54. Bartholin's Abscess

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Overhead Lights / SCD's Machine / Bair Hugger machine / Diathermy machine / Suction Canaster Tree / Peri Table (Ask Surgeon) / Stool for Surgeon

Operating Table and patient positioning requirements



Lithotomy position
with direct placement
legholders

Position: Lithotomy/ Arms Out

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes: A Bartholin's cyst is a fluid-filled lump near the vaginal opening

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

55. B.S.O – Bilateral Salpingopaxy Oophorectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendant Stack and Monitors
Overhead Lights
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree
Ligature Machine
3 Ltr Glycine

Notes: A bilateral salpingo-oophorectomy is a surgery to remove both fallopian tubes and both ovaries

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

56. Cone Biopsy of the Cervix

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: This procedure removes a cone-shaped piece of tissue containing the abnormal cells from the cervix

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

57. D&C – Dilatation and Curettage

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is a procedure to remove tissue from inside the uterus

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

58. Ectopic Pregnancy - Laparoscopically

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Salpingostomy and salpingectomy are two laparoscopic surgeries used to treat some ectopic pregnancies

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

59. Hysteroscopy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is a procedure used to examine the inside of the womb (uterus)

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

60. Hysterectomy / Total Abdominal Hysterectomy / T.A.H

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: A partial hysterectomy removes the uterus. A total hysterectomy removes the uterus and the cervix

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

61. Hysterectomy / Vaginal / Laparoscopic

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is a procedure to remove the uterus through an incision in the vagina

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

62. L.L.E.T.Z – Large Loop Excision of Transformation Zone

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is an operation done to remove abnormal cells from the cervix or the neck of the womb

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

63. L.U.C.C.S – Lower Uterine Segment Caesarean Section

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is the most commonly used type of Caesarean section.

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

64. Pelvic Mass

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is a growth that happens near or in the fallopian tubes, ovaries, uterus, and connecting tissues

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

65. P.P.H – Post Partum Haemorrhage

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is heavy bleeding after the birth

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

66. Salpingostomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is the surgical removal of a fallopian tube

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

67. T.A.H – Total Abdominal Hysterectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is the Surgical removal of the uterus along with the cervix through the abdomen

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

68. Vaginal Hysterectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is a procedure to remove the uterus through an incision in the vagina

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

69. Trial By Forceps

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Is an attempt to deliver a baby naturally before reverting to Caesarean Section

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

70. Ventouse

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is a method to assist delivery of a baby using a vacuum device

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

71. Ventrosuspension

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is the surgical fixation of a displaced uterus to the anterior abdominal wall

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

72. Vulvectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: is a procedure where a surgeon removes all or part of the vulva

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

73. 3rd Degree Tear

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: is a tear that extends into the muscle that controls the anus (the anal sphincter)

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trendelenburg (consult surgical team)

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

74. ***** Maxillo Facial

[\(Home\)](#)



75. C.A.T / Combined Approach Tympanoplasty / M.R.M / Modified Radical Meatoplasty

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

76. Tracheostomy / Dental Extractions / Bilateral Neck Dissection / Lip Split / Resection of Lesion / Radical Forearm Flap Reconstruction

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

77. ***** Neuro

[\(Home\)](#)



78. Craniotomy - With Stealth

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.


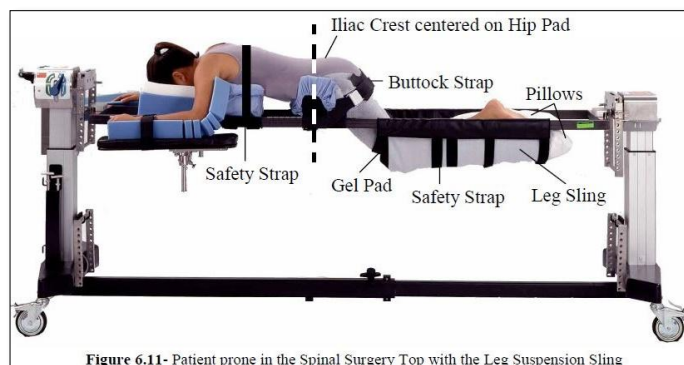


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling

Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Mayfield/Doro Head Section w/ Skull Clamp	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do NOT over-tighten). Place skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile blue control plate and pointer (found in Stealth drawer) on the mayo stand with the head clamp and adjustable Medtronic arm. Attach foot pedal and position on floor at head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Only SDC required only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill remains attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. <u>Note:</u> If semi lateral Collar & Cuff will be required.

79. INTER-CRANIAL ANEURYSM – With Stealth


(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

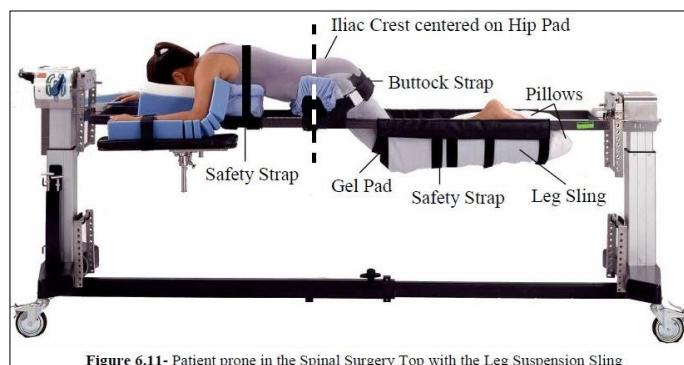

Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Doro Head Section	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do NOT over-tighten). Place Doro skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile blue control plate and pointer (found in Stealth drawer) on the mayo stand with the head clamp and adjustable Medtronic arm. Attach foot pedal and position on floor at head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
High Suction Unit	Fitted to anaesthetic ceiling boom. Place unit to patient's head, beside anaesthetic machine.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill remains attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Config of Tube to "Left and Right". Set User to "Infrared 800". Ensure eye piece fitted to correct side before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. Note: If semi lateral Collar & Cuff will be required.

80. Craniotomy / Shunt – With Axiom


(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

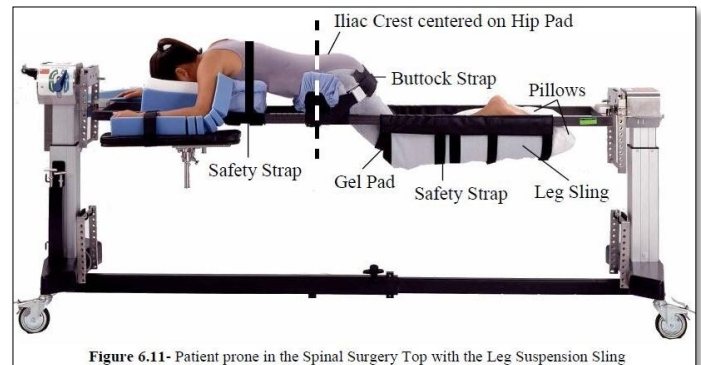

Equipment	Position and Settings
Eschmann Operating Table (Head Section Removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Mayfield/Doro Head Section w/ Horseshoe	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do NOT over-tighten).
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile corded tracer (found in Stealth drawer) on the mayo stand with adjustable Medtronic arm. Note: Use Medtronic arm with black frame attached, use tongue depressor or comb as a spacer when fitting to the Eschmann rail.
Medtronic Stealth Axiom	Hang Axiom on the foot end of the operating table, to the patient's left. Connect Axiom to Stealth system with corresponding coloured cables of which there are 3 as well as the power cord, ie: Green to green, blue to blue, etc. Connect foot pedal and position on floor to head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. SDC, camera and light box required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to be attached to IV pole behind suction unit with 1x 1L bag of room temperature sodium chloride hung above. Foot pedal to be placed at head end of operating table.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. Note: If semi lateral Collar & Cuff will be required.

81. Sub-Dural Haematoma / Burr Hole / EVD / ICP (Emergency)


(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

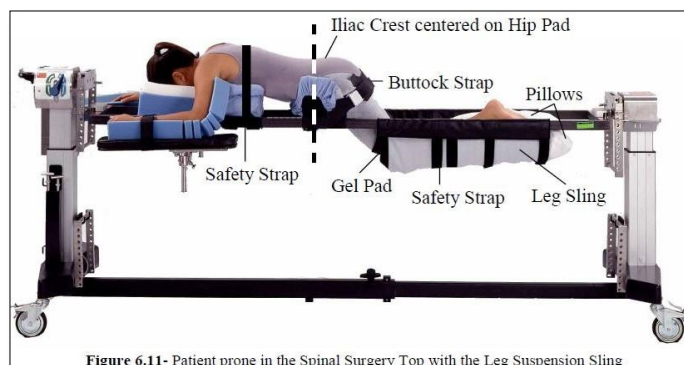

Equipment	Position and Settings
Eschmann Operating Table (Head Section Removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Mayfield/Doro Head Section w/ Horseshoe	Fit to head end of table. Tape horseshoe gels if loose and cover. Ensure all sections secure together firmly (do NOT over-tighten).
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Only SDC required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Extras Required	Shoulder roll (size may vary), 2x Arm gels, 2x J boards, 1x Pillow, 2x Heel gels, Half-length gel mat/Megadyne, SCD machine, Side support w/ Leg strap required if tilting operating table, bear hugger, foam for pressure areas. <u>Note:</u> If semi lateral Collar & Cuff will be required.

82. Craniotomy- Intraoperative MRI With Skull Clamp


(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

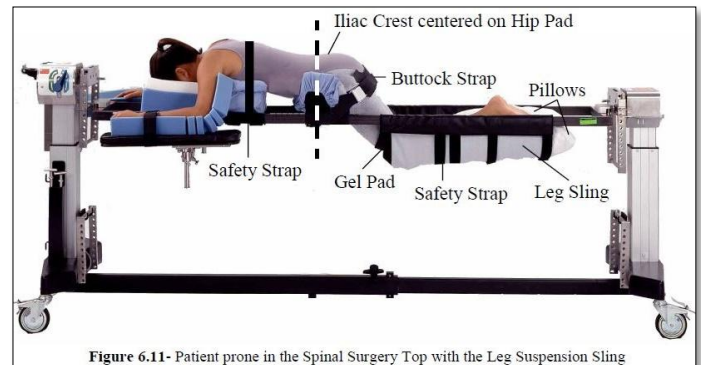

Equipment	Position and Settings
Maquet Magnus w/ Transfer Bed and Trolley	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted.
Carbon Fibre Headset w/ Carbon Fibre Clamp (MRI Compatible Tray)	Fit square plate to head end of table with four lug screws. Use black handled 'star' screwdriver to loosen all joints. Place carbon fibre head clamp (with un-threaded centre hole) on Mayo stand with MRI safe pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Settings for Bi/Monopolar, from left to right, are as follows: 15/0/25. Note: Do NOT use Megadyne gel mattress for MRI transfers).
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile blue control plate, and tracer (found in Stealth drawer) on the mayo stand with the head clamp and adjustable <u>MRI compatible</u> Medtronic arm. Attach foot pedal and position on floor at head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Only SDC required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	1x Pillow, 2x MRI J boards, 2x Heel gels, Half-length gel mat, 2x Arm gels, Shoulder roll (size may vary), SCD machine, Side support w/ Leg strap required if tilting operating table, 2x MRI clearance spacers, 1x Extra Maquet knuckle and ENT arm rest found OT14 (only if ENT surgeon present), bear hugger, foam for pressure areas.

83. Trans-Sphenoidal Tumour Resection – Intraoperative MRI With Head Ring


(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

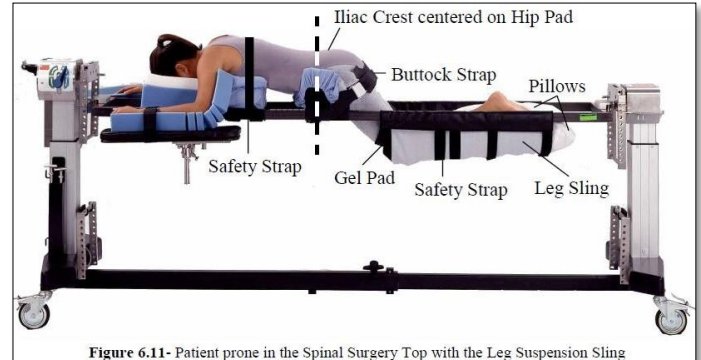

Equipment	Position and Settings
Maquet Magnus w/ Transfer Bed and Trolley	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Head ring placed under patient's head. Note: If table slide not in correct orientation, table remote will alarm when use attempted.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Settings for Bi/Monopolar, from left to right, are as follows: 15/0/25. Note: Do NOT use Megadyne gel mattress for MRI transfers).
Medtronic Stealth	Position Stealth to left side of diathermy. Place unsterile corded tracer (found in Stealth drawer) on the mayo stand with adjustable MRI compatible Medtronic arm. Note: If using ENT user settings scrub team to provide unsterile metal tracer.
Medtronic Stealth Axiom	Hang Axiom on the foot end of the operating table, to the patient's left. Connect Axiom to Stealth system with corresponding coloured cables of which there are 3 as well as the power cord, ie: Green to green, blue to blue, etc. Connect foot pedal and position on floor to head end of operating table.
Sonopet	Position Sonopet to left side of Stealth. Place room temperature 500mL bag of sodium chloride, unopened, on IV hanging rail provided. Position foot pedal on floor at head end of operating table.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. SDC, camera and light box required.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to be attached to IV pole behind suction unit with 1x 1L bag of room temperature sodium chloride hung above. Foot pedal to be placed at head end of operating table.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Left and Right". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing, eg. if operating on the left side, eye piece to be fitted to right side of microscope.
Extras Required	1x Pillow, 2x MRI J boards, 2x Heel gels, Half-length gel mat, 2x Arm gels, Shoulder roll (size may vary), SCD machine, Side support w/ Leg strap required if tilting operating table, 2x MRI clearance spacers, 1x Extra Maquet knuckle and ENT elbow rest found OT14 (required only if ENT surgeon present), bear hugger, foam for pressure areas.

84. Cervical Laminectomy – With Pillows “BOWS” With Xray


(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

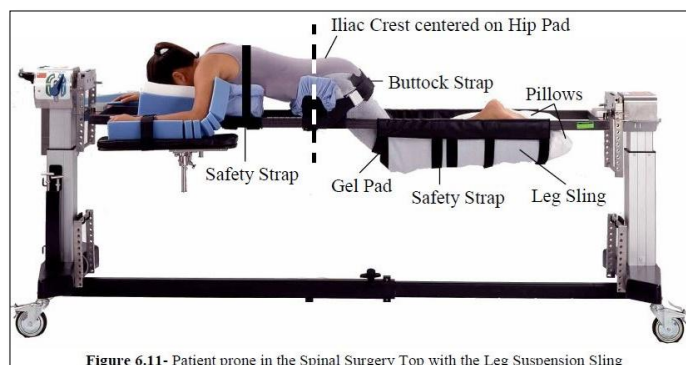

Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Arm boards removed. Sheet draped laterally across table, on top of pillows, for arm tuck. Brakes applied.
Mayfield/Doro Head Section	Fit to head end of table. Horseshoe not required. Ensure all sections secure together firmly (do NOT over-tighten). Place skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to “Face to Face”. Set User to “Neurosurgery User”. Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	5x Pillows (four taped together in pairs, one at the feet), 3x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas

85. Cervical Laminectomy – With Montreal Mattress – With Xray

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

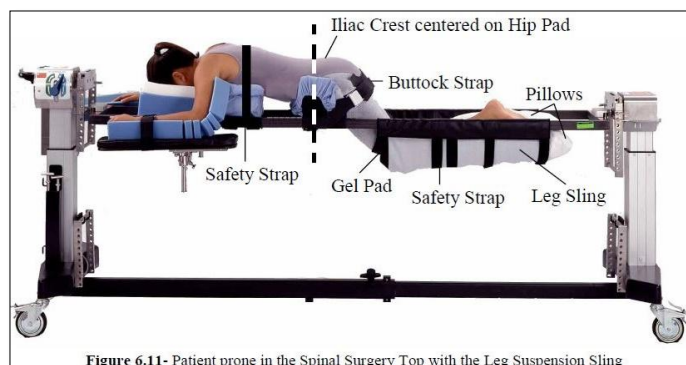

Equipment	Position and Settings
Eschmann Operating Table (Head section removed)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Arm boards removed. Sheet draped laterally across table, on top of Montreal Mattress, for arm tuck. Brakes applied.
Montreal Mattress	Placed directly onto Eschmann pads, to head end of table.
Mayfield/Doro Head Section	Fit to head end of table. Horseshoe not required. Ensure all sections secure together firmly (do NOT over-tighten). Place skull clamp on Mayo stand with pins.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x Pillows, 1x sheet, 3x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas.

86. Cervical Laminectomy – Compress Roll – With Xray

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

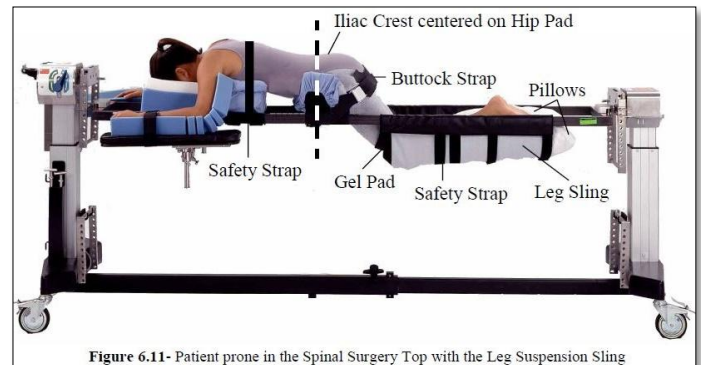


Figure 6.11- Patient prone in the Spinal Surgery Top with the Leg Suspension Sling


Equipment	Position and Settings
Jackson Operating Table w/ Flat Top	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pin top "H" bar to both head end, and foot end of Jackson table. Note: Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Spinal Frame	Head rest and sling removed. Pre-fit frame with chest pad, Regular Patient hip pads, 2x foot plates and all Mizuno-Osi pad covers. Have 2 Jackson pins ready to fit to top "H" frame when. 6 (six) straps will be required to secure patient for the roll, these will be found with Doro Frame inside Blue "Spinal Kit" in the set-up room.
Jackson Compatible Doro Frame w/ Skull Clamp	Doro frame will secure to central "H" bar at head-end of Jackson operating table. Patient will be pinned and secured before the roll occurs.
Jackson Pad Pack	1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Jackson Table w/ Flat Top	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pin top "H" frame to head end of Jackson table. 1x bed sheet draped across for arm tuck.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	4x Pillows, 1x gel mat, 2x sheets, 3x roll of wide Elastoplast, 6x straps, SCD, bear hugger, foam for pressure areas.

87. Anterior Cervical Discectomy Fusion (ACDF) With Xray V1

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Li Yang

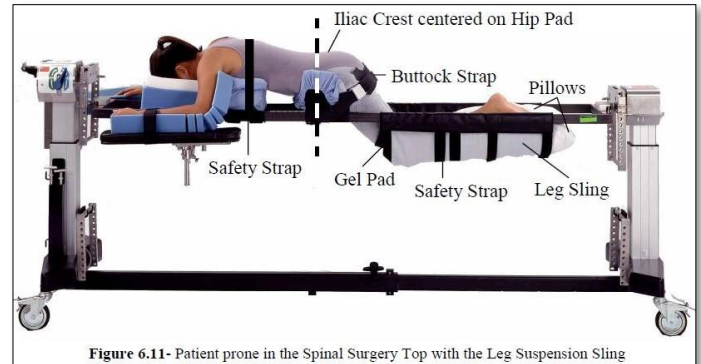


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Arm boards removed. Sheet draped laterally across table for arm tuck. Desired head-ring placed, on absorbent pad, at head end of table. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll (size may vary), 2x arm gel, 1x sheet (arm tuck), 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas.

88. Anterior Cervical Discectomy Fusion (ACDF) With Xray V2

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Li Yang

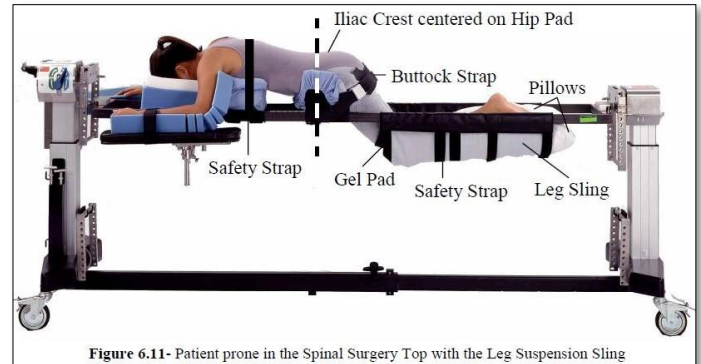


Equipment	Position and Settings
Jackson Table w/ Flat Top	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pin top "H" bar to head end of Jackson table. 1x bed sheet draped across for arm tuck. Note: Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll, 2x arm gel, 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas

89. Anterior Cervical Discectomy Fusion (ACDF) With Xray V3

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Jonathan, Dr. Stephenson & Dr. Withers

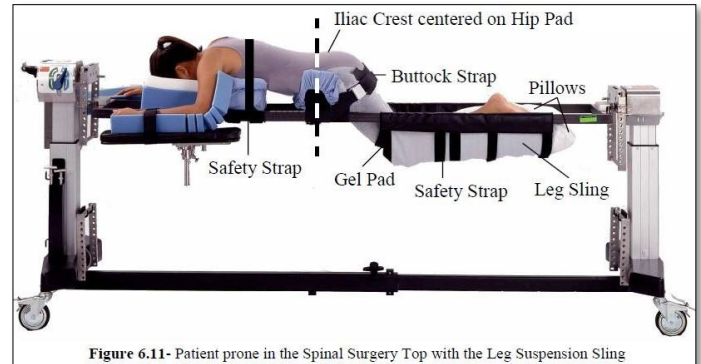


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Arm boards removed. Sheet draped laterally across table for arm tuck. Desired head-ring placed, on absorbent pad, at head end of table. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed toward head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll (size may vary), 2x arm gel, 1x sheet (arm tuck), 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas

90. Anterior Cervical Discectomy Fusion (ACDF) With Xray V4

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Wayne Ng

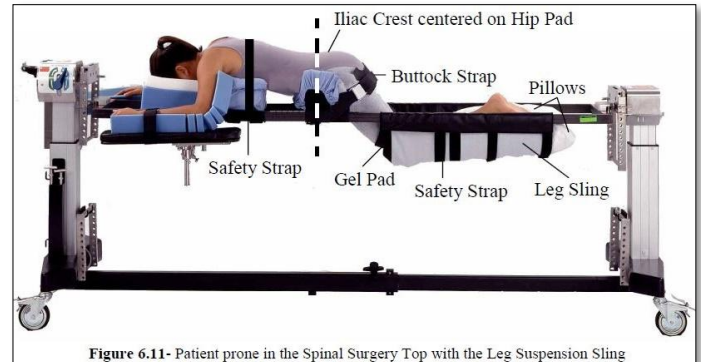


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Arm boards removed. Sheet draped laterally across table for arm tuck. Gel head-ring placed at head end on top of absorbent pad. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Reg" with operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	1x gel head-ring, 1x folded towel, 1x rolled towel, 1x shoulder roll, 2x arm gel, 1x Pillows (under knees), 2x heel gel, 1x roll of wide Elastoplast, SCD, bear hugger, foam for pressure areas.

91. Anterior Cervical Discectomy Fusion (ACDF) With Xray V5

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Withers, Dr. Stephenson, Dr. Li Yang & Dr. Poulgrain

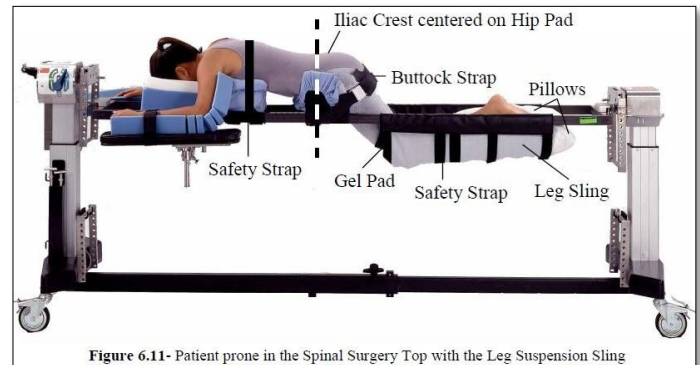


Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). Note: Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, chest plate, 2x regular patient pads, sling fitted with gel mattress and 3 pillows. Black Jackson knuckle to be fitted to frame for surgical retractor, confirm position with surgical registrar.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam, 1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 3x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger.

92. Laminectomy / Microdiscectomy – With Xray V1

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Jonathan

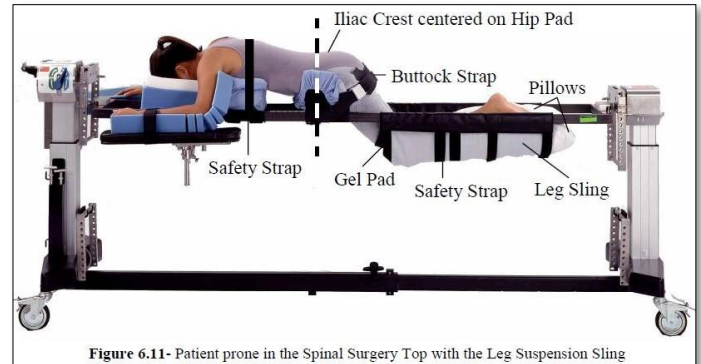


Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). Note: Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, chest plate, 2x thigh pads, sling fitted with gel mattress and 3 pillows. Black Jackson knuckle to be fitted to frame for surgical retractor, confirm position with surgical registrar.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam, 1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 3x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger

93. Laminectomy / Microdiscectomy – With Xray V2

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Wayne Ng

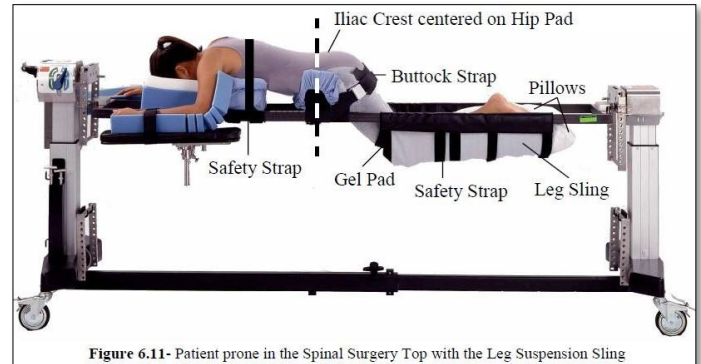


Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Head-end of spinal frame pinned at 5 th hole from the bottom of "H" bar, foot-end of spinal frame pinned at lowest hole. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). Note: Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, Wilson Frame, 2x foot plates with gel mattress and 2 pillows. Black Jackson knuckle to be fitted to frame for surgical retractor, confirm position with surgical registrar.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, and to left side of stack. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 3x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger.

94. Spinal Fusion (Inc TLIF) With O-Arm

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Stephenson, Dr. Wayne Ng & Dr. Li Yang

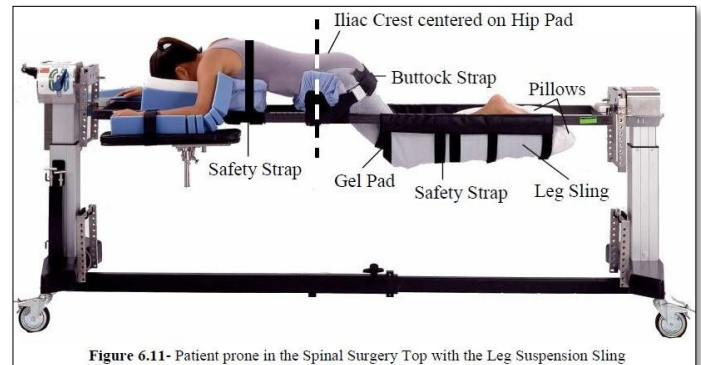


Equipment	Position and Settings
Jackson Operating Table w/Spinal Frame	Position table laterally, from left-to-right, under ceiling light podium with head end to anaesthetic machine and foot end towards theatre window. Pre-fit and position both arm-boards, remove left arm-board only and store under table (fit when patient has been positioned). Note: Ensure brakes applied, all table pins are secured correctly, and base lug is fastened.
Jackson Positioning Configuration	Fit from head-end to foot-end: Arm boards, face plate, chest plate, 4x regular patient pads, 2x foot plate with gel mattress and 2 pillows.
Jackson Pad Pack	1x Face foam (confirm style with anaesthetic consultant), 2x arm foam, 1x chest pad, 2x patient pad covers.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor toward head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, beside Stealth. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Medtronic Stealth	Positioned to left of theatre stack. VGA cable to connect to ANA socket on theatre stack with feed linked to Monitor 1.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece secured before balancing.
Extras Required	Face foam, Jackson pack, 2x pillows, 1x gel mat, 1x sheet, SCD, foam for pressure areas, 2x bear hugger

95. Spinal Fusion (XLIF) With Xray

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Stephenson, Dr. Wayne Ng & Dr. Li Yang

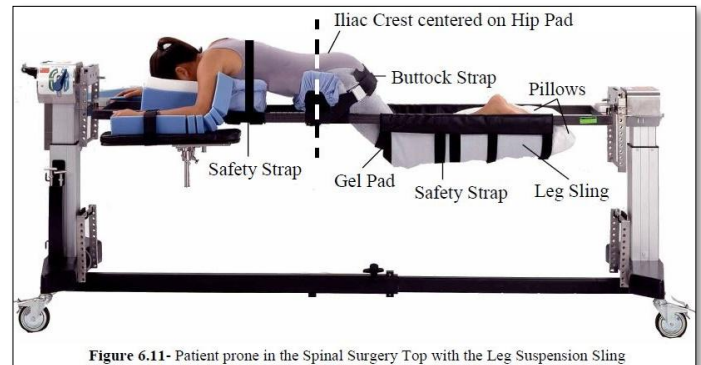


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor at head end of operating table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Medtronic IPC (Midas Rex) or Stryker Core Drill (see DR Preference)	Drill to remain attached to stack. Foot pedal to be placed at head end of operating table and attached to console once the patient is positioned.
Microscope	Powered on with light turned off. Turn Focus Light off. Set Configuration of Tube to "Face to Face". Set User to "Neurosurgery User". Ensure eye piece fitted to correct side, and secured, before balancing.
Extras Required	2x Pillows, 1x shoulder roll, 2x lateral supports, 1x arm gutter, 4x Elastoplast (wide), SCD, bear hugger, foam for pressure areas

96. Carpal Tunnel Repair (Right)

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: Dr. Stephenson, Dr. Wayne Ng & Dr. Li Yang

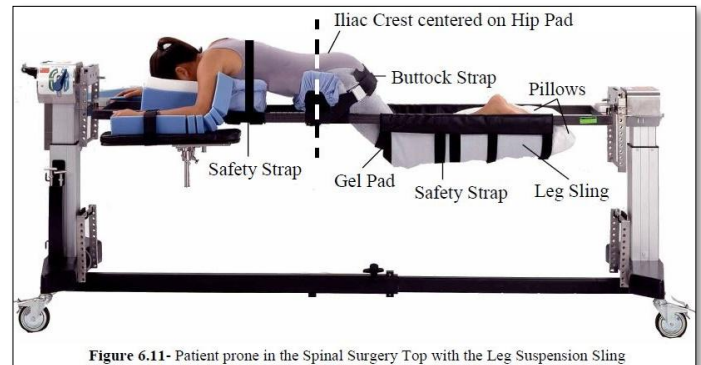


Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table straight, front-to-back, under ceiling light podium, with foot end towards the rear of theatre. Left arm-board fitted. Brakes applied.
Arm Table	To be fitted to patient's right once positioned on the bed.
Tourniquet	Note: Only Dr. Poulgrain will use tourniquet, and only if procedure performed under general anaesthesia.
Diathermy	Position diathermy at foot end of the operating table with room to walk behind. Position foot pedal on floor under arm table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand to right side of diathermy. Ensure high and low suction tubing is attached to the correct outlet. Low suction operating pressure set between 10-20Psi.
Theatre Stack	Position theatre stack to right side of suction unit. Turn on SDC only.
Extras Required	1x Pillows, 1x shoulder roll, SCD, bear hugger, foam for pressure areas

97. Carpal Tunnel Repair (Left)

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.



Consultants: All

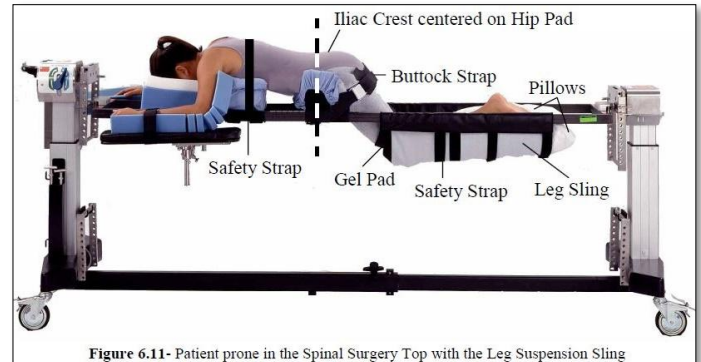

Equipment	Position and Settings
Eschmann Operating Table (Head section fitted)	Position table laterally, from left-to-right, under ceiling light podium, with foot end towards theatre window. Arm boards removed. Brakes applied.
Arm Table	To be fitted to patient's left once positioned on the bed.
Tourniquet	Note: Only Dr. Poulgrain will use tourniquet, and only if procedure performed under general anaesthesia.
Diathermy	Position diathermy at foot end of the operating table, to right of theatre stack. Position foot pedal on floor under arm table. Standard settings for Bi/Monopolar, from left to right, are as follows: 15/0/25.
Four-way Suction Unit	Position suction stand at foot end of operating table, beside Stealth. Ensure high and low suction tubing is attached to the correct outlet. Suction regulator set to "Full".
Theatre Stack	Position theatre stack to foot end of operating table. Turn on SDC only.
Extras Required	1x Pillows, 2x J-boards, 1x shoulder roll, SCD, bear hugger, foam for pressure areas

98. ***** Orthopaedics

[\(Home\)](#)



99. P&P / Pin and Plate / Canulated Hip Screw

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Tucked In

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

100. Archilles Tendon Repair

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Tucked In

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

101. Carpel Tunnel Release

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

102. Cubital Tunnel Release

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

103. D.P.C / Direct Primary Closure

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Tale / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

104. Dupuytren's Contracture

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Tucked In

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

105. Arthroscopy Knee

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Bone Foam / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

106. M.U.A / Manipulation under Anaesthetic / Ulna - Radius

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

107. O.I.F / Open Reduction Internal Fixation / Ankle

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

108. O.I.F / Open Reduction Internal Fixation / Clavicle

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Table – Beach Chair
 SCD's Machine
 Bair Hugger machine
 Diathermy machine
 Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Beach Chair

Setup: ...

Notes:

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

109. O.I.F / Open Reduction Internal Fixation / Distal Humorous

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

110. O.I.F / Open Reduction Internal Fixation / Proximal Humorous

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

111. O.I.F / Open Reduction Internal Fixation / Femur

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

112. O.I.F / Open Reduction Internal Fixation / Olecranon / Elbow

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

113. R.C.R / Rotator Cuff Repair

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Table Beach Chair
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Beach Chair

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

114. Tendo/ Repair / Nerve Repair / Upper Limb

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

115. Tibial Plateau

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

116. T.K.R / Total Knee Replacement

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

117. T.H.R / Total Hip Replacement

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

118. Vac Dressing Change

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

119. ***** Paediatrics

[\(Home\)](#)



120. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

)

Notes: A ????? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

121. ?????

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

?????

Operating Table and patient positioning requirements



Position: ?????

Setup: ?????

)

Notes: A ????? is a ?????

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

122. ***** Thoracic

[\(Home\)](#)



123. Anterior Mediastinoscopy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

124. Lobectomy / Excision of Lung Lobe

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

125. Lung Lavage

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

126. Mediastinotomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

127. Pleurectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

128. Peritoneal Shunt Insertion / Pleuro

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

129. Pneumonectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

130. Thoracoscopy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

131. Thoracotomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

132. ***** Urology

[\(Home\)](#)



133. Circumcision

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

134. Cystectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

135. Cystoscopy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

136. Dorsal Slit

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

137. Excision Of Bladder Endometrioma (Laparoscopically)

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Treguard (consult surgical team)

Notes: May Require Treguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

138. Hydrocele

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

139. Ileal Conduit

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

140. Stent Insertion

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

141. Laparoscopic Deroofing of Renal Cyst

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

142. Lithotripsy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

143. Lithopaxy / Litholapaxy / Cisto-Litholapaxy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

144. Nephrectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

145. Nephrostomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

146. Orchidectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

147. Orchidopexy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

148. Percutaneous Nephrolithotomy / P.C.N.L

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

Starting in Lithotomy – Then Going Prone

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

149. Prostatectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

150. Radical Cystectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

151. Torsion of Testes

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

152. T.U.R.B.T / Trans Urethral Resection of Bladder Tumour

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

153. T.U.R.P / Trans Urethral Resection Prostatectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

Pendent Stack Moved Into position
SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lithotomy/ Arms Tucked In

Setup: ½ Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Table Head End Removed / Table Light End Attached / Leg Stirrups / Sheet on Table (Under Patient) / Bair Hugger / Warm Blanket

May Require Trenguard (consult surgical team)

Notes: May Require Trenguard (Consult surgical team)

Procedural Variations

....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

154. Ureterolithotomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Lateral or Prone (ask surgeon)

Setup - Lateral: Gel Mat / Diathermy Plate / Arm Boards / Arm Gutter / Rotator Knuckles / Front and Back Lateral Supports / Pillow for between Legs / Sheet on Table (Under Patient) / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

155. Vasectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

156. ***** Vascular

[\(Home\)](#)



157. A.A.A / Abdominal Aortic Aneurysm

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree
Light Source
Cell Saver

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

158. A.K.A / Above Knee Amputation / B.K/A / Below Knee Amputation

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

159. A.V / Arteriovenous / Fistula

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out / Arm Table

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then Arm Table / Sheet on Table (Under Patient) / Heal Gels / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

160. Carotid Endarterectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Tucked In

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2 until anaesthetised, then both arms tucked in / Sheet on Table (Under Patient) / Heal Gels / Gel Head Ring / Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

161. E.V.A.R / Endovascular Aneurysm Repair

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

162. Femoral Embolectomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position: Supine / Arms Out

Setup: Gel Mat / Diathermy Plate / Arm Boards x 2
/ Sheet on Table (Under Patient) / Heal Gels /
Surgical Access Bair Hugger / Warm Blanket

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

163. Fasciotomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

164. F.P.B / Femoral Popliteal Bypass

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

165. Fistulotomy

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

166. Formation of RC (Radio Cephalic) AVF (Arteria Venous Fistula)

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

167. H.L.S / High Ligation & Strip / G.S.V / Greater Saphenous Vein

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canaster Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised

168. Ligation & Avulsion of Veins

(Home) Important: Confirm all requirements with surgical team prior to setup. This includes Theatre table orientation, patient positioning and theatre equipment requirements.

In Theatre Requirements



In Room Equipment:

SCD's Machine
Bair Hugger machine
Diathermy machine
Suction Canister Tree

Notes: Position Pendant Lights:

Operating Table and patient positioning requirements



Position:

Setup: ...

Notes:

Procedural Variations

.....

In theatre assistance requirements:

EG: Reposition Patient once anaesthetised